

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
 Data File : PL075871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 15:22
 Operator : AR\AJ
 Sample : N3390-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-2-061722RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:50:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.637	6067349	14198053	8.990	8.460
28)	SA Decachlor...	11.636	10.378	31758651	59656373	51.874	42.341
Target Compounds							
11)	B alpha-Chl...	8.474	7.403	3930780	9147914	5.154	5.010
12)	B 4,4'-DDE	8.656	7.620	3992264	5659212	6.032	3.540 #
13)	MA Dieldrin	8.811	7.758	704651	11682866	0.975	6.902 #
16)	A 4,4'-DDD	9.201	8.202	5058852	1707154	9.246	1.298m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
Data File : PL075871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 15:22
Operator : AR\AJ
Sample : N3390-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
PT-2-061722RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2022
Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:50:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

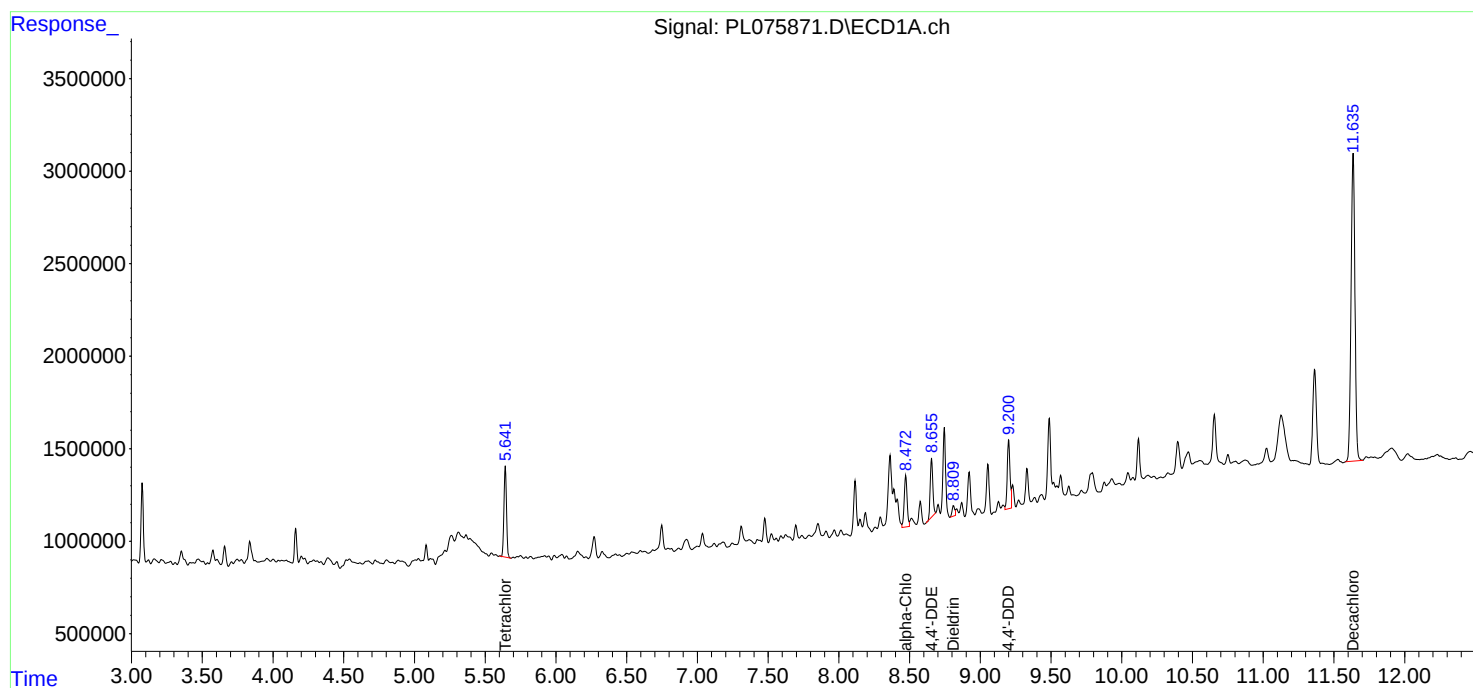

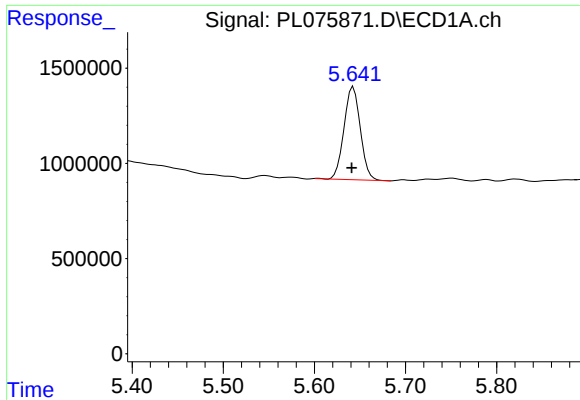


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 6067349
Conc: 8.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-2-061722RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

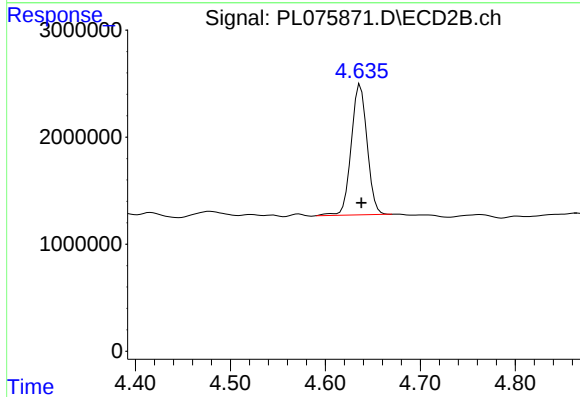


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 14198053
Conc: 8.46 ng/ml

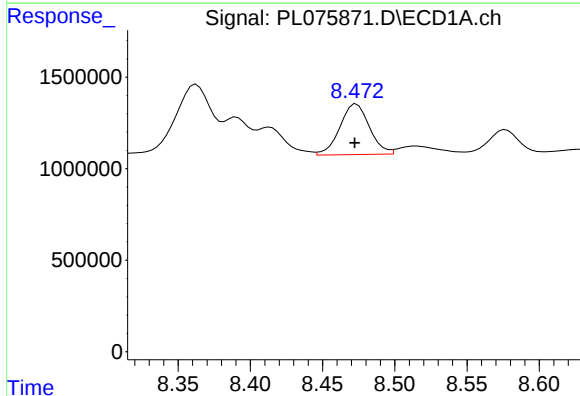


#11 alpha-Chlordane

R.T.: 8.474 min
Delta R.T.: 0.001 min
Response: 3930780
Conc: 5.15 ng/ml

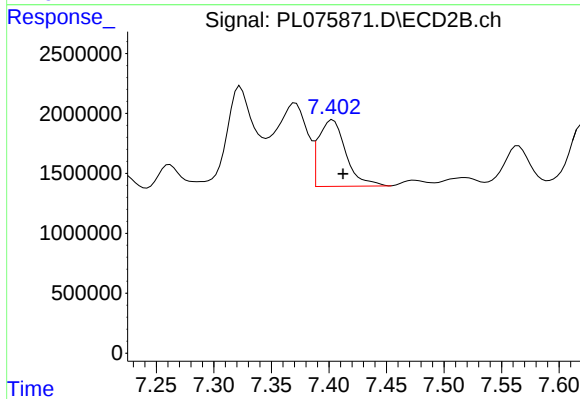

#11 alpha-Chlordane

R.T.: 7.403 min
Delta R.T.: -0.009 min
Response: 9147914
Conc: 5.01 ng/ml

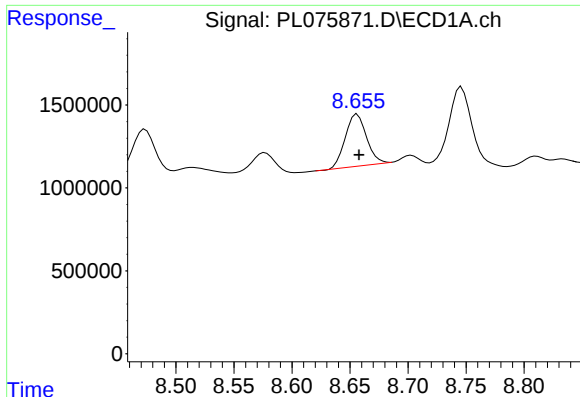


#12 4,4'-DDE

R.T.: 8.656 min
Delta R.T.: -0.002 min
Response: 3992264
Conc: 6.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-2-061722RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

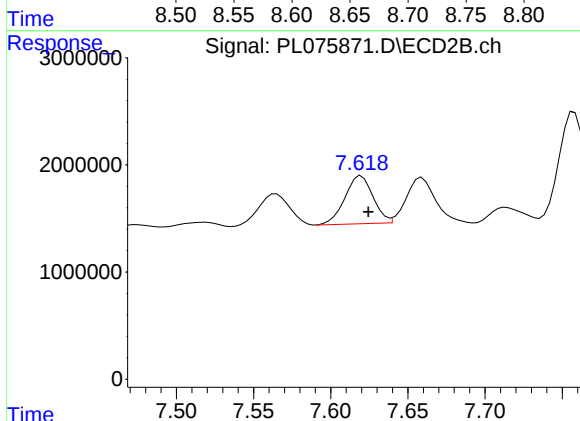


#12 4,4'-DDE

R.T.: 7.620 min
Delta R.T.: -0.005 min
Response: 5659212
Conc: 3.54 ng/ml

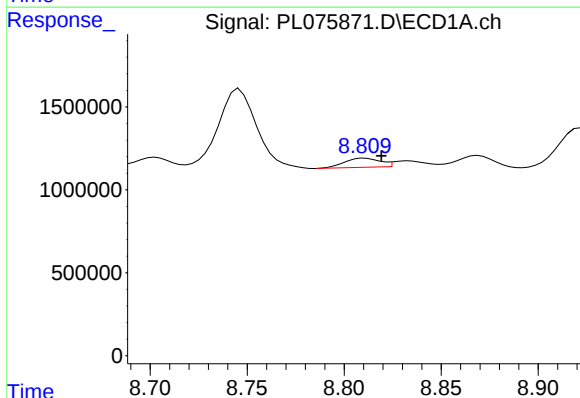


#13 Dieldrin

R.T.: 8.811 min
Delta R.T.: -0.008 min
Response: 704651
Conc: 0.98 ng/ml

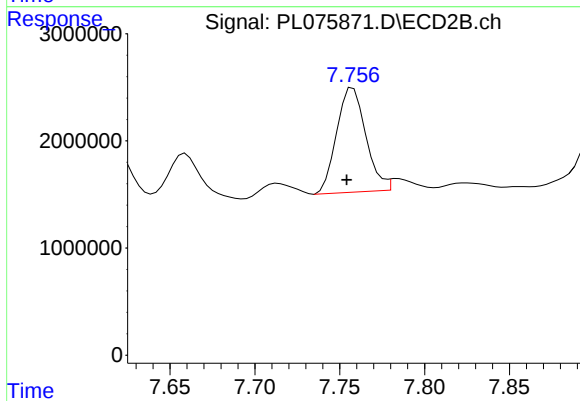

#13 Dieldrin

R.T.: 7.758 min
Delta R.T.: 0.004 min
Response: 11682866
Conc: 6.90 ng/ml

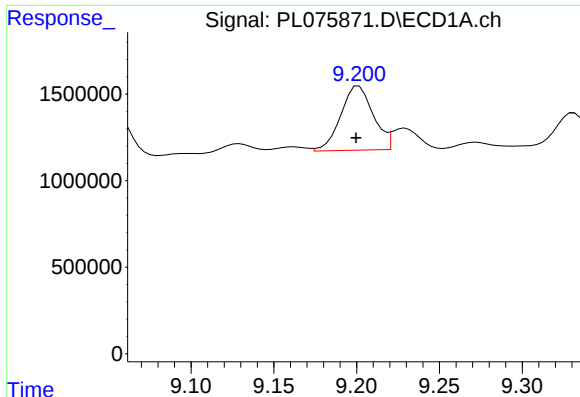


#16 4,4'-DDD

R.T.: 9.201 min
Delta R.T.: 0.002 min
Response: 5058852
Conc: 9.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-2-061722RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

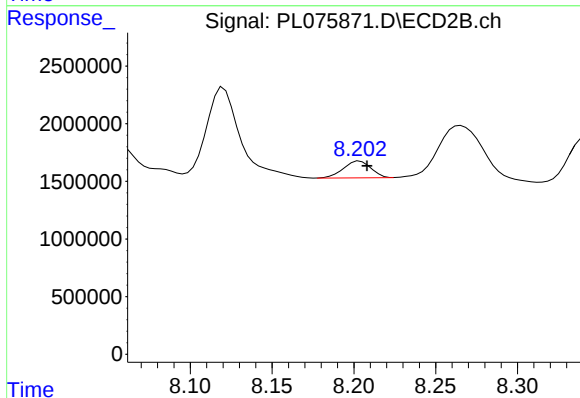


#16 4,4'-DDD

R.T.: 8.202 min
Delta R.T.: -0.006 min
Response: 1707154
Conc: 1.30 ng/ml m

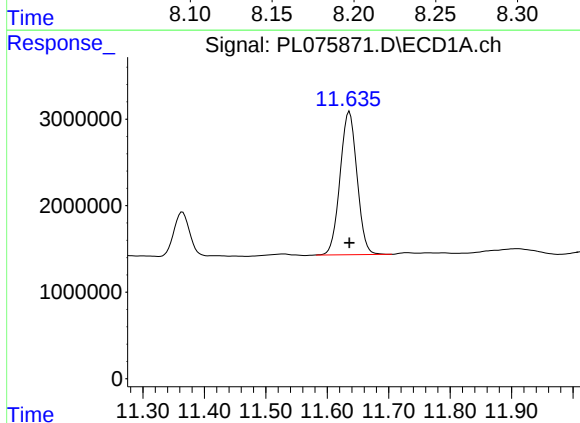

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 31758651
Conc: 51.87 ng/ml

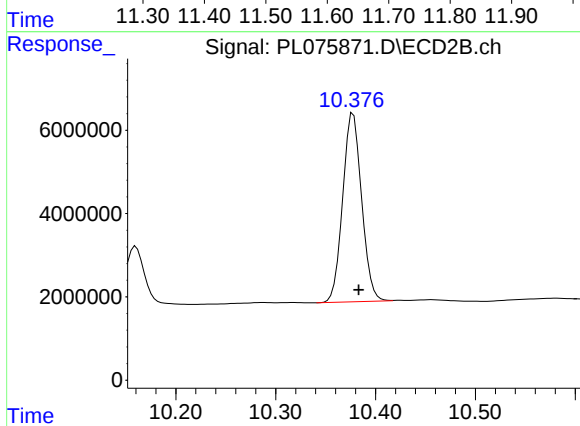

#28 Decachlorobiphenyl

R.T.: 10.378 min
Delta R.T.: -0.006 min
Response: 59656373
Conc: 42.34 ng/ml