

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062123\
 Data File : PD075939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 13:06
 Operator : AR\AJ
 Sample : PIBLK171
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:25:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.767	43691882	20839576	21.856	20.555
27)	SA Decachlor...	9.089	7.912	103.0E6	43038862	44.900	45.830
Target Compounds							
4)	MA Heptachlor	4.944	0.000	3623395	0	1.117	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062123\
Data File : PD075939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 13:06
Operator : AR\AJ
Sample : PIBLK171
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:25:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

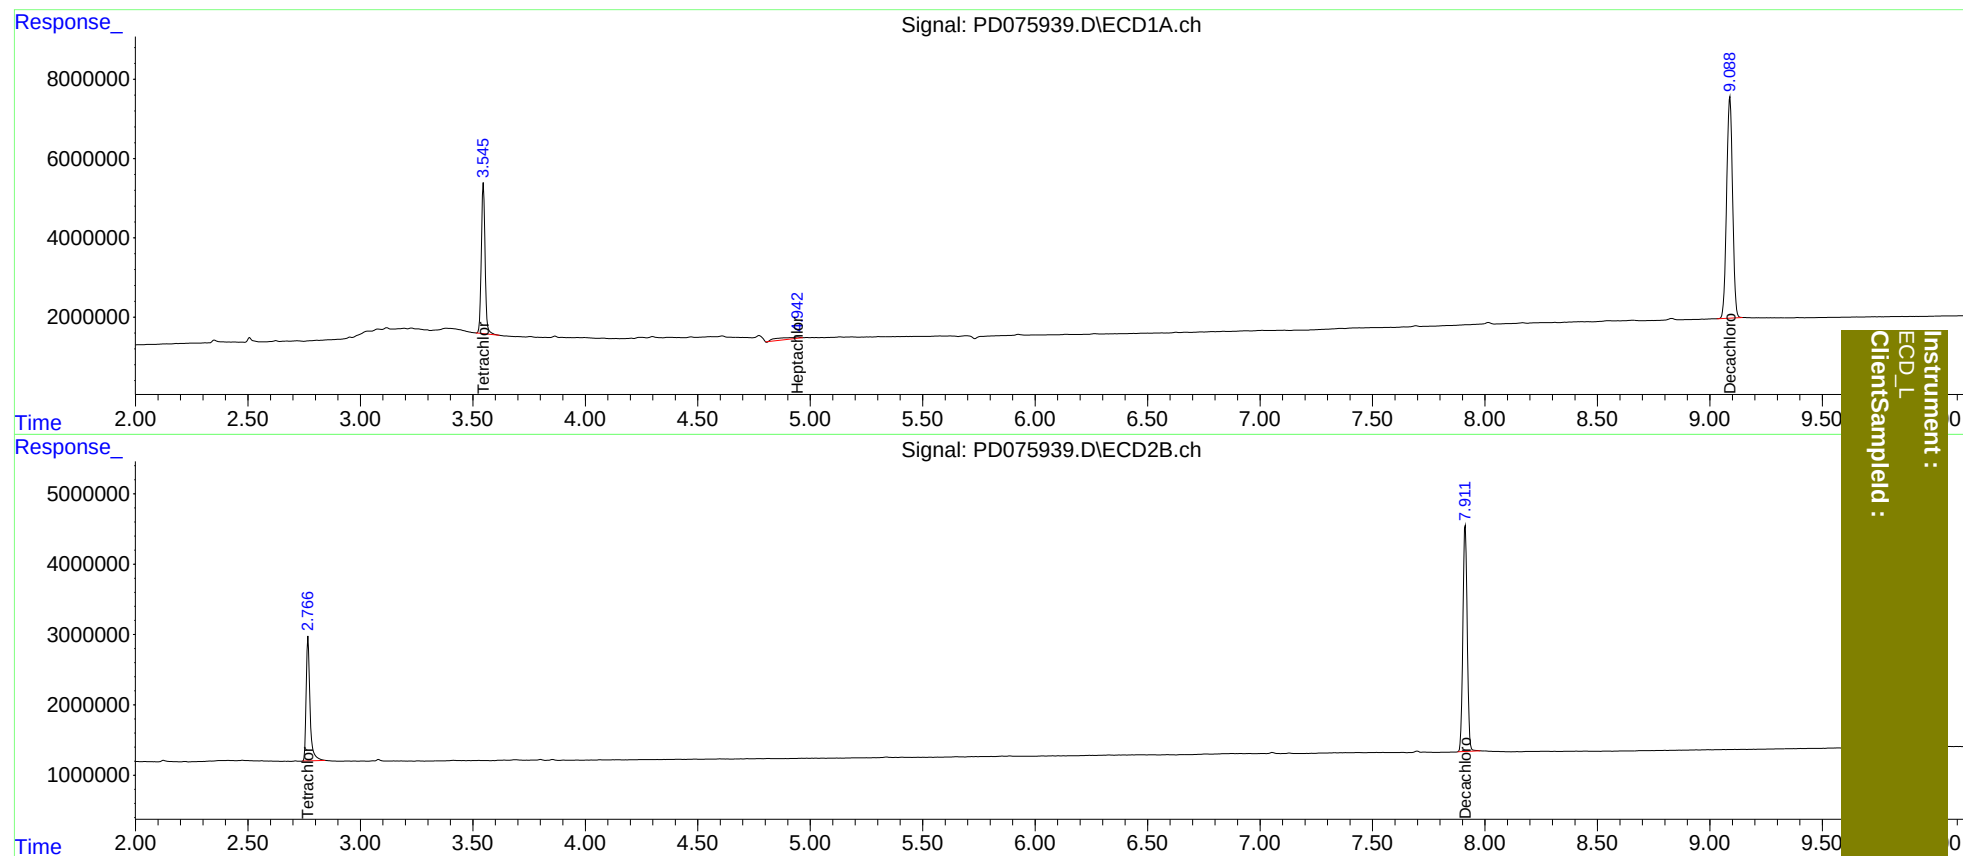


Instrument :
ECD_1
ClientSampled :
0

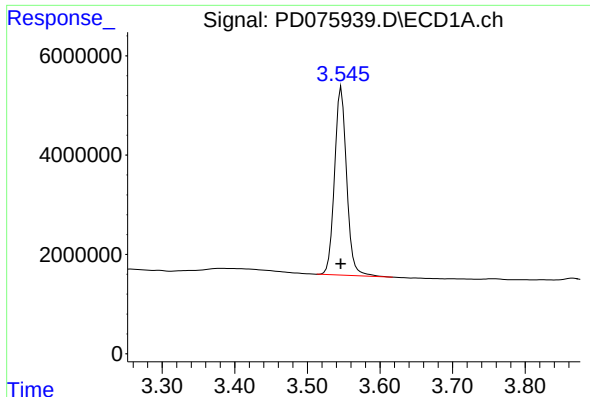

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 43691882
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

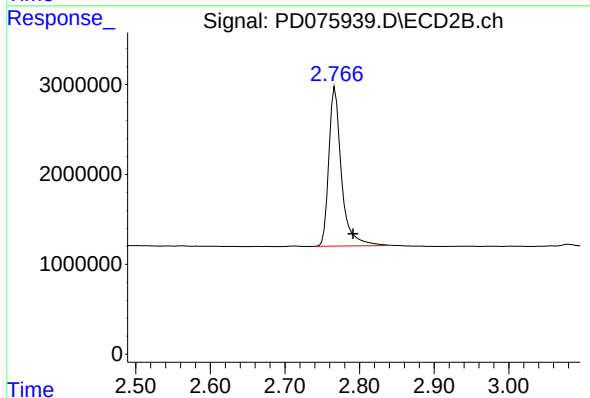


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: -0.024 min
Response: 20839576
Conc: 20.55 ng/ml

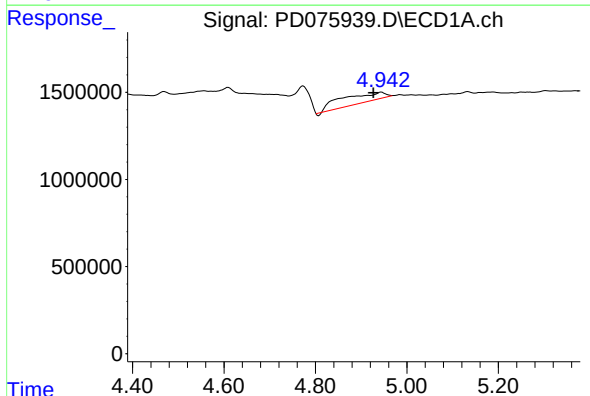


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.017 min
Response: 3623395
Conc: 1.12 ng/ml

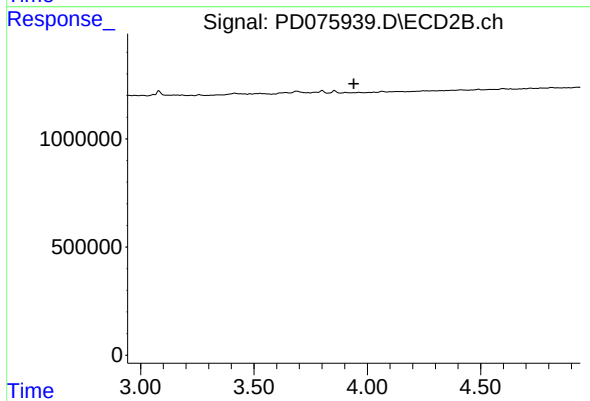

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

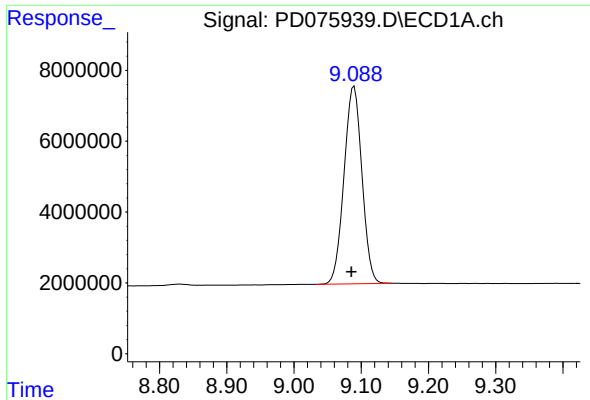

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.004 min
Response: 102980926
Conc: 44.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

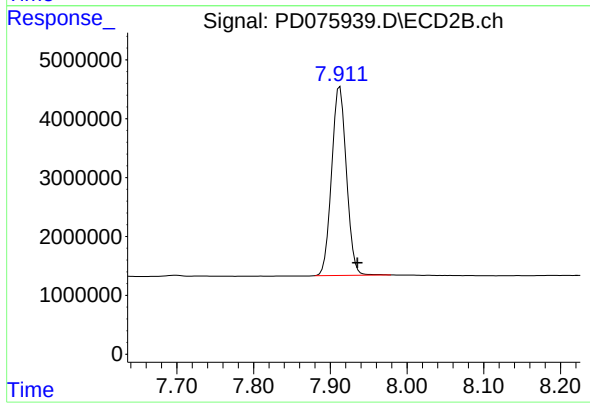

#27 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: -0.023 min
Response: 43038862
Conc: 45.83 ng/ml