

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062123\
 Data File : PD075947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 15:23
 Operator : AR\AJ
 Sample : 03121-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:34:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.768	48148453	22391501	24.085	22.086
27)	SA Decachlor...	9.087	7.912	82134189	33369492	35.811	35.533
Target Compounds							
4)	MA Heptachlor	4.946	0.000	4623385	0	1.426	N.D. #
8)	B Heptachlo...	0.000	4.793f	0	265357	N.D.	0.202
15)	B Endosulfa...	0.000	5.888f	0	417613	N.D.	0.372


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062123\
Data File : PD075947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 15:23
Operator : AR\AJ
Sample : 03121-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:34:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

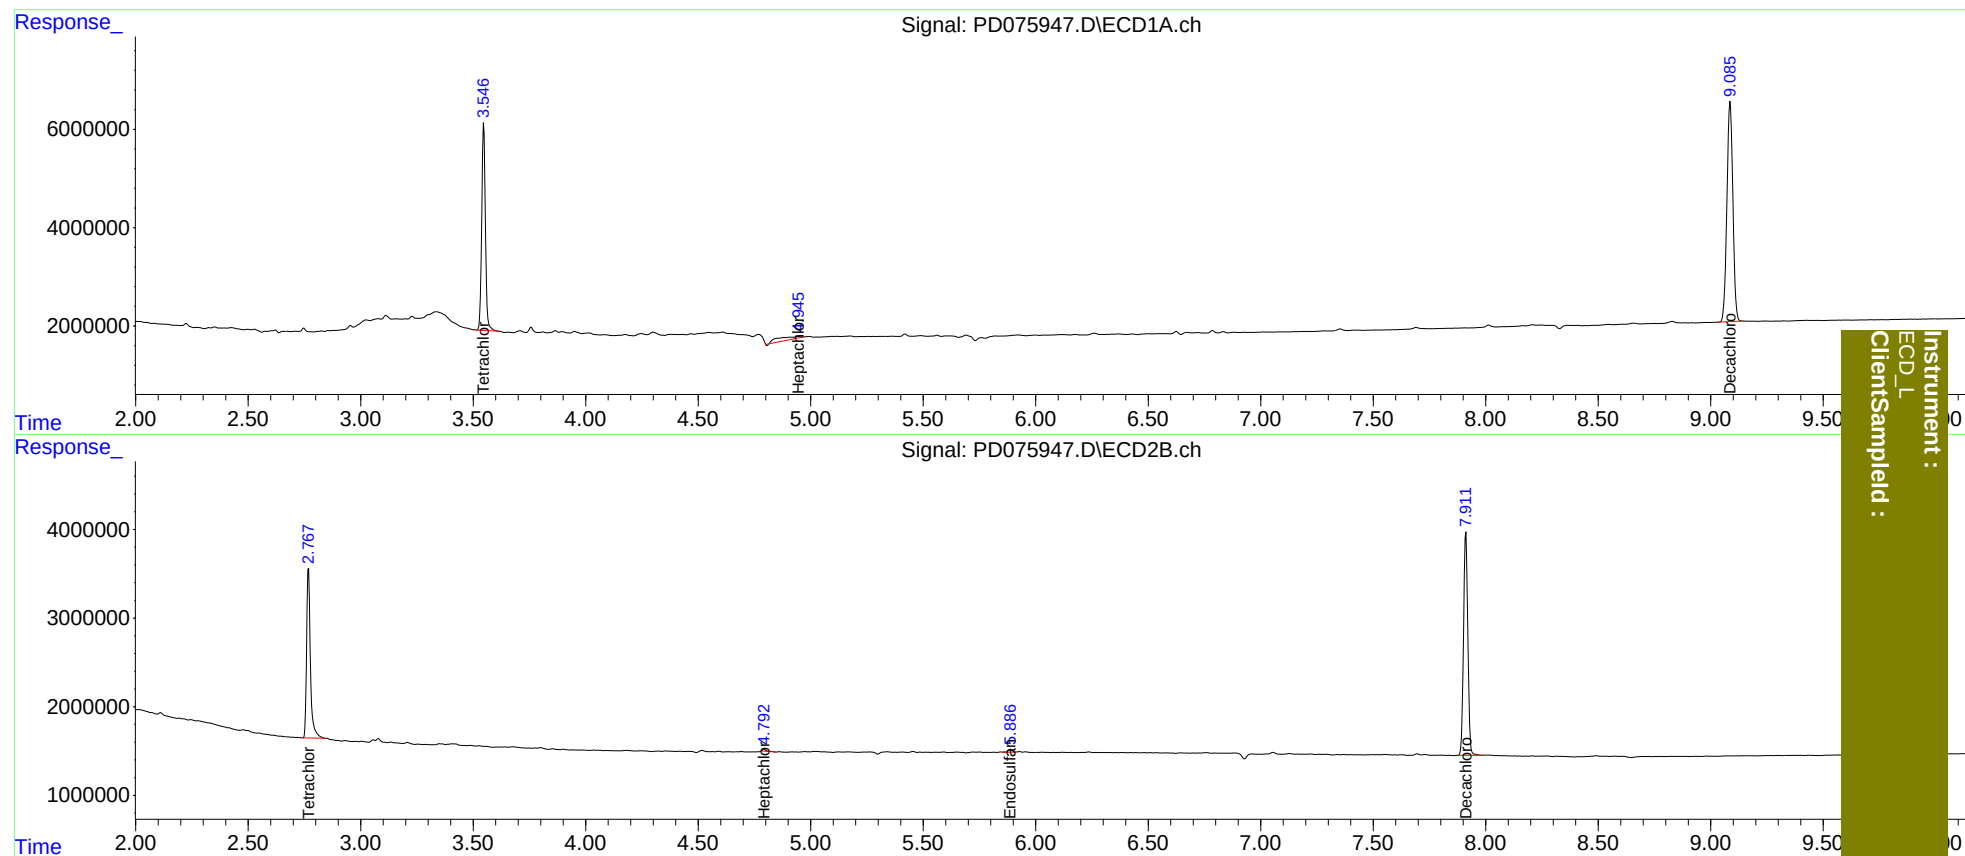


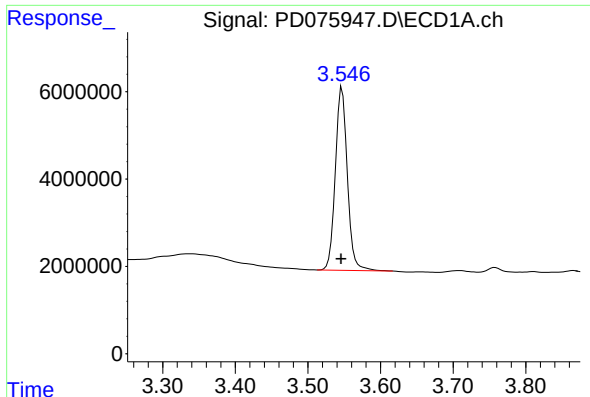

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.001 min
Response: 48148453
Conc: 24.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

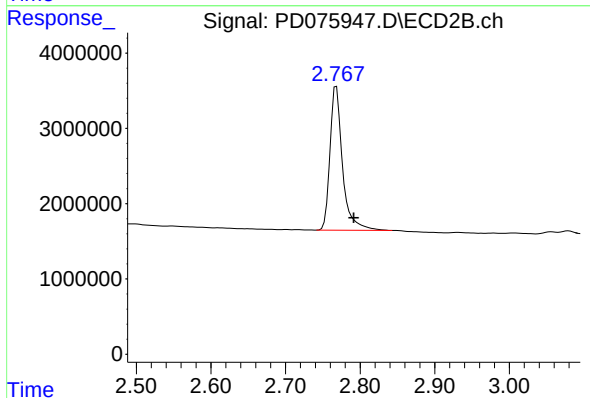


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.023 min
Response: 22391501
Conc: 22.09 ng/ml

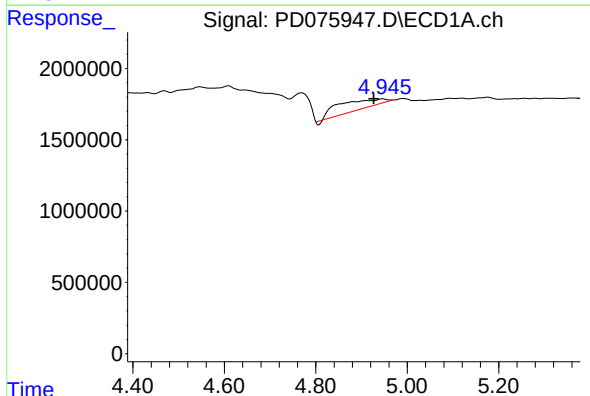


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.019 min
Response: 4623385
Conc: 1.43 ng/ml

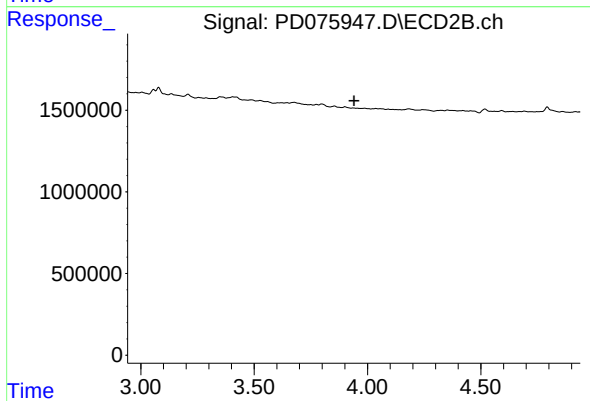

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

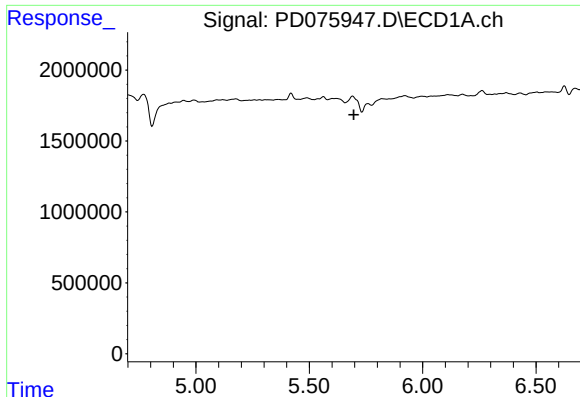

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.697 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

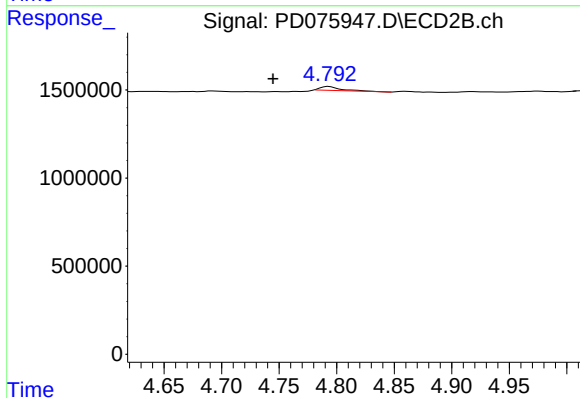


#8 Heptachlor epoxide

R.T.: 4.793 min
Delta R.T.: 0.048 min
Response: 265357
Conc: 0.20 ng/ml

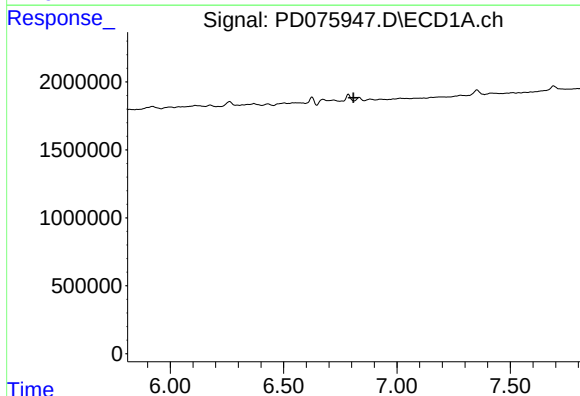


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.809 min
Response: 0
Conc: N.D.

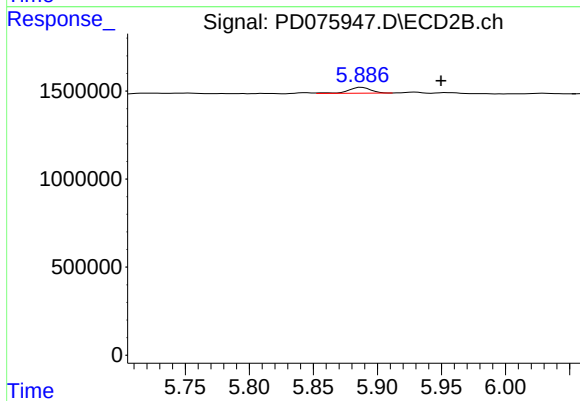

#15 Endosulfan II


R.T.: 5.888 min
Delta R.T.: -0.062 min
Response: 417613
Conc: 0.37 ng/ml

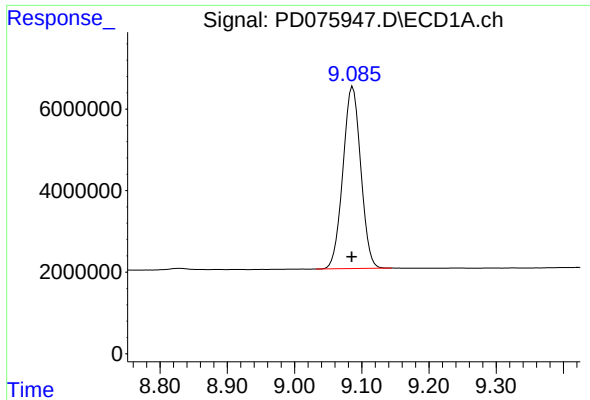

#27 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.001 min
Response: 82134189
Conc: 35.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

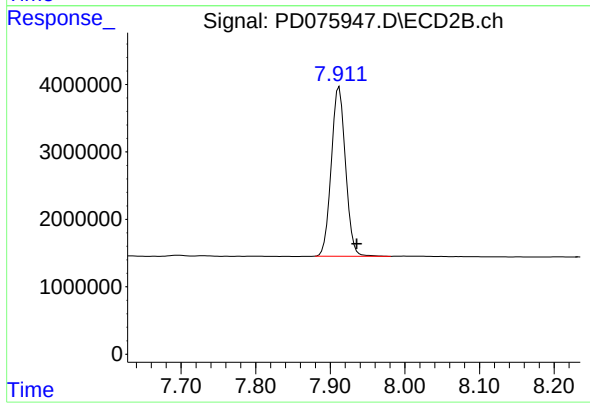

#27 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: -0.024 min
Response: 33369492
Conc: 35.53 ng/ml