

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062123\
 Data File : PD075952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 16:44
 Operator : AR\AJ
 Sample : PIBLK172
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:38:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.768	44248409	20664825	22.134	20.382
2) SA Decachlor...	9.084	7.910	108.3E6	43297840	47.214	46.105
Target Compounds						
3) MA gamma-BHC...	0.000	3.609	0	110207	N.D.	<MDL
4) MA Heptachlor	4.941	0.000	3962309	0	1.222	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062123\
Data File : PD075952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 16:44
Operator : AR\AJ
Sample : PIBLK172
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:38:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

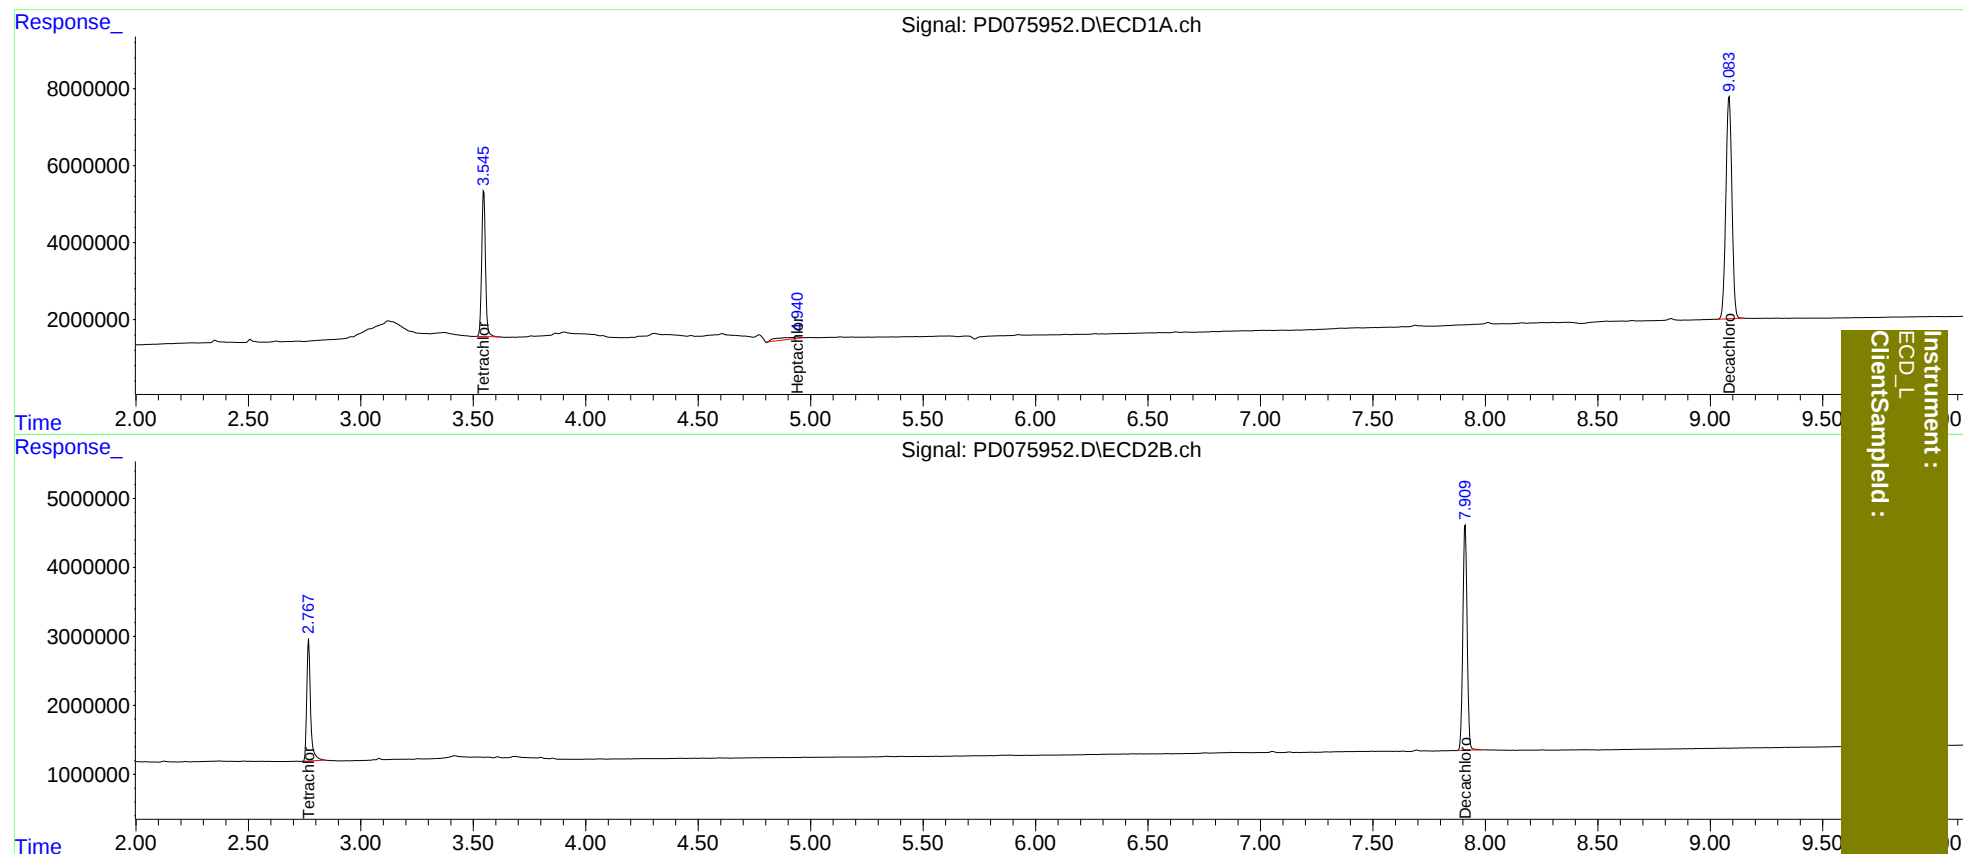


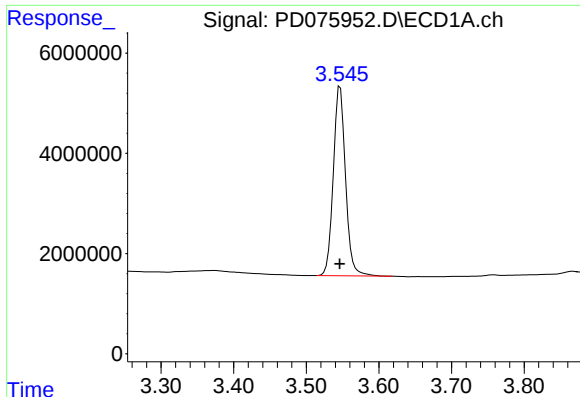

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 44248409
Conc: 22.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

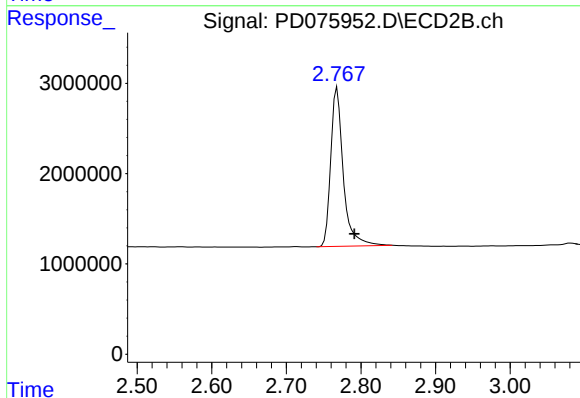


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.023 min
Response: 20664825
Conc: 20.38 ng/ml

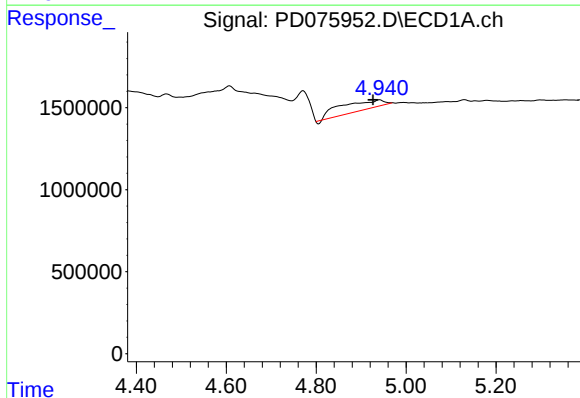


#4 Heptachlor

R.T.: 4.941 min
Delta R.T.: 0.014 min
Response: 3962309
Conc: 1.22 ng/ml

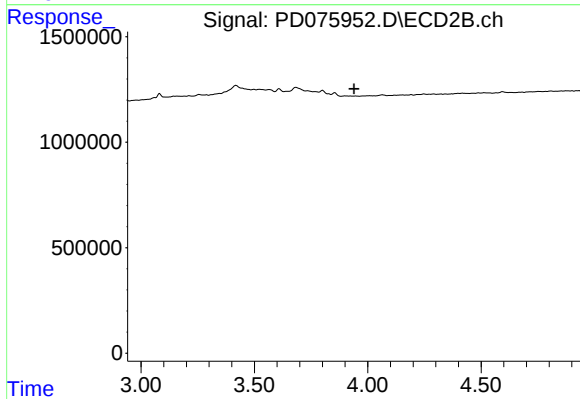

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.941 min
Response: 0
Conc: N.D.

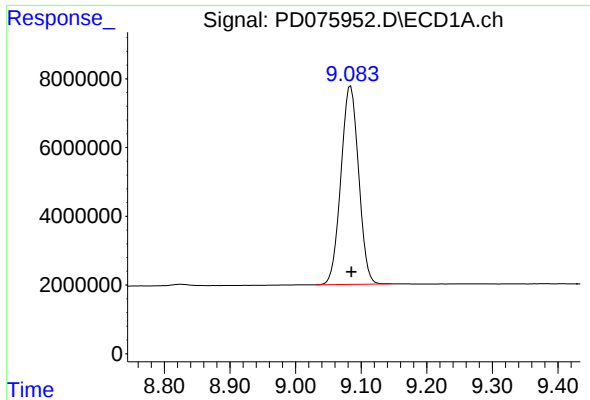

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.001 min
Response: 108288293
Conc: 47.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

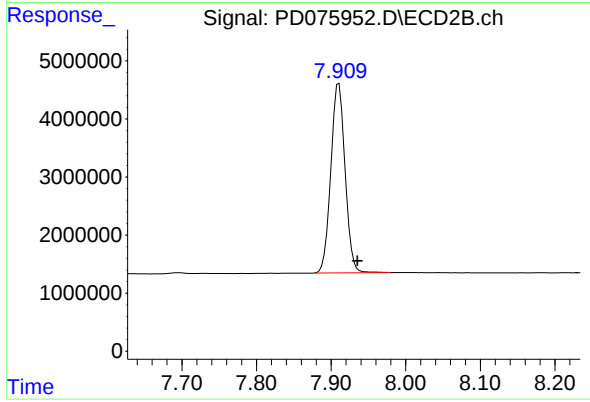

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.025 min
Response: 43297840
Conc: 46.11 ng/ml