

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
 Data File : PL083575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 13:26
 Operator : AR\AJ
 Sample : 03302-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2023
 Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:31:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.451	2.754	43688030	63356441	19.766m	27.199 #
2) SA Decachlor...	8.988	7.960	38831310	47702296	20.378	19.422

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
Data File : PL083575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 13:26
Operator : AR\AJ
Sample : 03302-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2023
Supervised By : Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:31:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

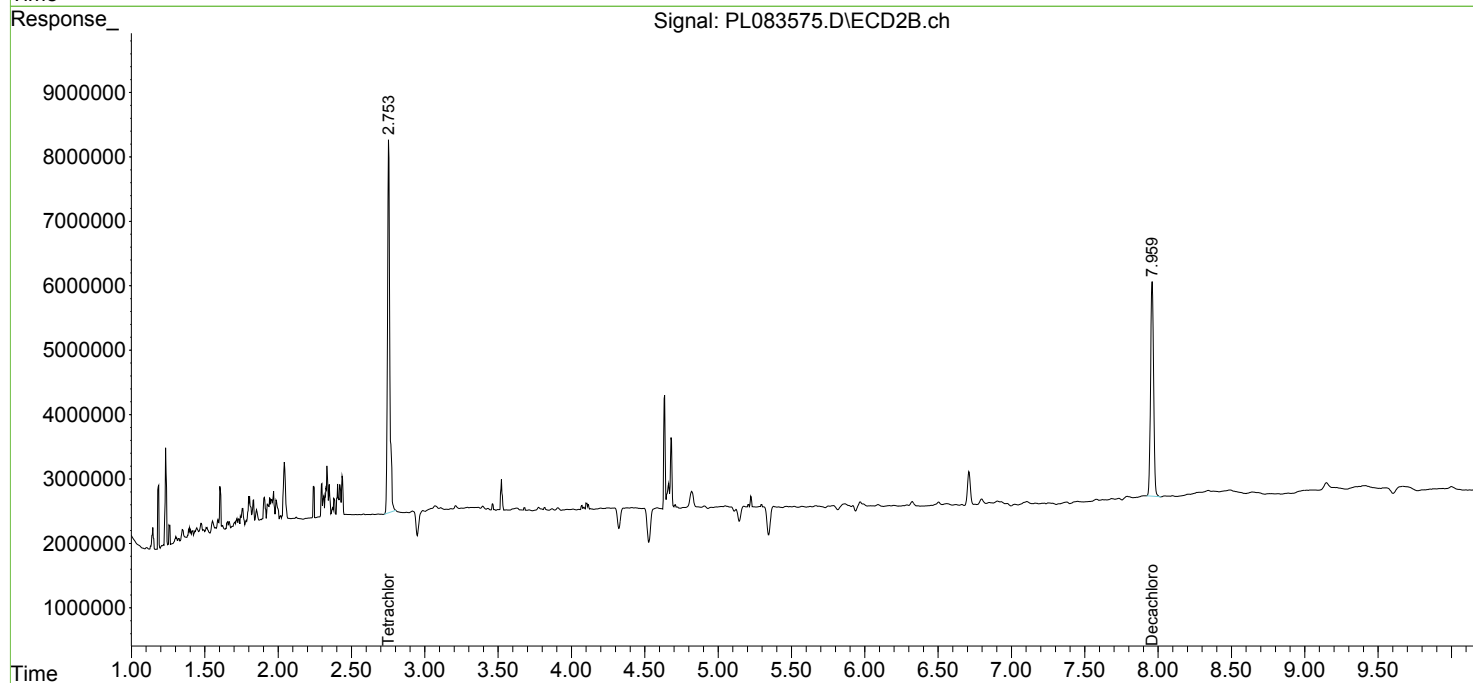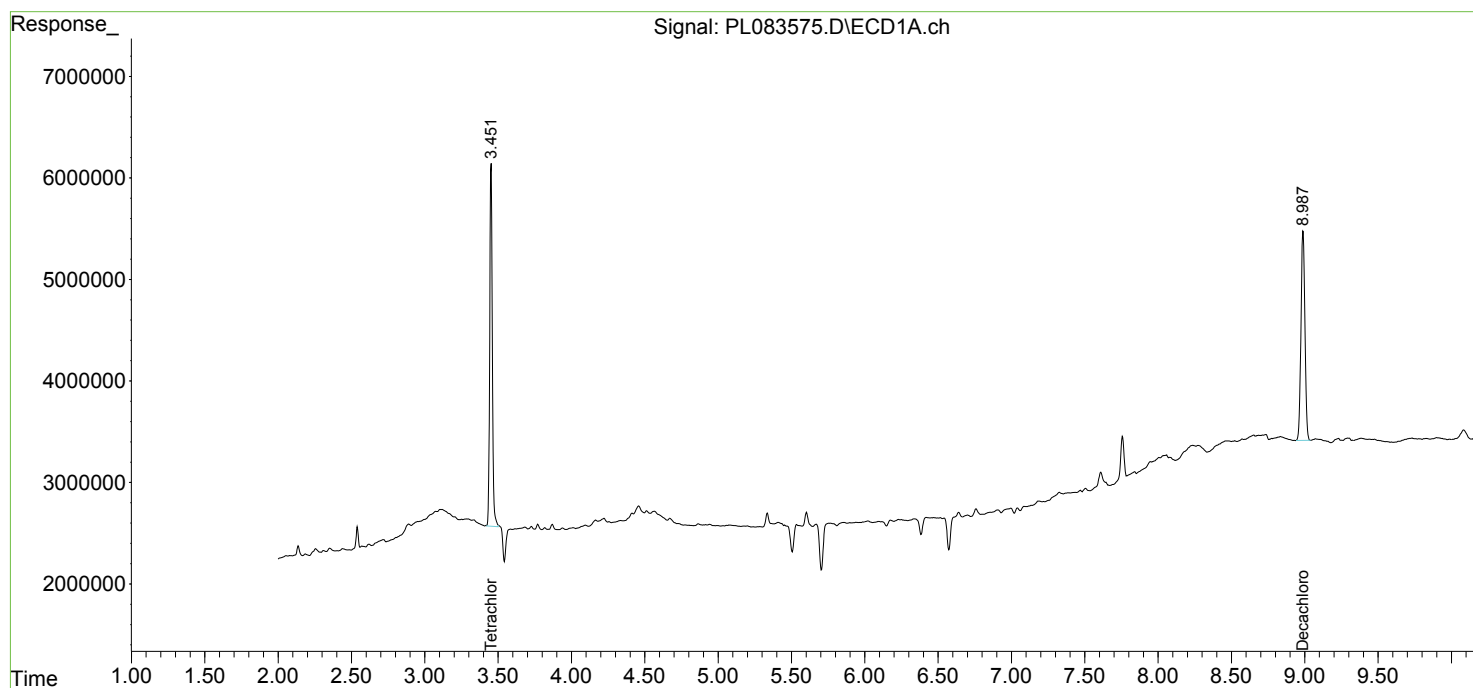

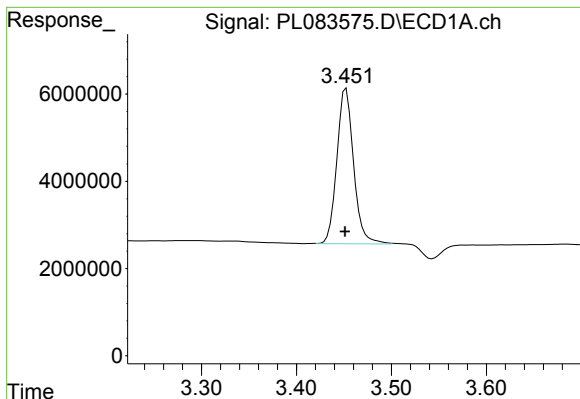


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 43688030
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

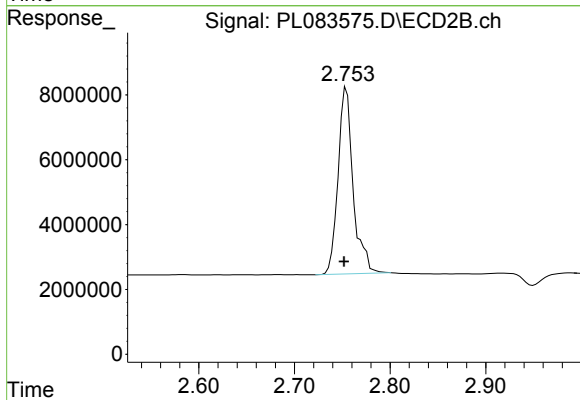


#1 Tetrachloro-m-xylene

R.T.: 2.754 min
Delta R.T.: 0.003 min
Response: 63356441
Conc: 27.20 ng/ml

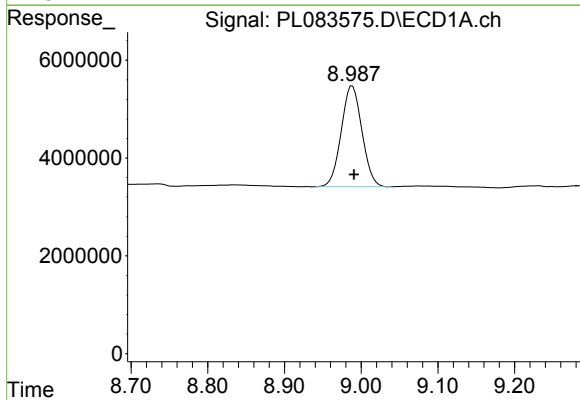

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.002 min
Response: 38831310
Conc: 20.38 ng/ml

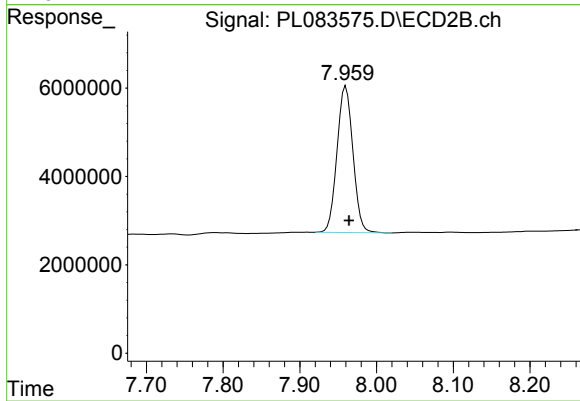

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 47702296
Conc: 19.42 ng/ml