

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
 Data File : PL083579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 14:21
 Operator : AR\AJ
 Sample : 03302-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2023
 Supervised By : Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:35:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	2.753	46305576	52020377	20.950m	22.332
28)	SA Decachlor...	8.989	7.961	42258565	52237475	22.177	21.268

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
Data File : PL083579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 14:21
Operator : AR\AJ
Sample : 03302-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2023
Supervised By : Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:35:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

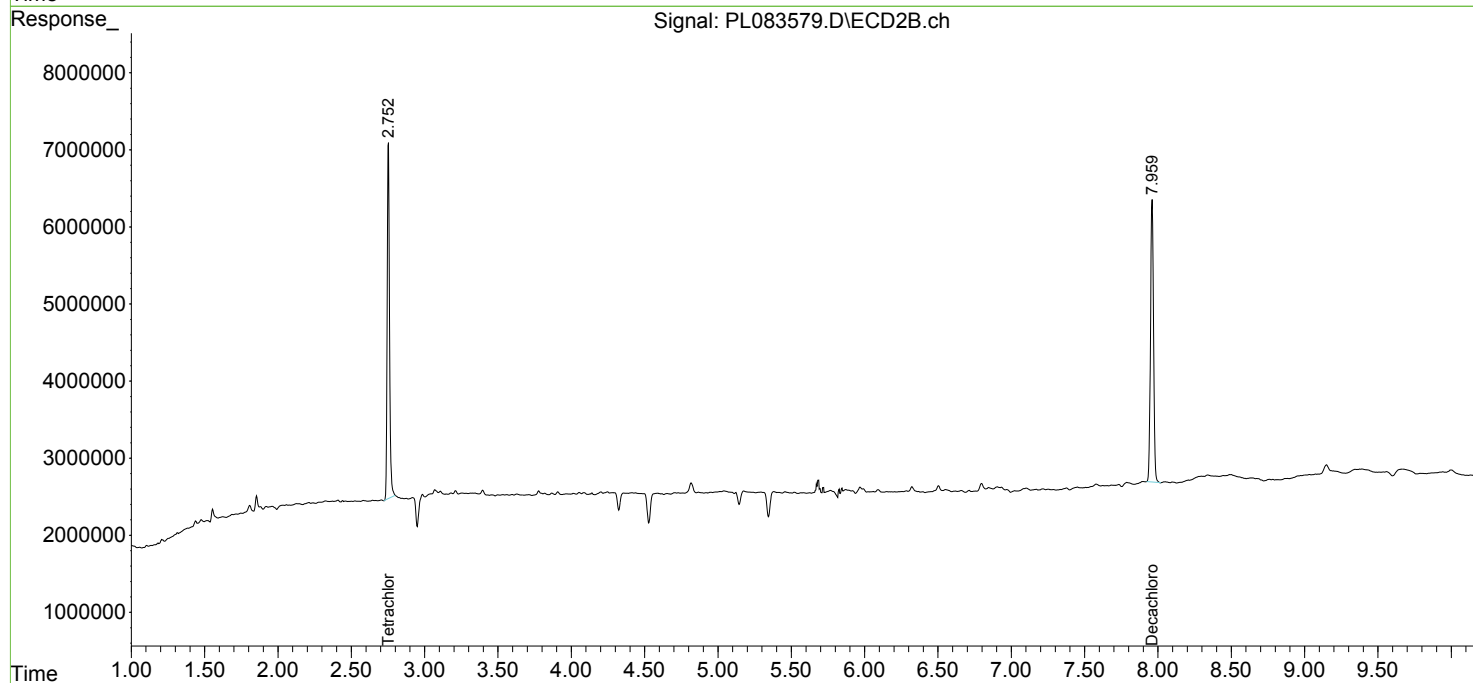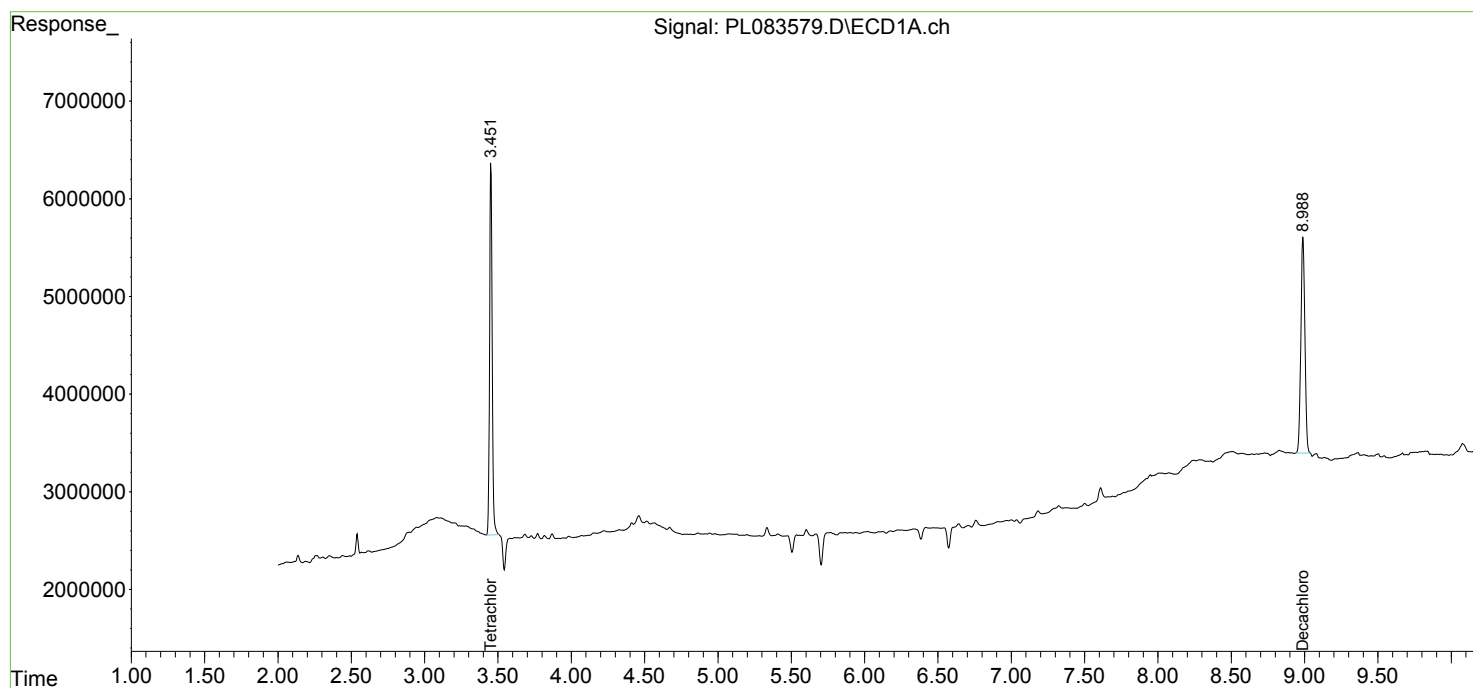

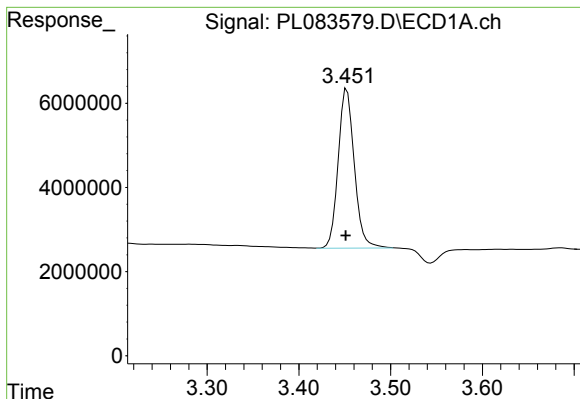


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 46305576
Conc: 20.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

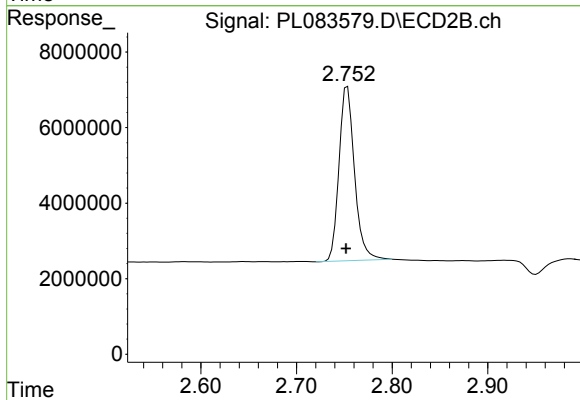


#1 Tetrachloro-m-xylene

R.T.: 2.753 min
Delta R.T.: 0.001 min
Response: 52020377
Conc: 22.33 ng/ml

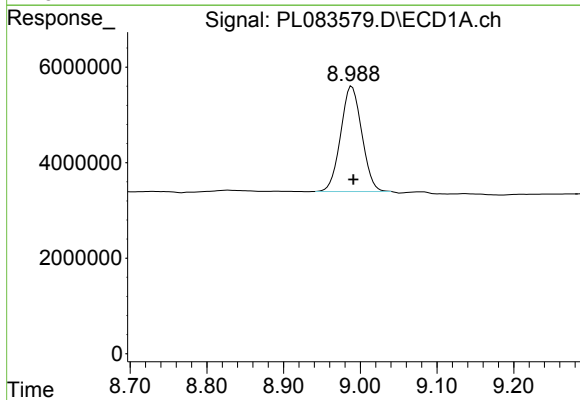

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.002 min
Response: 42258565
Conc: 22.18 ng/ml

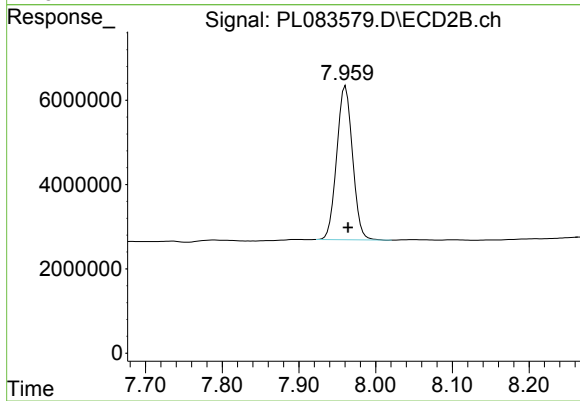

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.003 min
Response: 52237475
Conc: 21.27 ng/ml