

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
 Data File : PL083606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 21:32
 Operator : AR\AJ
 Sample : 03328-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSIT-SW02-8-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:54:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.452	2.752	30442395	28879585	13.773	12.398
28) SA Decachlor...	8.988	7.959	31629631	37091041	16.599	15.102

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
Data File : PL083606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 21:32
Operator : AR\AJ
Sample : 03328-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMPOSIT-SW02-8-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:54:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

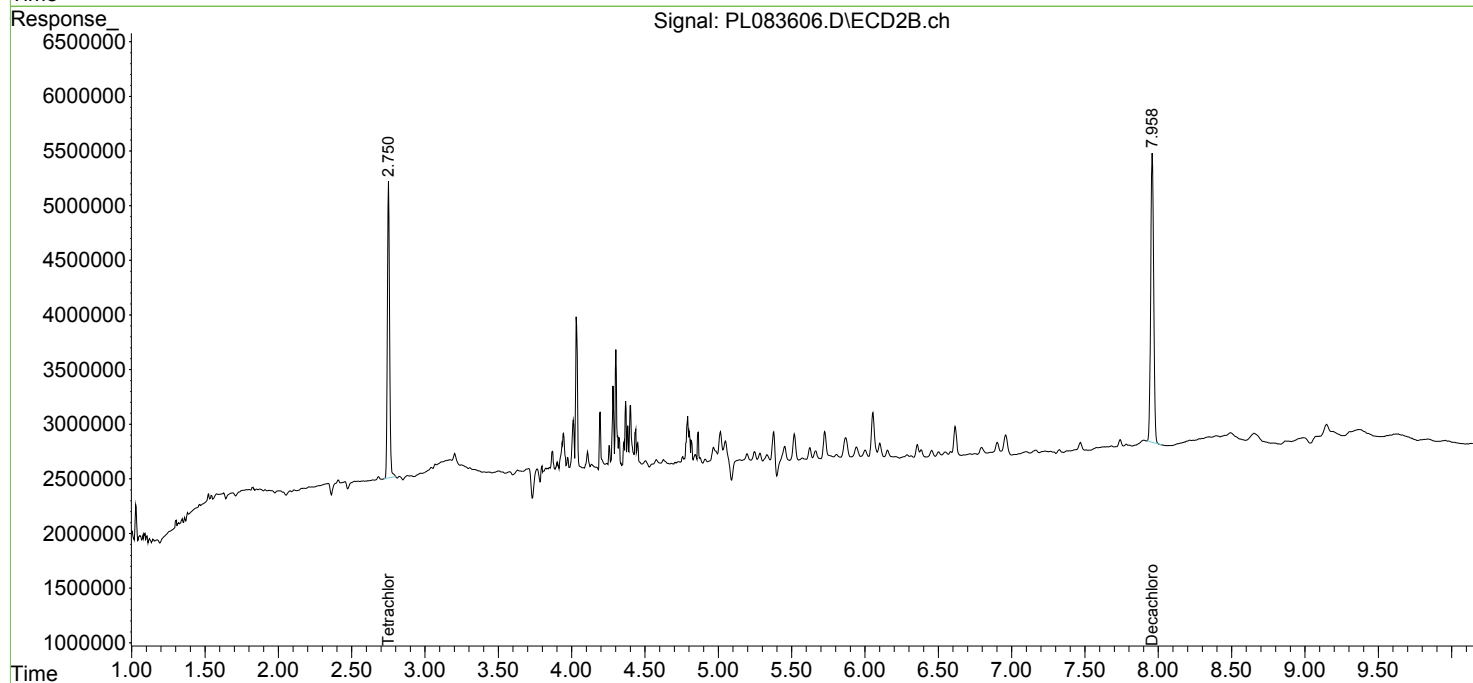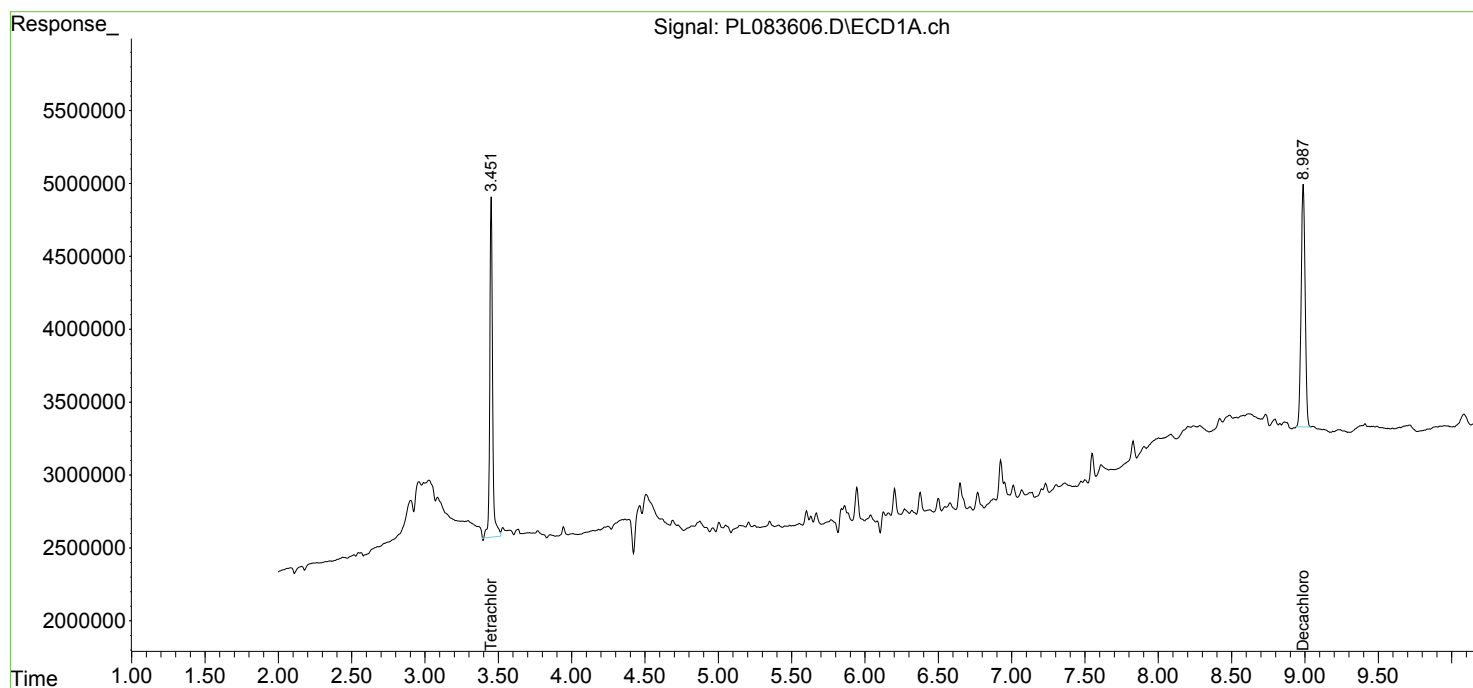


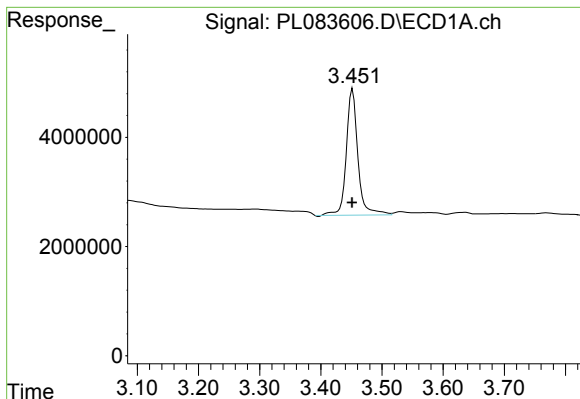

#1 Tetrachloro-m-xylene


R.T.: 3.452 min
Delta R.T.: 0.001 min
Response: 30442395
Conc: 13.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSIT-SW02-8-15

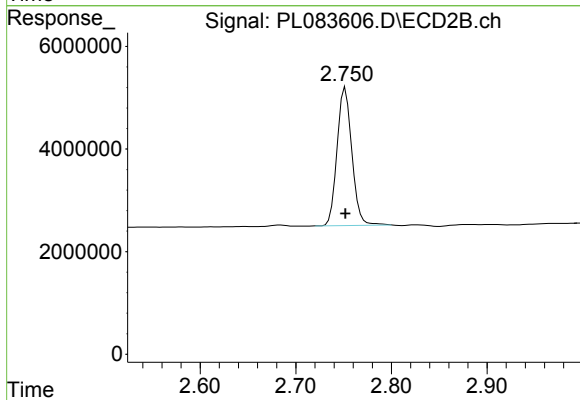


#1 Tetrachloro-m-xylene

R.T.: 2.752 min
Delta R.T.: 0.000 min
Response: 28879585
Conc: 12.40 ng/ml

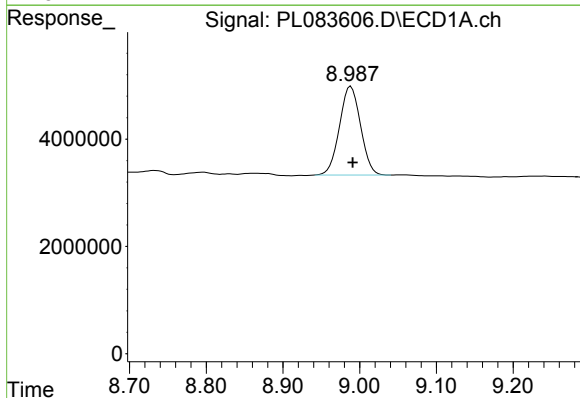

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.002 min
Response: 31629631
Conc: 16.60 ng/ml

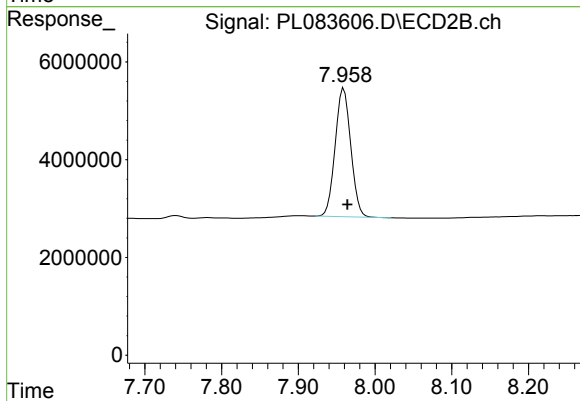

#28 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.005 min
Response: 37091041
Conc: 15.10 ng/ml