

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
 Data File : PL083610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 22:27
 Operator : AR\AJ
 Sample : 03330-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSITE-MC03

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2023
 Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 07:19:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.452	2.751	32100484	35732990	14.523	15.340
28) SA Decachlor...	8.990	7.960	36192632	42924168	18.993	17.477
Target Compounds						
10) B gamma-Chl...	5.861	4.986	32542044	29772487	13.527m	10.063m#
11) B alpha-Chl...	5.946	5.051	64903026	49198094	27.401	16.631 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
Data File : PL083610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 22:27
Operator : AR\AJ
Sample : 03330-01
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMPOSITE-MC03


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2023
Supervised By : Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 07:19:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

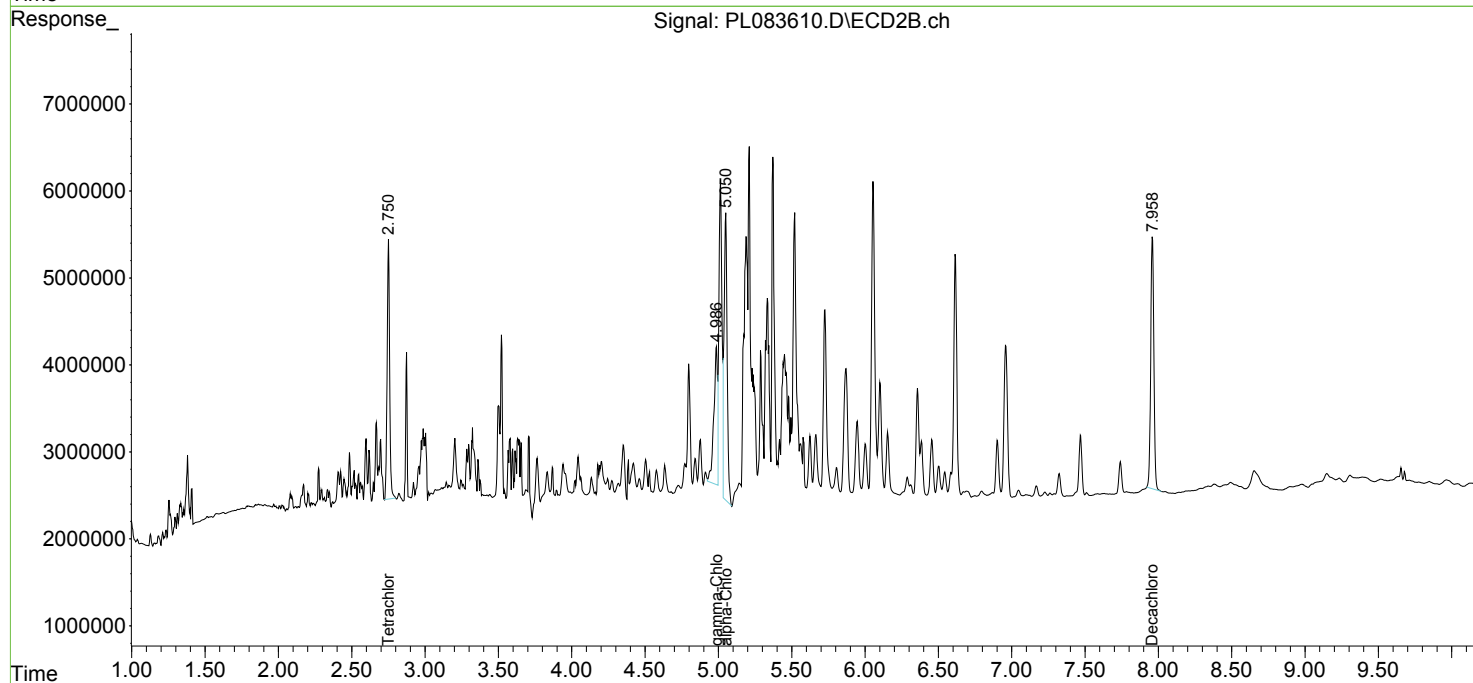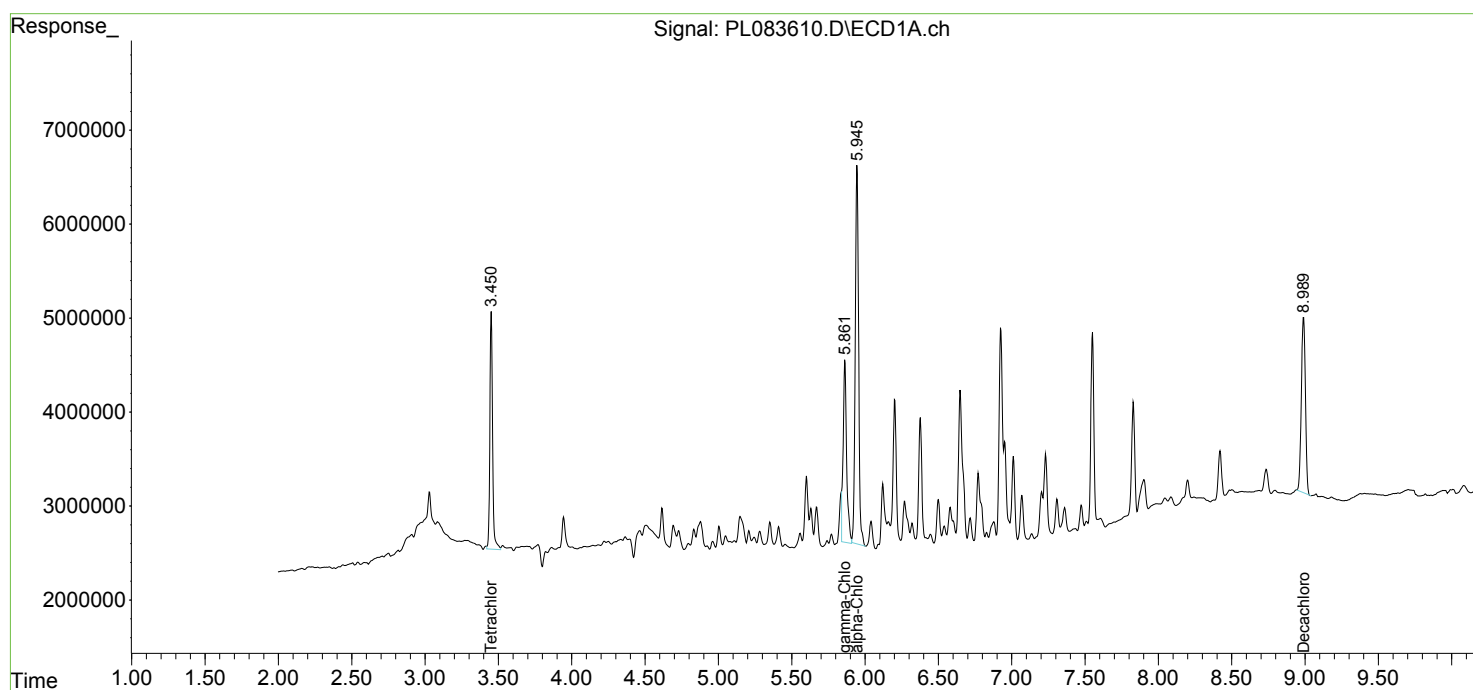

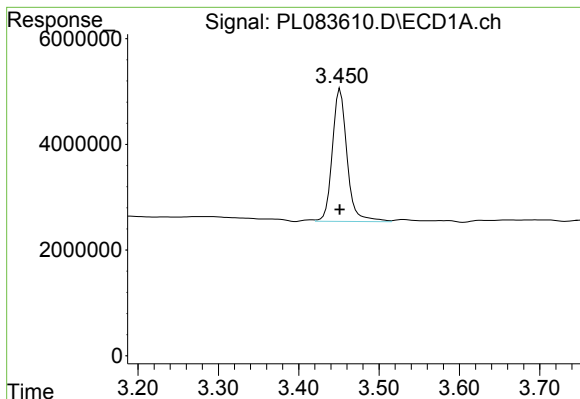


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: 0.000 min
Response: 32100484
Conc: 14.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-MC03


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

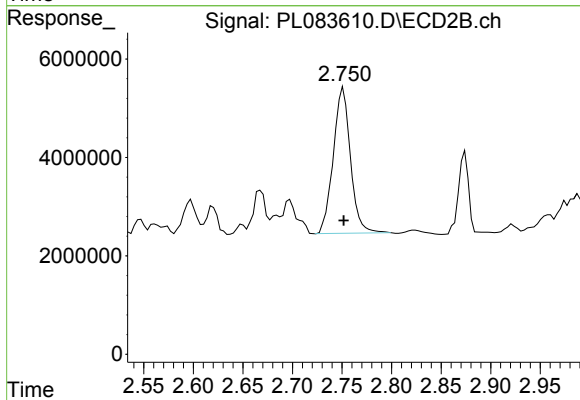


#1 Tetrachloro-m-xylene

R.T.: 2.751 min
Delta R.T.: 0.000 min
Response: 35732990
Conc: 15.34 ng/ml

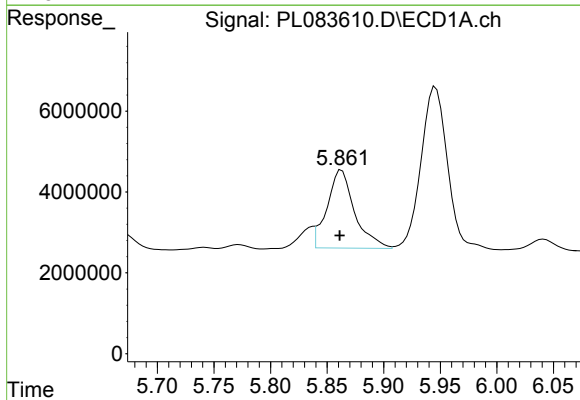


#10 gamma-Chlordane

R.T.: 5.861 min
Delta R.T.: 0.000 min
Response: 32542044
Conc: 13.53 ng/ml m

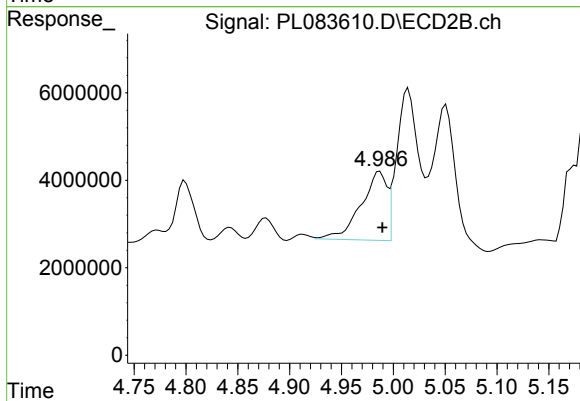

#10 gamma-Chlordane

R.T.: 4.986 min
Delta R.T.: -0.004 min
Response: 29772487
Conc: 10.06 ng/ml m

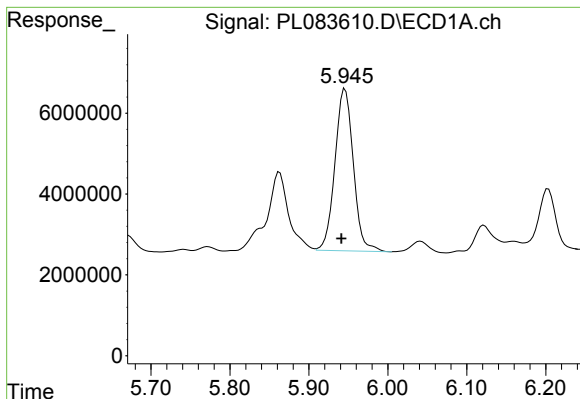


#11 alpha-Chlordane

R.T.: 5.946 min
Delta R.T.: 0.005 min
Response: 64903026
Conc: 27.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-MC03


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

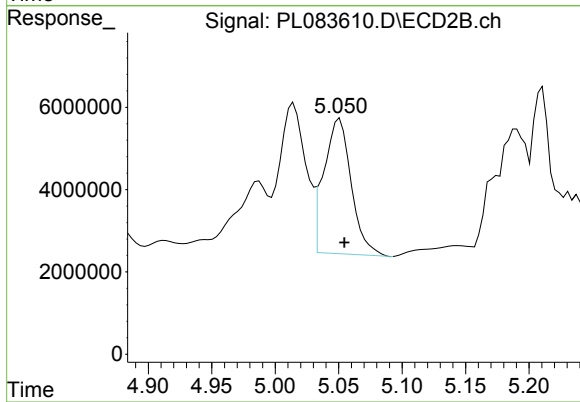


#11 alpha-Chlordane

R.T.: 5.051 min
Delta R.T.: -0.004 min
Response: 49198094
Conc: 16.63 ng/ml

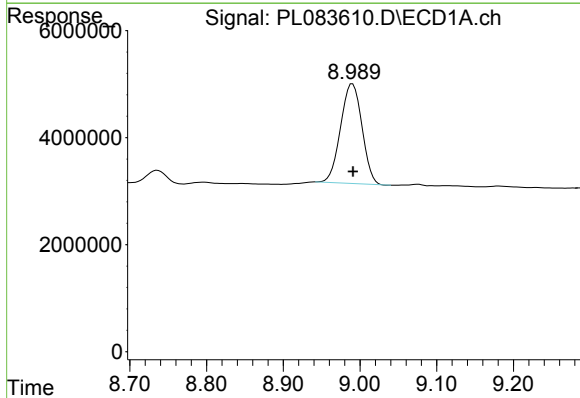

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 36192632
Conc: 18.99 ng/ml

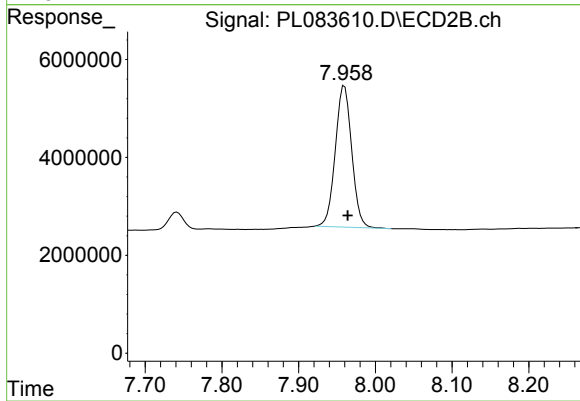

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 42924168
Conc: 17.48 ng/ml