

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
 Data File : PL083611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 22:41
 Operator : AR\AJ
 Sample : 03330-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSITE-MC01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2023
 Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 07:19:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.452	2.750	30337241	37810221	13.725	16.232m
28)	SA Decachlor...	8.989	7.960	33491085	39565467	17.576	16.109
Target Compounds							
10)	B gamma-Chl...	5.862	4.985	14854905	8921390	6.175	3.015m#
11)	B alpha-Chl...	5.946	5.050	29232814	24701718	12.341	8.350 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062023\
Data File : PL083611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 22:41
Operator : AR\AJ
Sample : 03330-07
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMPOSITE-MC01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2023
Supervised By : Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 07:19:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

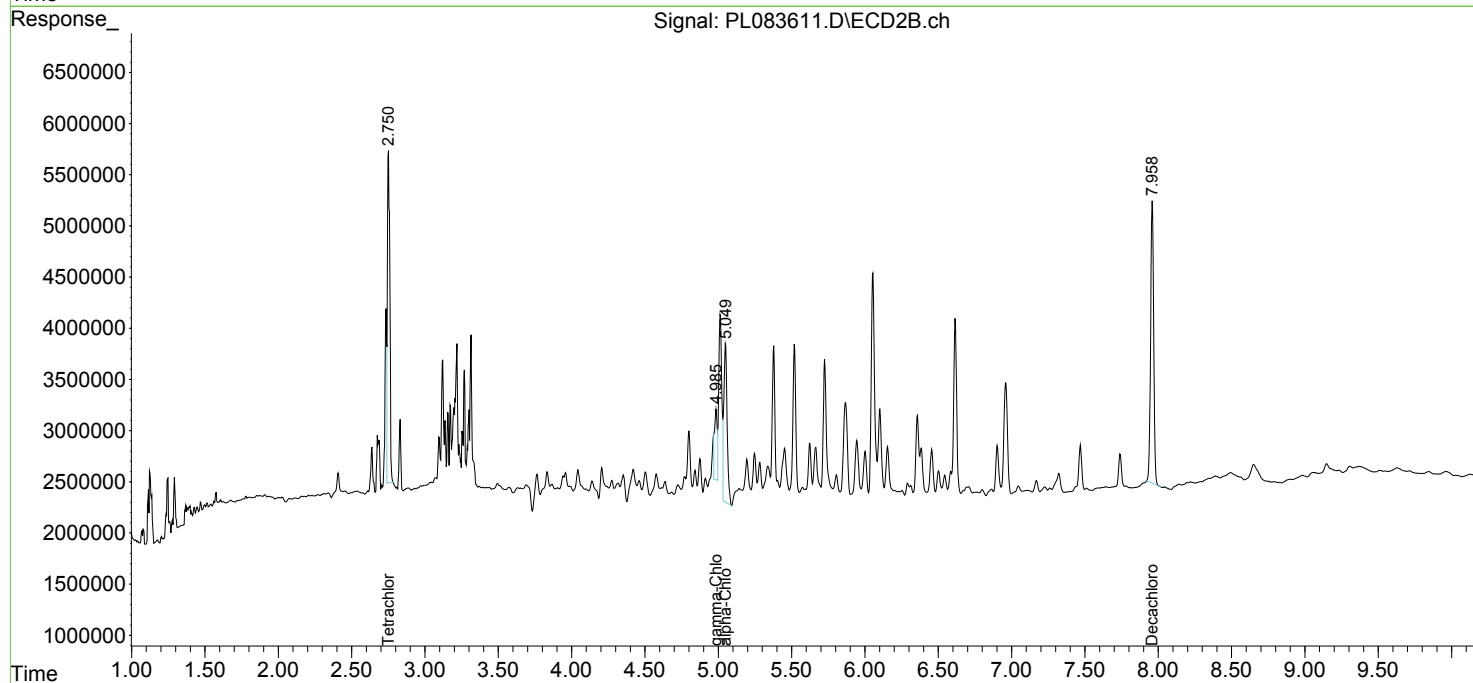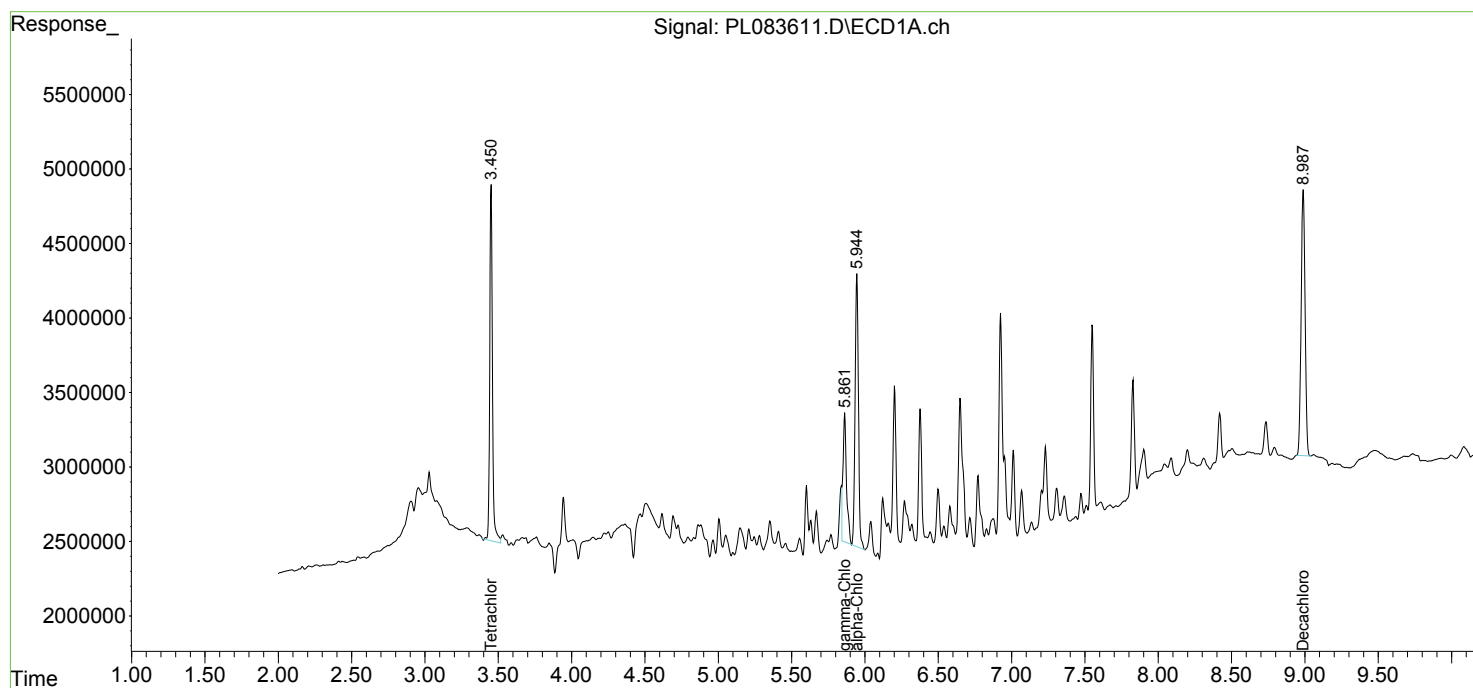

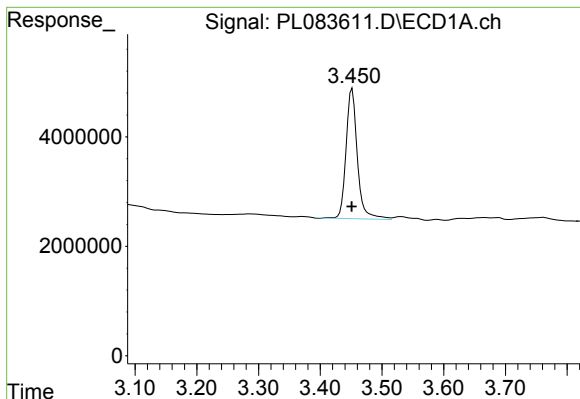


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: 0.000 min
Response: 30337241
Conc: 13.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-MC01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

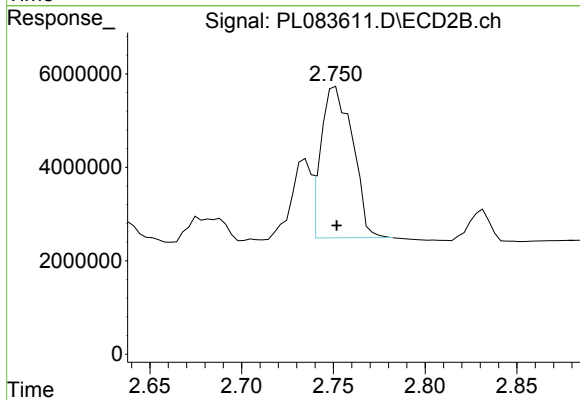


#1 Tetrachloro-m-xylene

R.T.: 2.750 min
Delta R.T.: -0.002 min
Response: 37810221
Conc: 16.23 ng/ml m

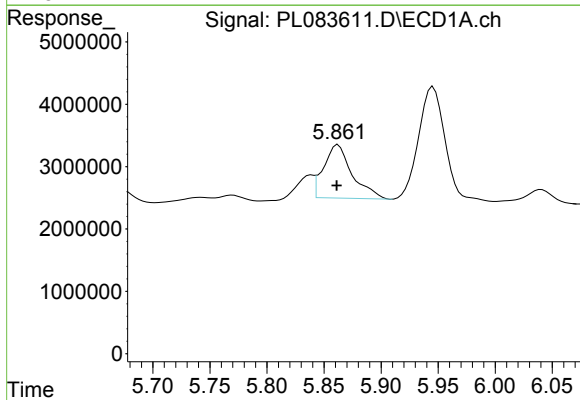


#10 gamma-Chlordane

R.T.: 5.862 min
Delta R.T.: 0.001 min
Response: 14854905
Conc: 6.17 ng/ml

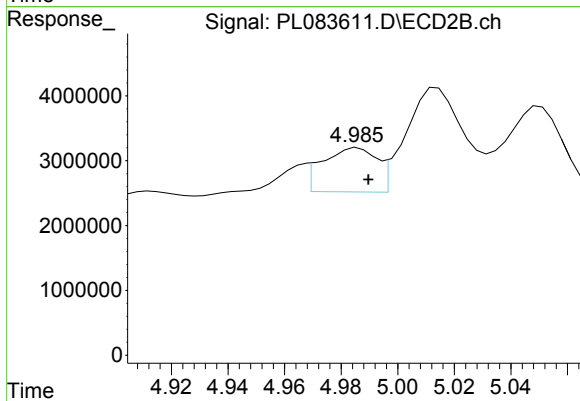

#10 gamma-Chlordane

R.T.: 4.985 min
Delta R.T.: -0.005 min
Response: 8921390
Conc: 3.02 ng/ml m

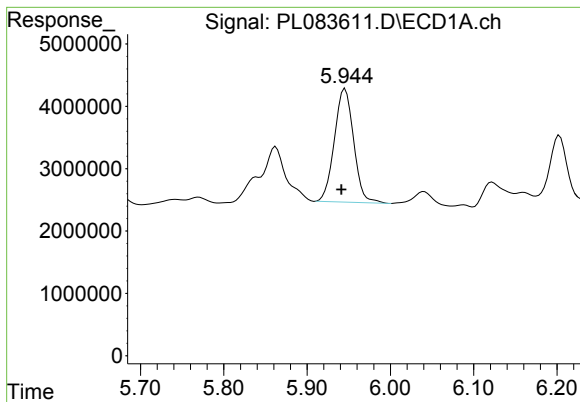


#11 alpha-Chlordane

R.T.: 5.946 min
Delta R.T.: 0.005 min
Response: 29232814
Conc: 12.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-MC01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

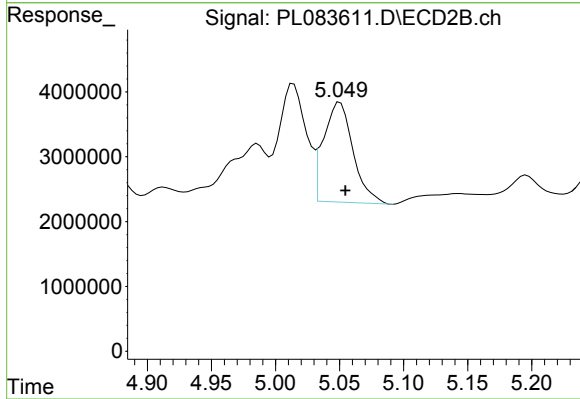


#11 alpha-Chlordane

R.T.: 5.050 min
Delta R.T.: -0.004 min
Response: 24701718
Conc: 8.35 ng/ml

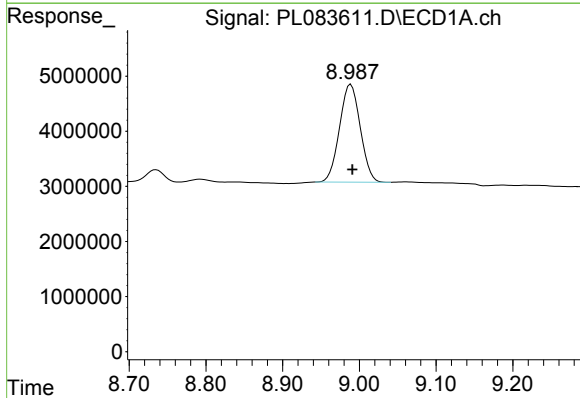

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.002 min
Response: 33491085
Conc: 17.58 ng/ml

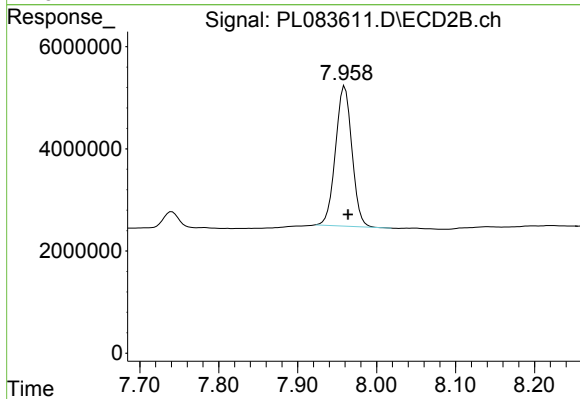

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 39565467
Conc: 16.11 ng/ml