

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062024\
 Data File : PL090261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2024 17:19
 Operator : AR\AJ
 Sample : P2977-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OSTL-A1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2024
 Supervised By :Ankita Jodhani 06/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:32:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.791	40801093	27677167	19.487m	19.303
2)	SA Decachlor...	9.057	7.934	17587290	17240316	11.961	11.602
Target Compounds							
17)	MA 4,4'-DDT	7.027	6.052	769053	1371978	0.418	0.903m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062024\
Data File : PL090261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2024 17:19
Operator : AR\AJ
Sample : P2977-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OSTL-A1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2024
Supervised By : Ankita Jodhani 06/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:32:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

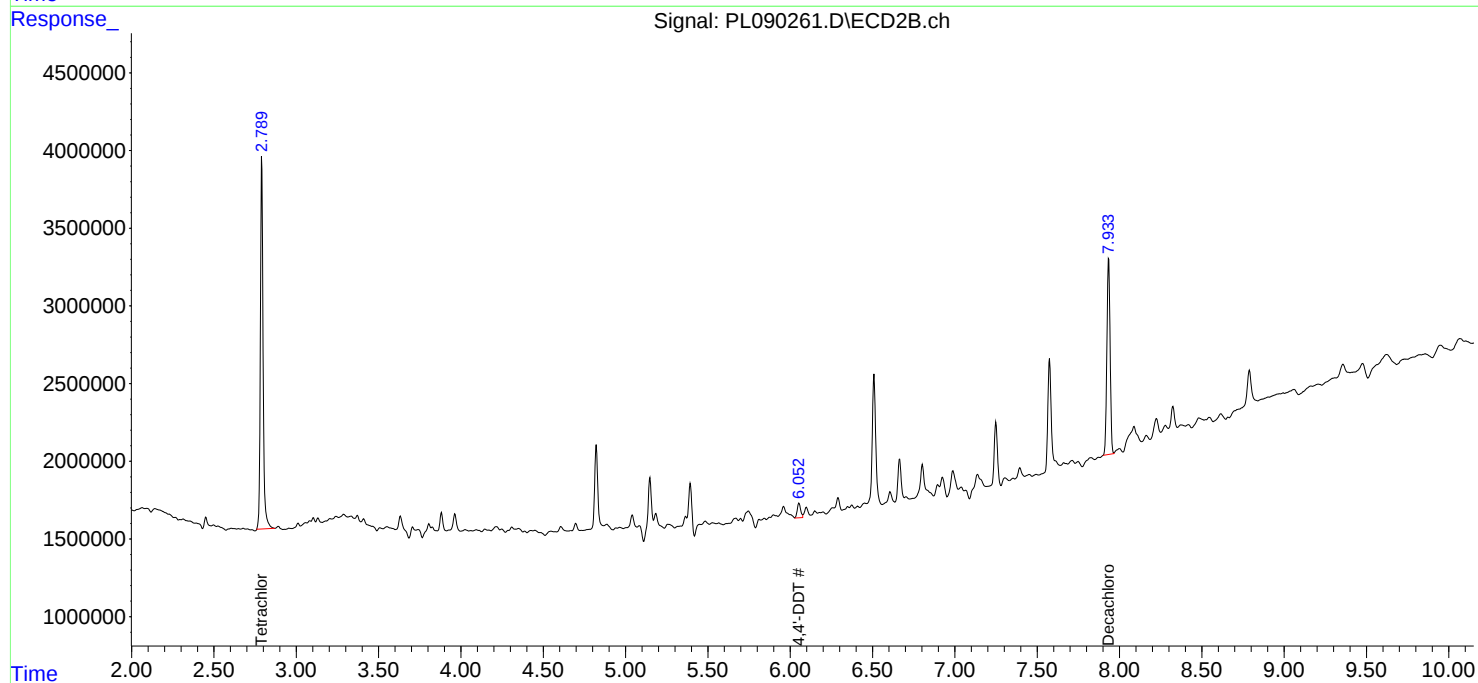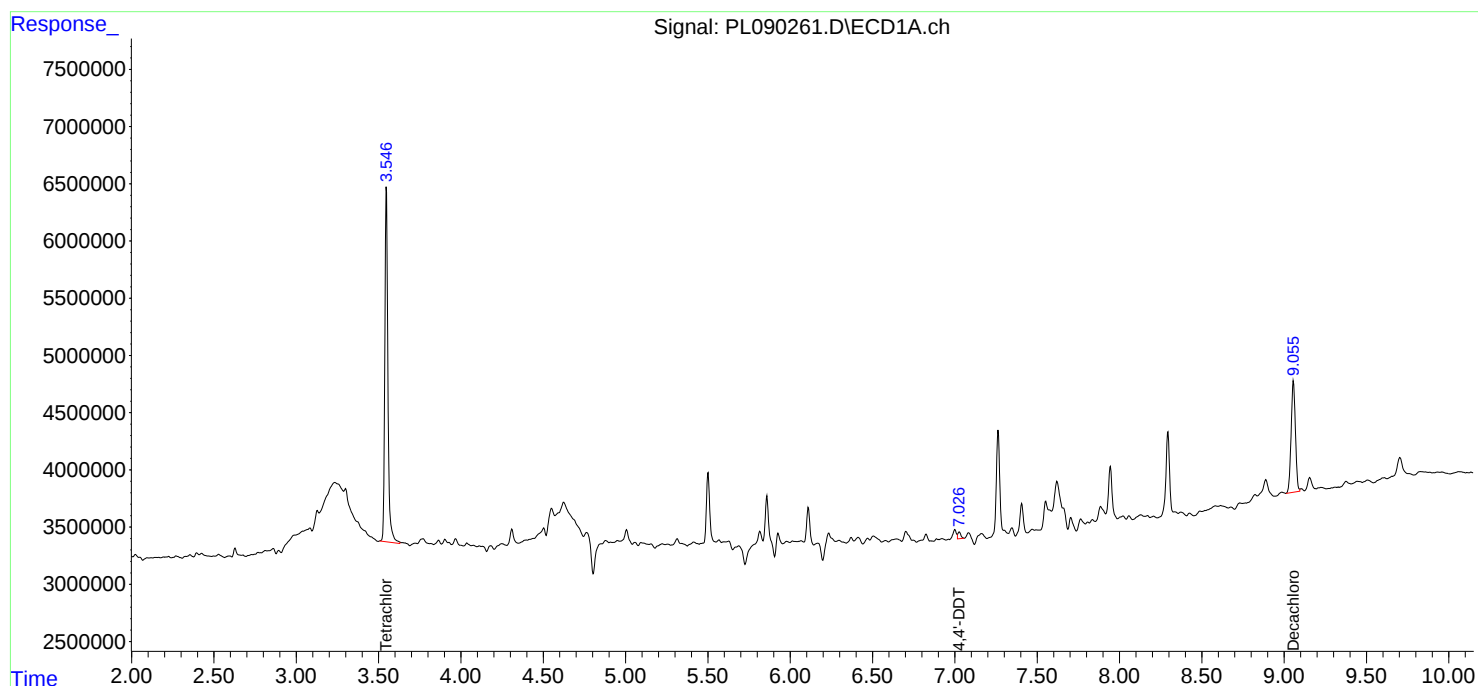

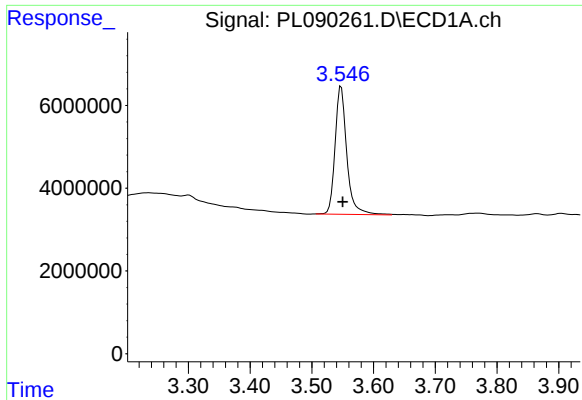


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.004 min
Response: 40801093
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
OSTL-A1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2024
Supervised By :Ankita Jodhani 06/21/2024

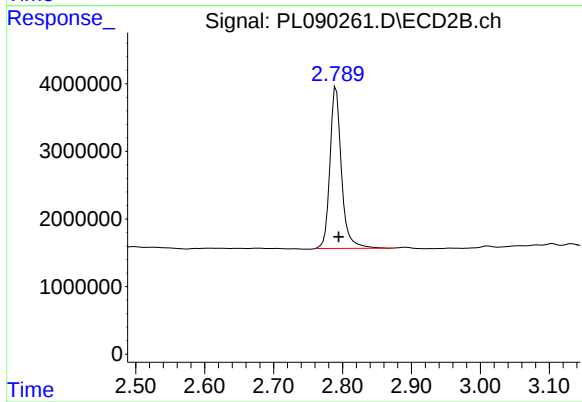


#1 Tetrachloro-m-xylene

R.T.: 2.791 min
Delta R.T.: -0.004 min
Response: 27677167
Conc: 19.30 ng/ml

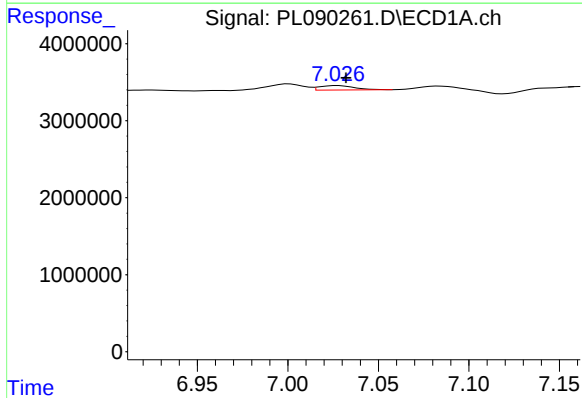


#17 4,4'-DDT

R.T.: 7.027 min
Delta R.T.: -0.005 min
Response: 769053
Conc: 0.42 ng/ml

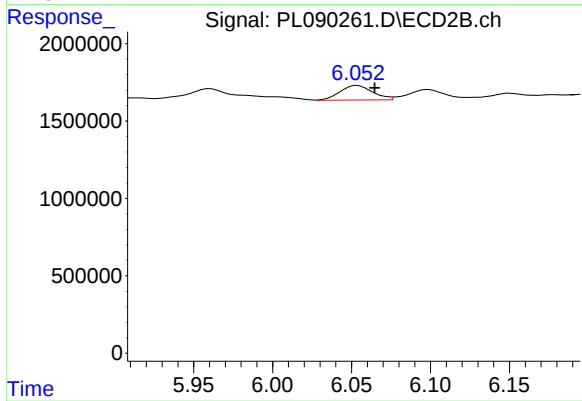

#17 4,4'-DDT

R.T.: 6.052 min
Delta R.T.: -0.012 min
Response: 1371978
Conc: 0.90 ng/ml m

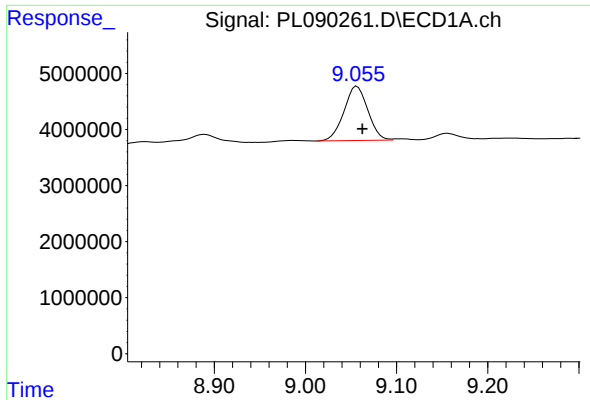


#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.006 min
Response: 17587290
Conc: 11.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
OSTL-A1

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2024
Supervised By :Ankita Jodhani 06/21/2024

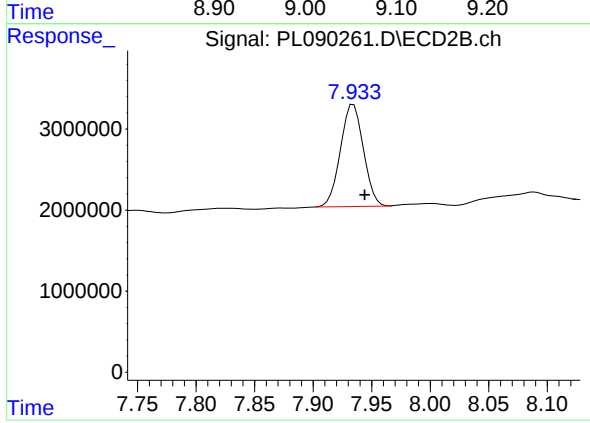

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: -0.009 min
Response: 17240316
Conc: 11.60 ng/ml