

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062024\
 Data File : PL090266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2024 18:28
 Operator : AR\AJ
 Sample : P2977-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OSTL-A6

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2024
 Supervised By :Ankita Jodhani 06/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:37:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.790	41128767	29182341	19.644m	20.353
2)	SA Decachlor...	9.053	7.933	16629012	17038025	11.309m	11.466
Target Compounds							
17)	MA 4,4'-DDT	7.027	6.055	725642	1376784	0.394	0.907 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062024\
Data File : PL090266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2024 18:28
Operator : AR\AJ
Sample : P2977-06
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OSTL-A6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2024
Supervised By : Ankita Jodhani 06/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:37:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

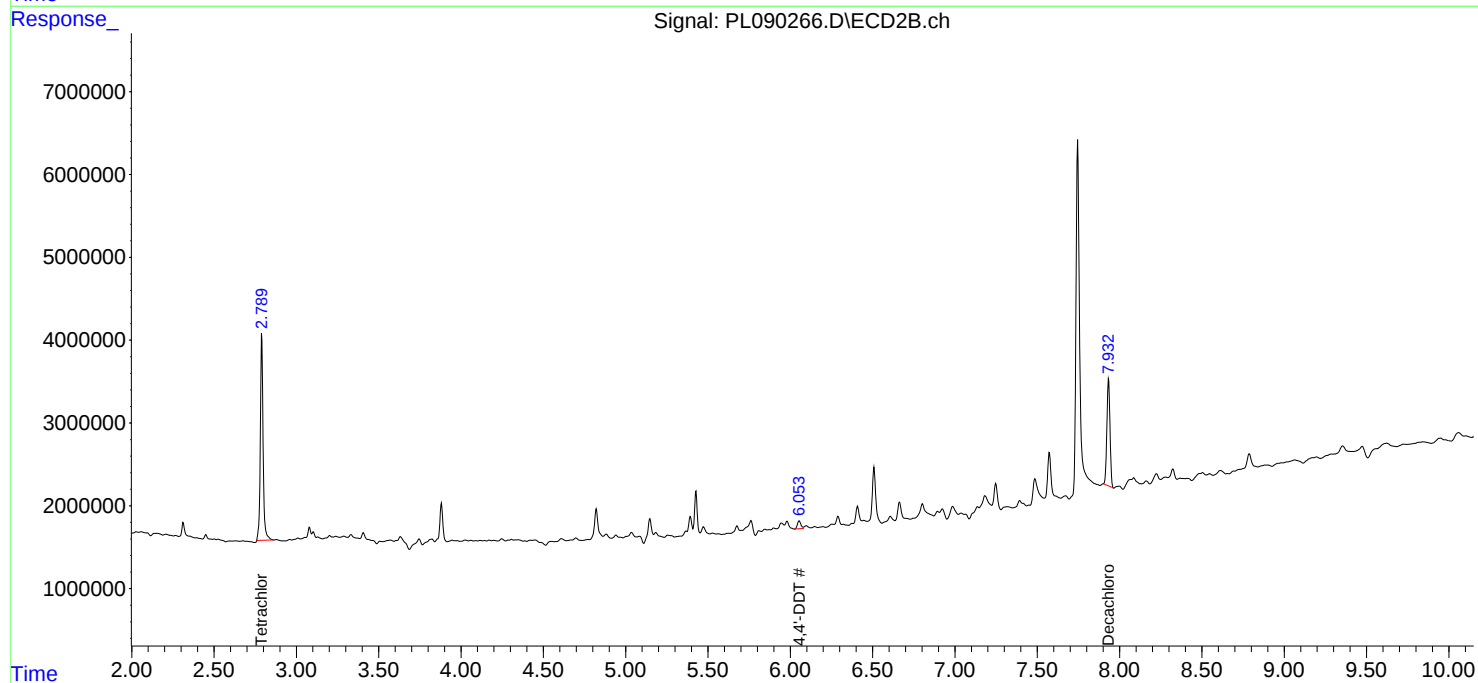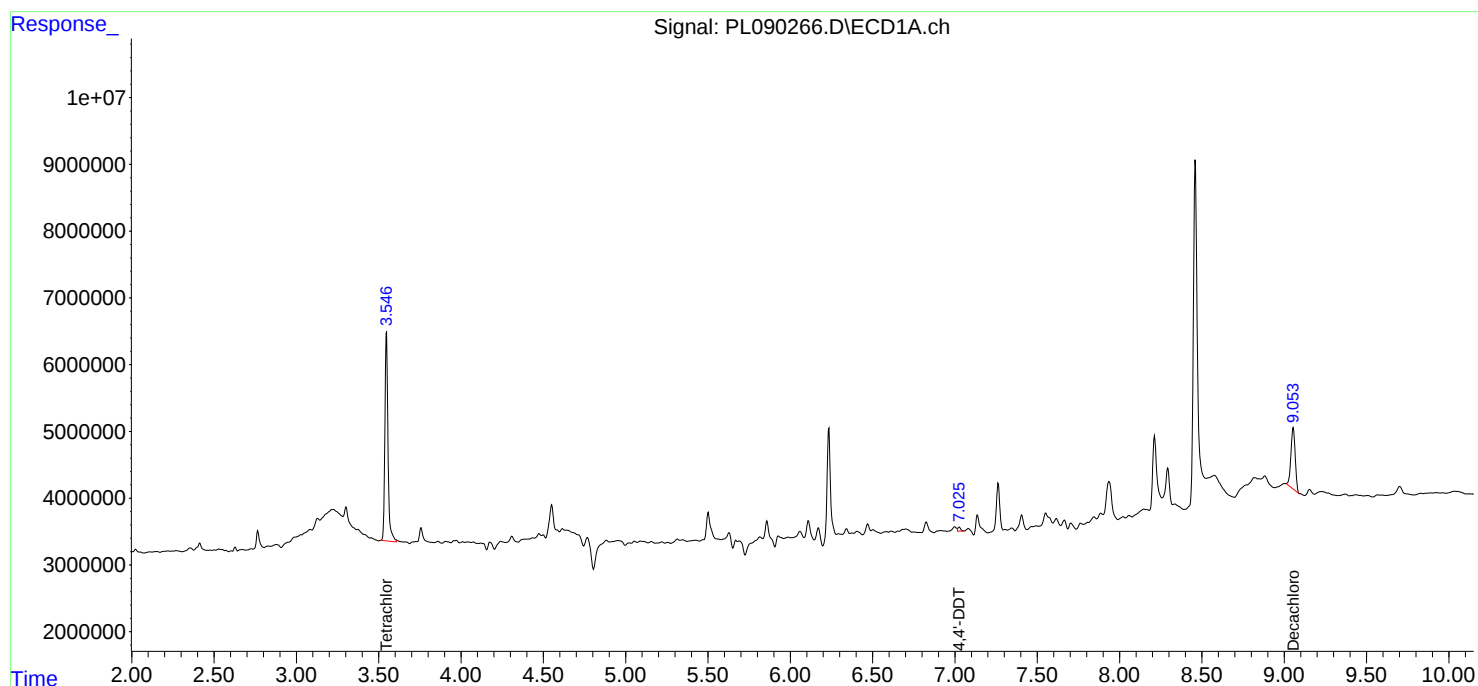

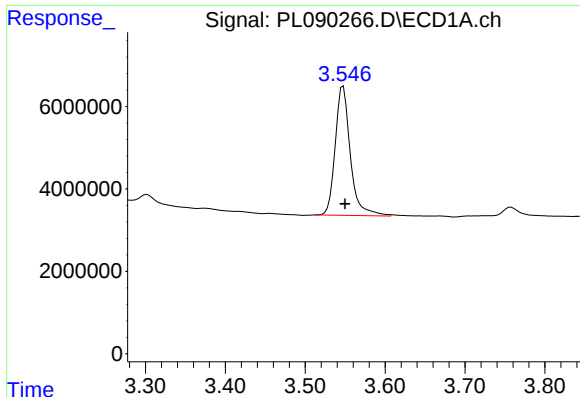


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.004 min
Response: 41128767
Conc: 19.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
OSTL-A6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2024
Supervised By :Ankita Jodhani 06/21/2024

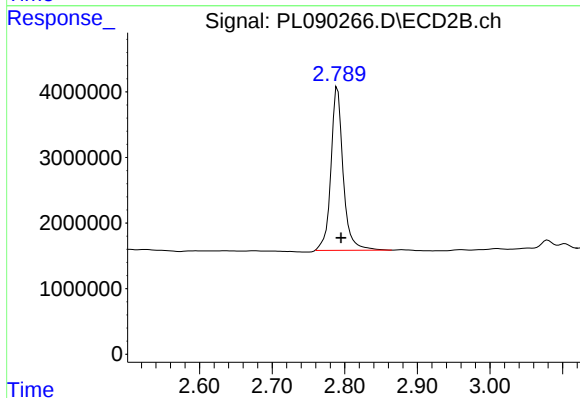


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: -0.005 min
Response: 29182341
Conc: 20.35 ng/ml

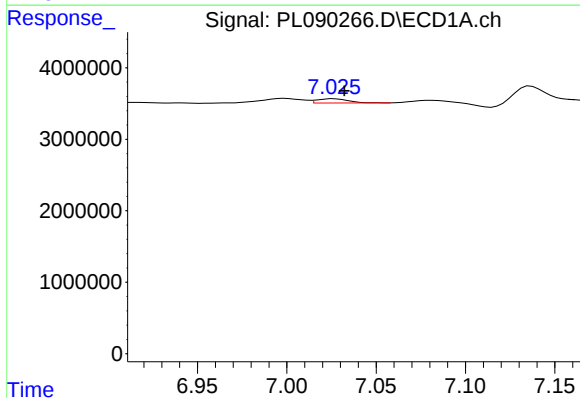


#17 4,4'-DDT

R.T.: 7.027 min
Delta R.T.: -0.006 min
Response: 725642
Conc: 0.39 ng/ml

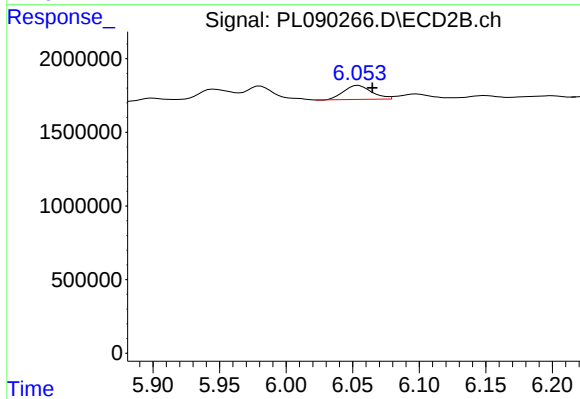

#17 4,4'-DDT

R.T.: 6.055 min
Delta R.T.: -0.010 min
Response: 1376784
Conc: 0.91 ng/ml

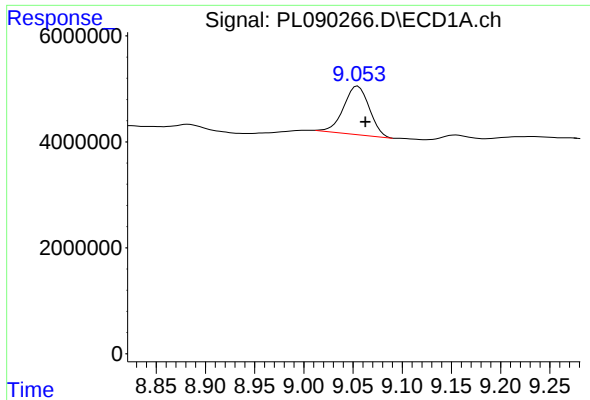


#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.009 min
Response: 16629012
Conc: 11.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
OSTL-A6

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2024
Supervised By :Ankita Jodhani 06/21/2024

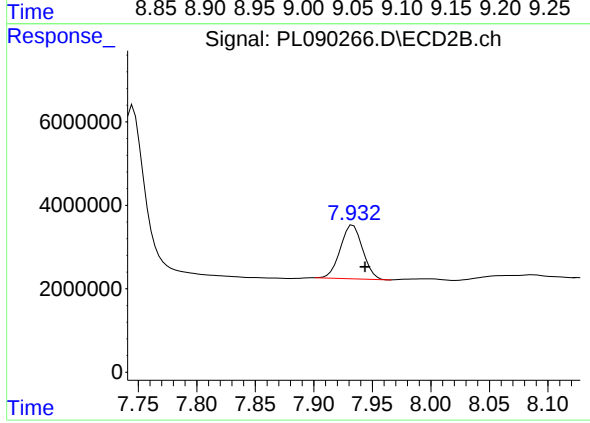

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: -0.010 min
Response: 17038025
Conc: 11.47 ng/ml