

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062119\
 Data File : PL049749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 13:37
 Operator : SM\AJ
 Sample : K3446-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-007-B255-061819

Manual Integrations
 APPROVED

Ankita
 6/24/2019 9:21:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 23:10:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.934	173.1E6	44997572	15.347	14.697
28)	SA Decachlor...	7.990	8.972	135.1E6	37031492	10.634	11.031
Target Compounds							
12)	B 4,4'-DDE	5.431	6.260	24821376	4766036	1.490m	1.373m
17)	MA 4,4'-DDT	6.176	7.051	23239258	5456792	1.750m	1.863m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062119\
Data File : PL049749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 13:37
Operator : SM\AJ
Sample : K3446-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-007-B255-061819


Manual Integrations
APPROVED

Ankita
6/24/2019 9:21:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 23:10:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

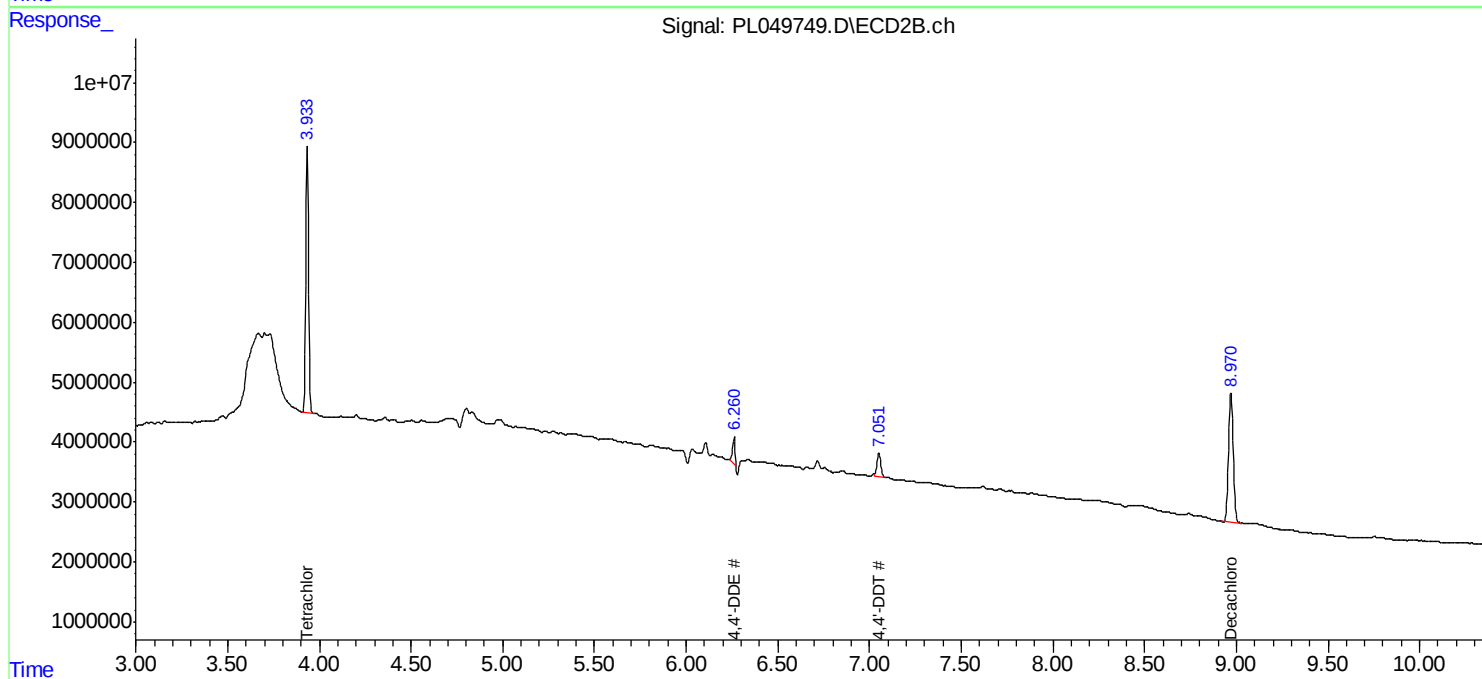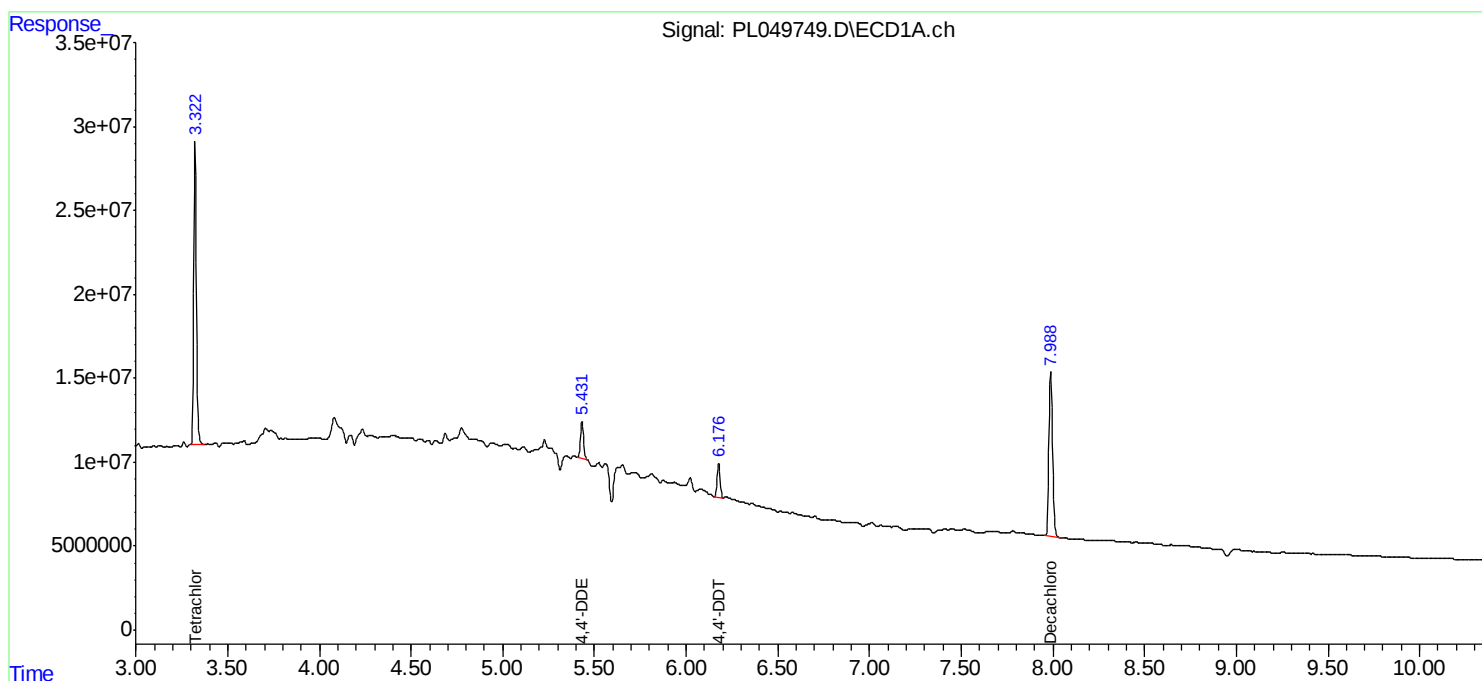

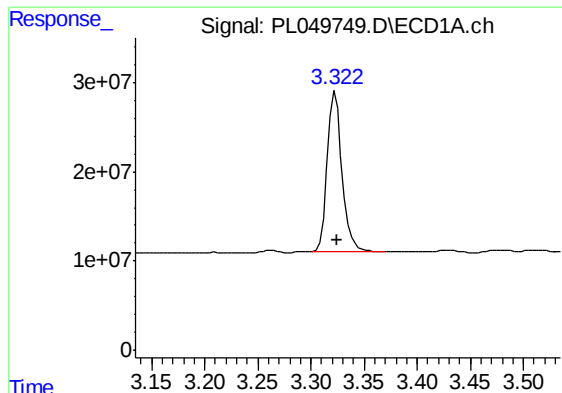


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 173075979
Conc: 15.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-007-B255-061819


Manual Integrations
APPROVED

Ankita
6/24/2019 9:21:17 AM

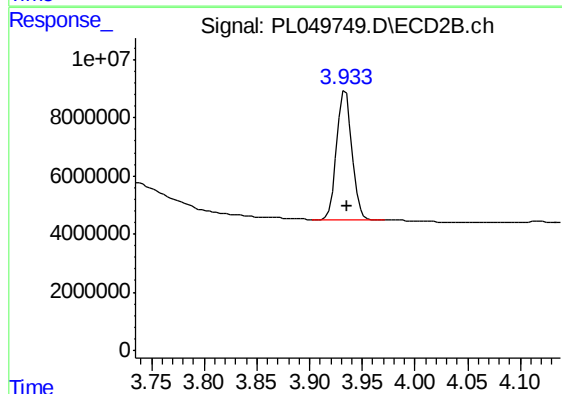


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.001 min
Response: 44997572
Conc: 14.70 ng/ml

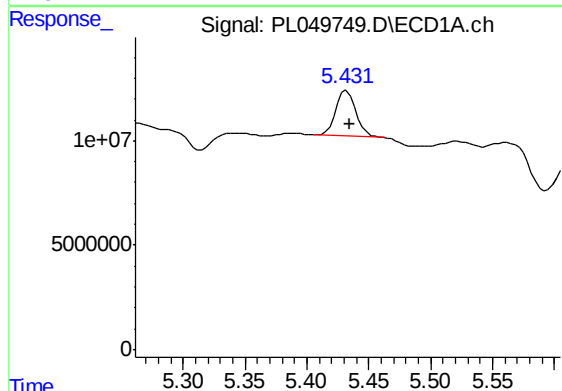


#12 4,4'-DDE

R.T.: 5.431 min
Delta R.T.: -0.003 min
Response: 24821376
Conc: 1.49 ng/ml m

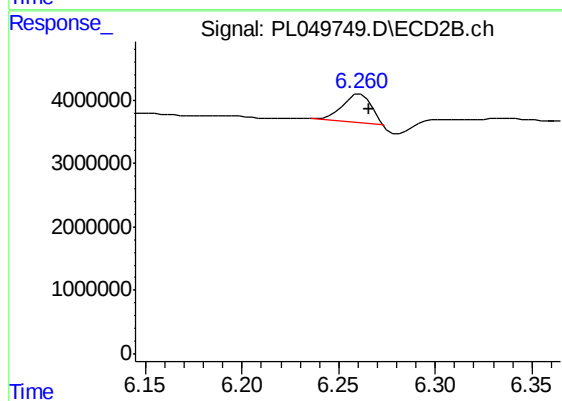

#12 4,4'-DDE

R.T.: 6.260 min
Delta R.T.: -0.006 min
Response: 4766036
Conc: 1.37 ng/ml m

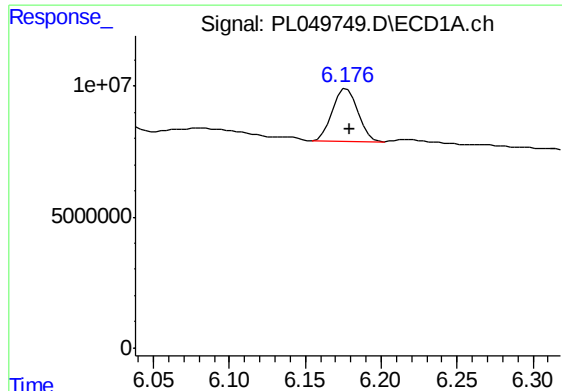


#17 4,4'-DDT

R.T.: 6.176 min
Delta R.T.: -0.004 min
Response: 23239258
Conc: 1.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PST-007-B255-061819


Manual Integrations
APPROVED

Ankita
6/24/2019 9:21:17 AM

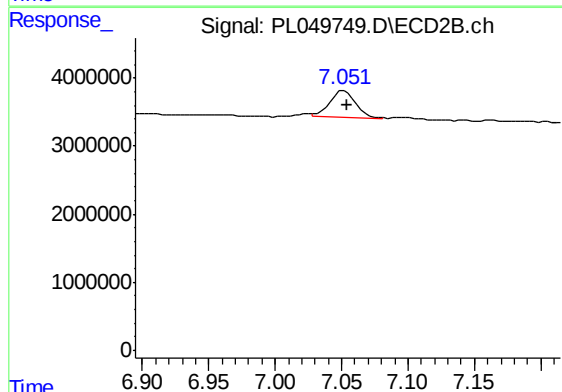


#17 4,4'-DDT

R.T.: 7.051 min
Delta R.T.: -0.003 min
Response: 5456792
Conc: 1.86 ng/ml m

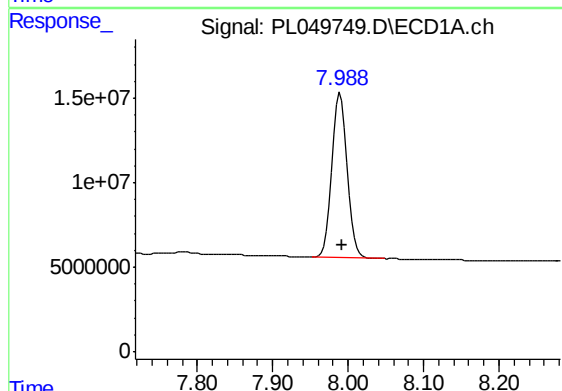

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 135116340
Conc: 10.63 ng/ml

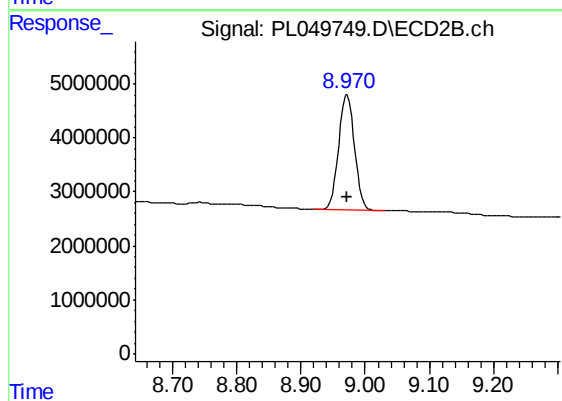

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.001 min
Response: 37031492
Conc: 11.03 ng/ml