

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 11:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:30:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	11165392	19435203	20.309	20.616
28)	SA Decachlor...	10.223	11.430	14053902	20249866	19.831	20.330
Target Compounds							
3)	MA gamma-BHC...	5.596	0.000	485843	0	0.648	N.D. #
4)	MA Heptachlor	5.987f	0.000	451333	0	0.598	N.D. #
6)	B beta-BHC	5.987	0.000	451333	0	1.261	N.D. #
7)	B delta-BHC	0.000	7.000f	0	1822577	N.D.	1.550 #
8)	B Heptachlo...	0.000	7.995	0	400598	N.D.	0.400 #
15)	B Endosulfa...	0.000	9.181f	0	107411	N.D.	0.135 #
18)	B Endrin al...	8.377	0.000	751938	0	1.485	N.D. #
21)	B Endrin ke...	9.128	0.000	552774	0	0.726	N.D. #
23)	Chlordane-1	0.000	6.940f	0	262402	N.D.	9.292 #
24)	Chlordane-2	6.485	0.000	283866	0	10.601	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 11:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

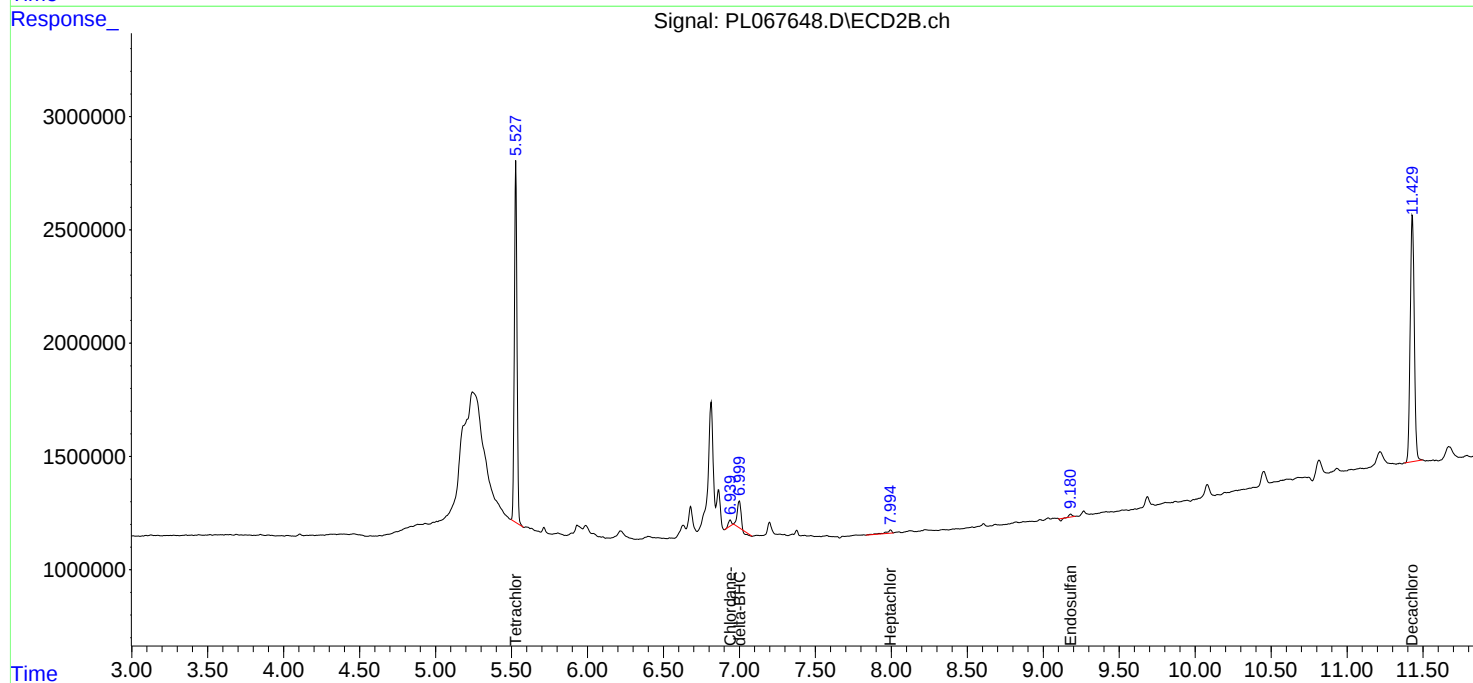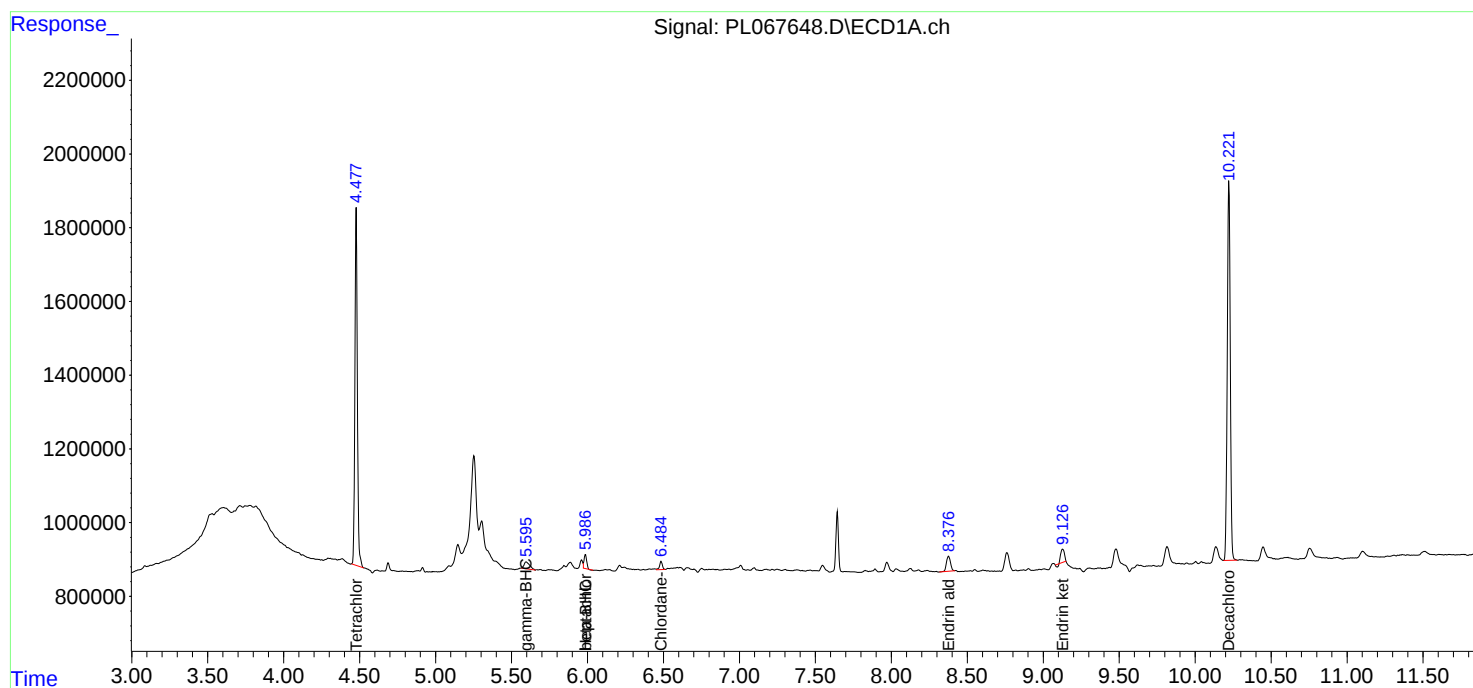


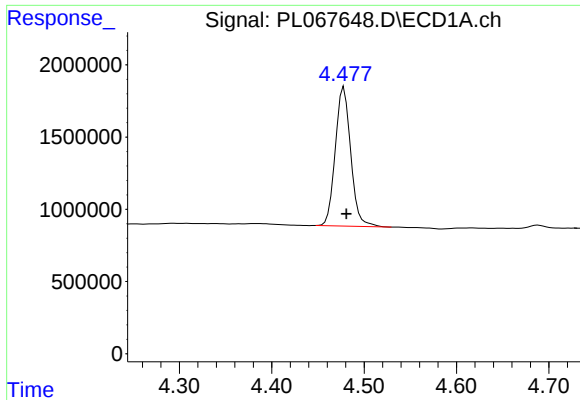

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11165392
Conc: 20.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

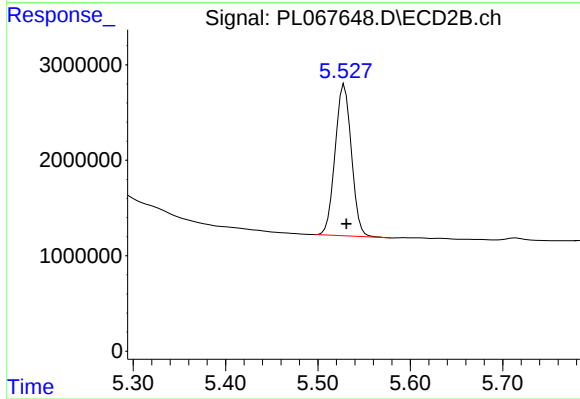


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 19435203
Conc: 20.62 ng/ml

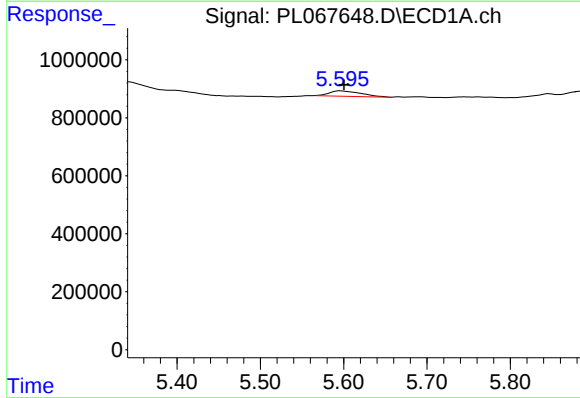


#3 gamma-BHC (Lindane)

R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 485843
Conc: 0.65 ng/ml

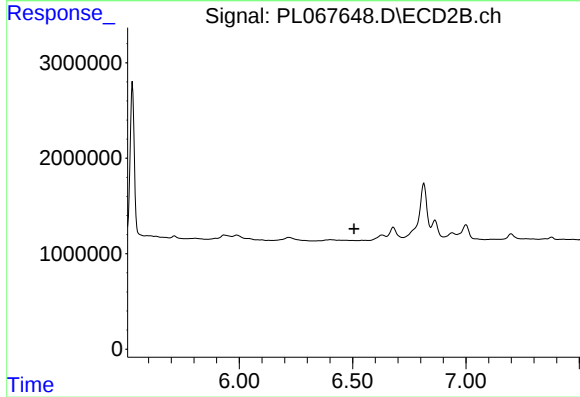

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

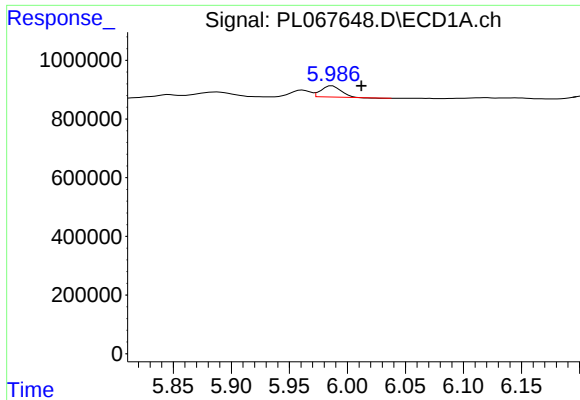

#4 Heptachlor


R.T.: 5.987 min
Delta R.T.: -0.025 min
Response: 451333
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

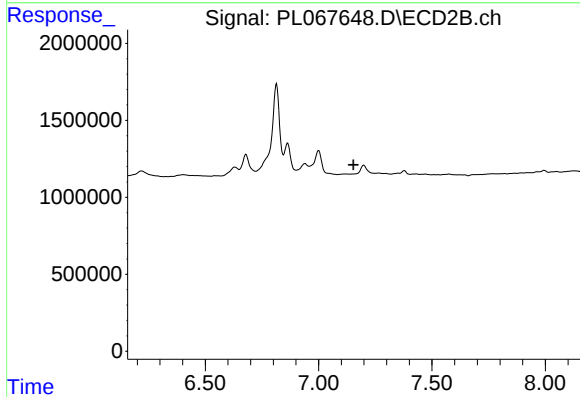


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

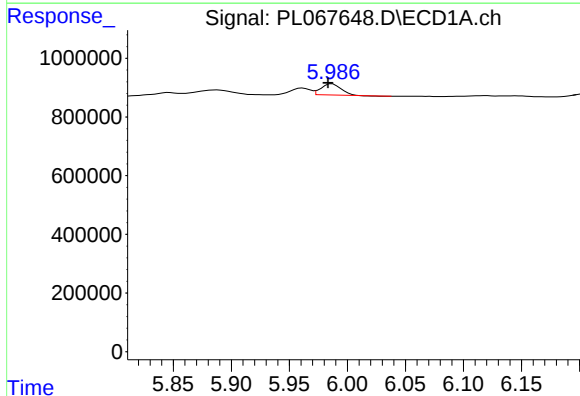


#6 beta-BHC

R.T.: 5.987 min
Delta R.T.: 0.004 min
Response: 451333
Conc: 1.26 ng/ml

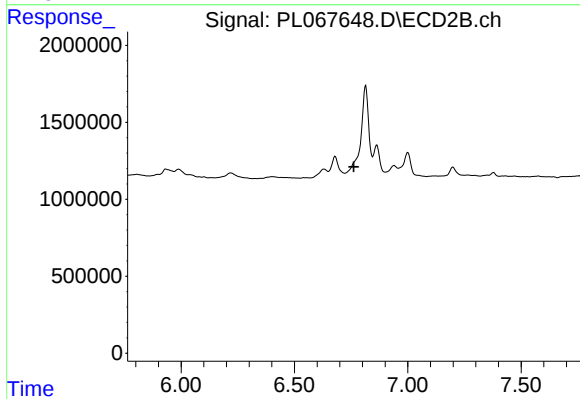

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

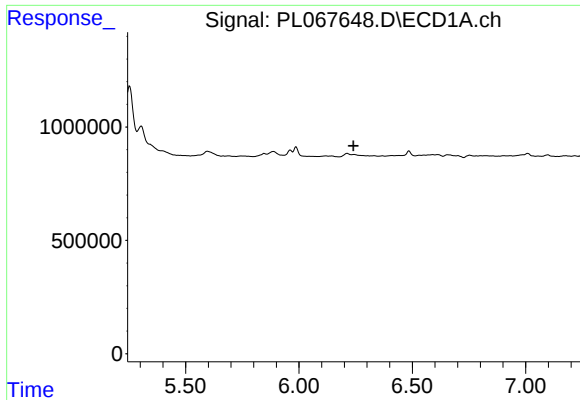

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

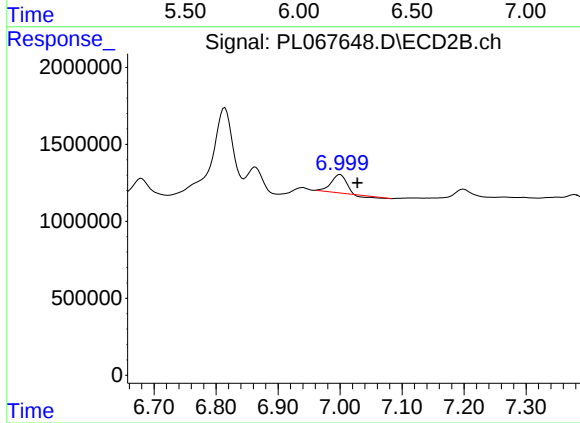


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 1822577
Conc: 1.55 ng/ml

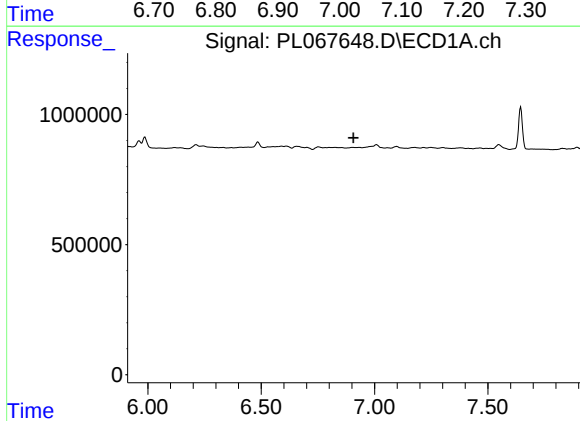


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

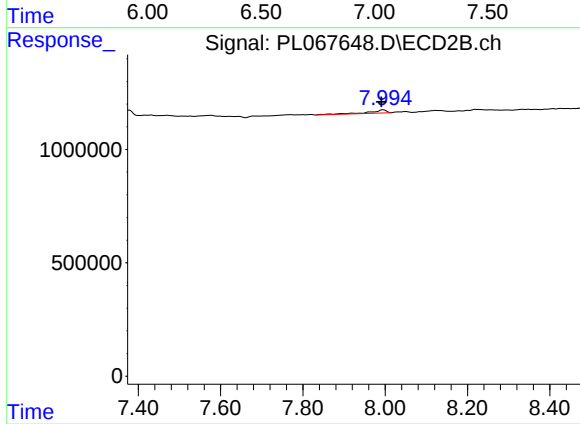

#8 Heptachlor epoxide


R.T.: 7.995 min
Delta R.T.: 0.004 min
Response: 400598
Conc: 0.40 ng/ml

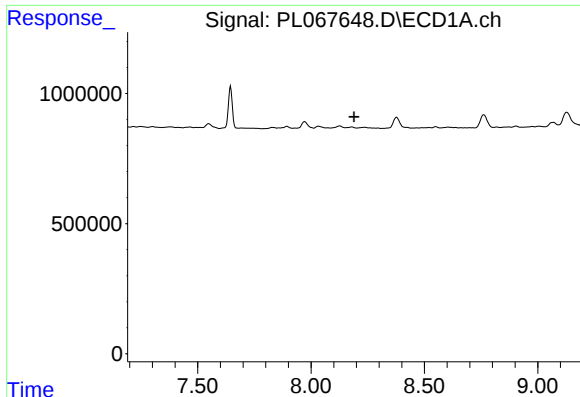

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

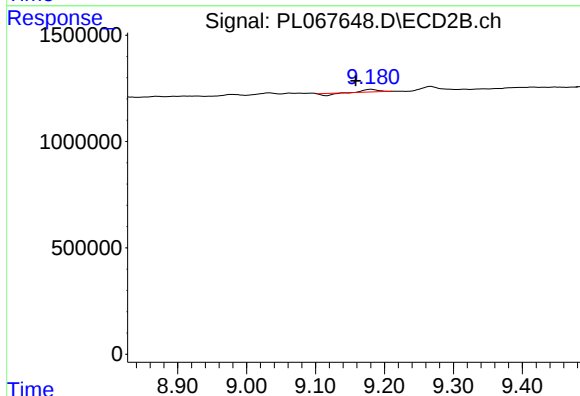


#15 Endosulfan II

R.T.: 9.181 min
Delta R.T.: 0.023 min
Response: 107411
Conc: 0.13 ng/ml

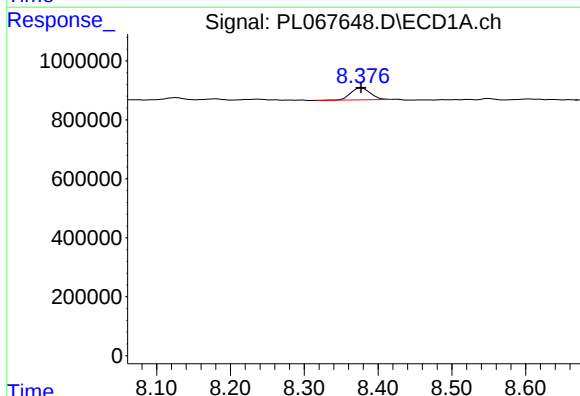


#18 Endrin aldehyde

R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 751938
Conc: 1.49 ng/ml

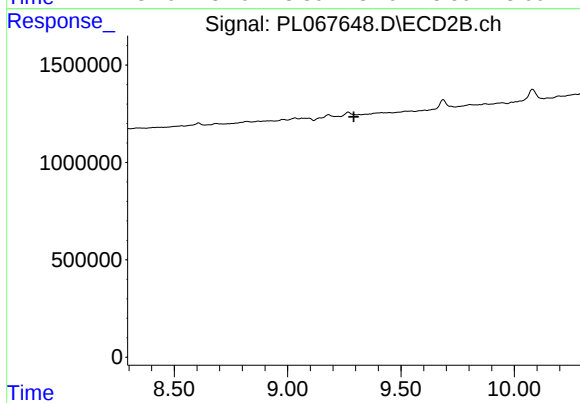

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.292 min
Response: 0
Conc: N.D.

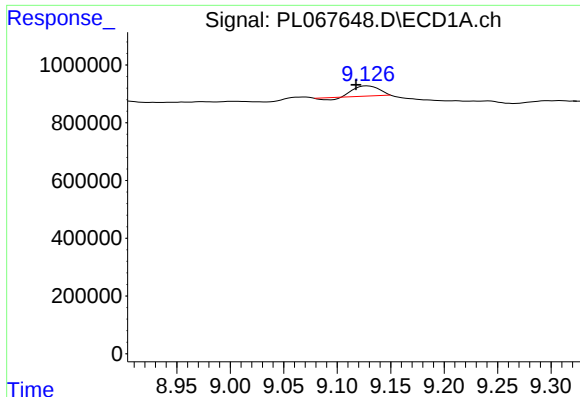

#21 Endrin ketone


R.T.: 9.128 min
Delta R.T.: 0.010 min
Response: 552774
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

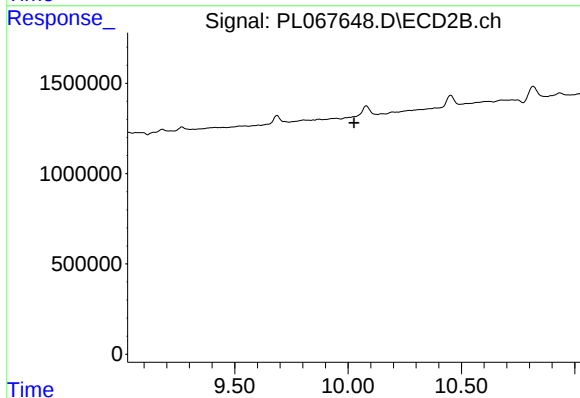


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

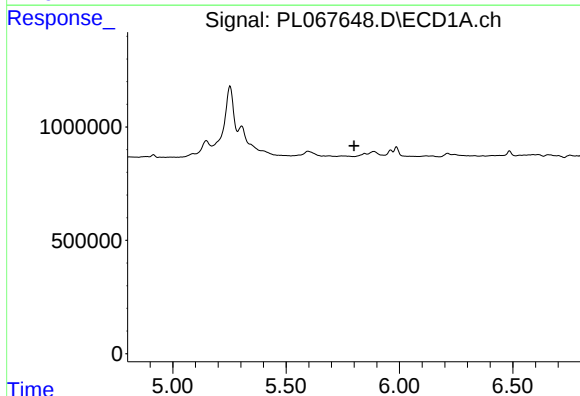


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.800 min
Response: 0
Conc: N.D.

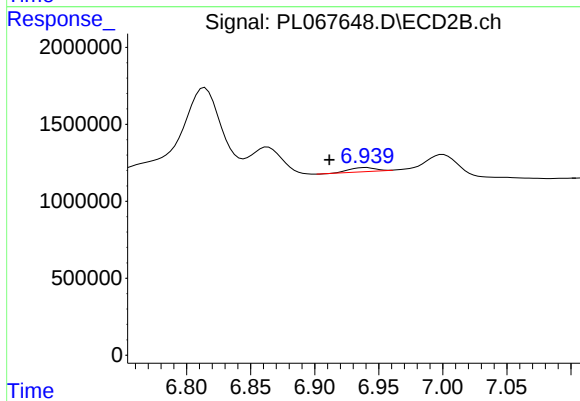

#23 Chlordane-1


R.T.: 6.940 min
Delta R.T.: 0.029 min
Response: 262402
Conc: 9.29 ng/ml

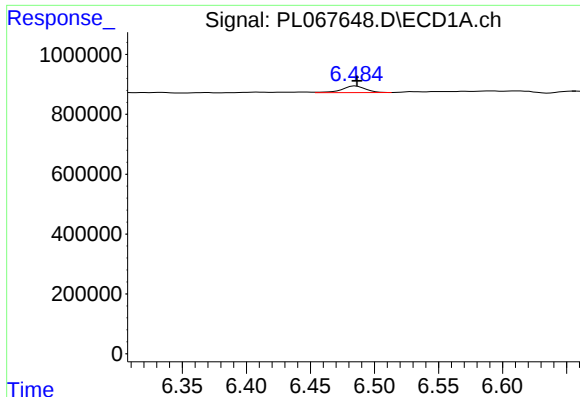

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 283866
Conc: 10.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

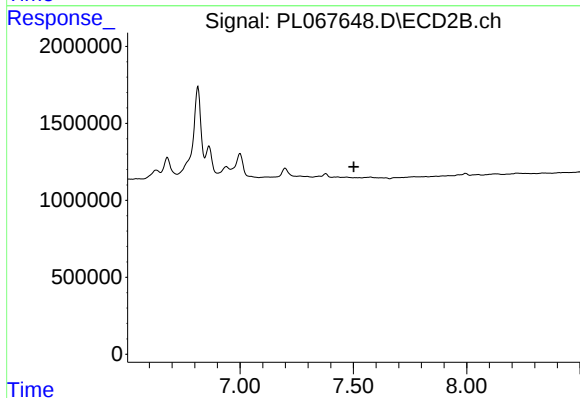


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

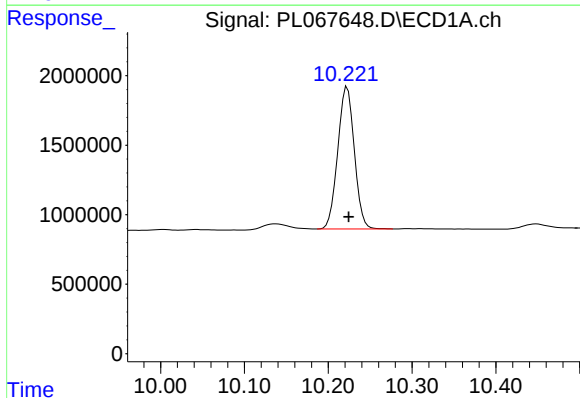

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.002 min
Response: 14053902
Conc: 19.83 ng/ml

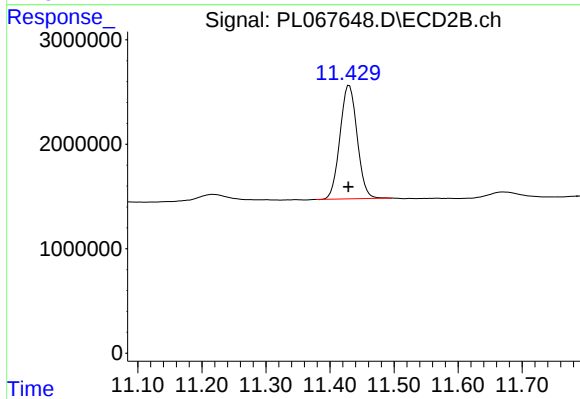

#28 Decachlorobiphenyl

R.T.: 11.430 min
Delta R.T.: 0.001 min
Response: 20249866
Conc: 20.33 ng/ml