

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 14:18
 Operator : AR\AJ
 Sample : M2709-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-AMND-COMP-N(CL-22)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:32:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	11672608	20742297	21.231	22.002
28)	SA Decachlor...	10.220	11.427	14698175	21819056	20.740	21.905
Target Compounds							
2)	A alpha-BHC	0.000	6.088f	0	364601	N.D.	0.295 #
3)	MA gamma-BHC...	5.599	0.000	816664	0	1.090	N.D. #
5)	MB Aldrin	6.335	0.000	758596	0	1.031	N.D. #
6)	B beta-BHC	5.964f	0.000	273982	0	0.766	N.D. #
12)	B 4,4'-DDE	0.000	8.540	0	477206	N.D.	0.527 #
13)	MA Dieldrin	7.592	0.000	168288	0	0.240	N.D. #
15)	B Endosulfa...	0.000	9.179f	0	426660	N.D.	0.535 #
20)	A Methoxychlor	8.890f	0.000	206103	0	0.580	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 14:18
Operator : AR\AJ
Sample : M2709-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:32:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

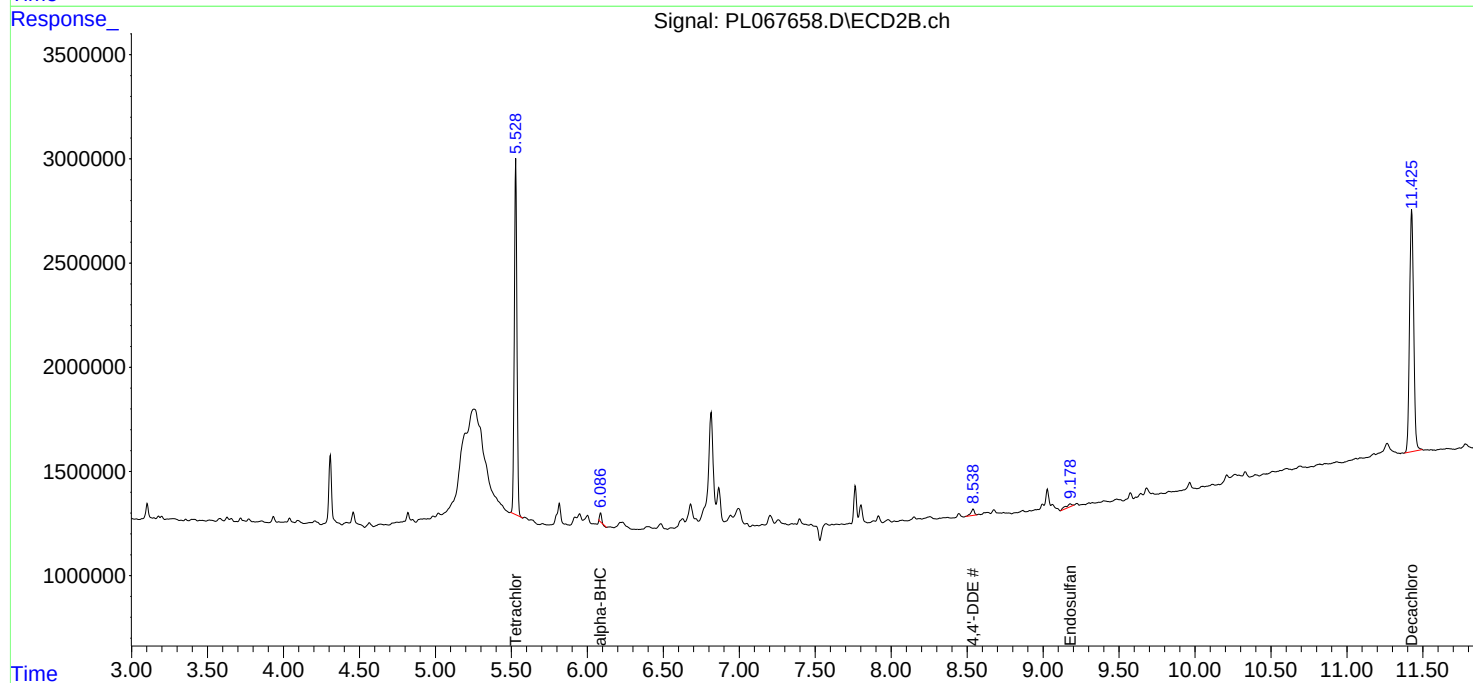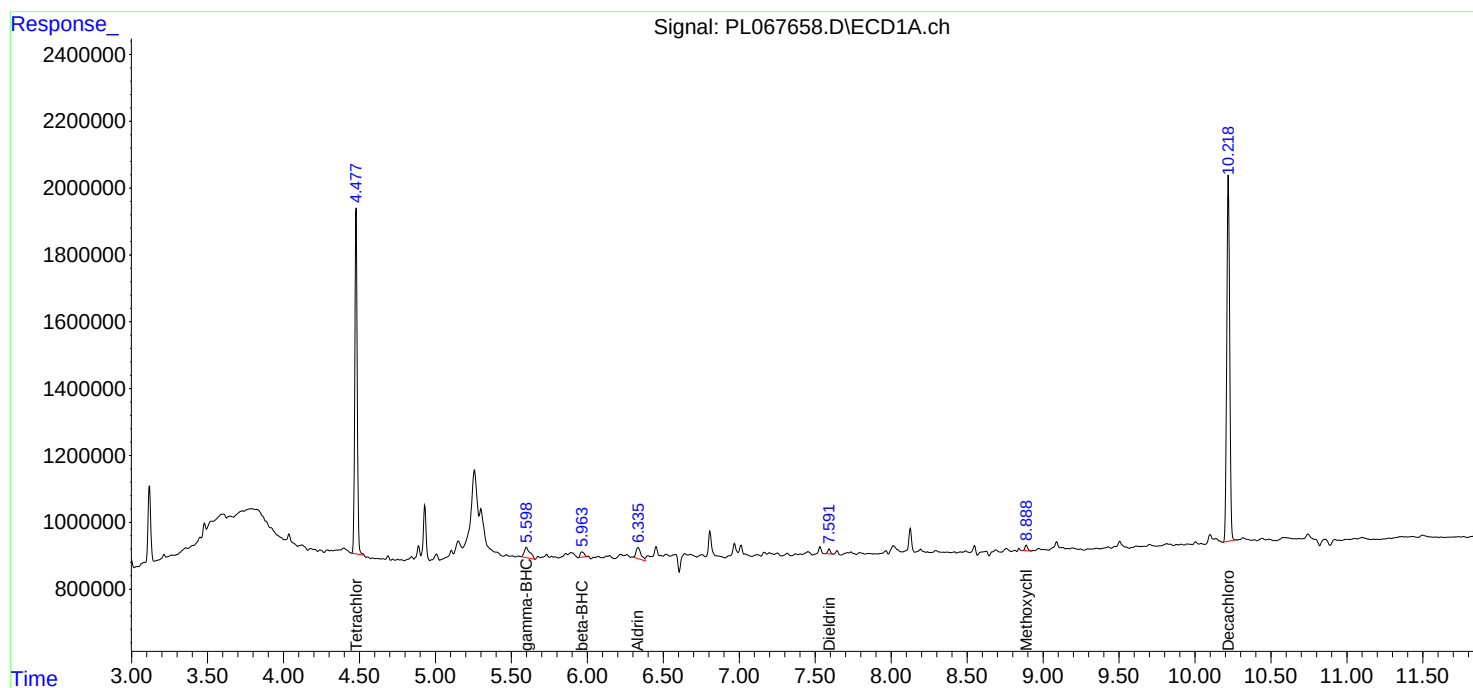


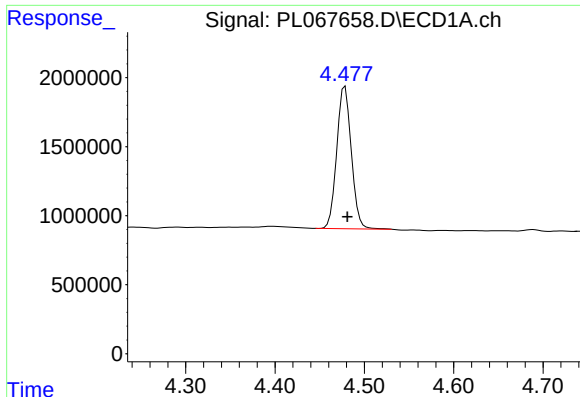

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11672608
Conc: 21.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

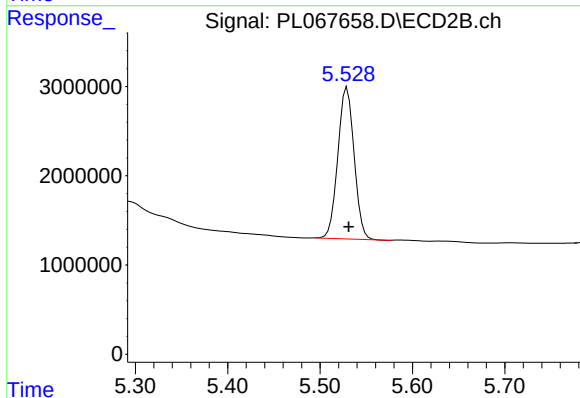


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 20742297
Conc: 22.00 ng/ml

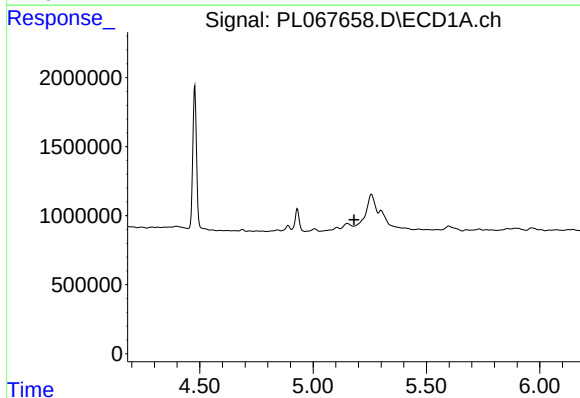


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.181 min
Response: 0
Conc: N.D.

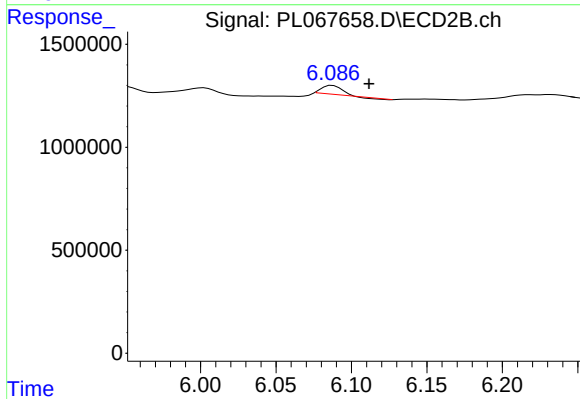

#2 alpha-BHC


R.T.: 6.088 min
Delta R.T.: -0.024 min
Response: 364601
Conc: 0.29 ng/ml

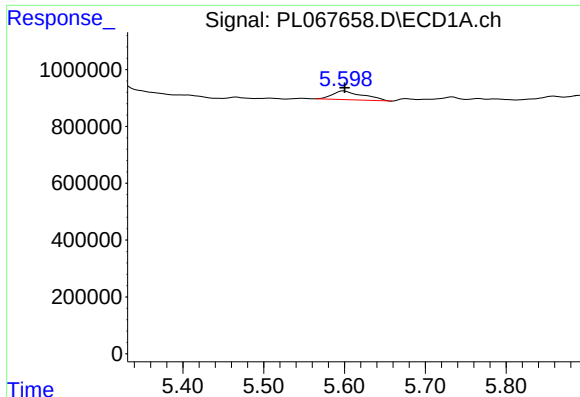

#3 gamma-BHC (Lindane)


R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 816664
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

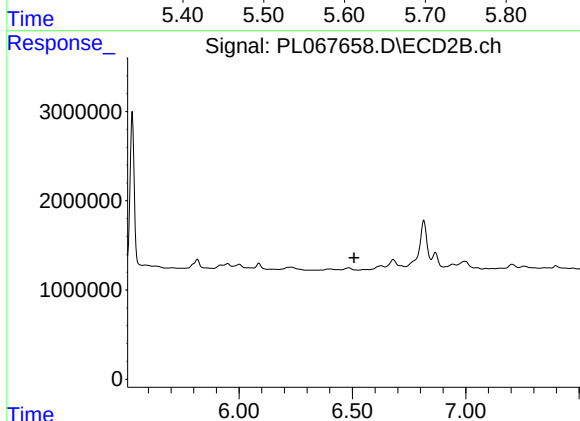


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

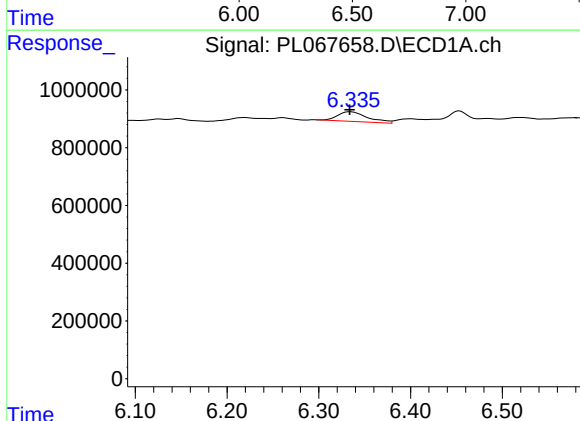


#5 Aldrin

R.T.: 6.335 min
Delta R.T.: 0.000 min
Response: 758596
Conc: 1.03 ng/ml

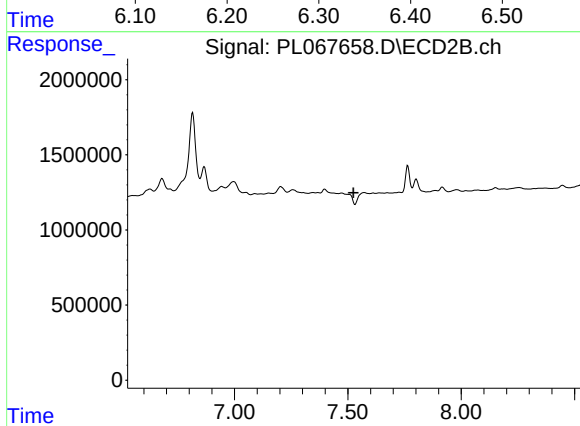

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

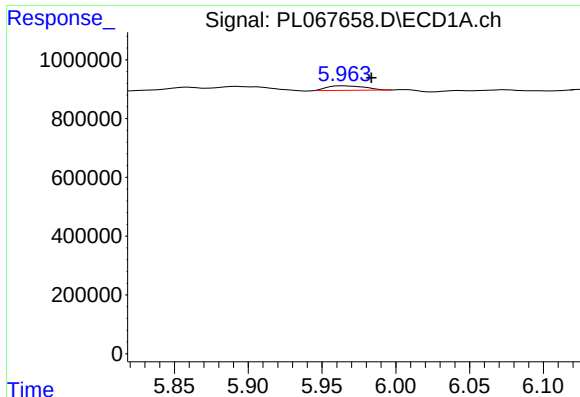

#6 beta-BHC


R.T.: 5.964 min
Delta R.T.: -0.019 min
Response: 273982
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

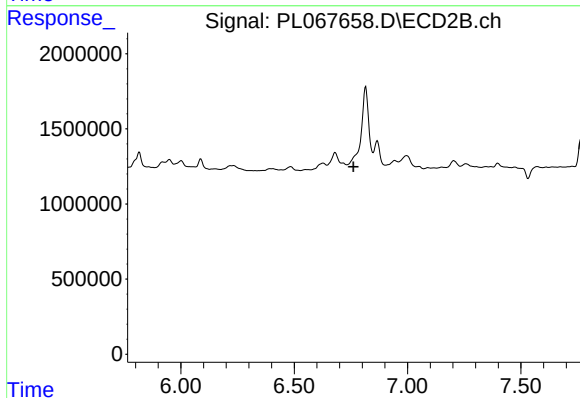


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

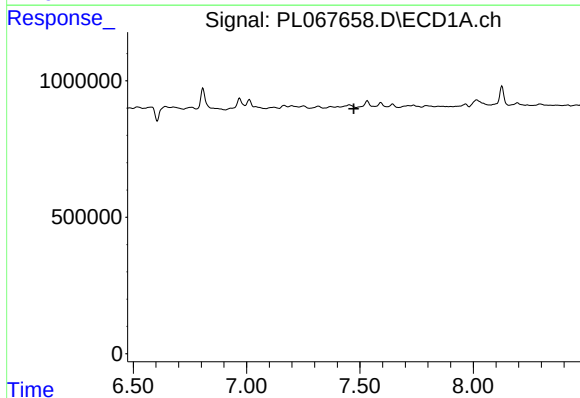


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.473 min
Response: 0
Conc: N.D.

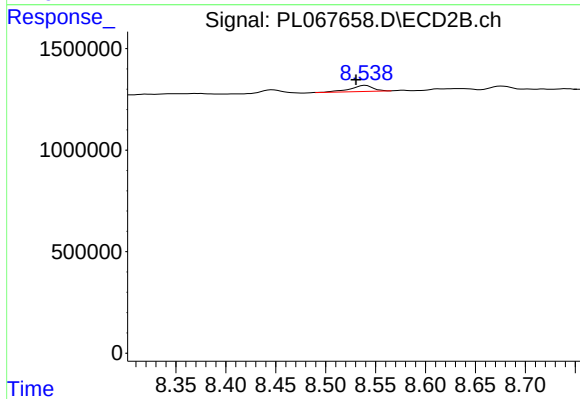

#12 4,4'-DDE


R.T.: 8.540 min
Delta R.T.: 0.010 min
Response: 477206
Conc: 0.53 ng/ml

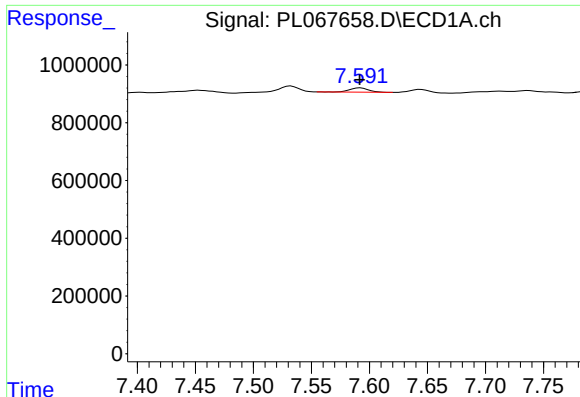

#13 Dieldrin


R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 168288
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

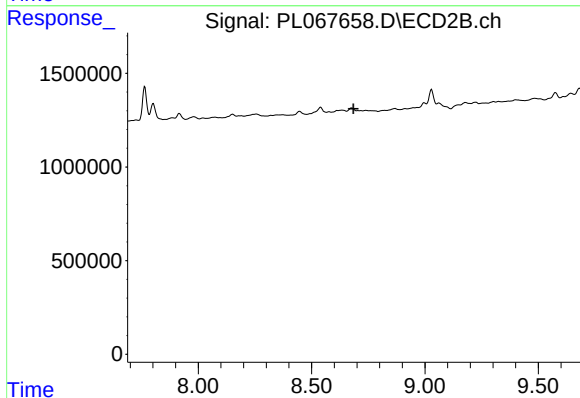


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.685 min
Response: 0
Conc: N.D.

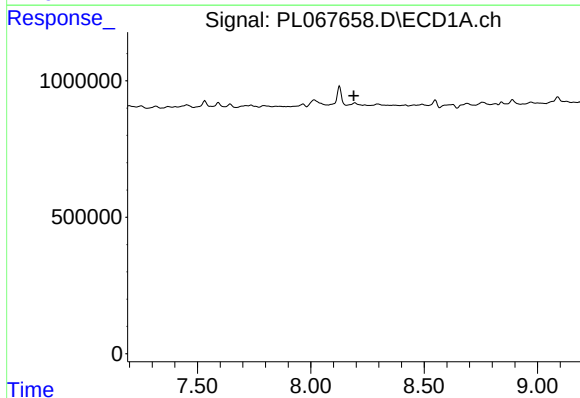


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

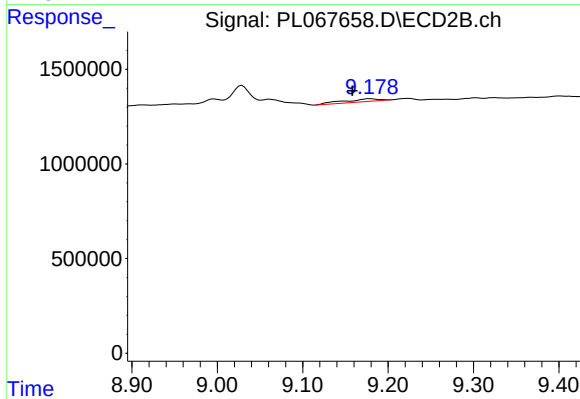

#15 Endosulfan II


R.T.: 9.179 min
Delta R.T.: 0.021 min
Response: 426660
Conc: 0.54 ng/ml

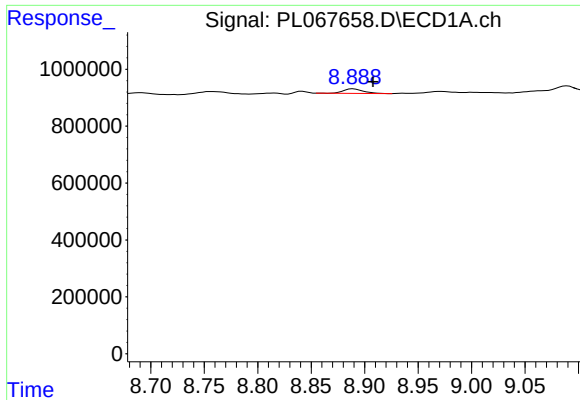

#20 Methoxychlor


R.T.: 8.890 min
Delta R.T.: -0.018 min
Response: 206103
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

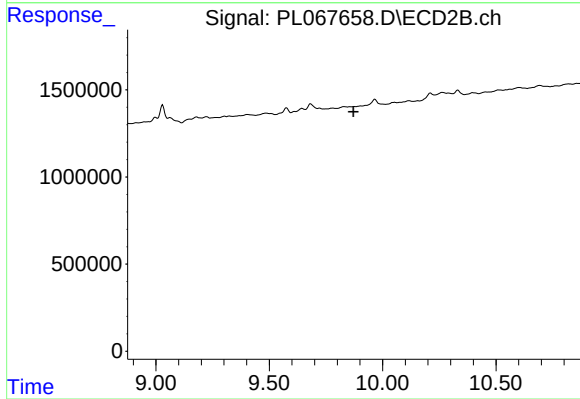


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.872 min
Response: 0
Conc: N.D.

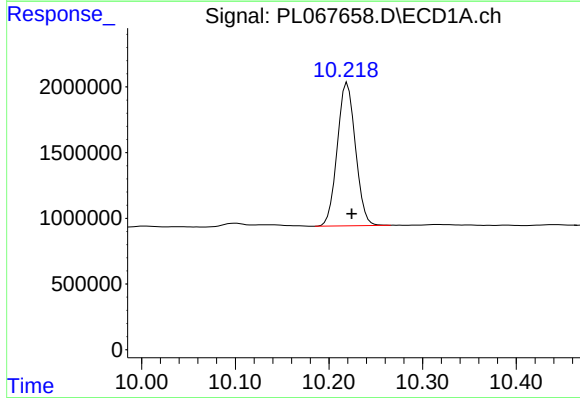

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 14698175
Conc: 20.74 ng/ml

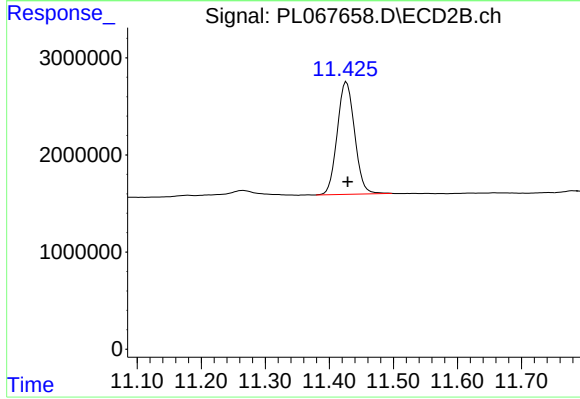

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 21819056
Conc: 21.91 ng/ml