

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 14:35
 Operator : AR\AJ
 Sample : M2709-17
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-AMND-COMP-O(CL-23)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:32:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	11763241	20454739	21.396	21.697
28)	SA Decachlor...	10.220	11.428	11028848	15121364	15.562	15.181
Target Compounds							
3)	MA gamma-BHC...	5.601	0.000	641133	0	0.855	N.D. #
5)	MB Aldrin	6.331	0.000	358219	0	0.487	N.D. #
6)	B beta-BHC	5.963f	0.000	195695	0	0.547	N.D. #
7)	B delta-BHC	0.000	7.000f	0	1089557	N.D.	0.927 #
13)	MA Dieldrin	0.000	8.676	0	489483	N.D.	0.539 #
15)	B Endosulfa...	0.000	9.179f	0	1657579	N.D.	2.079 #
20)	A Methoxychlor	8.891f	0.000	313670	0	0.882	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 14:35
Operator : AR\AJ
Sample : M2709-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-O(CL-23)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:32:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

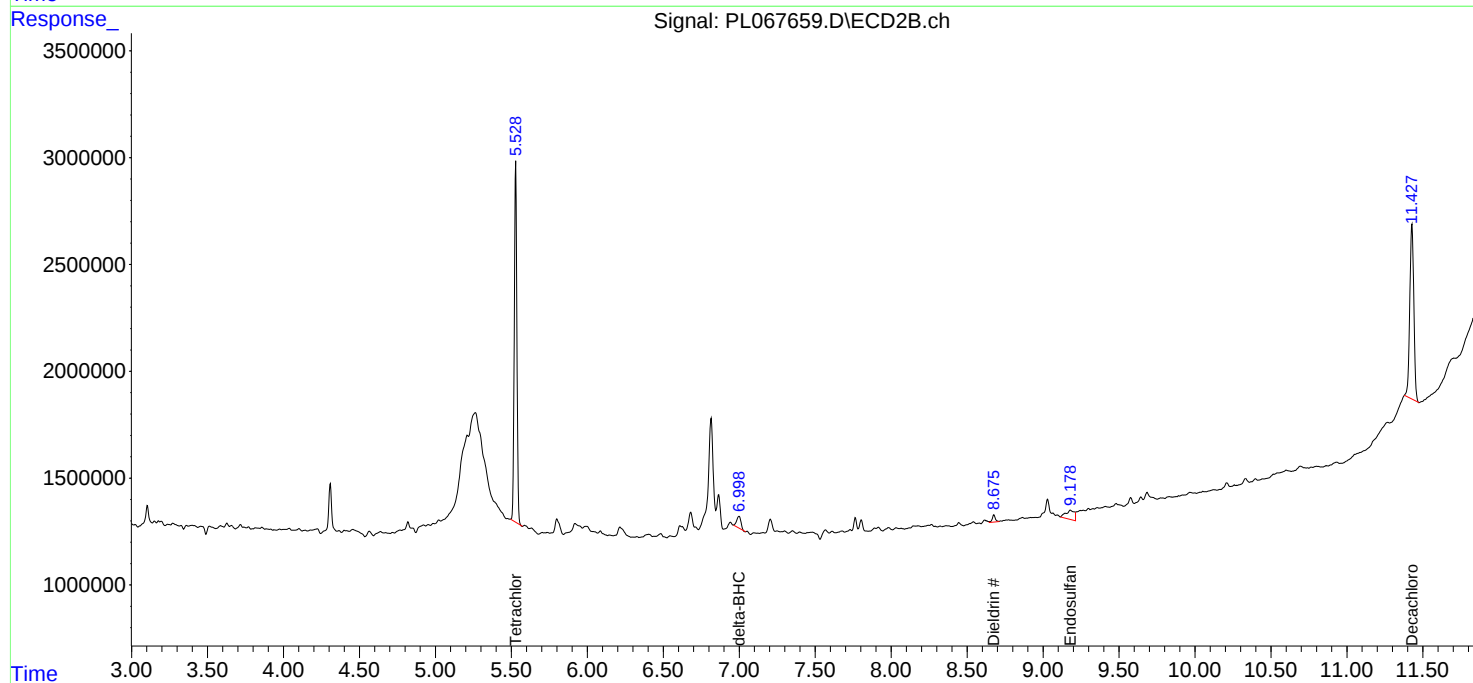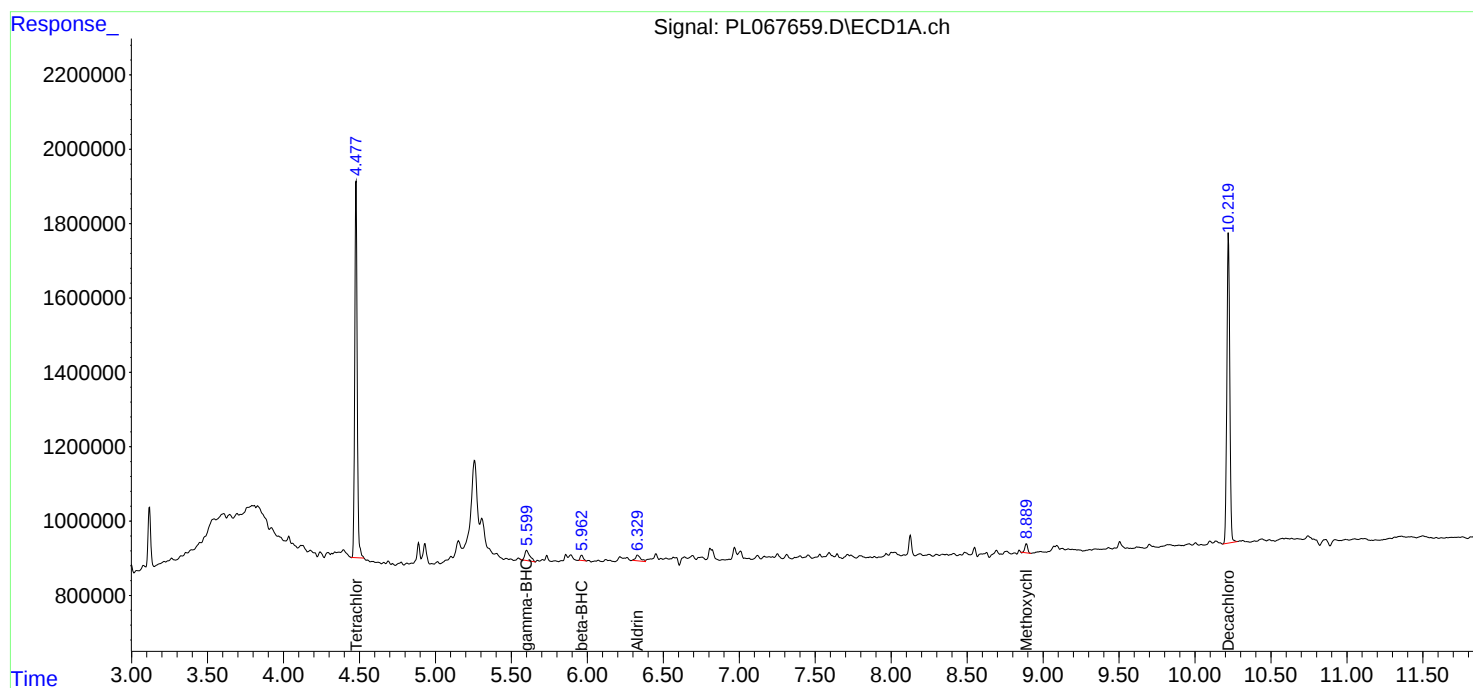


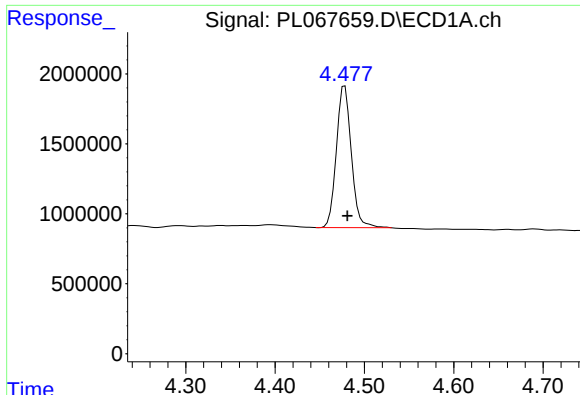

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11763241
Conc: 21.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-O(CL-23)

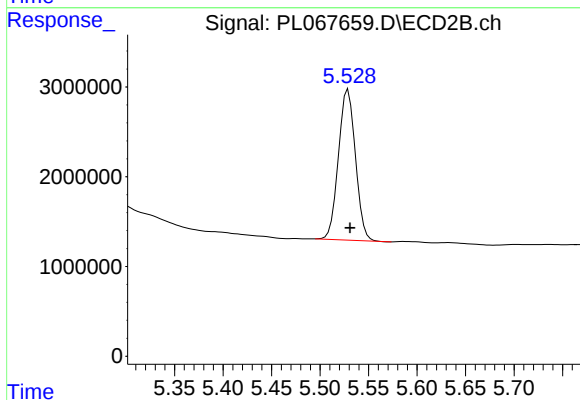


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 20454739
Conc: 21.70 ng/ml

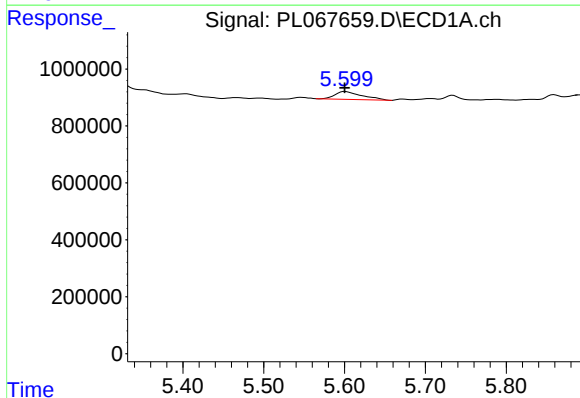


#3 gamma-BHC (Lindane)

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 641133
Conc: 0.86 ng/ml

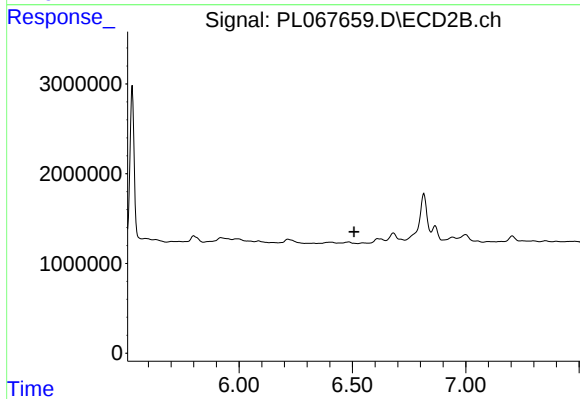

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

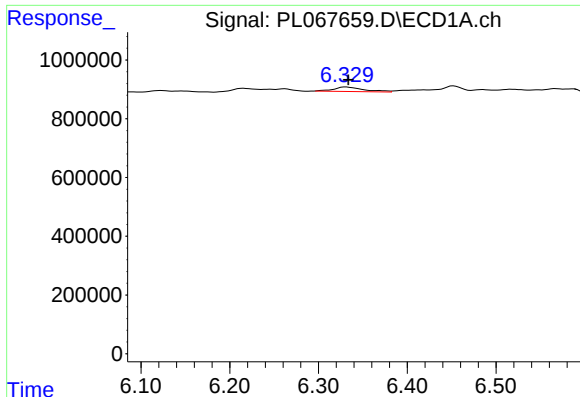

#5 Aldrin


R.T.: 6.331 min
Delta R.T.: -0.003 min
Response: 358219
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-O(CL-23)

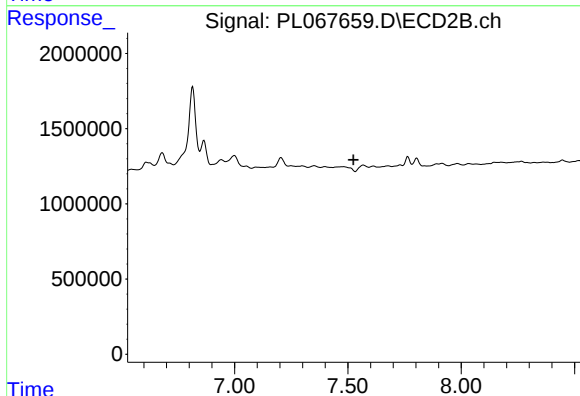


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

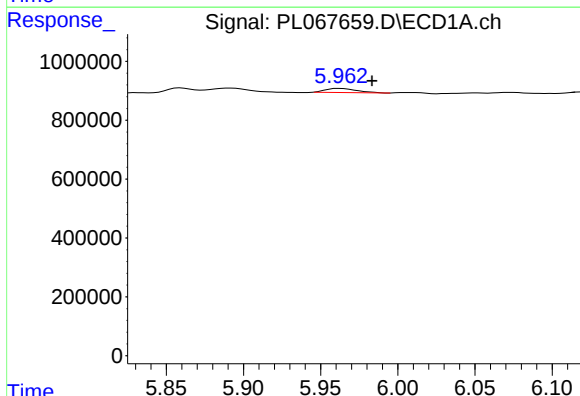


#6 beta-BHC

R.T.: 5.963 min
Delta R.T.: -0.021 min
Response: 195695
Conc: 0.55 ng/ml

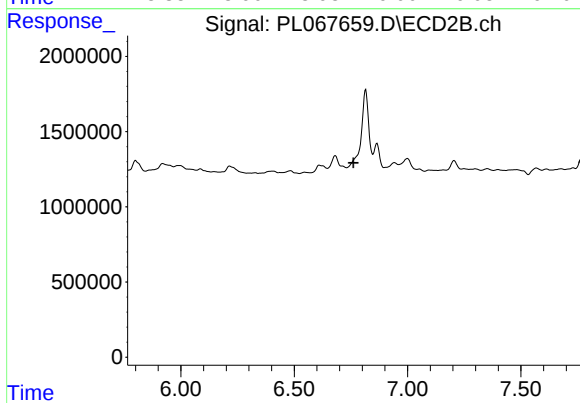

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

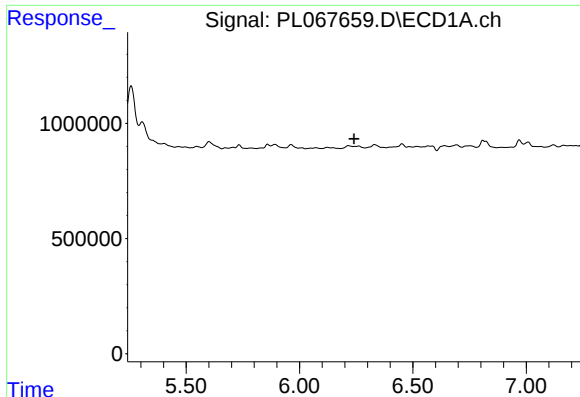

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-O(CL-23)

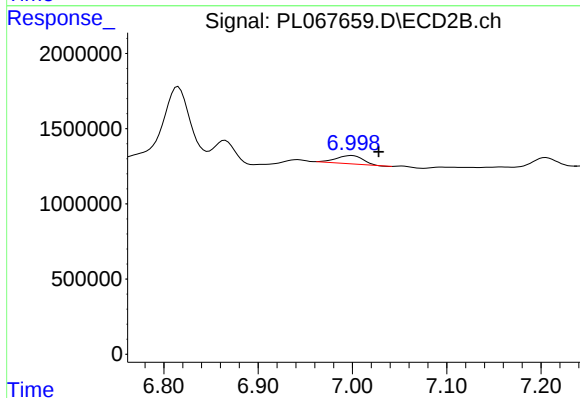


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 1089557
Conc: 0.93 ng/ml

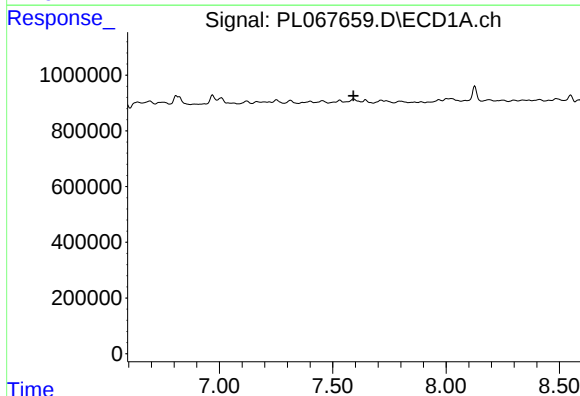


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.592 min
Response: 0
Conc: N.D.

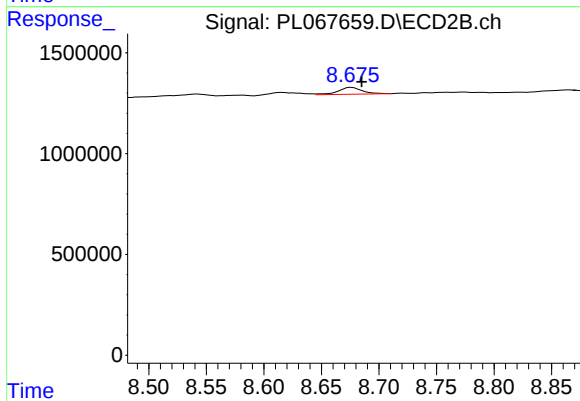

#13 Dieldrin


R.T.: 8.676 min
Delta R.T.: -0.009 min
Response: 489483
Conc: 0.54 ng/ml

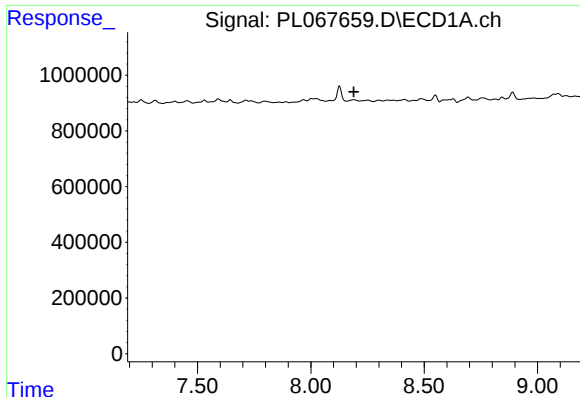

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-O(CL-23)

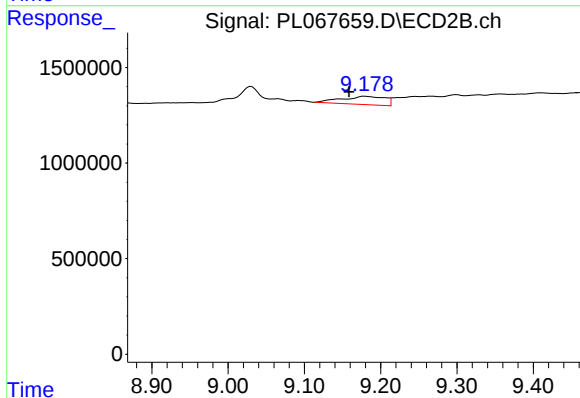


#15 Endosulfan II

R.T.: 9.179 min
Delta R.T.: 0.021 min
Response: 1657579
Conc: 2.08 ng/ml

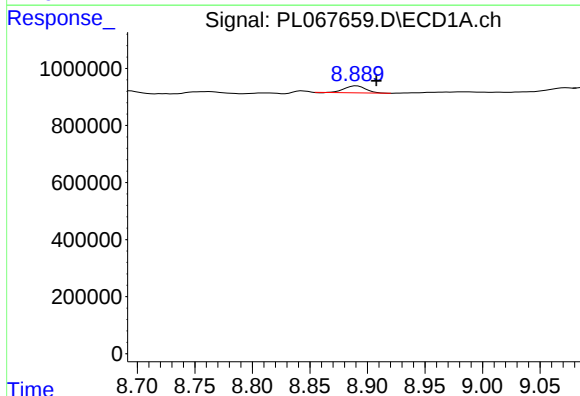


#20 Methoxychlor

R.T.: 8.891 min
Delta R.T.: -0.017 min
Response: 313670
Conc: 0.88 ng/ml

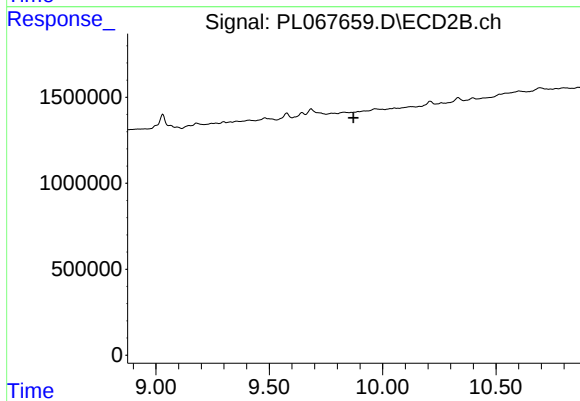

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.872 min
Response: 0
Conc: N.D.

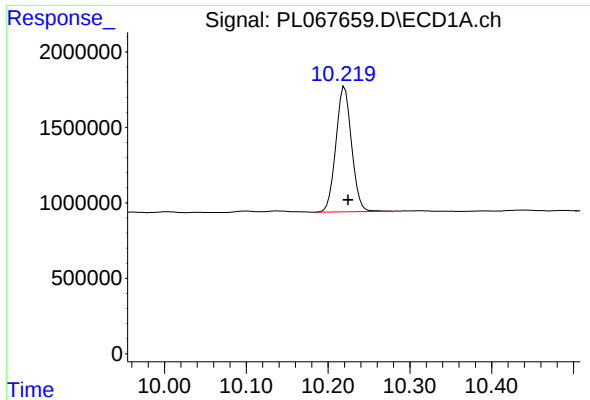

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 11028848
Conc: 15.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMND-COMP-O(CL-23)

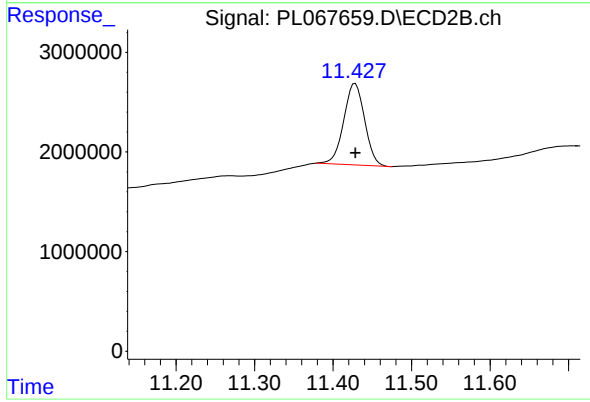

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 15121364
Conc: 15.18 ng/ml