

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 15:08
 Operator : AR\AJ
 Sample : PB137223TB
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB137223TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:32:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	10860993	19597191	19.755	20.788
28)	SA Decachlor...	10.220	11.427	14088698	20623524	19.880	20.705
Target Compounds							
3)	MA gamma-BHC...	5.600	0.000	581150	0	0.775	N.D. #
19)	B Endosulfa...	8.594	0.000	633079	0	0.997	N.D. #
23)	Chlordane-1	0.000	6.941f	0	391498	N.D.	13.864 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 15:08
Operator : AR\AJ
Sample : PB137223TB
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB137223TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:32:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

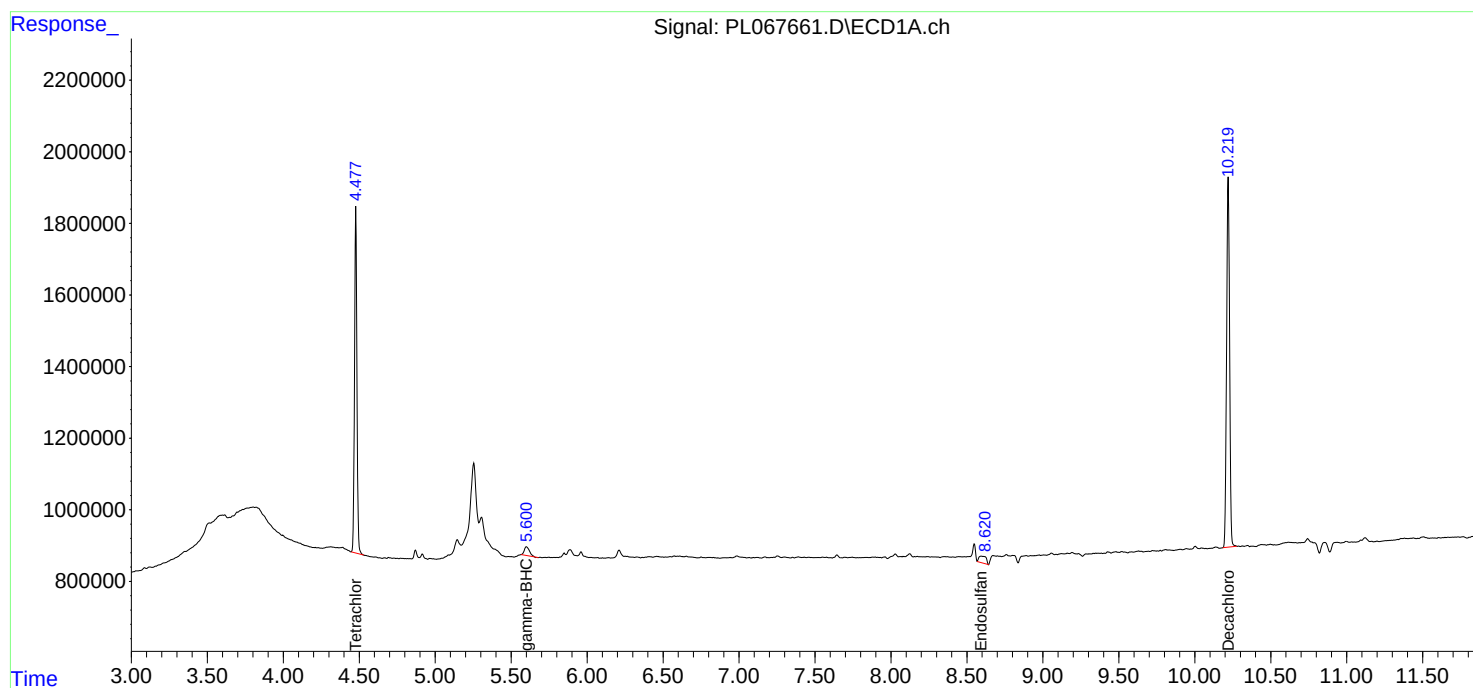


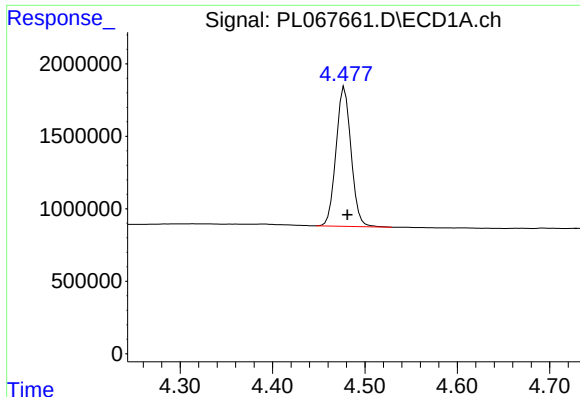

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10860993
Conc: 19.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137223TB

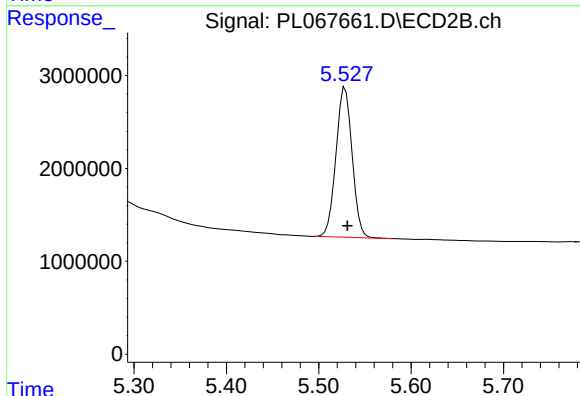


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 19597191
Conc: 20.79 ng/ml

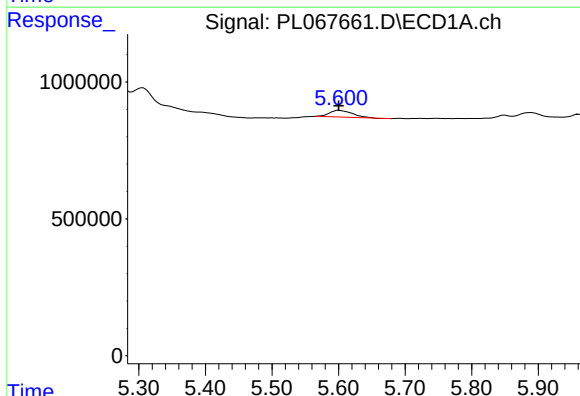


#3 gamma-BHC (Lindane)

R.T.: 5.600 min
Delta R.T.: 0.000 min
Response: 581150
Conc: 0.78 ng/ml

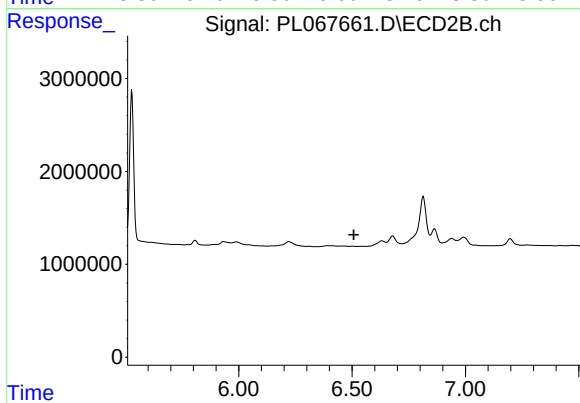

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

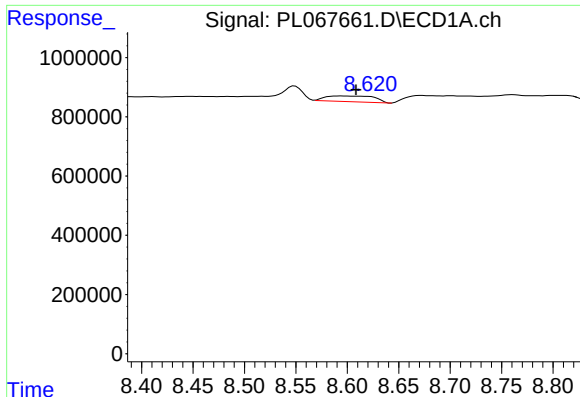

#19 Endosulfan Sulfate


R.T.: 8.594 min

Delta R.T.: -0.014 min

Response: 633079

Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137223TB

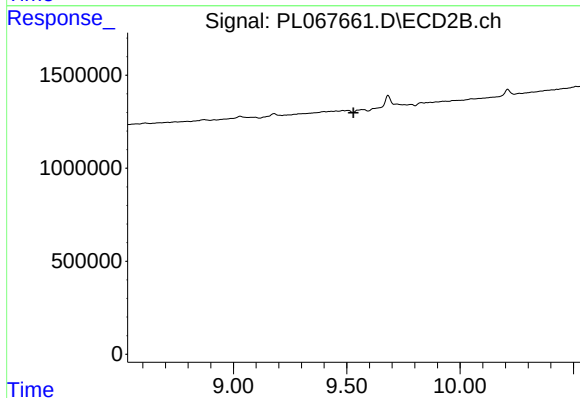


#19 Endosulfan Sulfate

R.T.: 0.000 min

Exp R.T. : 9.530 min

Response: 0

Conc: N.D.

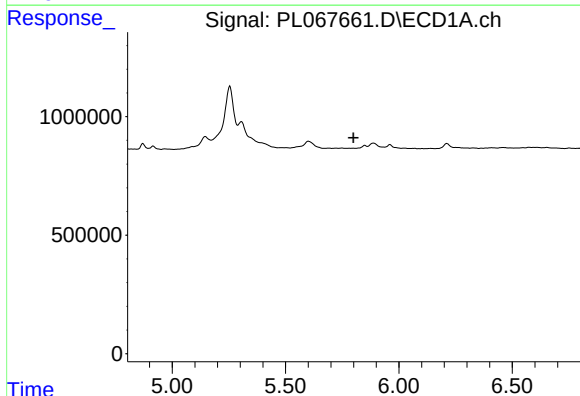


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T. : 5.800 min

Response: 0

Conc: N.D.

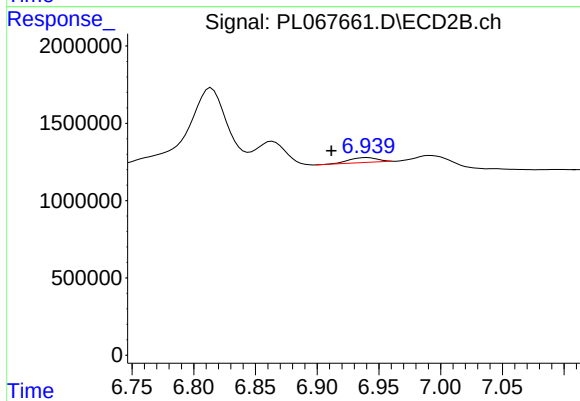


#23 Chlordane-1

R.T.: 6.941 min

Delta R.T.: 0.029 min

Response: 391498


Conc: 13.86 ng/ml

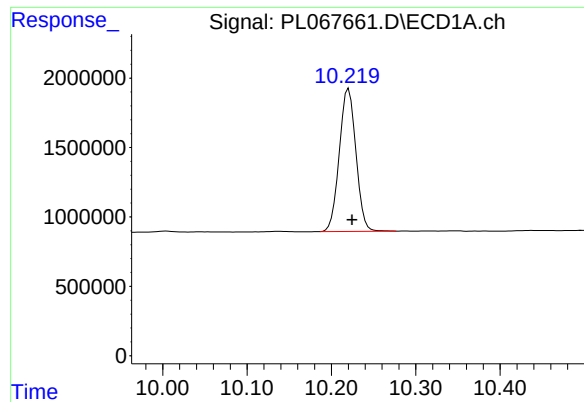

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 14088698
Conc: 19.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137223TB

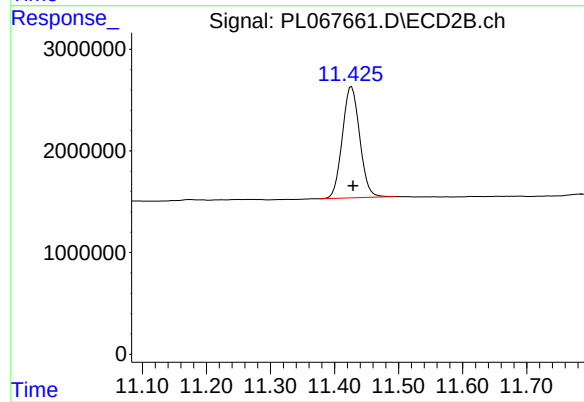

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 20623524
Conc: 20.71 ng/ml