

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 17:39
 Operator : AR\AJ
 Sample : PB137245BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB137245BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 04:21:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	8937147	16766343	16.256	17.785
28)	SA Decachlor...	10.221	11.429	12095591	18037840	17.068	18.109
Target Compounds							
3)	MA gamma-BHC...	5.609	0.000	387742	0	0.517	N.D. #
6)	B beta-BHC	5.961f	0.000	156654	0	0.438	N.D. #
7)	B delta-BHC	0.000	7.004f	0	419156	N.D.	0.357 #
23)	Chlordane-1	0.000	6.941f	0	272774	N.D.	9.660 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 17:39
Operator : AR\AJ
Sample : PB137245BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB137245BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 04:21:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

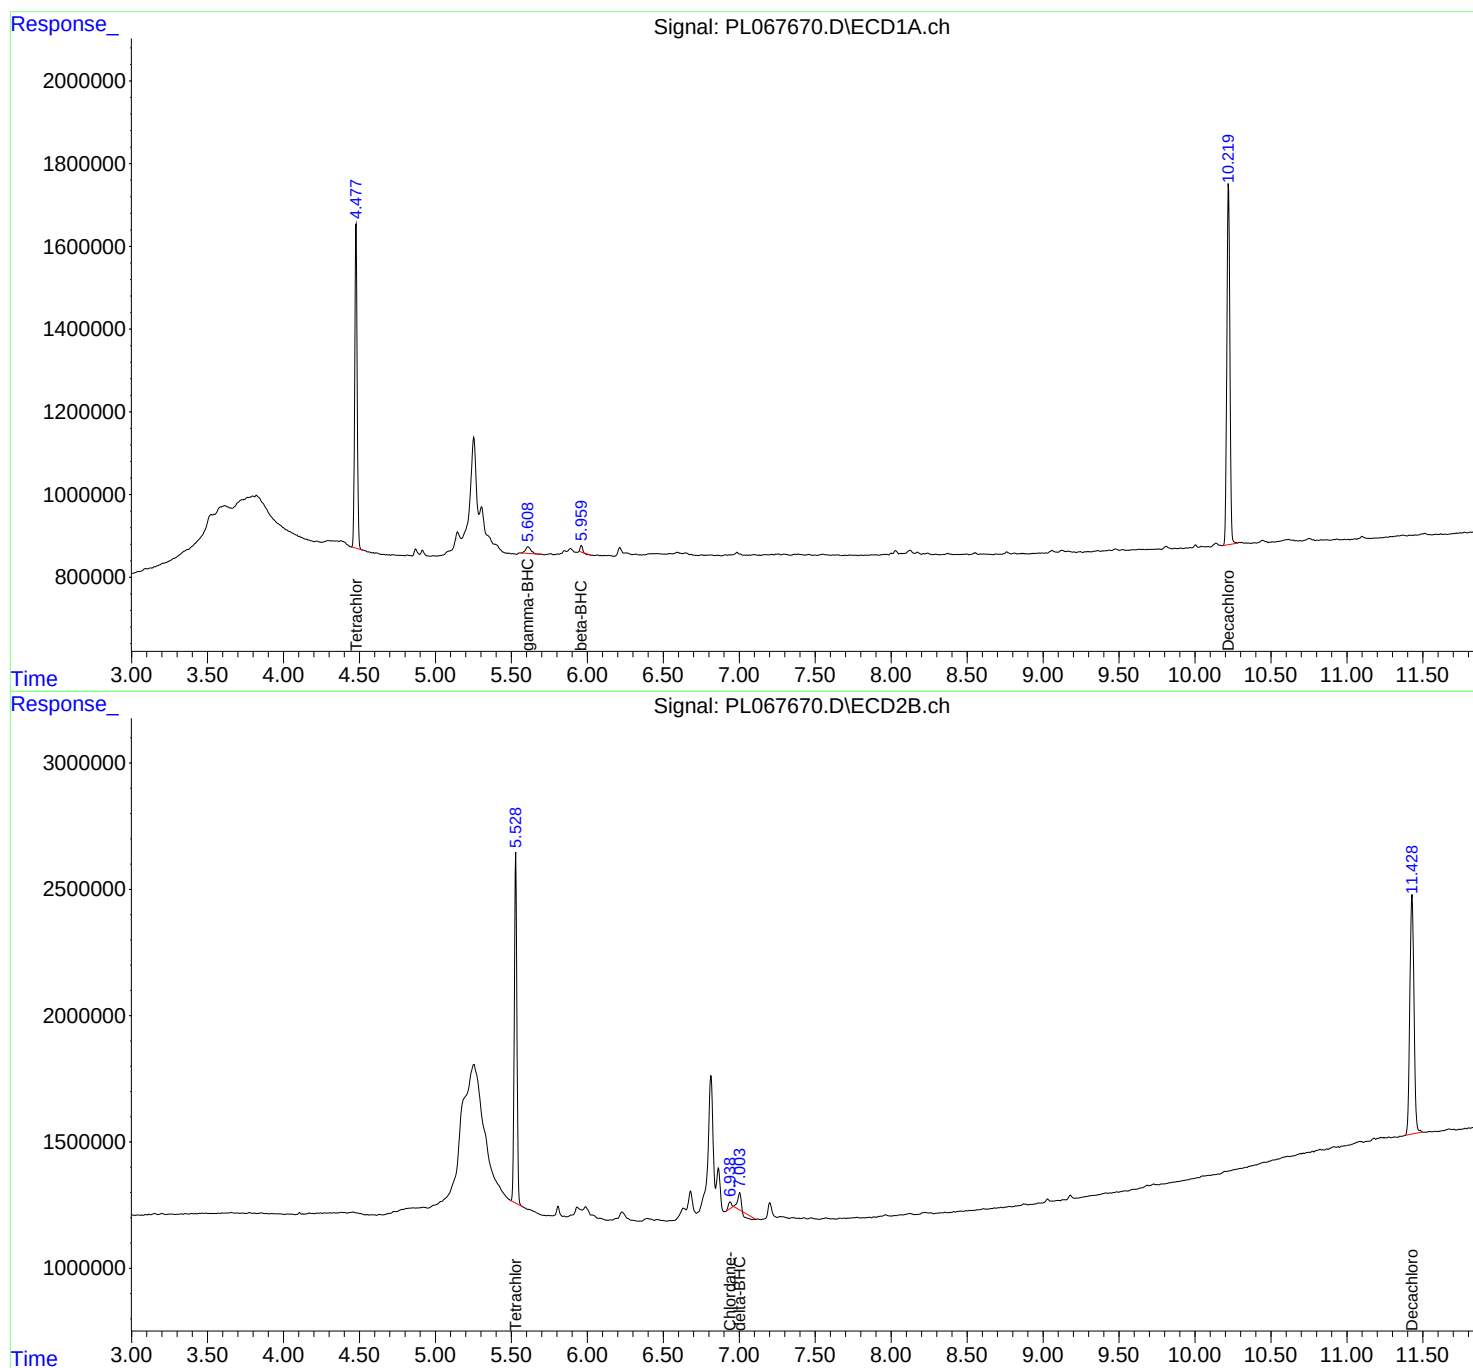


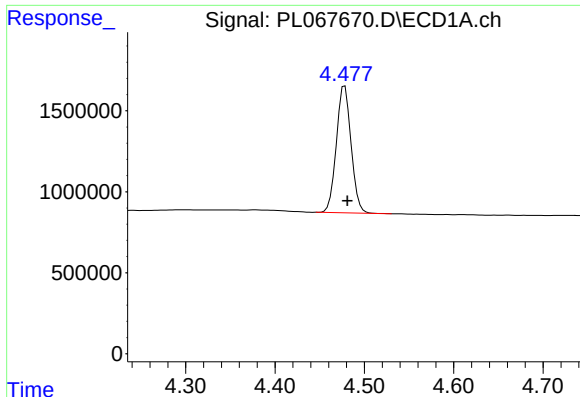

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 8937147
Conc: 16.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137245BL

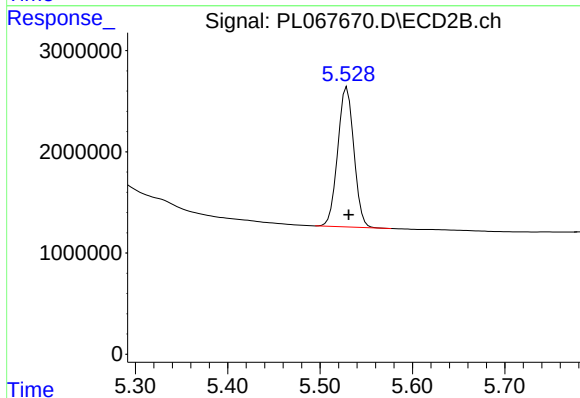


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 16766343
Conc: 17.78 ng/ml

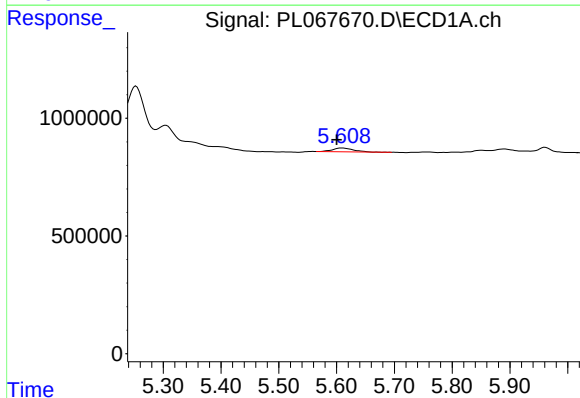


#3 gamma-BHC (Lindane)

R.T.: 5.609 min
Delta R.T.: 0.009 min
Response: 387742
Conc: 0.52 ng/ml

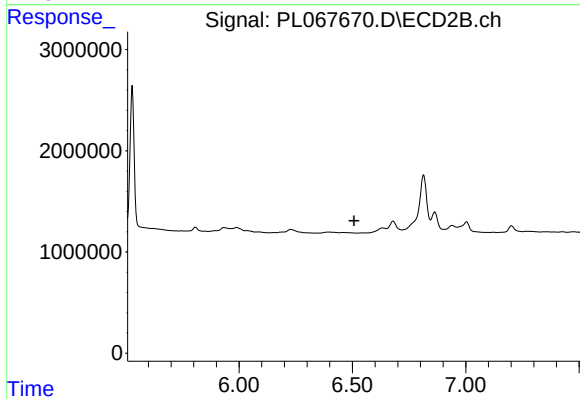

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

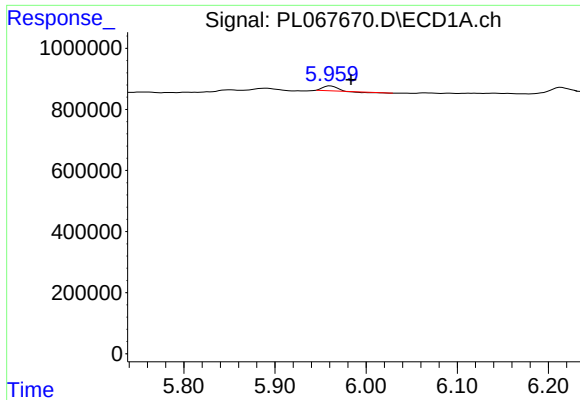

#6 beta-BHC


R.T.: 5.961 min
Delta R.T.: -0.023 min
Response: 156654
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137245BL

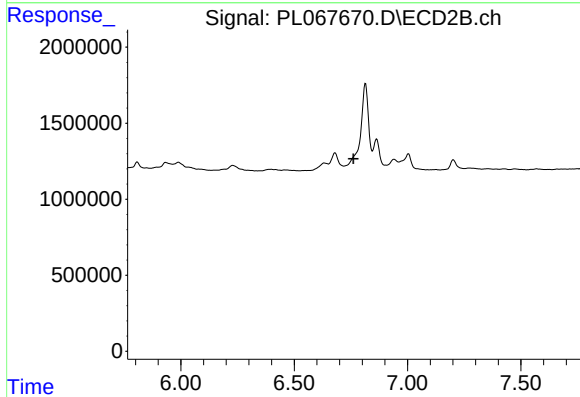


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

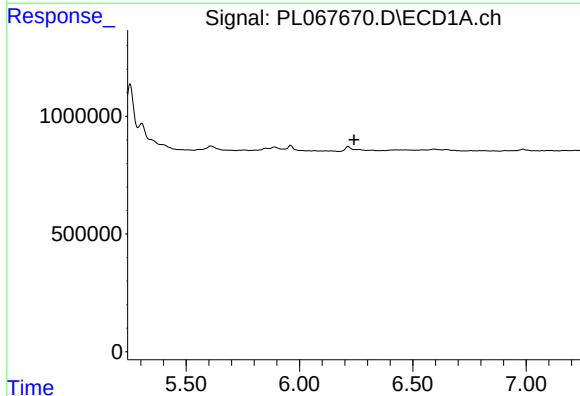


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

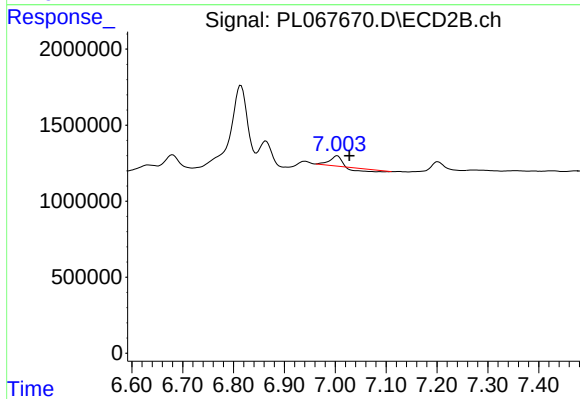

#7 delta-BHC


R.T.: 7.004 min
Delta R.T.: -0.024 min
Response: 419156
Conc: 0.36 ng/ml

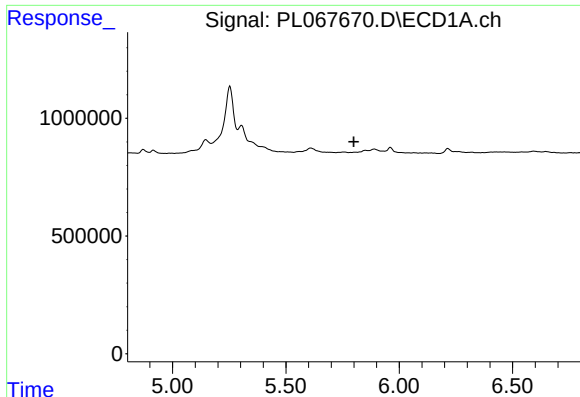

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137245BL

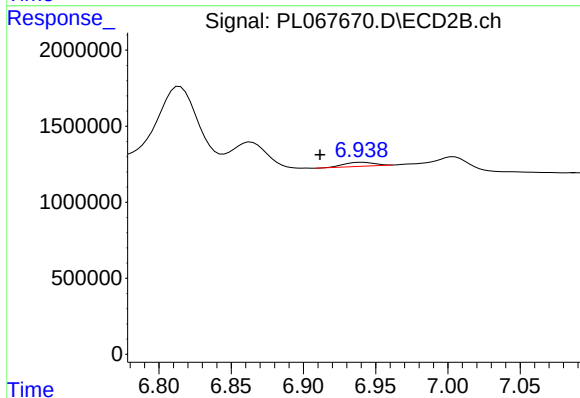


#23 Chlordane-1

R.T.: 6.941 min
Delta R.T.: 0.029 min
Response: 272774
Conc: 9.66 ng/ml

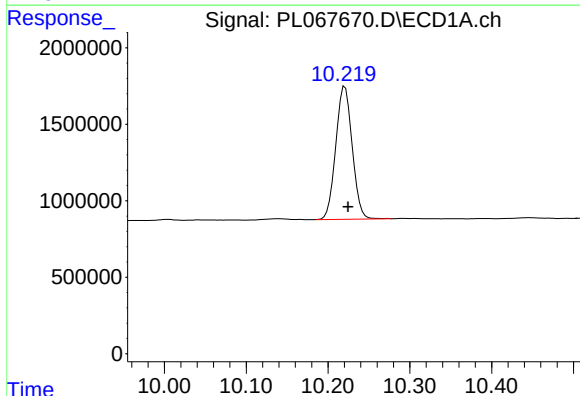

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 12095591
Conc: 17.07 ng/ml

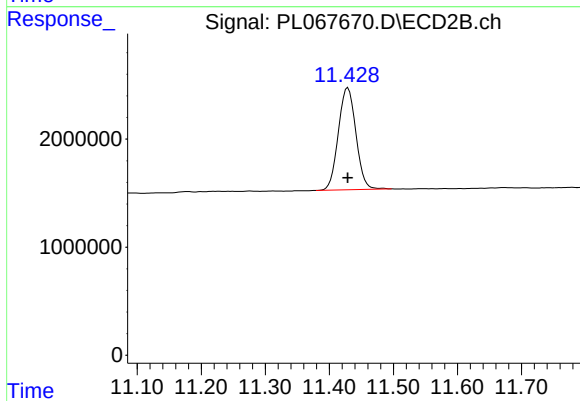

#28 Decachlorobiphenyl

R.T.: 11.429 min
Delta R.T.: 0.000 min
Response: 18037840
Conc: 18.11 ng/ml