

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 19:35
 Operator : AR\AJ
 Sample : M2746-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NEW-DORP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 04:22:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	11506602	21558194	20.929	22.868
28)	SA Decachlor...	10.221	11.428	15096493	22775388	21.302	22.866
Target Compounds							
2)	A alpha-BHC	0.000	6.088f	0	508172	N.D.	0.411 #
3)	MA gamma-BHC...	5.619f	0.000	359153	0	0.479	N.D. #
5)	MB Aldrin	6.337	0.000	659546	0	0.896	N.D. #
6)	B beta-BHC	5.962f	0.000	718140	0	2.007	N.D. #
7)	B delta-BHC	0.000	7.006f	0	2937823	N.D.	2.499 #
15)	B Endosulfa...	0.000	9.178f	0	595676	N.D.	0.747 #
19)	B Endosulfa...	8.590f	0.000	342265	0	0.539	N.D. #
21)	B Endrin ke...	0.000	10.004f	0	413974	N.D.	0.457 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 19:35
Operator : AR\AJ
Sample : M2746-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NEW-DORP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 04:22:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

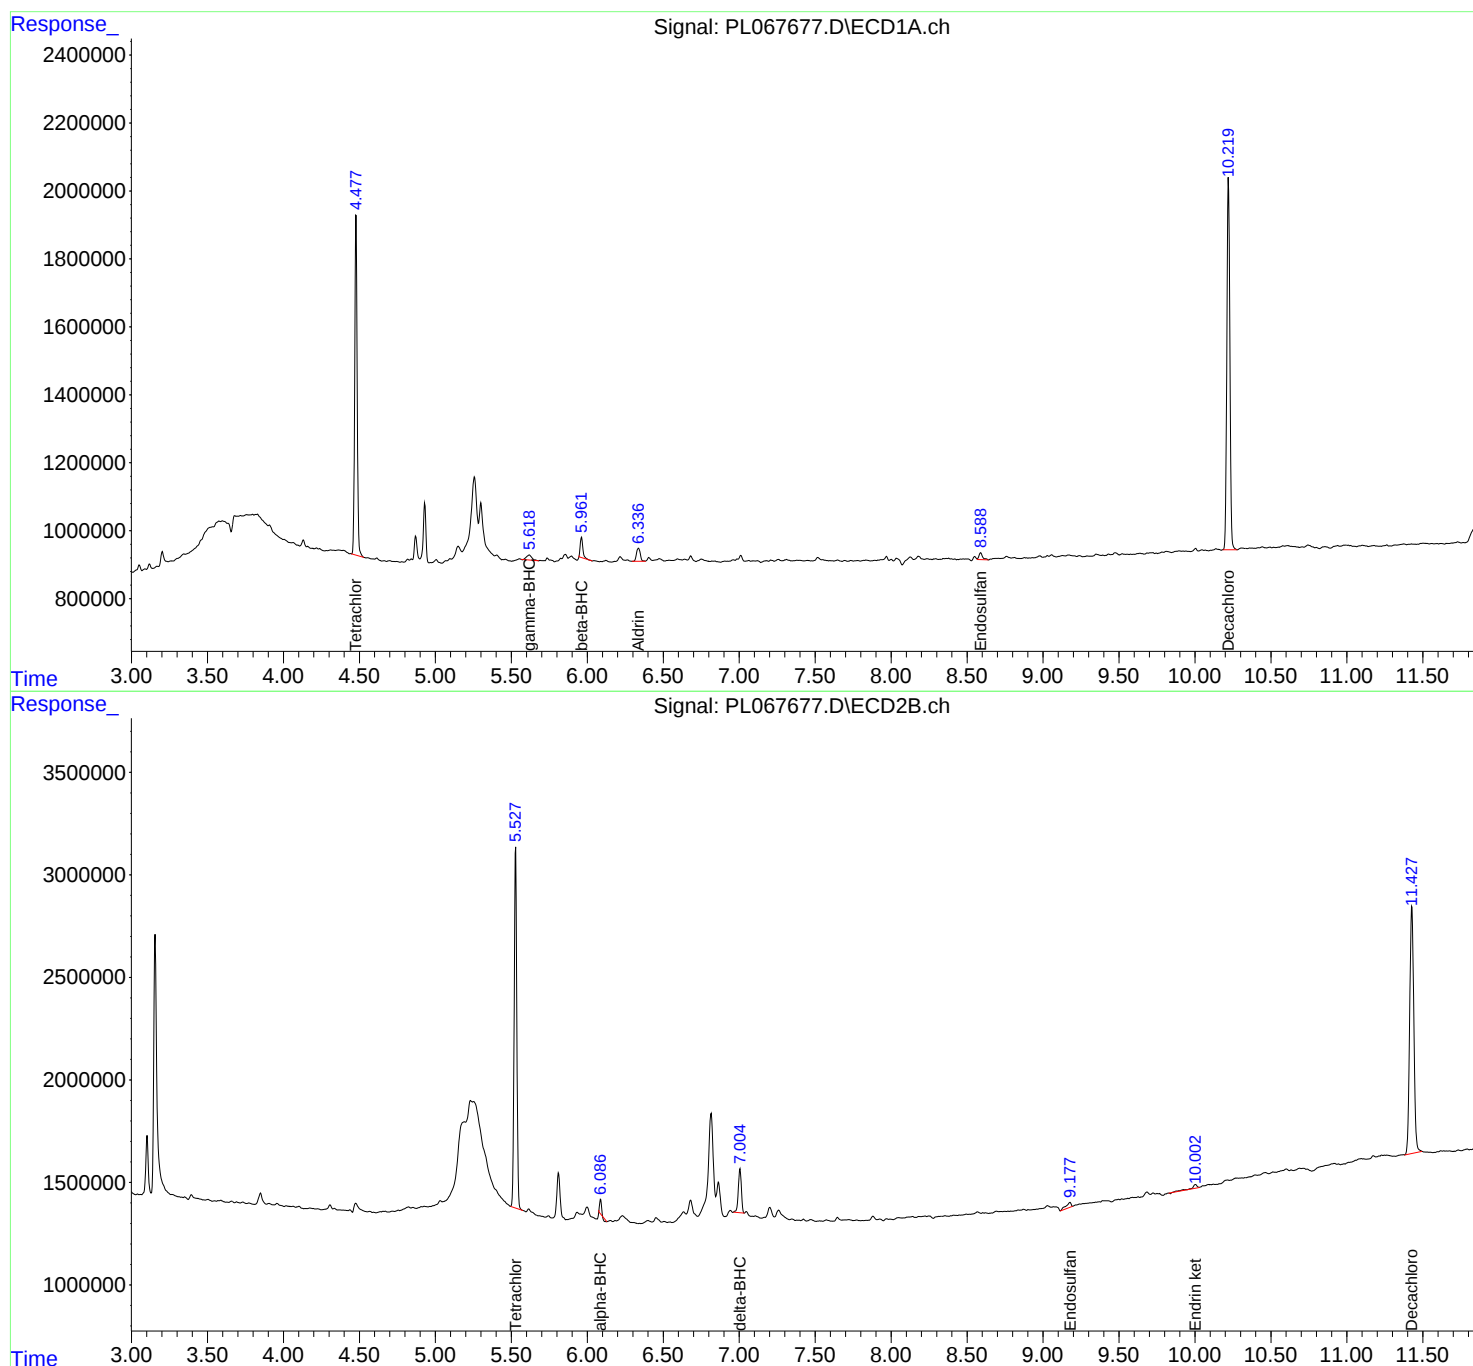


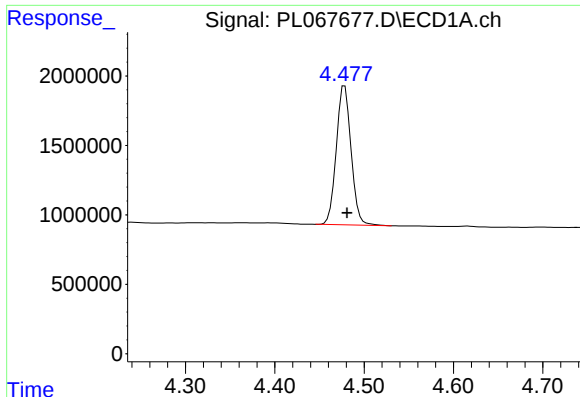

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11506602
Conc: 20.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
NEW-DORP-2

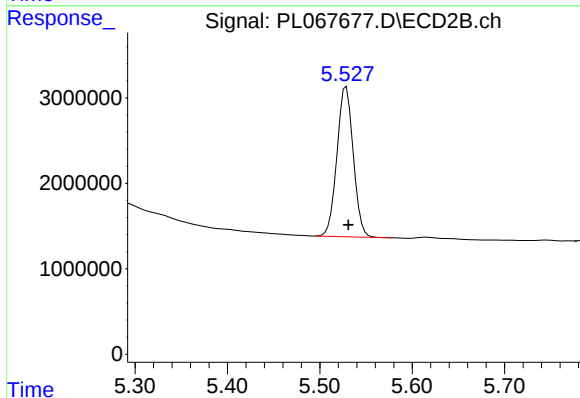


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 21558194
Conc: 22.87 ng/ml

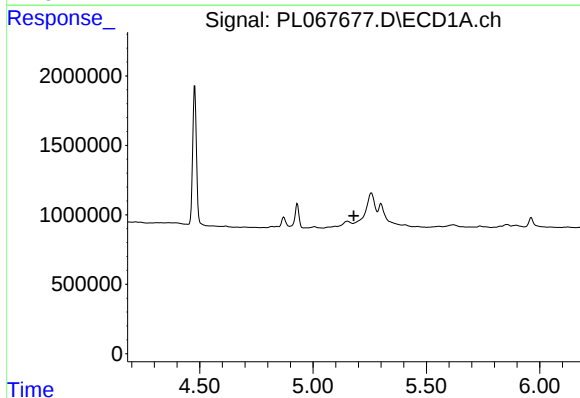


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.181 min
Response: 0
Conc: N.D.

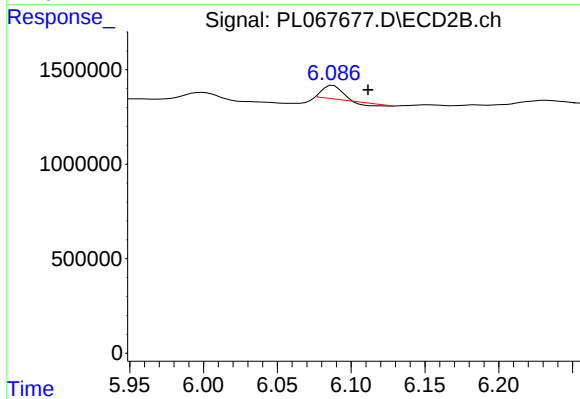

#2 alpha-BHC


R.T.: 6.088 min
Delta R.T.: -0.024 min
Response: 508172
Conc: 0.41 ng/ml

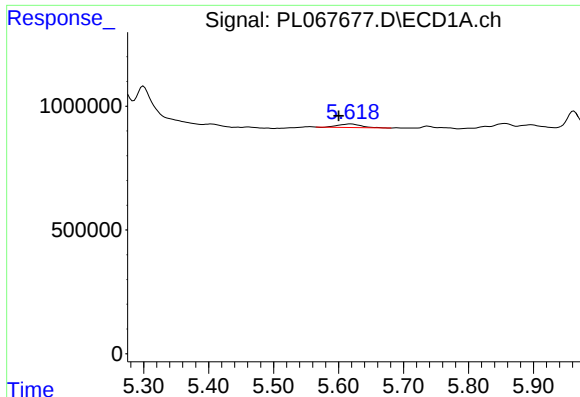

#3 gamma-BHC (Lindane)


R.T.: 5.619 min
Delta R.T.: 0.019 min
Response: 359153
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
NEW-DORP-2

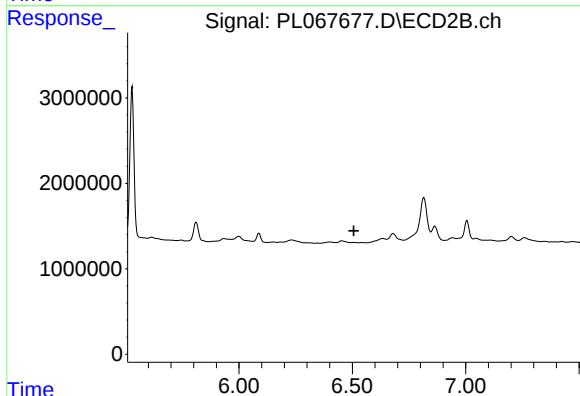


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

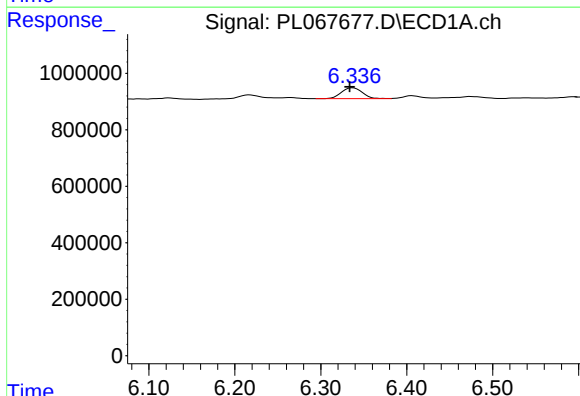


#5 Aldrin

R.T.: 6.337 min
Delta R.T.: 0.004 min
Response: 659546
Conc: 0.90 ng/ml

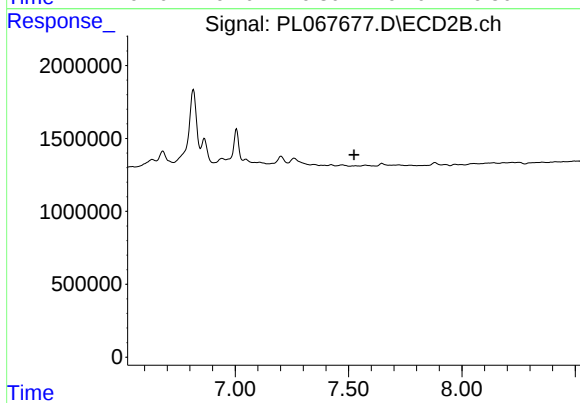

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

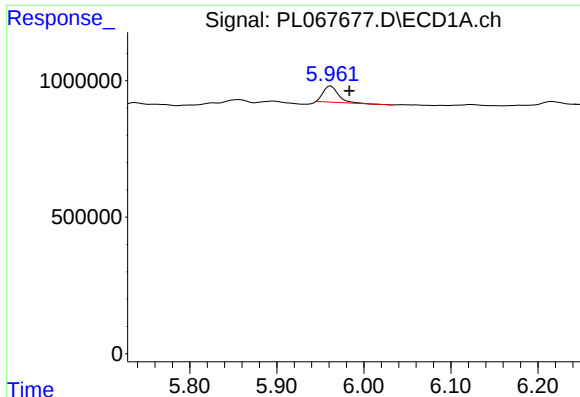

#6 beta-BHC


R.T.: 5.962 min
Delta R.T.: -0.021 min
Response: 718140
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
NEW-DORP-2

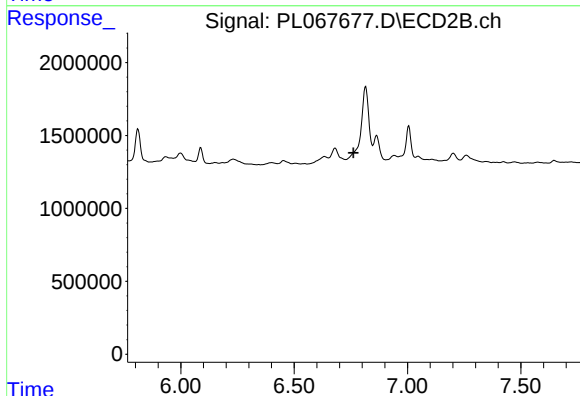


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

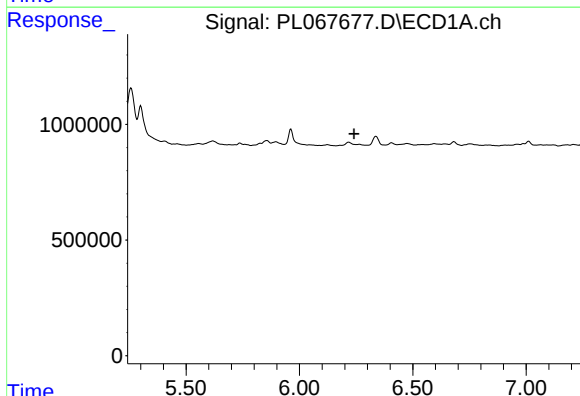


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

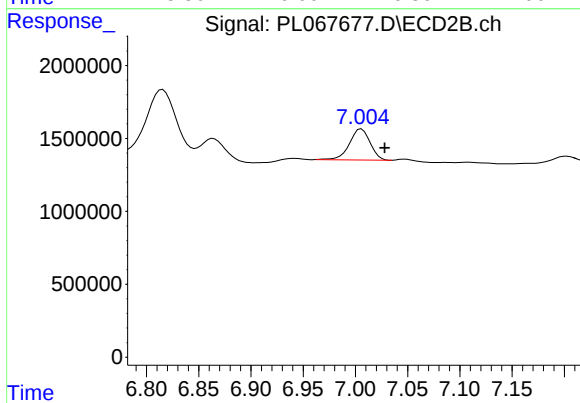

#7 delta-BHC


R.T.: 7.006 min
Delta R.T.: -0.022 min
Response: 2937823
Conc: 2.50 ng/ml

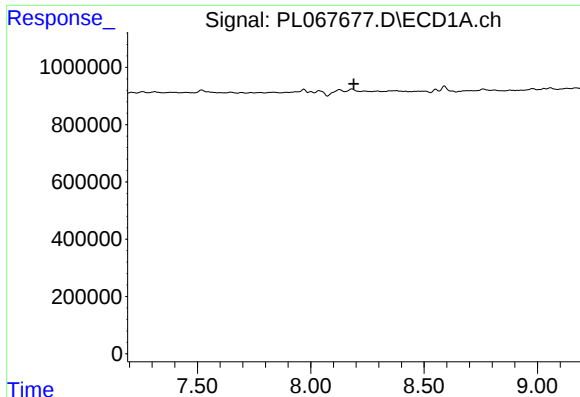

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NEW-DORP-2

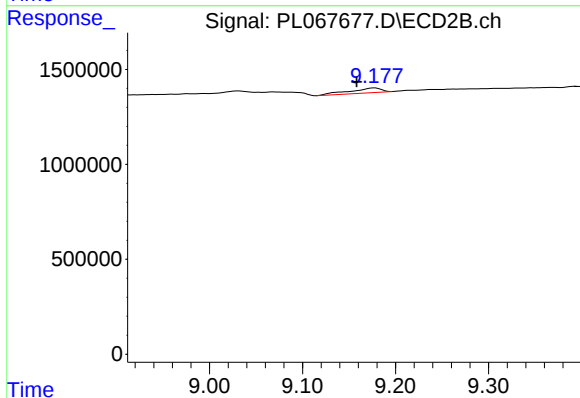


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 595676
Conc: 0.75 ng/ml

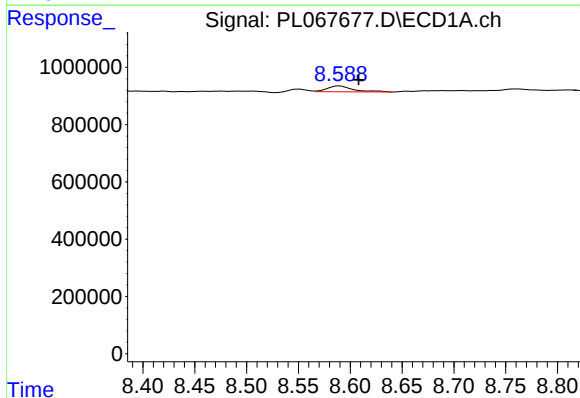


#19 Endosulfan Sulfate

R.T.: 8.590 min
Delta R.T.: -0.019 min
Response: 342265
Conc: 0.54 ng/ml

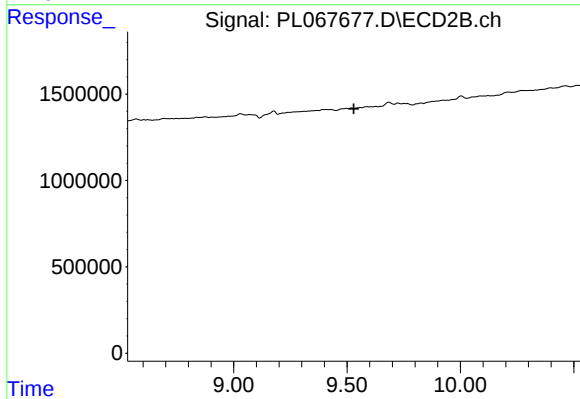

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.530 min
Response: 0
Conc: N.D.

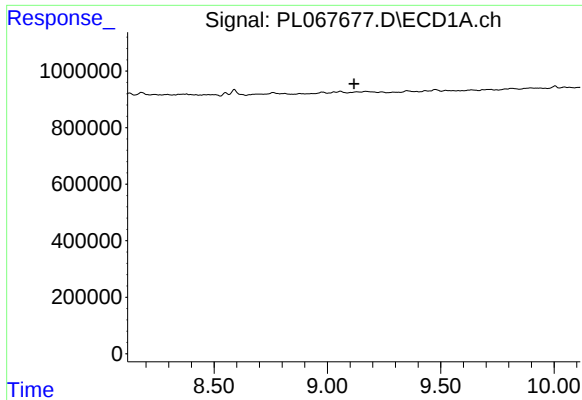

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NEW-DORP-2

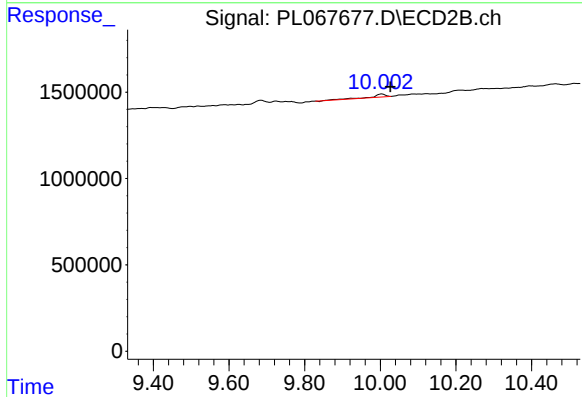


#21 Endrin ketone

R.T.: 10.004 min
Delta R.T.: -0.023 min
Response: 413974
Conc: 0.46 ng/ml

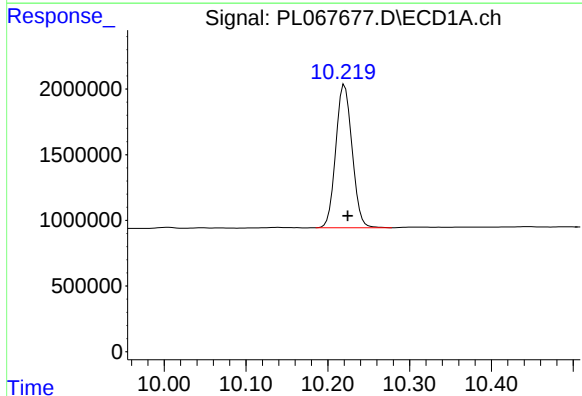

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 15096493
Conc: 21.30 ng/ml

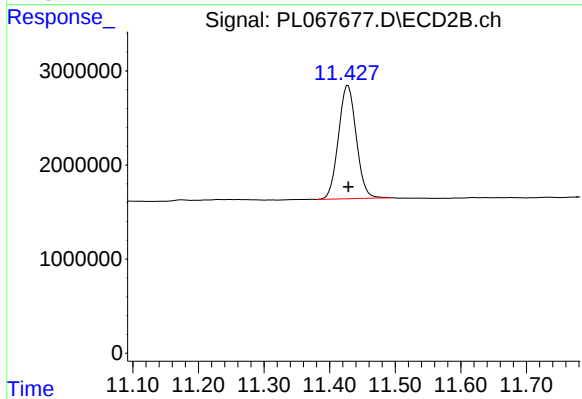

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 22775388
Conc: 22.87 ng/ml