

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 23:28
 Operator : AR\AJ
 Sample : M2771-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0338-COMPOSITE-DC-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 04:25:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	9543201	17096075	17.358	18.135
28)	SA Decachlor...	10.220	11.427	8592700	12869889	12.125	12.921
Target Compounds							
6)	B beta-BHC	5.960f	0.000	123762	0	0.346	N.D. #
7)	B delta-BHC	0.000	7.001f	0	1368778	N.D.	1.164 #
8)	B Heptachlo...	0.000	7.989	0	205169	N.D.	0.205 #
11)	B alpha-Chl...	7.254	0.000	268947	0	0.367	N.D. #
15)	B Endosulfa...	8.175f	9.179f	448020	326282	0.727	0.409 #
20)	A Methoxychlor	8.879f	0.000	283637	0	0.798	N.D. #
21)	B Endrin ke...	0.000	10.047f	0	192711	N.D.	0.213 #
24)	Chlordane-2	6.468f	0.000	840616	0	31.392	N.D. #
26)	Chlordane-4	7.254	0.000	268947	0	3.680	N.D. #
27)	Chlordane-5	8.175f	0.000	448020	0	20.477	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 23:28
Operator : AR\AJ
Sample : M2771-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 04:25:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

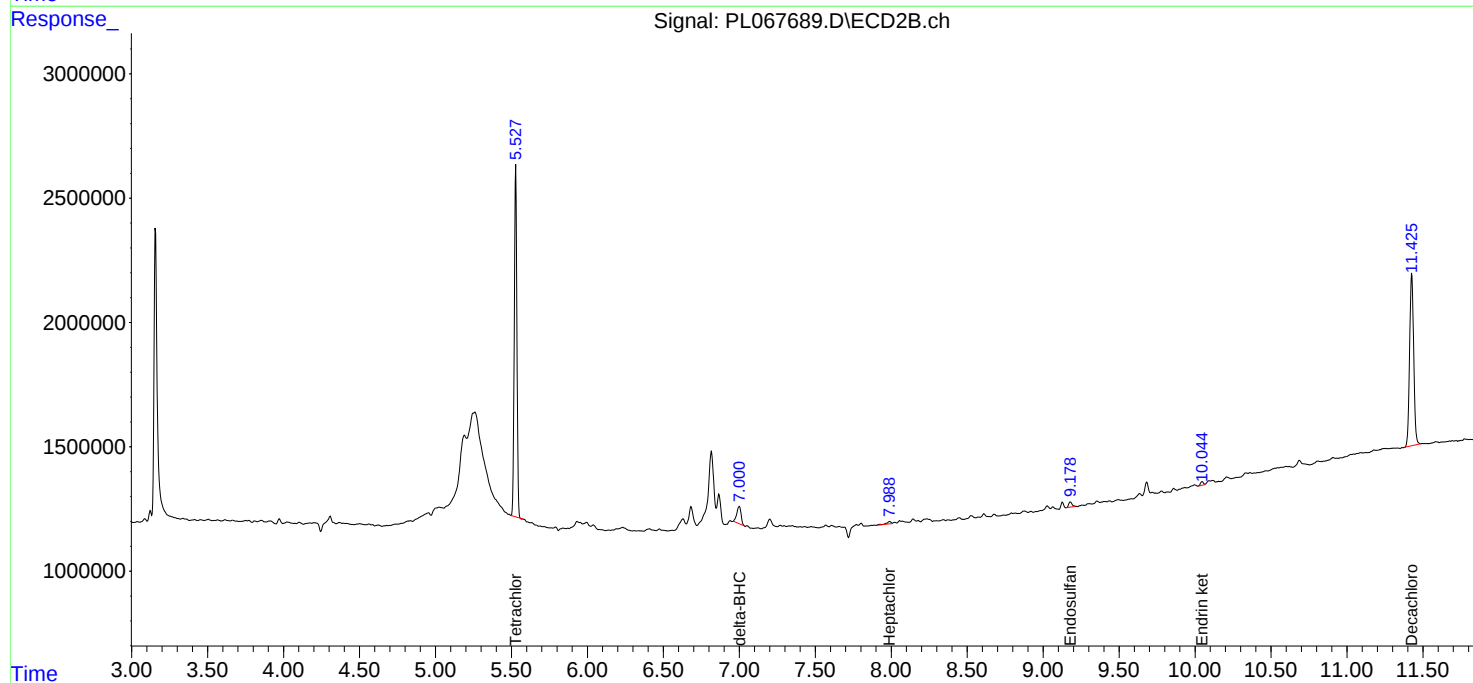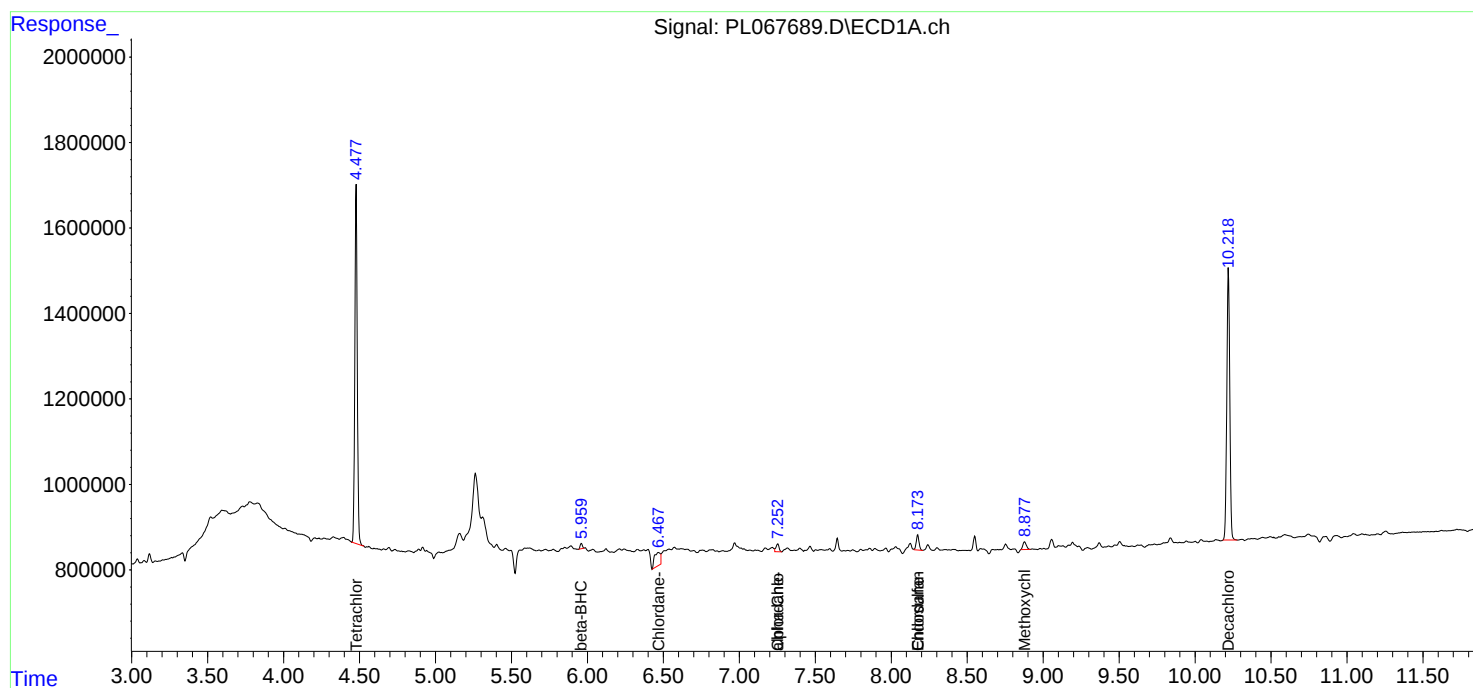


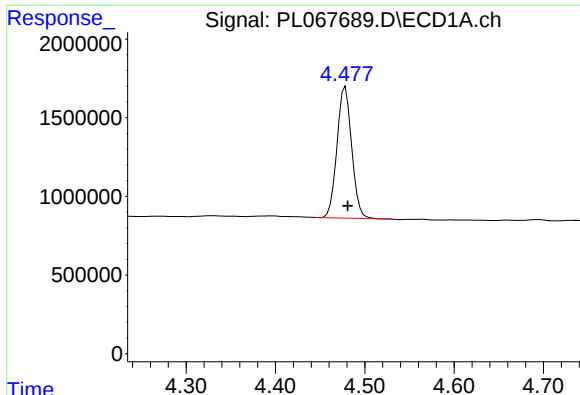

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 9543201
Conc: 17.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

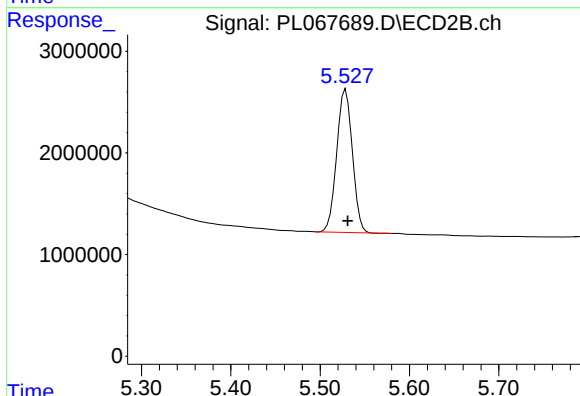


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 17096075
Conc: 18.13 ng/ml

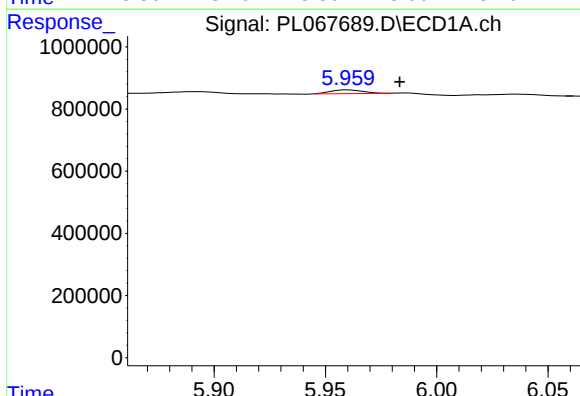


#6 beta-BHC

R.T.: 5.960 min
Delta R.T.: -0.023 min
Response: 123762
Conc: 0.35 ng/ml

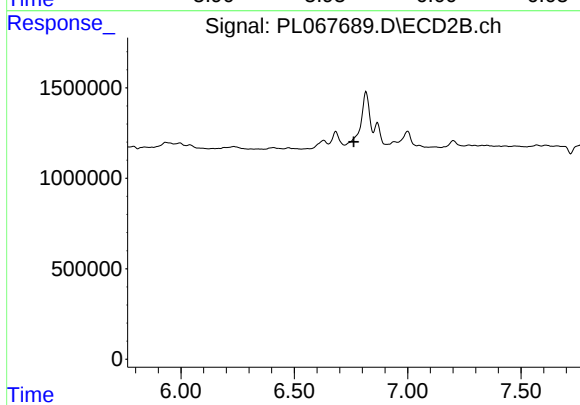

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

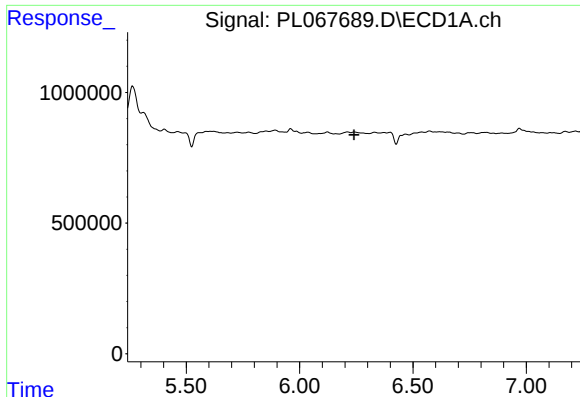

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

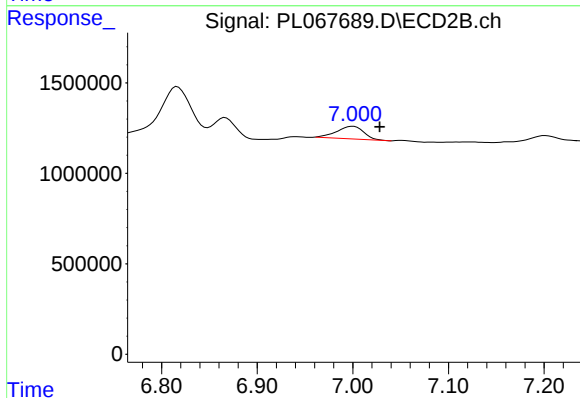


#7 delta-BHC

R.T.: 7.001 min
Delta R.T.: -0.028 min
Response: 1368778
Conc: 1.16 ng/ml

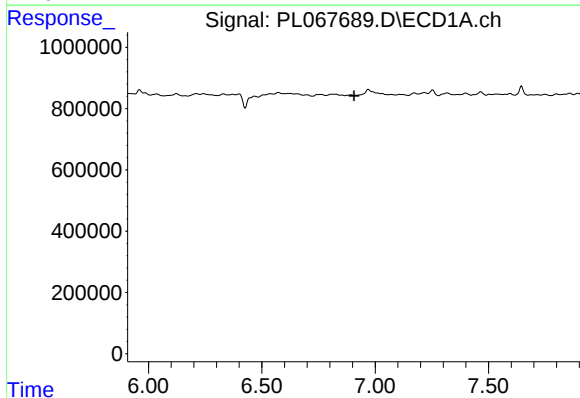


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

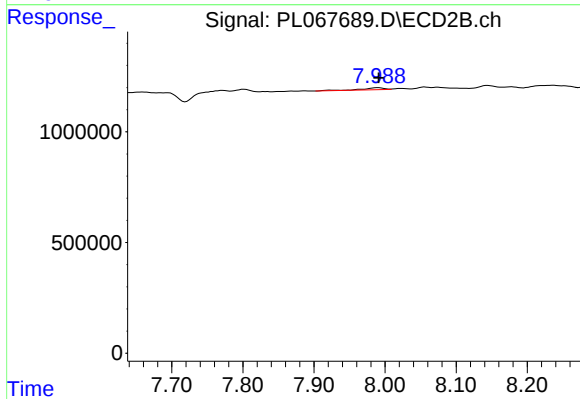

#8 Heptachlor epoxide


R.T.: 7.989 min
Delta R.T.: -0.002 min
Response: 205169
Conc: 0.20 ng/ml

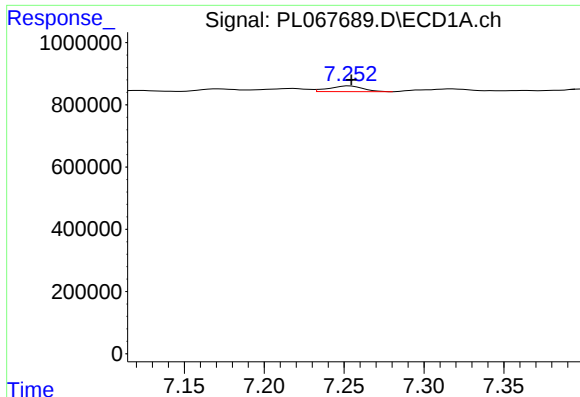

#11 alpha-Chlordane


R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 268947
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

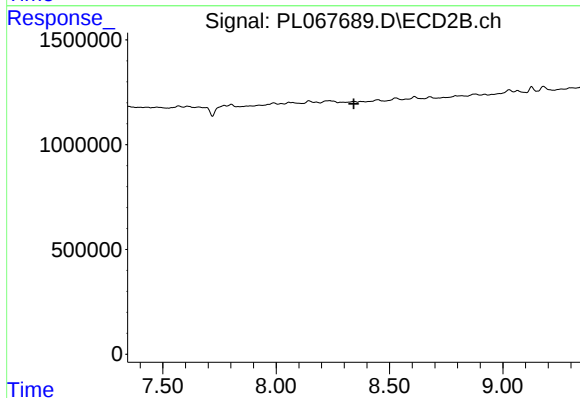


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

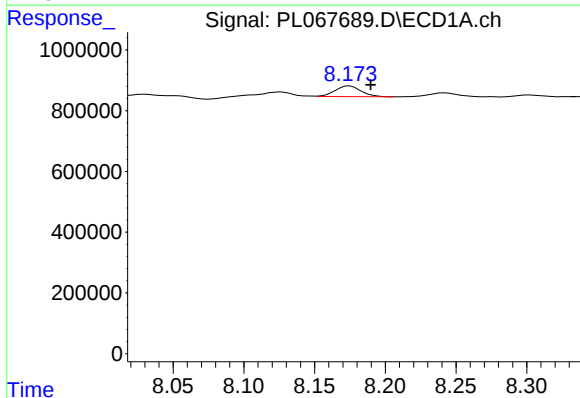


#15 Endosulfan II

R.T.: 8.175 min
Delta R.T.: -0.015 min
Response: 448020
Conc: 0.73 ng/ml

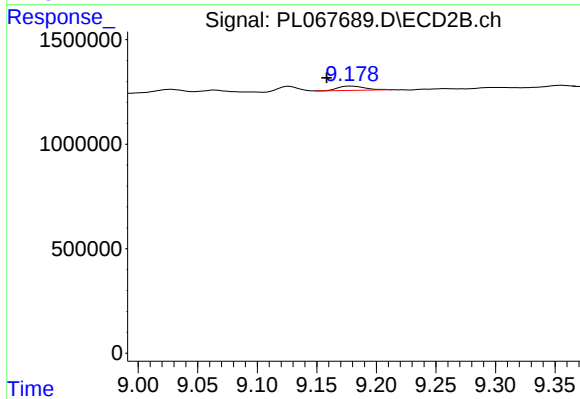

#15 Endosulfan II


R.T.: 9.179 min
Delta R.T.: 0.021 min
Response: 326282
Conc: 0.41 ng/ml

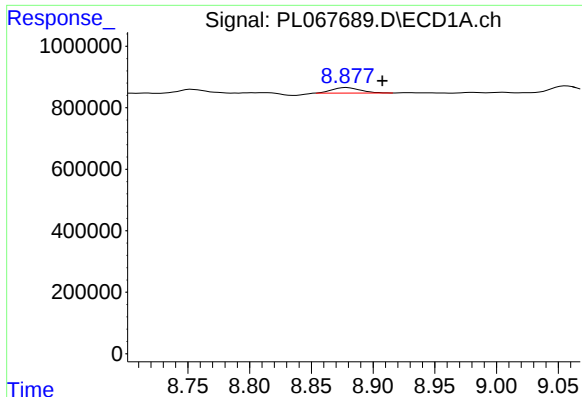

#20 Methoxychlor


R.T.: 8.879 min
Delta R.T.: -0.029 min
Response: 283637
Conc: 0.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

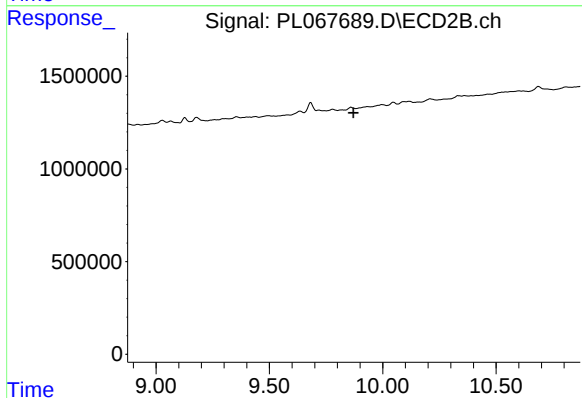


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.872 min
Response: 0
Conc: N.D.

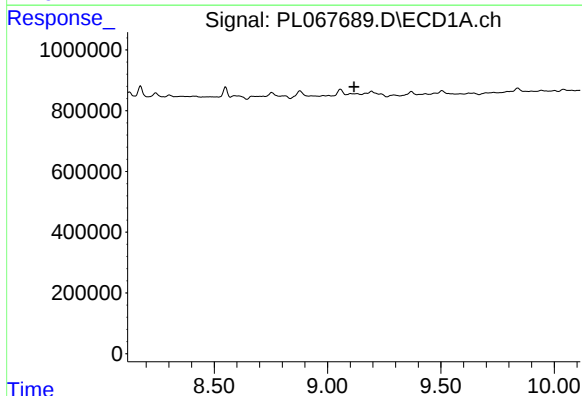


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

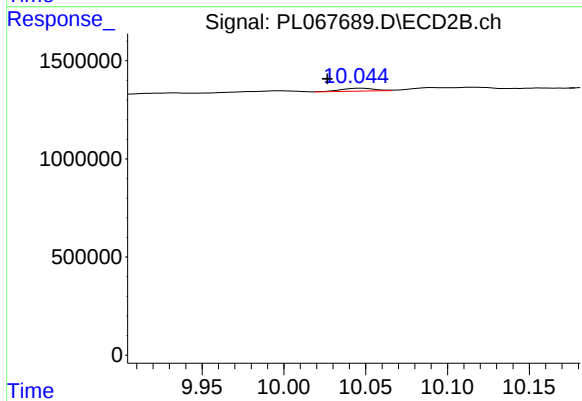

#21 Endrin ketone


R.T.: 10.047 min
Delta R.T.: 0.021 min
Response: 192711
Conc: 0.21 ng/ml

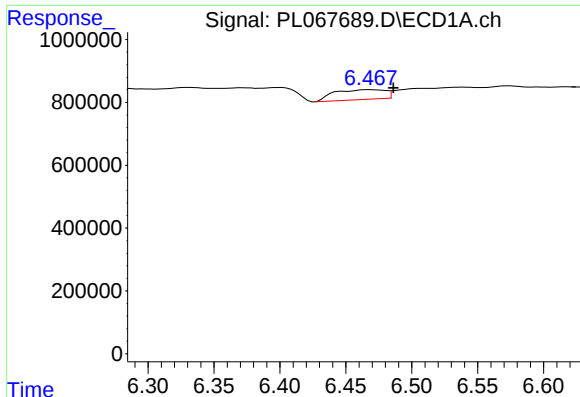

#24 Chlordane-2


R.T.: 6.468 min
Delta R.T.: -0.018 min
Response: 840616
Conc: 31.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

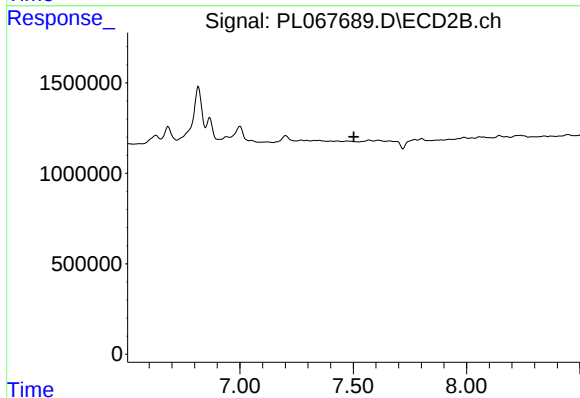


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

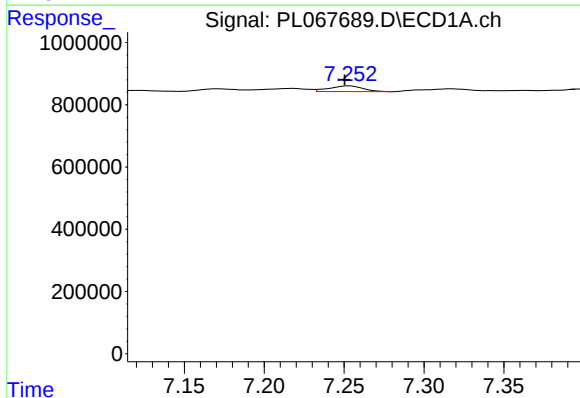


#26 Chlordane-4

R.T.: 7.254 min
Delta R.T.: 0.003 min
Response: 268947
Conc: 3.68 ng/ml

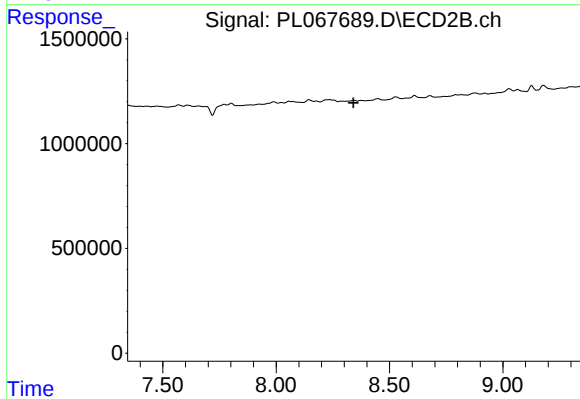

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

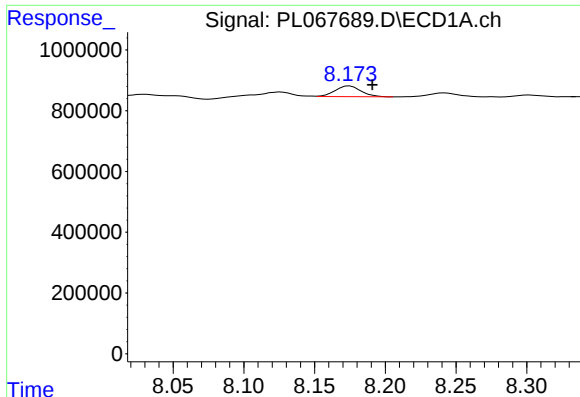

#27 Chlordane-5


R.T.: 8.175 min
Delta R.T.: -0.016 min
Response: 448020
Conc: 20.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
0338-COMPOSITE-DC-21

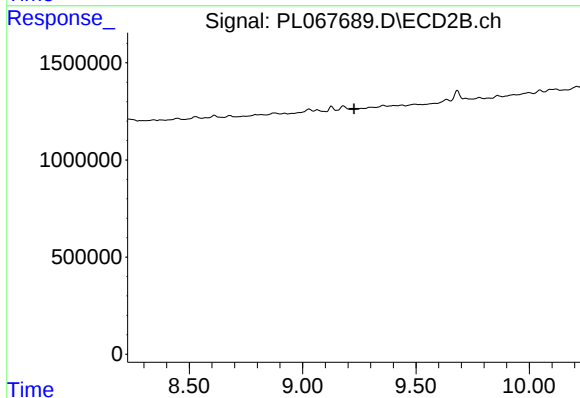


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

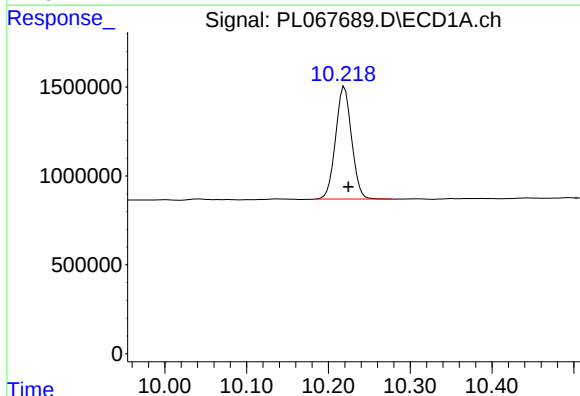

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 8592700
Conc: 12.12 ng/ml

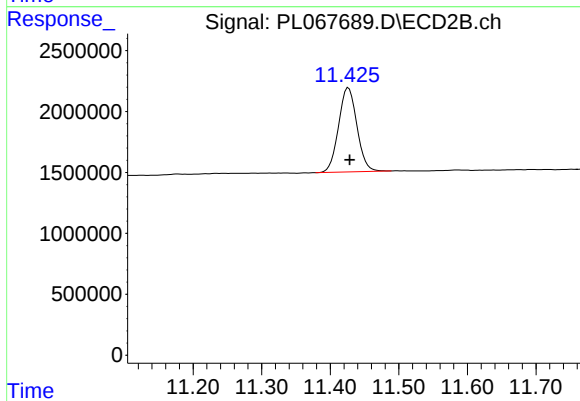

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 12869889
Conc: 12.92 ng/ml