

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062122\
 Data File : PL075890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2022 17:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:25:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.635	15198711	37101564	22.520	22.108
28)	SA Decachlor...	11.634	10.376	12344999	23513072	20.164	16.688
Target Compounds							
7)	B delta-BHC	0.000	6.400	0	403038	N.D.	0.188 #
9)	A Endosulfan I	8.533	0.000	93747	0	0.134	N.D. #
10)	B gamma-Chl...	8.382	0.000	1510963	0	1.946	N.D. #
11)	B alpha-Chl...	8.471	7.389f	113424	233907	0.149	0.128
15)	B Endosulfa...	9.303	0.000	200886	0	0.323	N.D. #
17)	MA 4,4'-DDT	0.000	8.460	0	92746	N.D.	0.066 #
19)	B Endosulfa...	0.000	8.760	0	438039	N.D.	0.298 #
20)	A Methoxychlor	0.000	9.032f	0	498202	N.D.	0.612 #
21)	B Endrin ke...	10.185f	0.000	756852	0	1.076	N.D. #
25)	Chlordane-3	8.382	0.000	1510963	0	14.634	N.D. #
26)	Chlordane-4	8.471	7.389f	113424	233907	0.896	1.271 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062122\
Data File : PL075890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2022 17:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:25:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

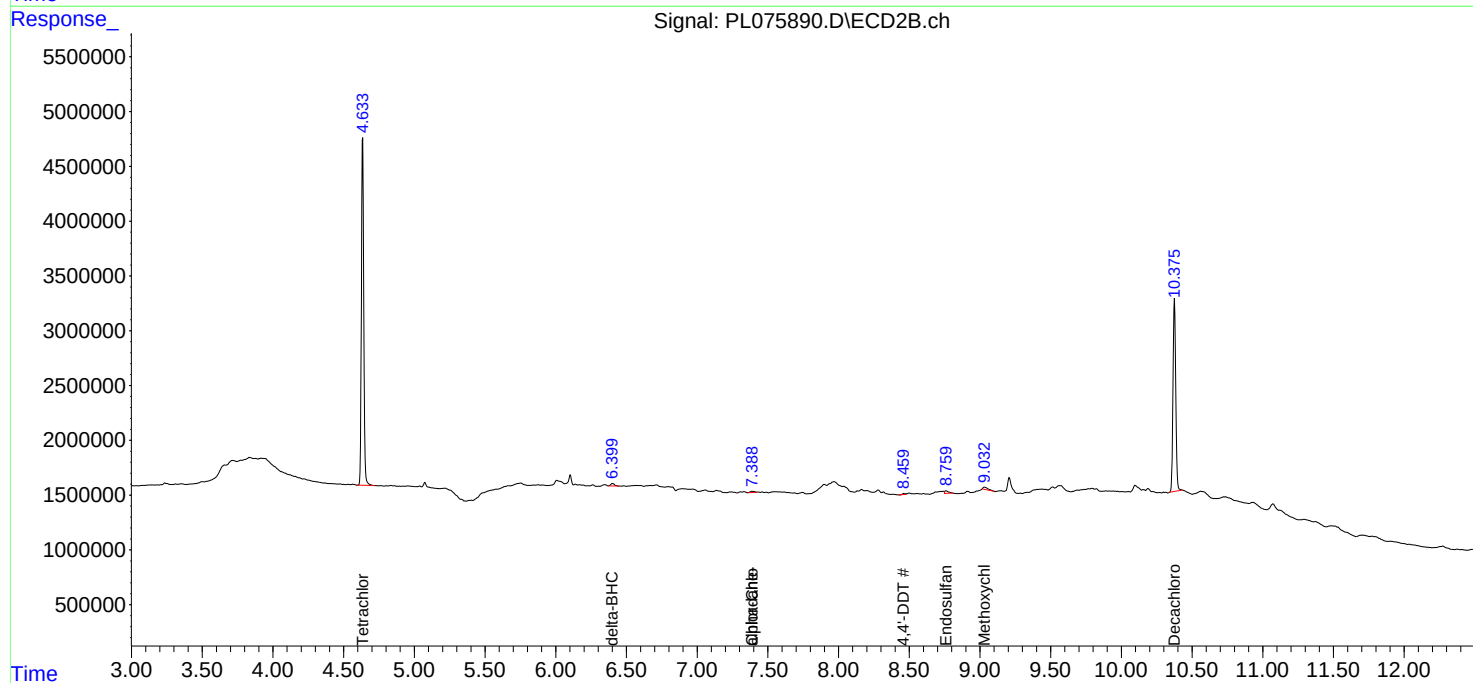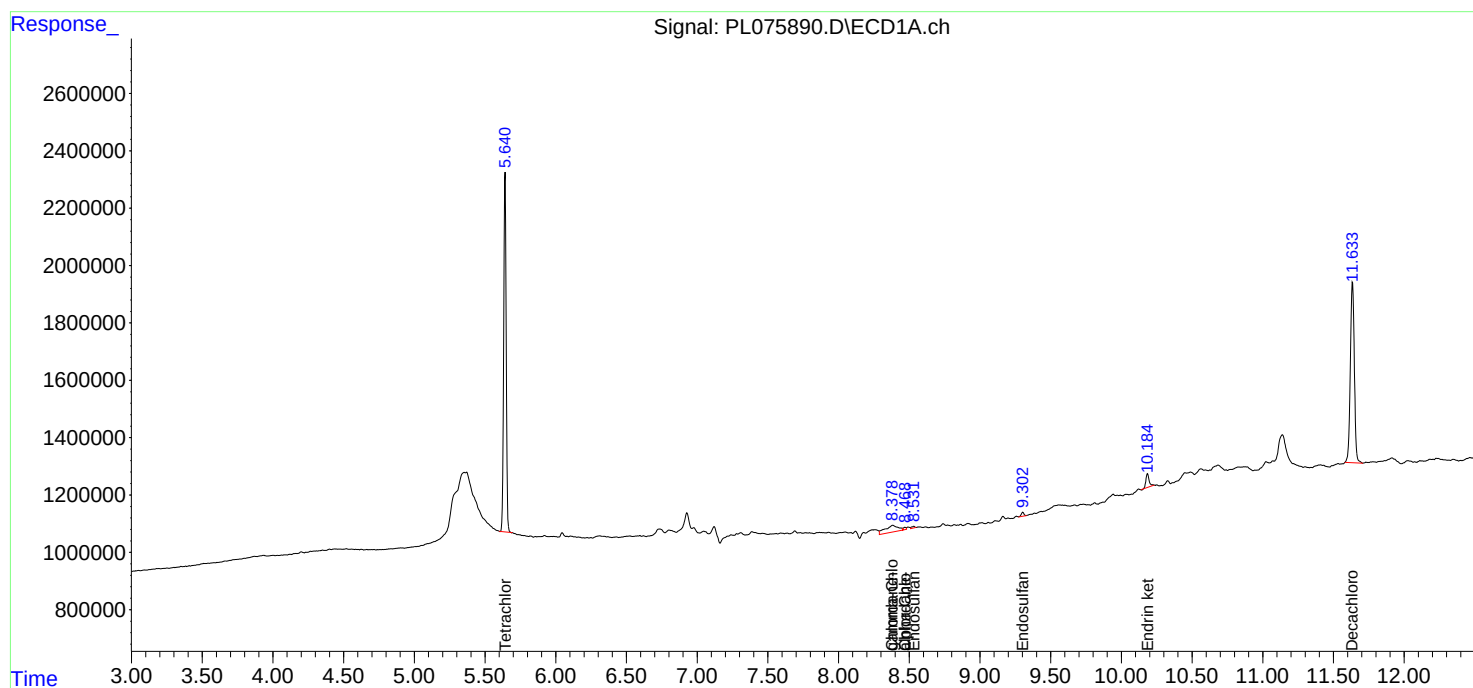


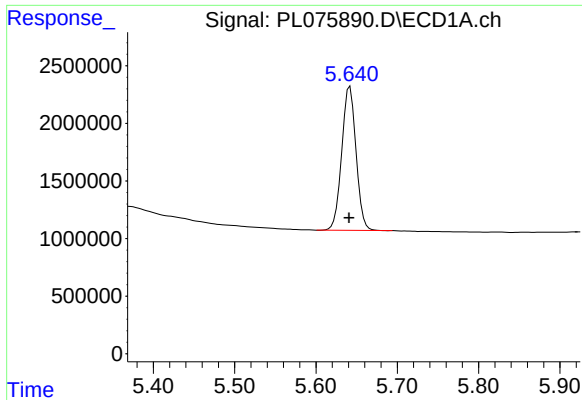

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 15198711
Conc: 22.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

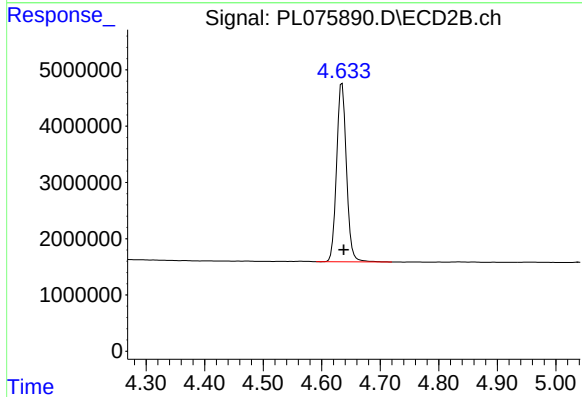


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 37101564
Conc: 22.11 ng/ml

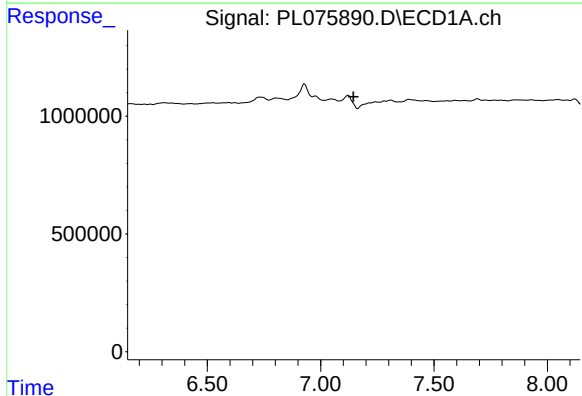


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

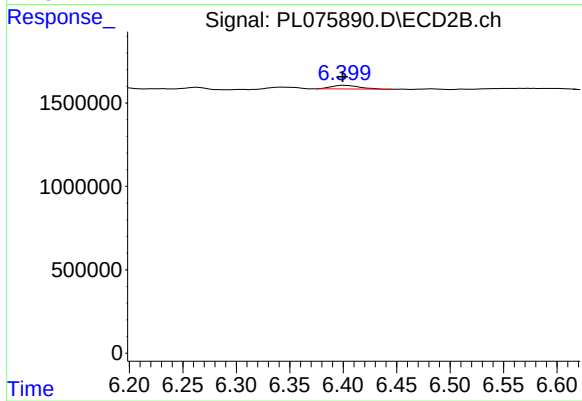

#7 delta-BHC


R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 403038
Conc: 0.19 ng/ml

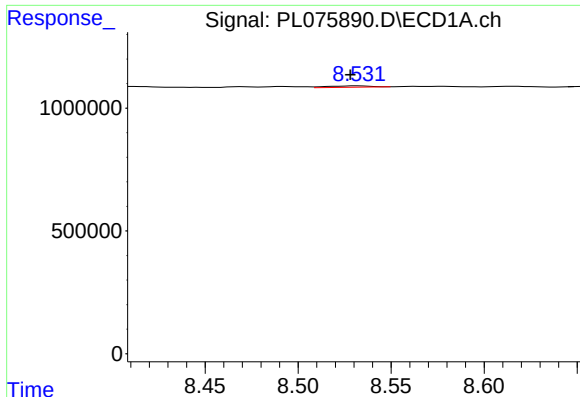

#9 Endosulfan I


R.T.: 8.533 min
Delta R.T.: 0.005 min
Response: 93747
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

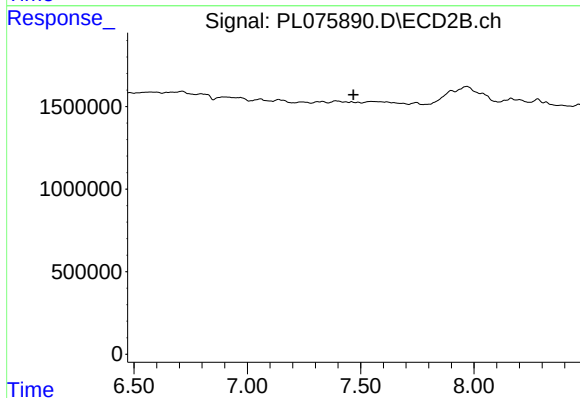


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

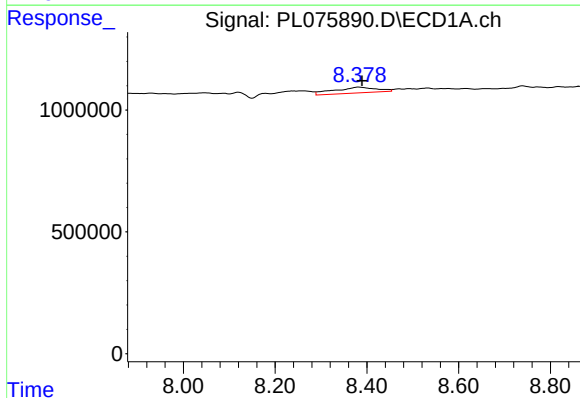


#10 gamma-Chlordane

R.T.: 8.382 min
Delta R.T.: -0.008 min
Response: 1510963
Conc: 1.95 ng/ml

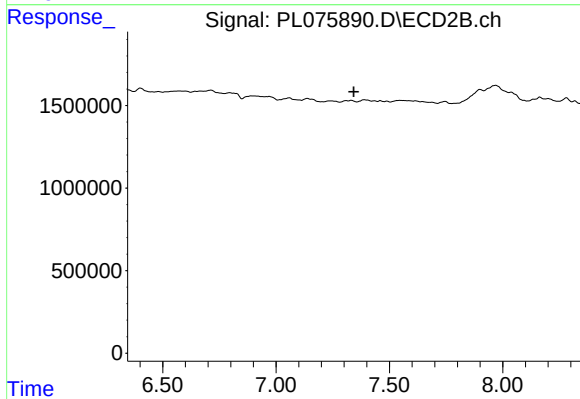

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

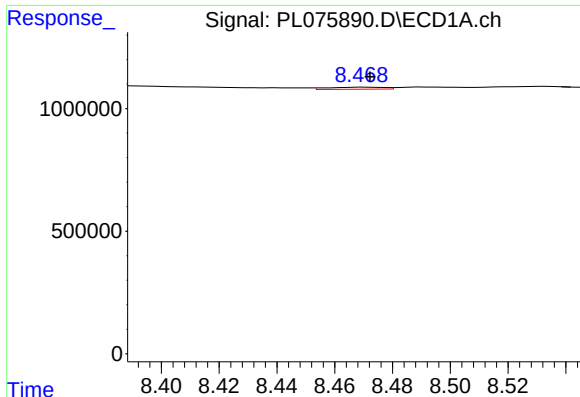

#11 alpha-Chlordane


R.T.: 8.471 min
Delta R.T.: -0.002 min
Response: 113424
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

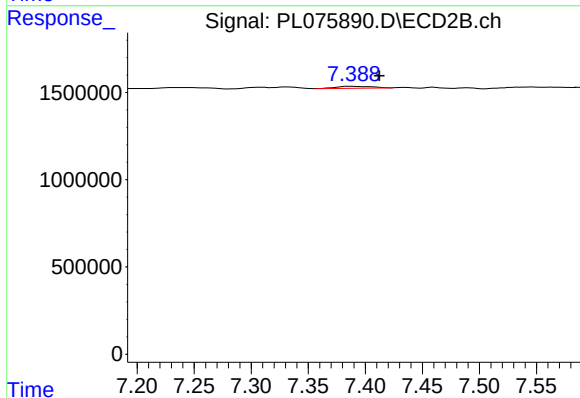


#11 alpha-Chlordane

R.T.: 7.389 min
Delta R.T.: -0.023 min
Response: 233907
Conc: 0.13 ng/ml

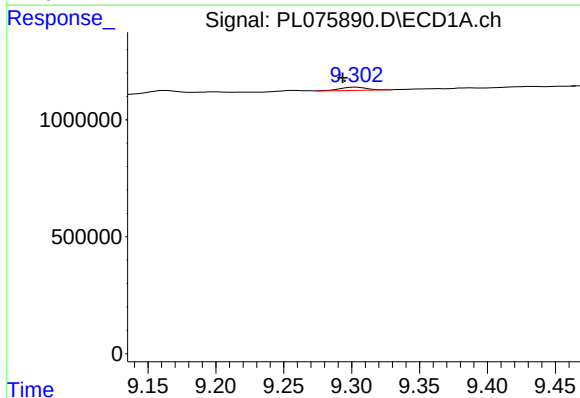


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.010 min
Response: 200886
Conc: 0.32 ng/ml

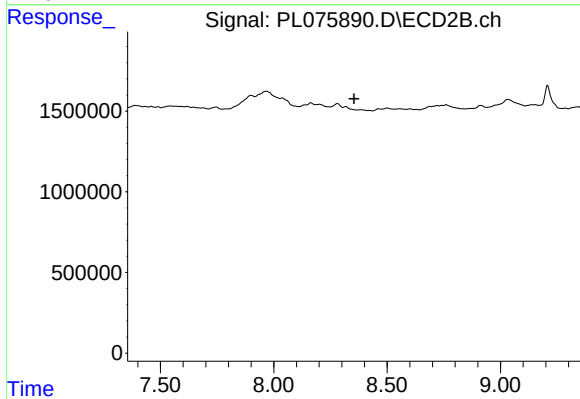

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

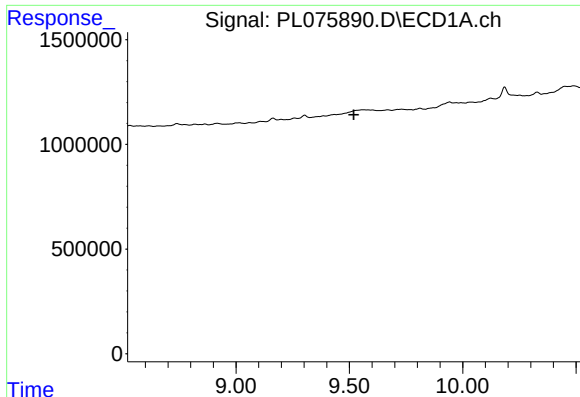

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

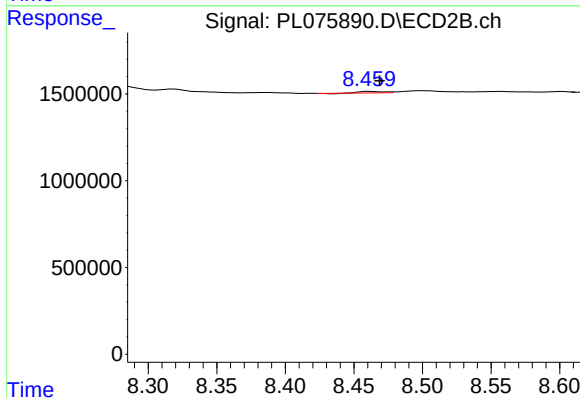


#17 4,4'-DDT

R.T.: 8.460 min
Delta R.T.: -0.008 min
Response: 92746
Conc: 0.07 ng/ml

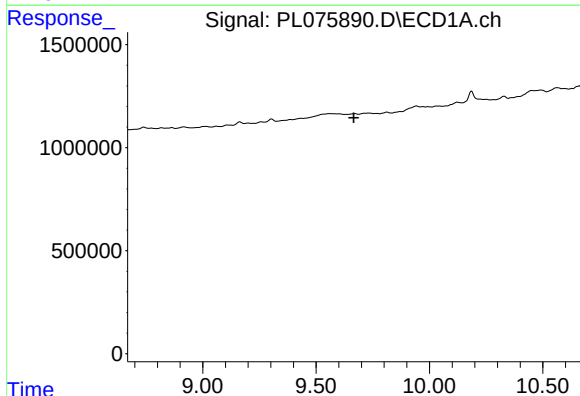


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.666 min
Response: 0
Conc: N.D.

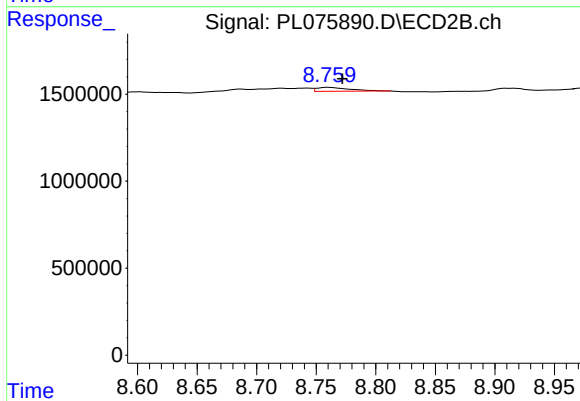

#19 Endosulfan Sulfate


R.T.: 8.760 min
Delta R.T.: -0.012 min
Response: 438039
Conc: 0.30 ng/ml

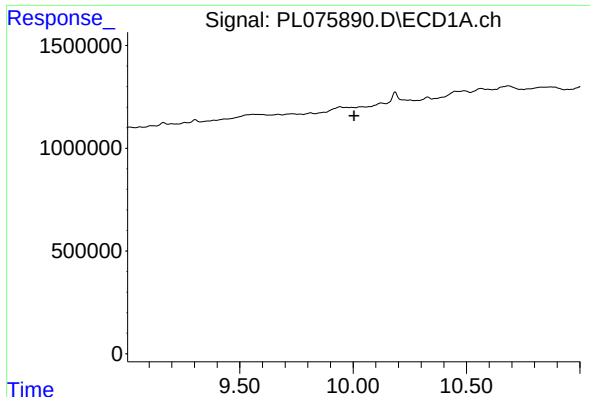

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 10.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

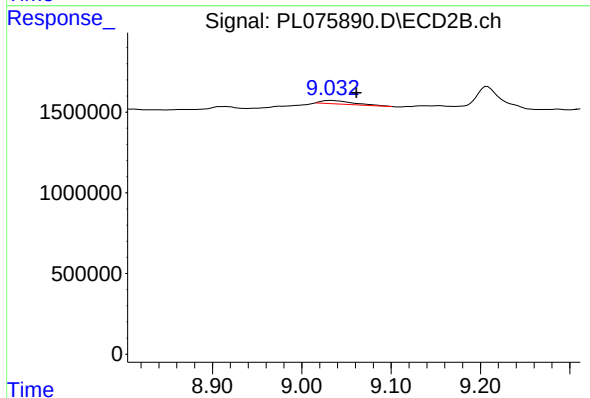


#20 Methoxychlor

R.T.: 9.032 min
Delta R.T.: -0.029 min
Response: 498202
Conc: 0.61 ng/ml

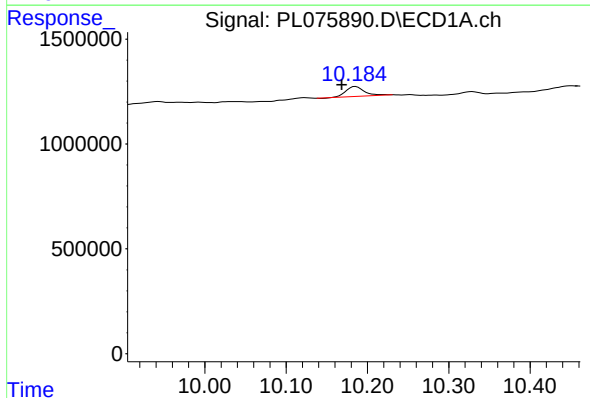


#21 Endrin ketone

R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 756852
Conc: 1.08 ng/ml

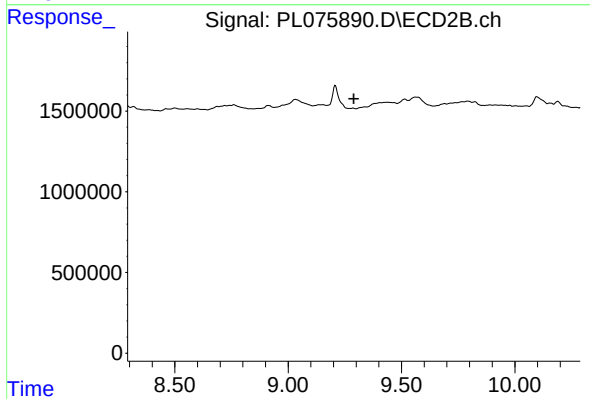

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.290 min
Response: 0
Conc: N.D.

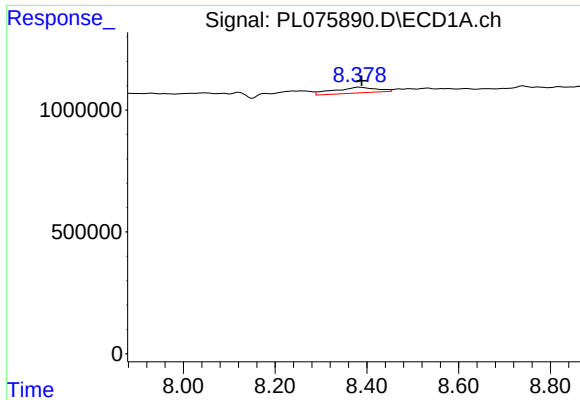

#25 Chlordane-3


R.T.: 8.382 min
Delta R.T.: -0.007 min
Response: 1510963
Conc: 14.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

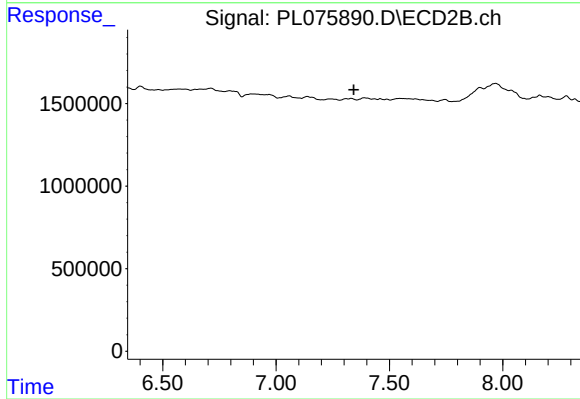


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

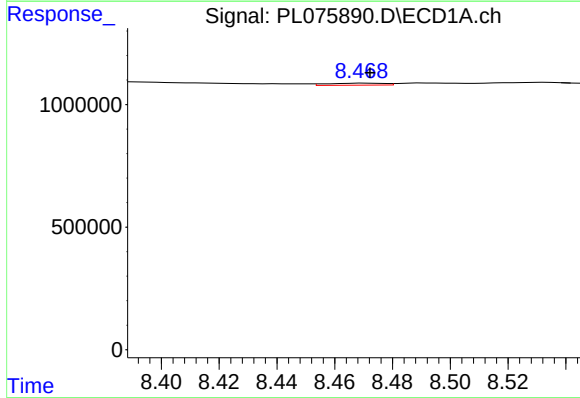


#26 Chlordane-4

R.T.: 8.471 min
Delta R.T.: -0.002 min
Response: 113424
Conc: 0.90 ng/ml

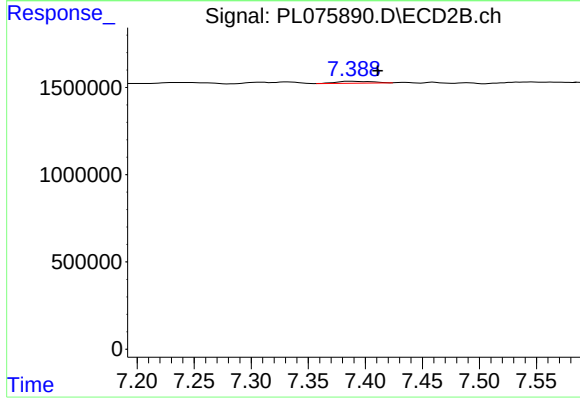

#26 Chlordane-4


R.T.: 7.389 min
Delta R.T.: -0.022 min
Response: 233907
Conc: 1.27 ng/ml

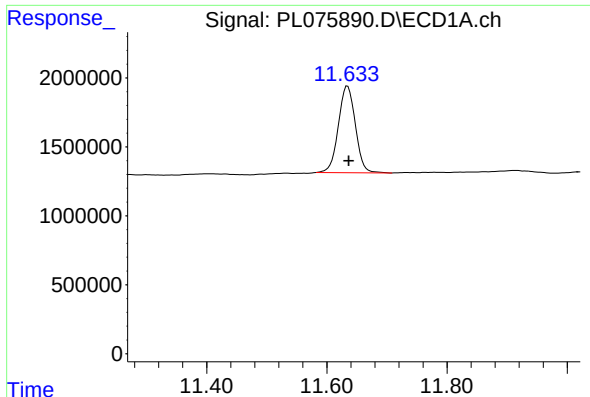

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.002 min
Response: 12344999
Conc: 20.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

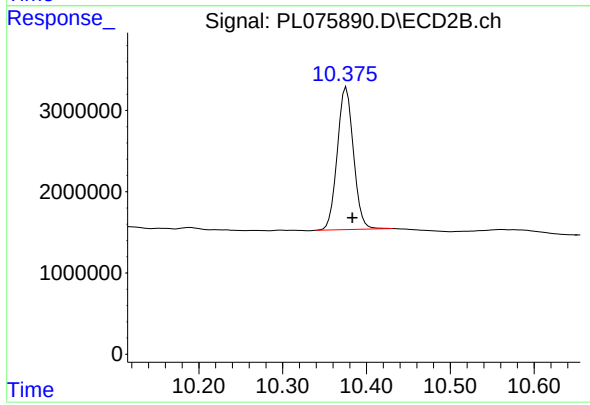

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: -0.007 min
Response: 23513072
Conc: 16.69 ng/ml