

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062122\
 Data File : PL075880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2022 14:03
 Operator : AR\AJ
 Sample : N3412-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-7-062022

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/22/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:21:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.647	4.636	9376116	22478573	13.893	13.395
2) SA Decachlor...	11.640	10.379	8335260	18262313	13.615	12.962

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062122\
Data File : PL075880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2022 14:03
Operator : AR\AJ
Sample : N3412-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-7-062022


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/22/2022
Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:21:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

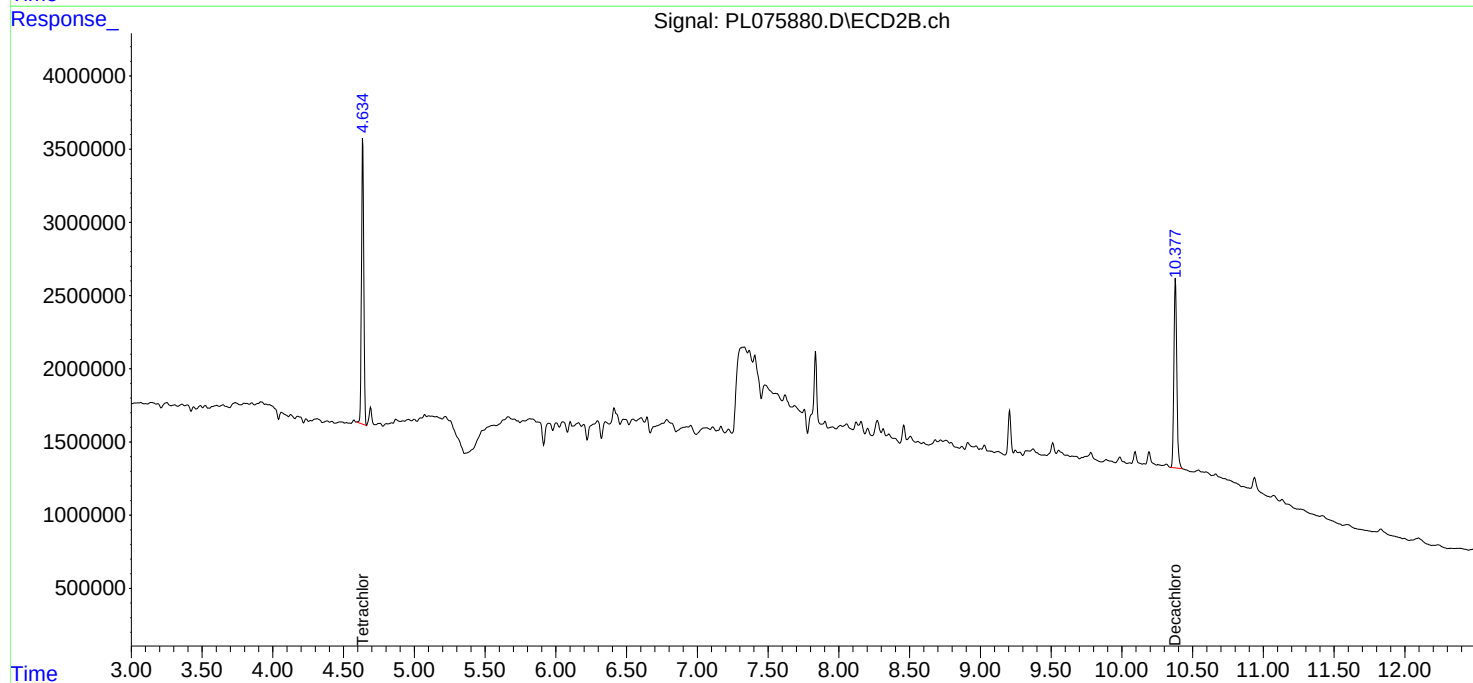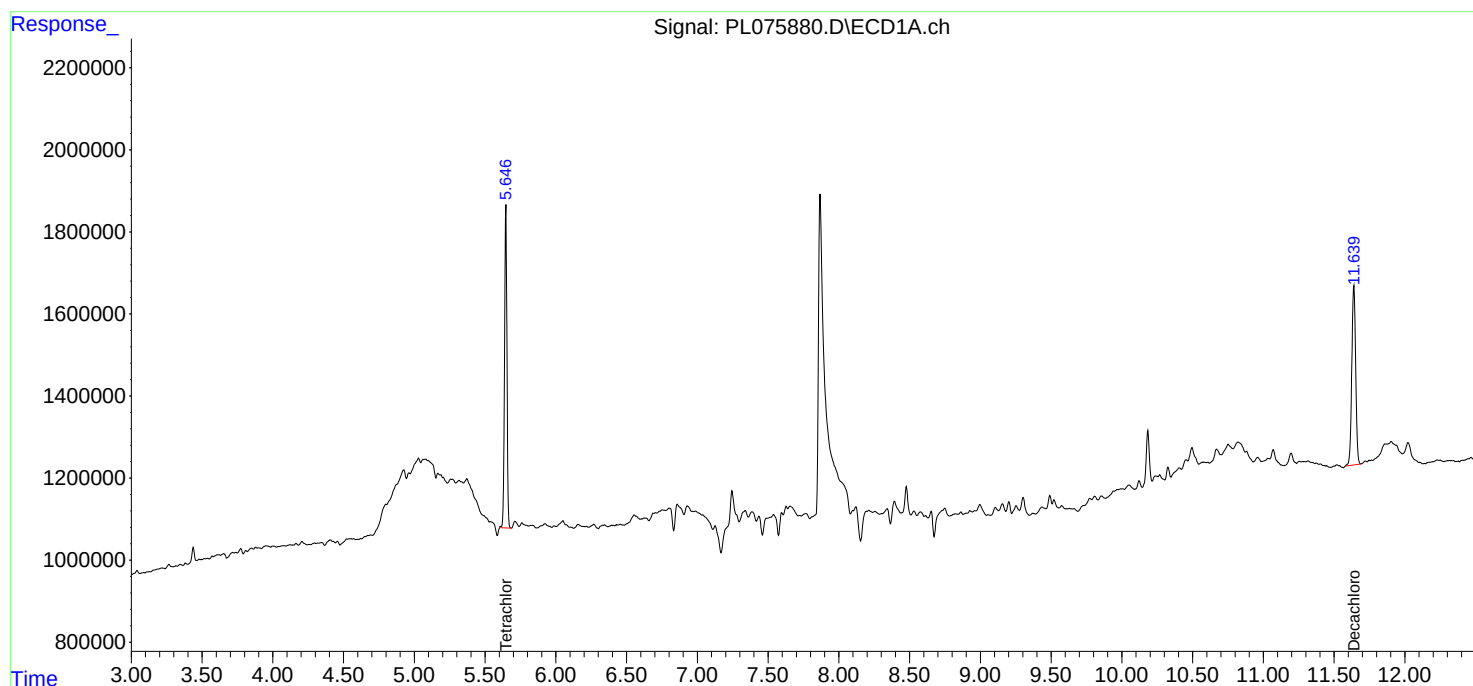

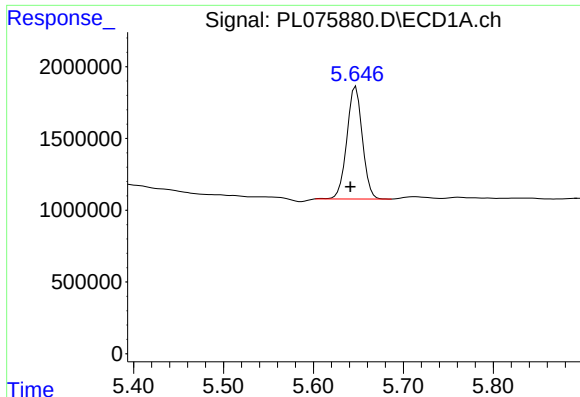


#1 Tetrachloro-m-xylene

R.T.: 5.647 min
Delta R.T.: 0.006 min
Response: 9376116
Conc: 13.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-7-062022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/22/2022
Supervised By :Ankita Jodhani 06/22/2022

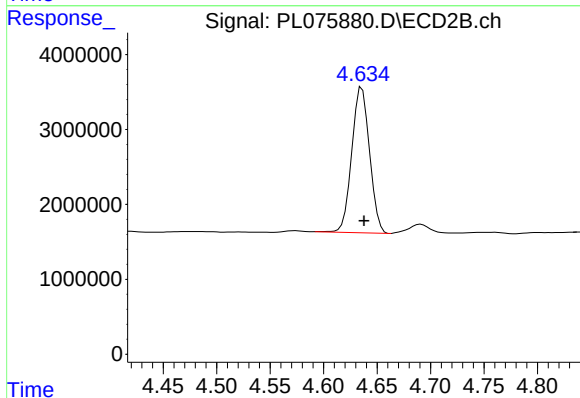


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 22478573
Conc: 13.39 ng/ml

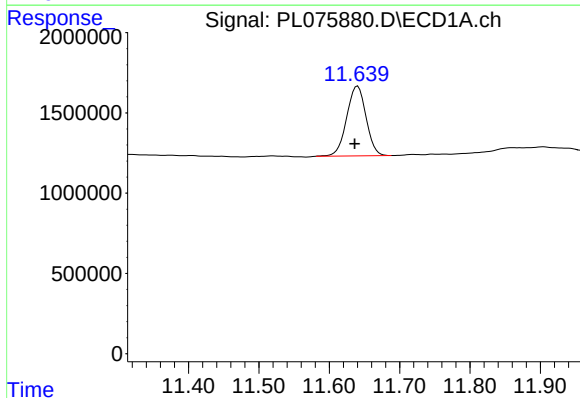

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.004 min
Response: 8335260
Conc: 13.61 ng/ml

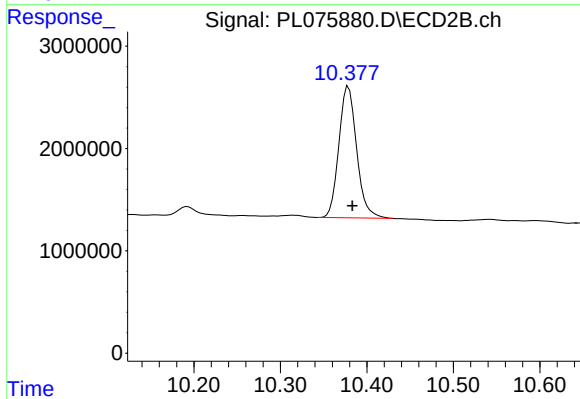

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 18262313
Conc: 12.96 ng/ml