

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062122\
 Data File : PL075882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2022 14:38
 Operator : AR\AJ
 Sample : N3373-12DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DS-7DDL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/22/2022
 Supervised By :Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:22:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	595460	1395781	0.882m	0.832
28)	SA Decachlor...	11.638	10.376	864433	2131906	1.412	1.513
Target Compounds							
13)	MA Dieldrin	8.810	7.757	9250575	45075537	12.805m	26.631m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062122\
Data File : PL075882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2022 14:38
Operator : AR\AJ
Sample : N3373-12DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DS-7DDL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/22/2022
Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:22:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

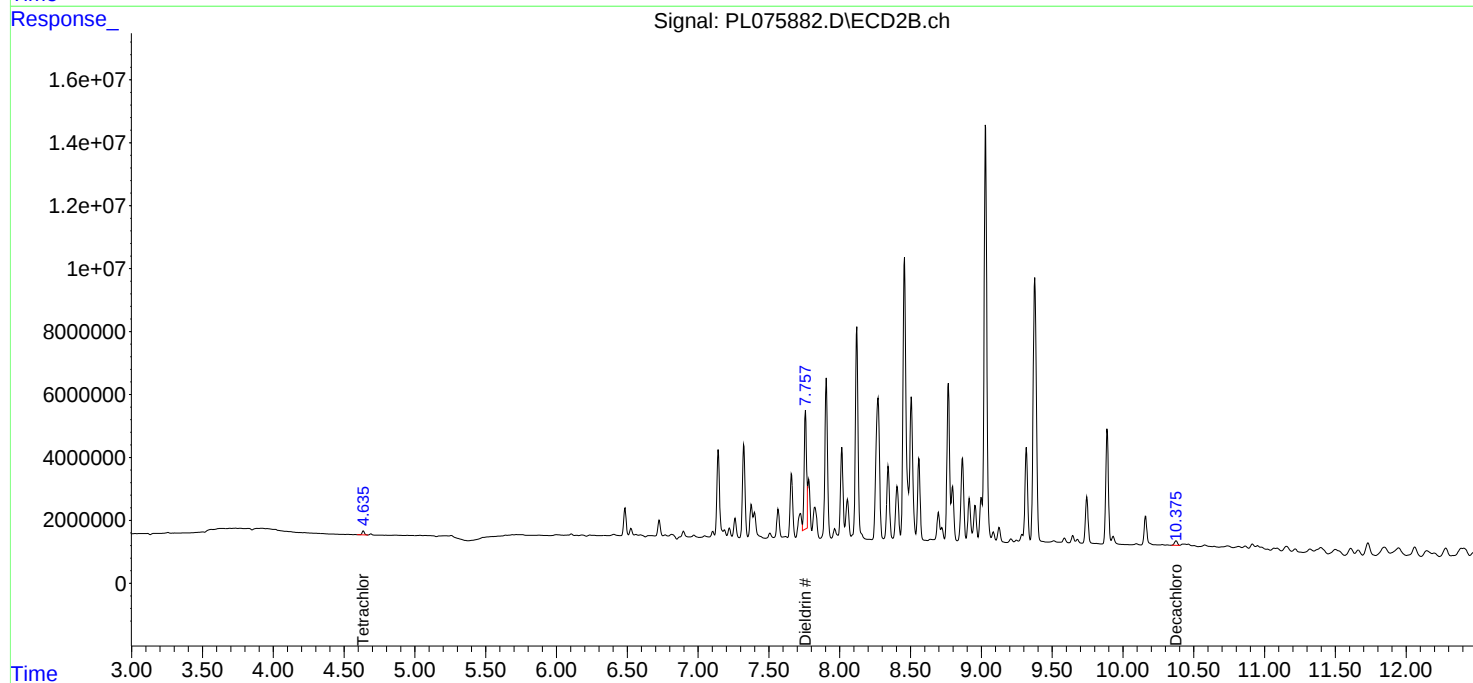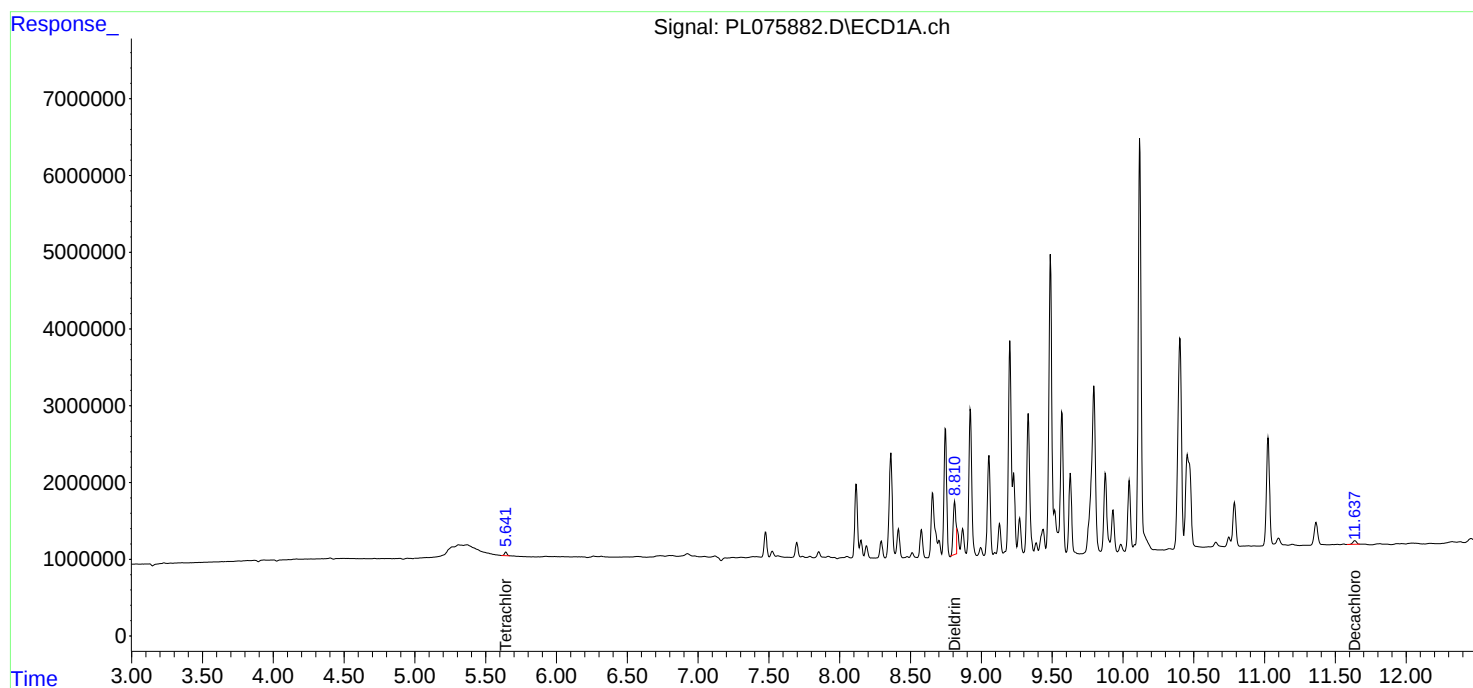

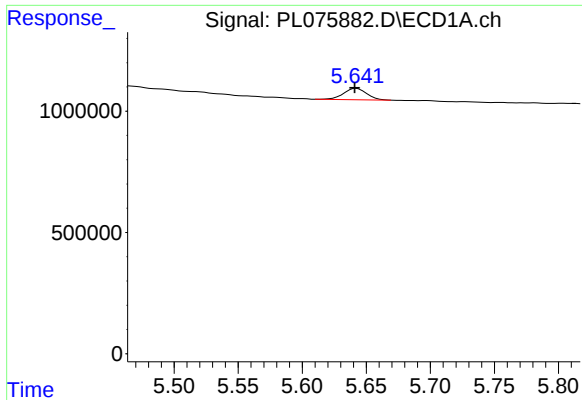


#1 Tetrachloro-m-xylene

R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 595460
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
DS-7DDL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/22/2022
Supervised By :Ankita Jodhani 06/22/2022

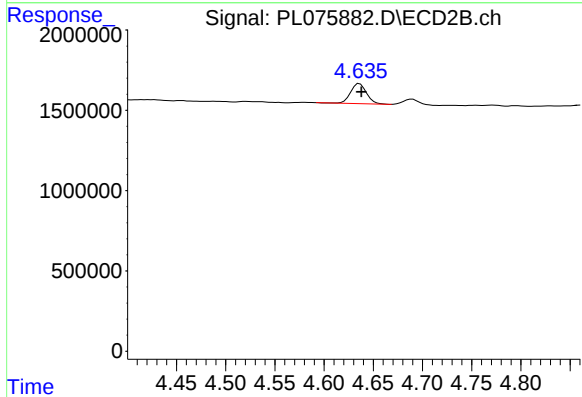


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 1395781
Conc: 0.83 ng/ml

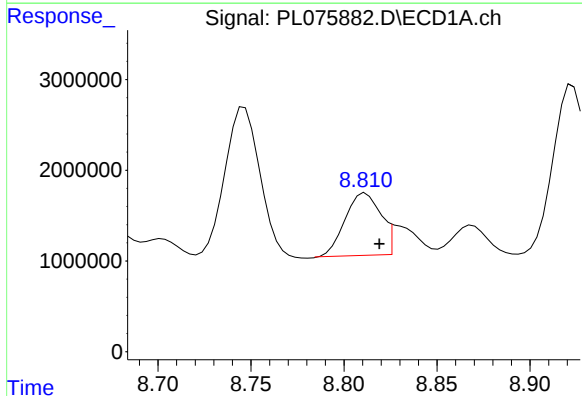


#13 Dieldrin

R.T.: 8.810 min
Delta R.T.: -0.009 min
Response: 9250575
Conc: 12.80 ng/ml m

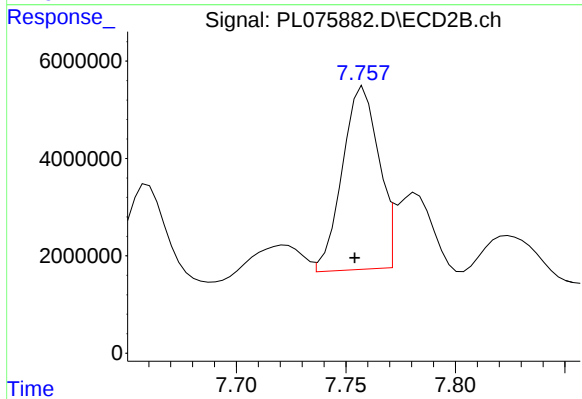

#13 Dieldrin

R.T.: 7.757 min
Delta R.T.: 0.003 min
Response: 45075537
Conc: 26.63 ng/ml m

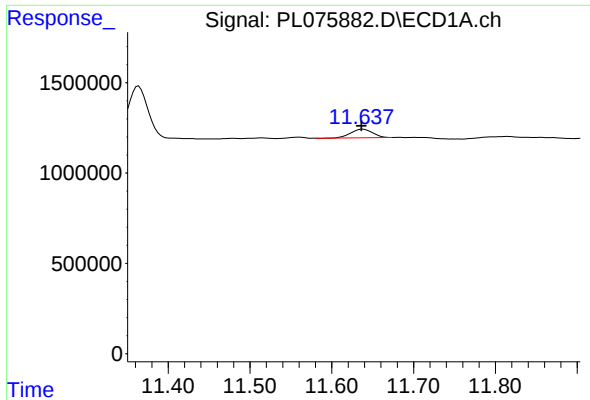


#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: 0.002 min
Response: 864433
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
DS-7DDL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/22/2022
Supervised By :Ankita Jodhani 06/22/2022

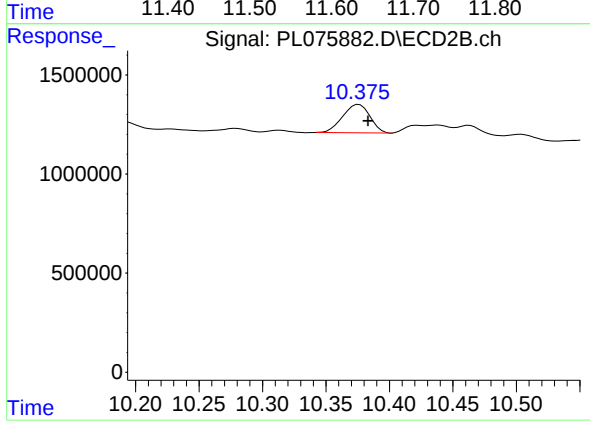

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: -0.007 min
Response: 2131906
Conc: 1.51 ng/ml