

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 14:41
 Operator : UA\AJ
 Sample : J3628-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:13:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	78871975	28765215	9.971	10.397
28)	SA Decachlor...	8.018	8.948	38840650	14259019	6.437	7.187
Target Compounds							
6)	B beta-BHC	4.256f	0.000	13365829	0	2.931	N.D. #
8)	B Heptachlo...	4.959f	0.000	40317351	0	4.304	N.D. #
10)	B gamma-Chl...	5.209	6.014	8474063	33492699	0.905	11.892 #
14)	MA Endrin	5.846	0.000	145.8E6	0	18.510	N.D. #
17)	MA 4,4'-DDT	6.200	0.000	17223417	0	2.668	N.D. #
23)	Chlordane-1	4.128	0.000	9616920	0	31.320	N.D. #
25)	Chlordane-3	5.209	6.014	8474063	33492699	7.972	85.641 #
27)	Chlordane-5	5.846	0.000	145.8E6	0	1114.228	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 14:41
Operator : UA\AJ
Sample : J3628-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:13:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

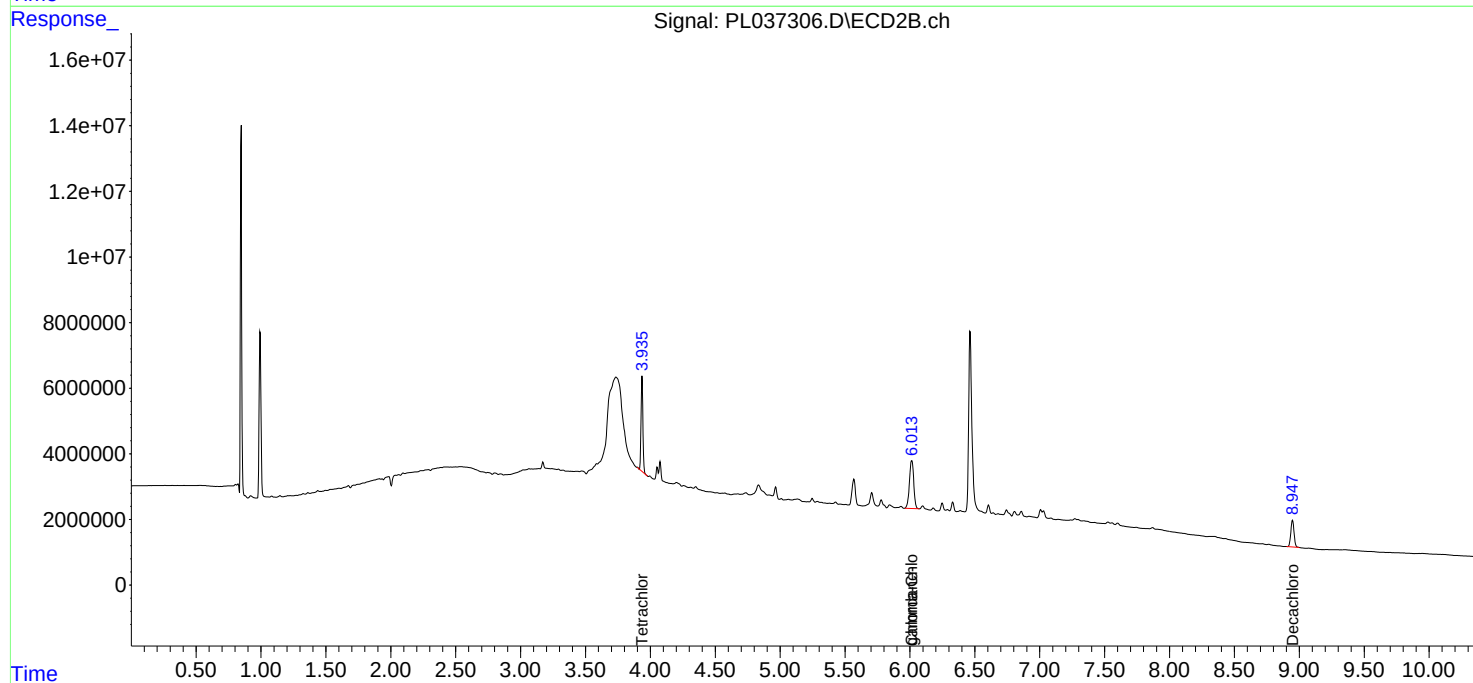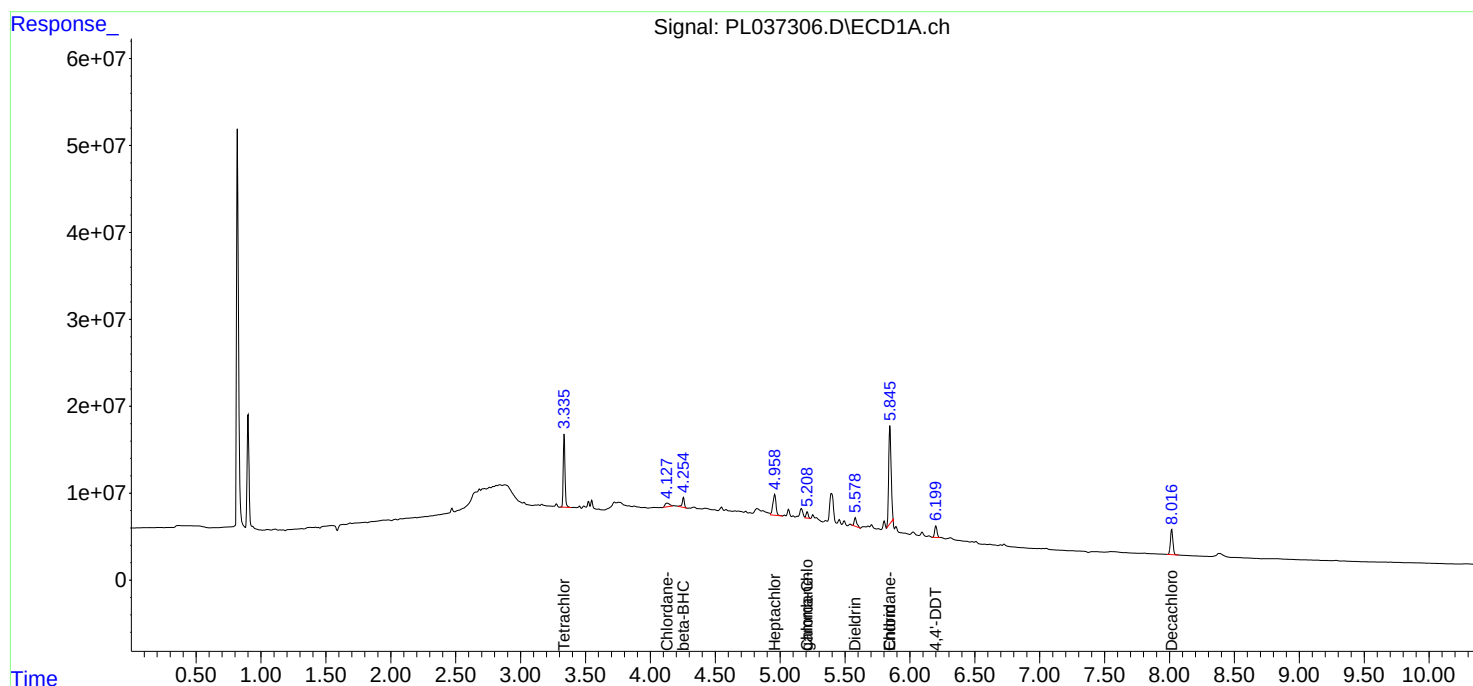


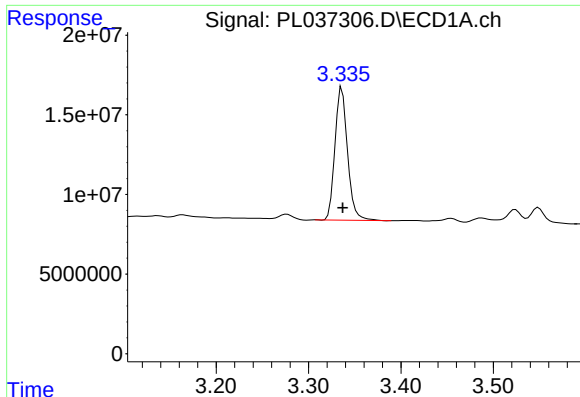

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 78871975
Conc: 9.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

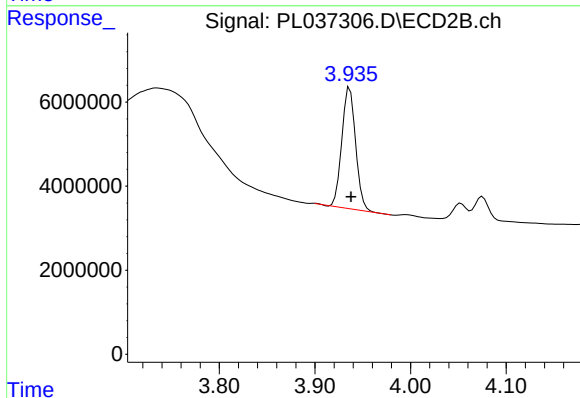


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.001 min
Response: 28765215
Conc: 10.40 ng/ml

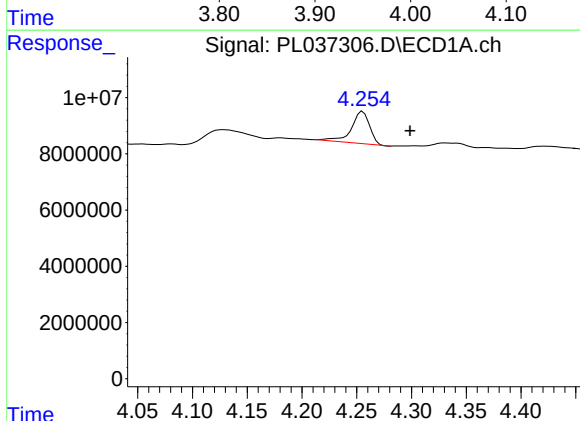


#6 beta-BHC

R.T.: 4.256 min
Delta R.T.: -0.043 min
Response: 13365829
Conc: 2.93 ng/ml

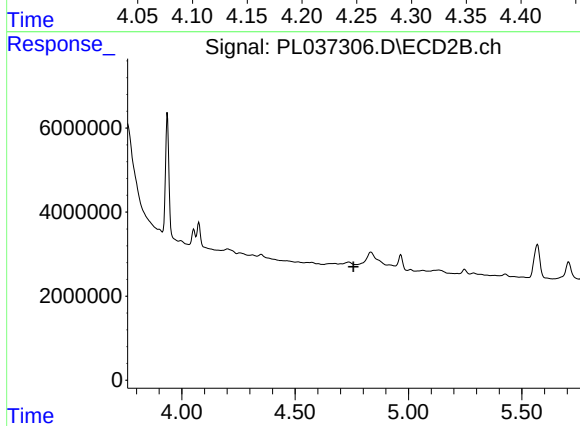

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

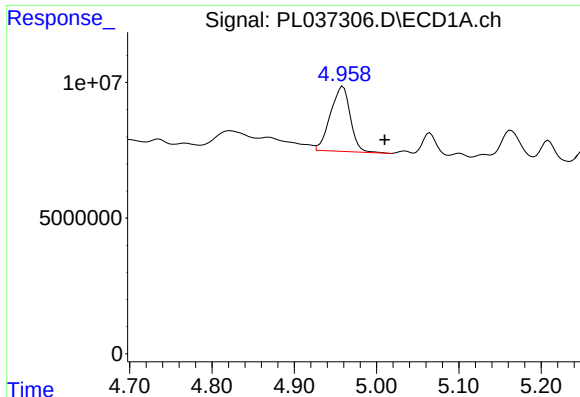

#8 Heptachlor epoxide


R.T.: 4.959 min
Delta R.T.: -0.051 min
Response: 40317351
Conc: 4.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

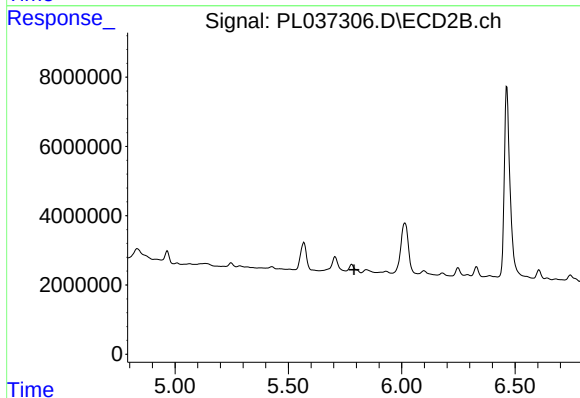


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

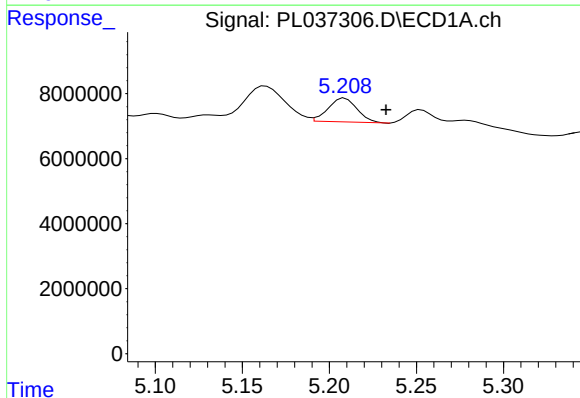


#10 gamma-Chlordane

R.T.: 5.209 min
Delta R.T.: -0.024 min
Response: 8474063
Conc: 0.90 ng/ml

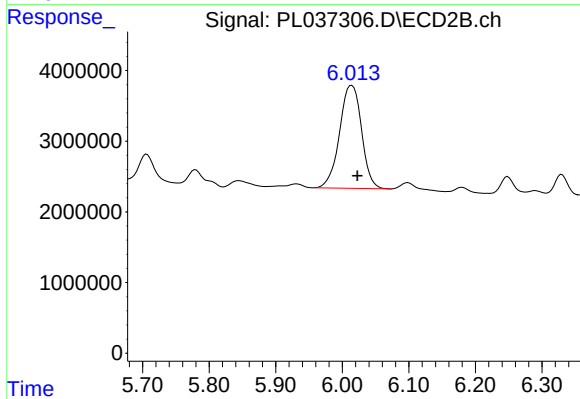

#10 gamma-Chlordane


R.T.: 6.014 min
Delta R.T.: -0.009 min
Response: 33492699
Conc: 11.89 ng/ml

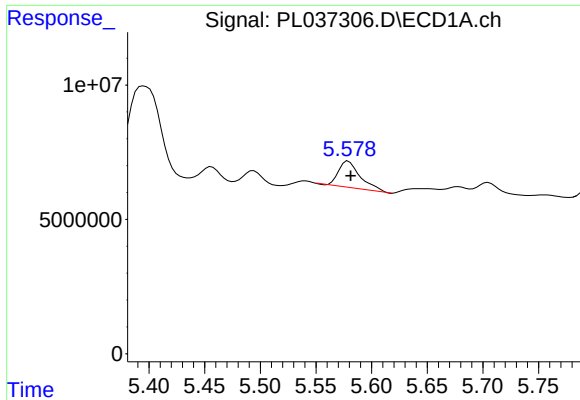

#13 Dieldrin


R.T.: 5.579 min
Delta R.T.: -0.002 min
Response: 13326720
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

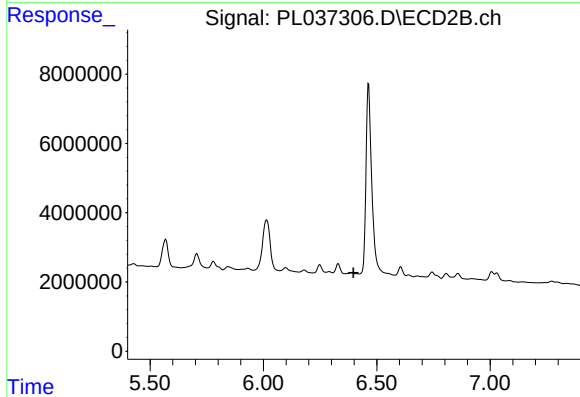


#13 Dieldrin

R.T.: 6.464 min
Delta R.T.: 0.066 min
Response: -9391980
Conc: N.D.

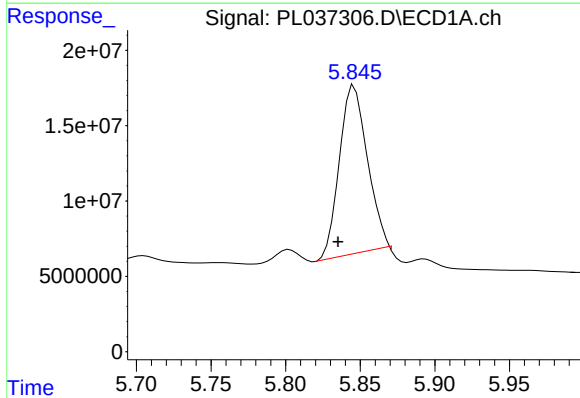


#14 Endrin

R.T.: 5.846 min
Delta R.T.: 0.011 min
Response: 145817101
Conc: 18.51 ng/ml

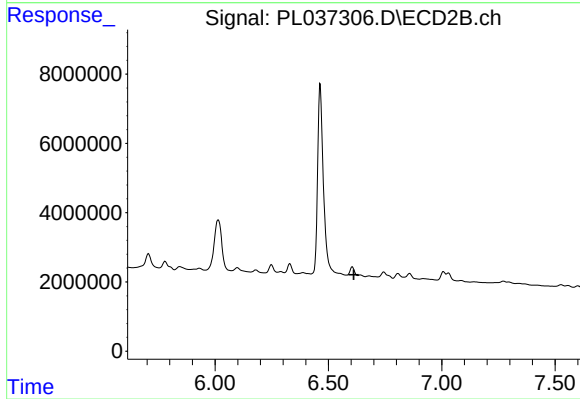

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

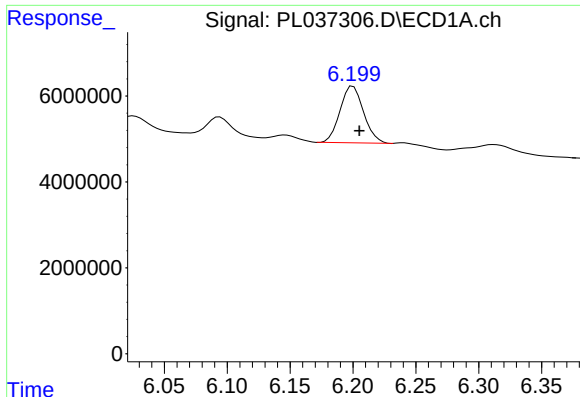

#17 4,4'-DDT


R.T.: 6.200 min
Delta R.T.: -0.005 min
Response: 17223417
Conc: 2.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

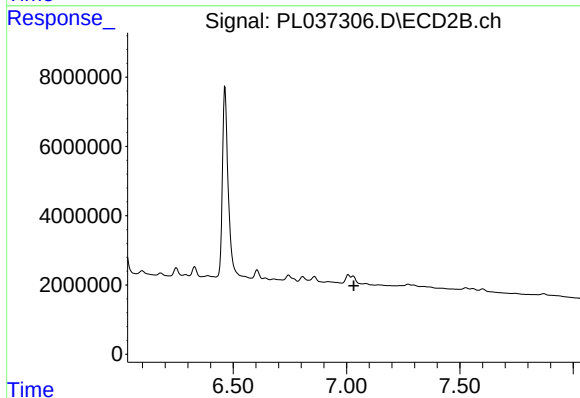


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

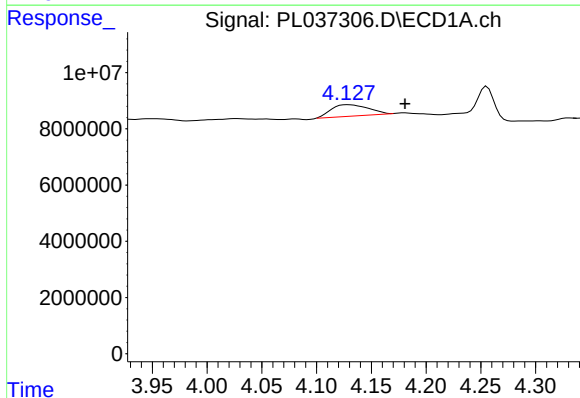


#23 Chlordane-1

R.T.: 4.128 min
Delta R.T.: -0.052 min
Response: 9616920
Conc: 31.32 ng/ml

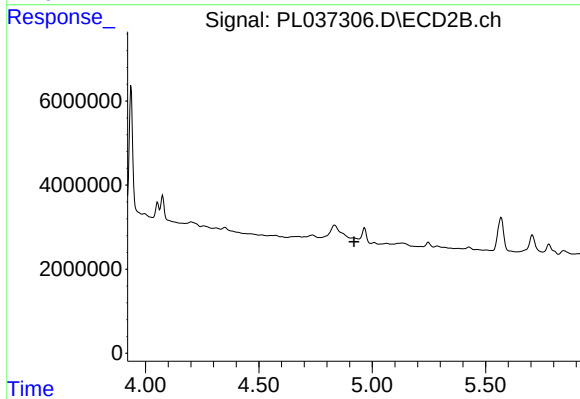

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

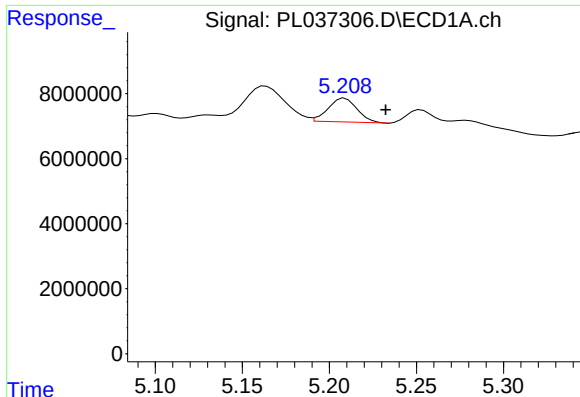

#25 Chlordane-3


R.T.: 5.209 min
Delta R.T.: -0.023 min
Response: 8474063
Conc: 7.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

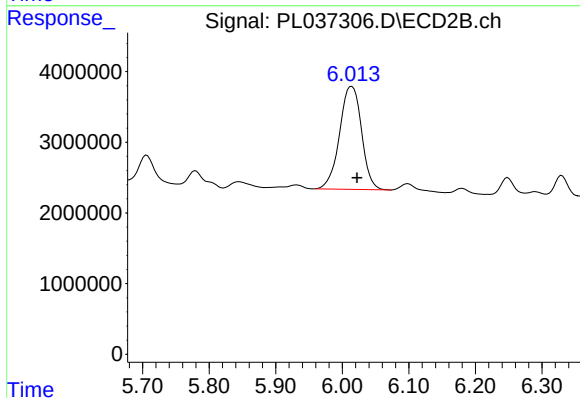


#25 Chlordane-3

R.T.: 6.014 min
Delta R.T.: -0.008 min
Response: 33492699
Conc: 85.64 ng/ml

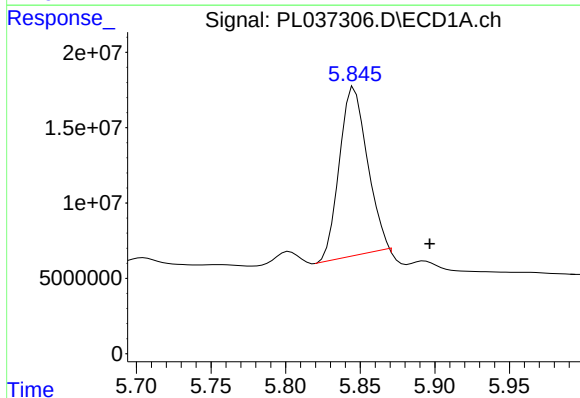


#27 Chlordane-5

R.T.: 5.846 min
Delta R.T.: -0.051 min
Response: 145817101
Conc: 1114.23 ng/ml

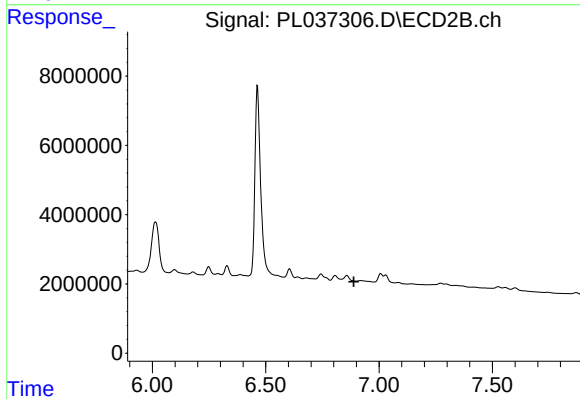

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

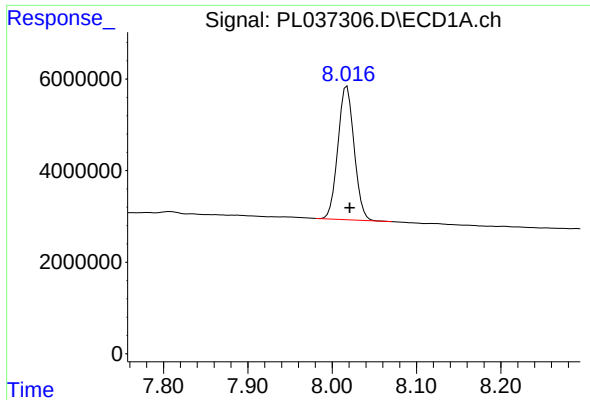

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 38840650
Conc: 6.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

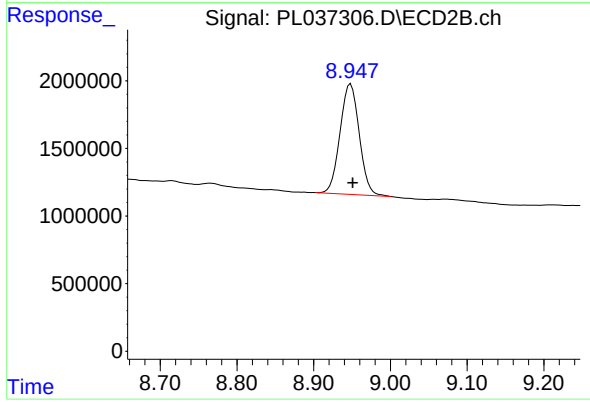

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 14259019
Conc: 7.19 ng/ml