

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 16:34
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:17:17 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	130.0E6	41734045	16.440	15.084
28)	SA Decachlor...	8.018	8.949	102.6E6	39136697	16.996	19.727
Target Compounds							
10)	B gamma-Chl...	5.164f	0.000	17150348	0	1.831	N.D. #
23)	Chlordane-1	4.120	0.000	18587030	0	60.534	N.D. #
25)	Chlordane-3	5.164	0.000	17150348	0	16.135	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 16:34
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:17:17 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

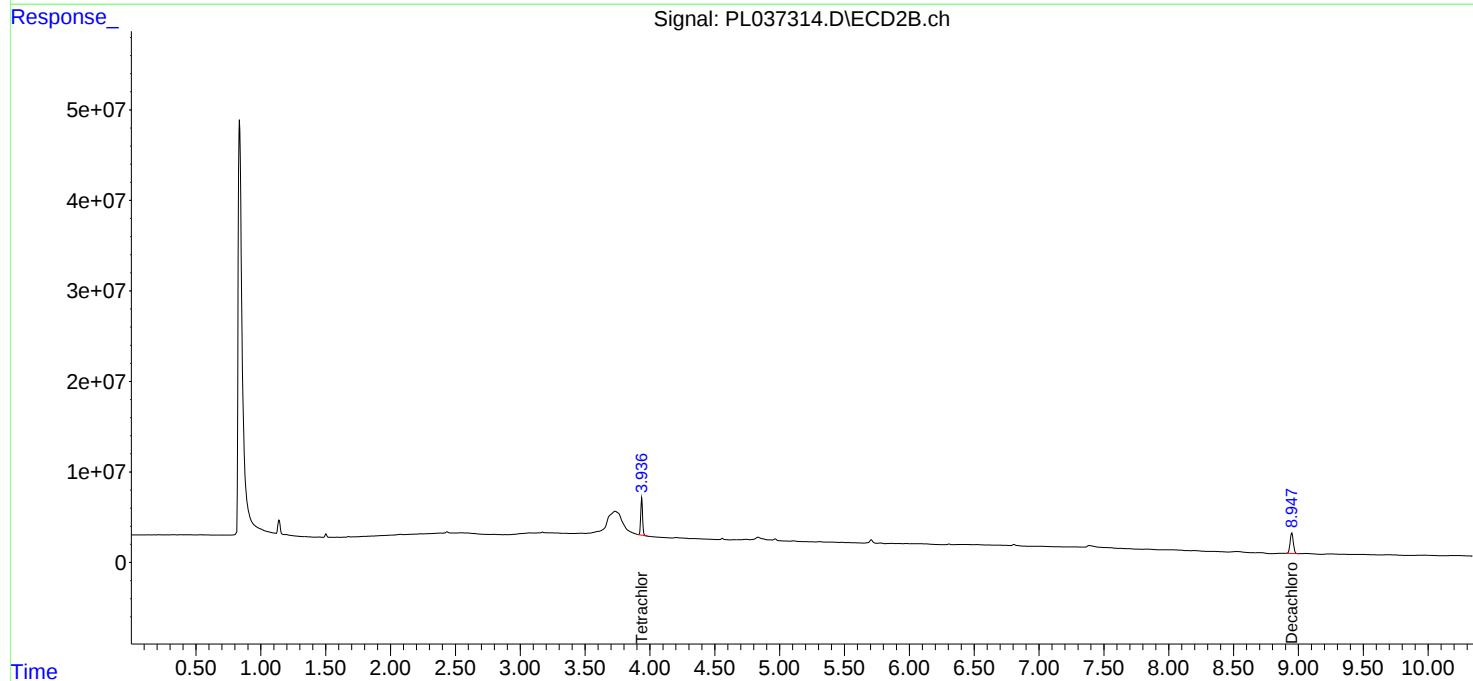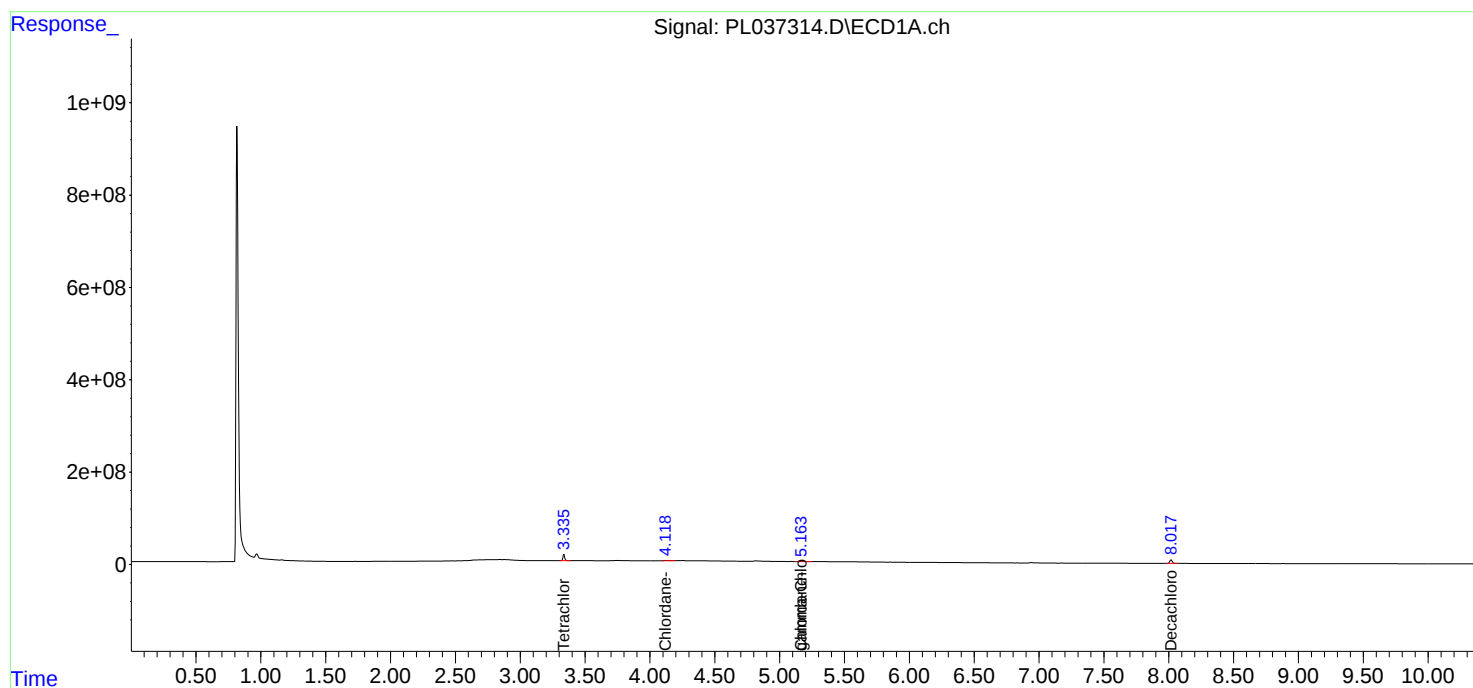


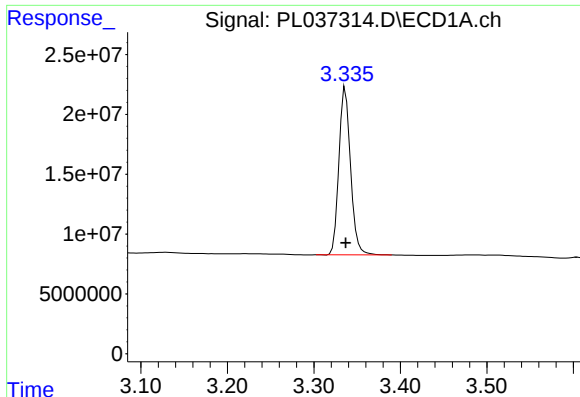

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 130047854
Conc: 16.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

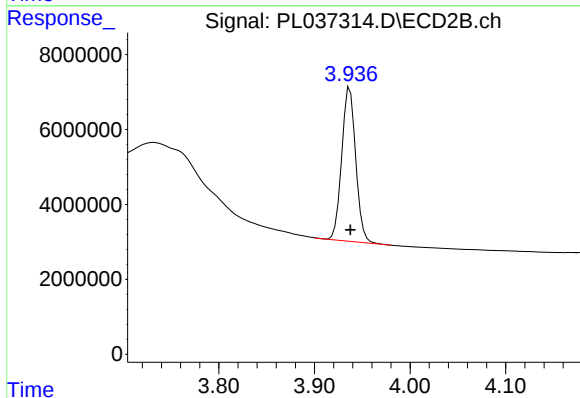


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 41734045
Conc: 15.08 ng/ml

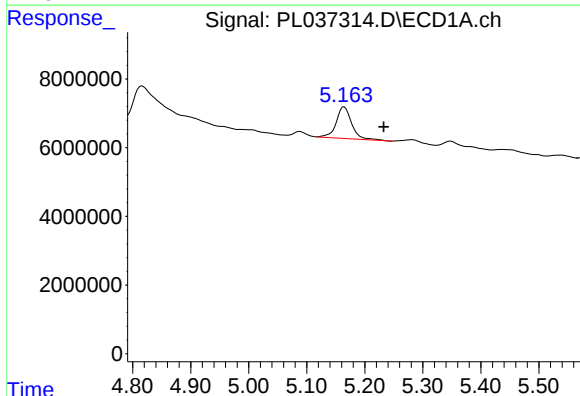


#10 gamma-Chlordane

R.T.: 5.164 min
Delta R.T.: -0.068 min
Response: 17150348
Conc: 1.83 ng/ml

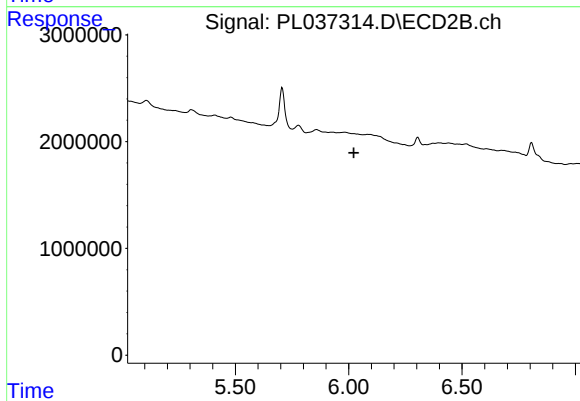

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

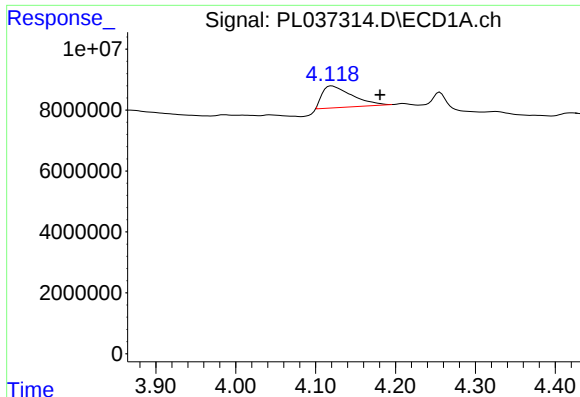

#23 Chlordane-1


R.T.: 4.120 min
Delta R.T.: -0.060 min
Response: 18587030
Conc: 60.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

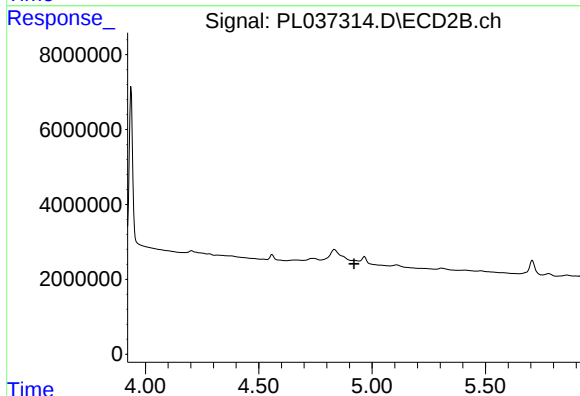


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

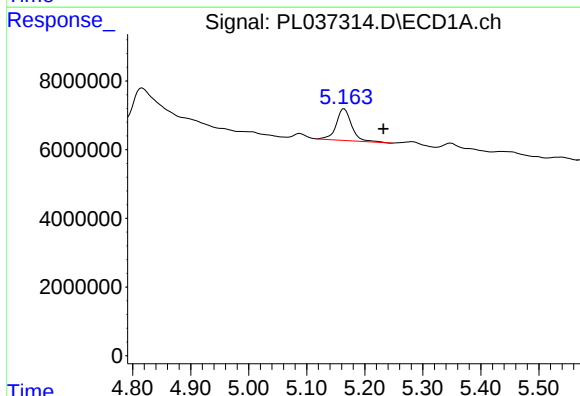


#25 Chlordane-3

R.T.: 5.164 min
Delta R.T.: -0.068 min
Response: 17150348
Conc: 16.14 ng/ml

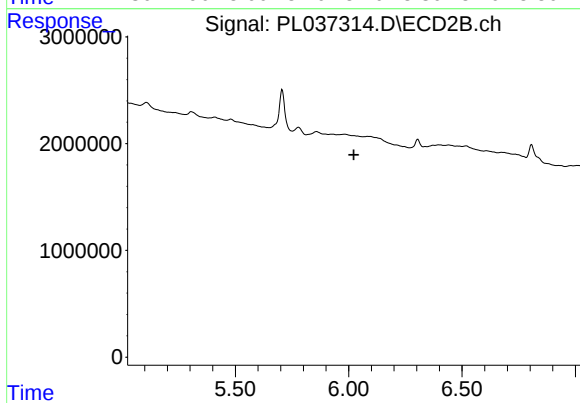

#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

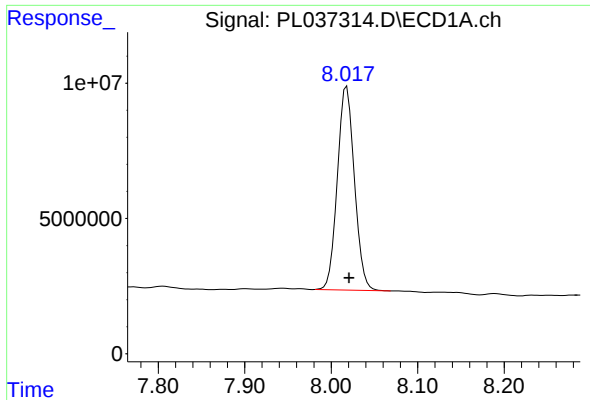

#28 Decachlorobiphenyl


R.T.: 8.018 min

Delta R.T.: -0.003 min

Response: 102553762

Conc: 17.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

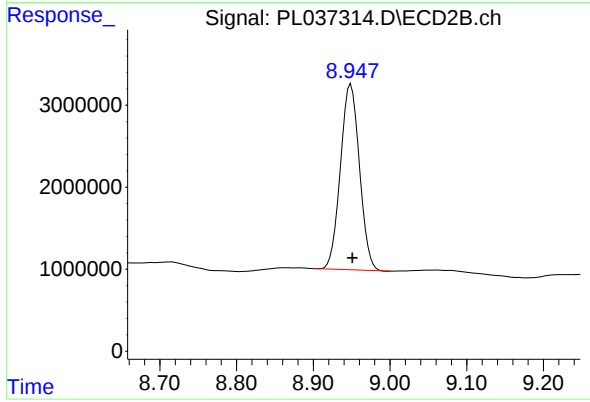

#28 Decachlorobiphenyl

R.T.: 8.949 min

Delta R.T.: -0.002 min

Response: 39136697

Conc: 19.73 ng/ml