

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 17:59
 Operator : UA\AJ
 Sample : J3665-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:19:05 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	141.8E6	51738817	17.928	18.700
28)	SA Decachlor...	8.017	8.948	83742515	31177494	13.878	15.715
Target Compounds							
6)	B beta-BHC	4.257f	0.000	10678569	0	2.341	N.D. #
8)	B Heptachlo...	5.070f	0.000	20477310	0	2.186	N.D. #
10)	B gamma-Chl...	5.165f	0.000	23118637	0	2.468	N.D. #
15)	B Endosulfa...	6.107	0.000	6753134	0	0.918	N.D. #
25)	Chlordane-3	5.165	0.000	23118637	0	21.750	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 17:59
Operator : UA\AJ
Sample : J3665-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:19:05 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

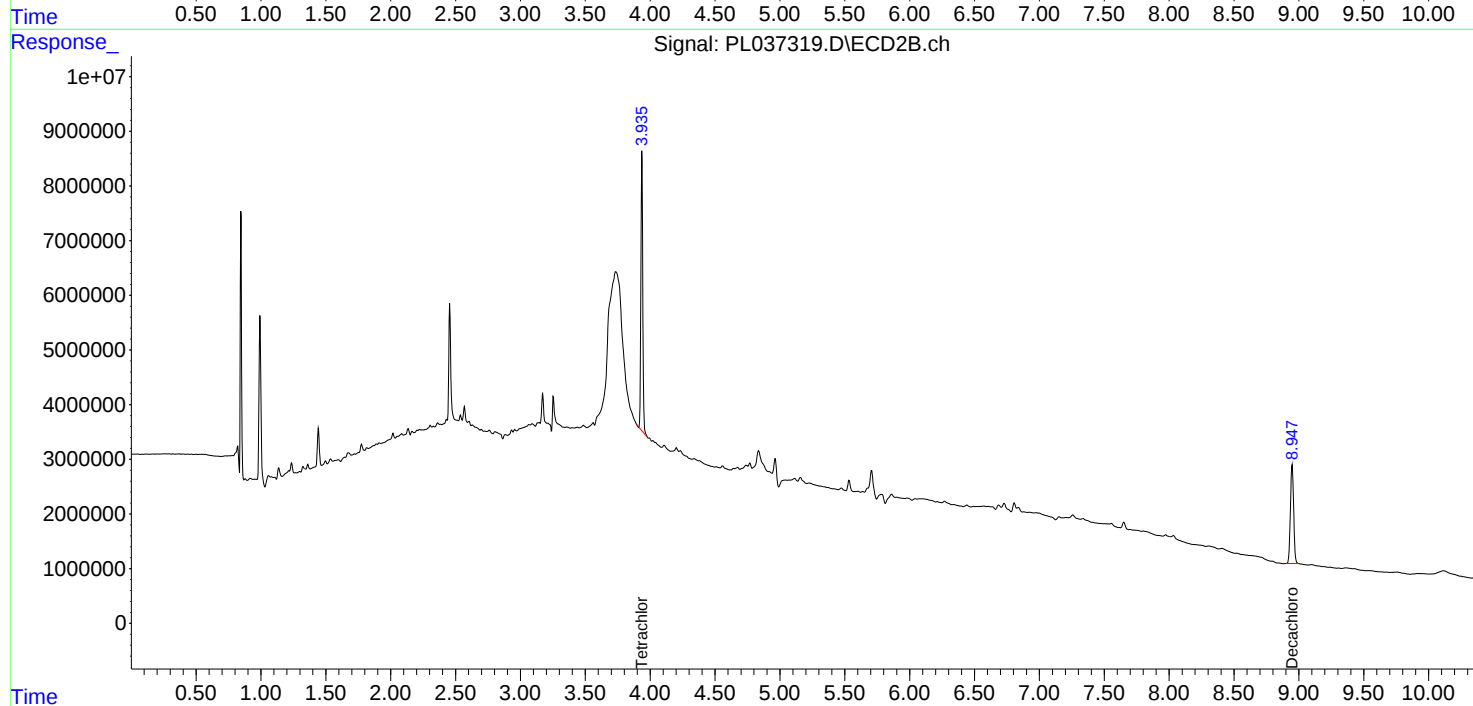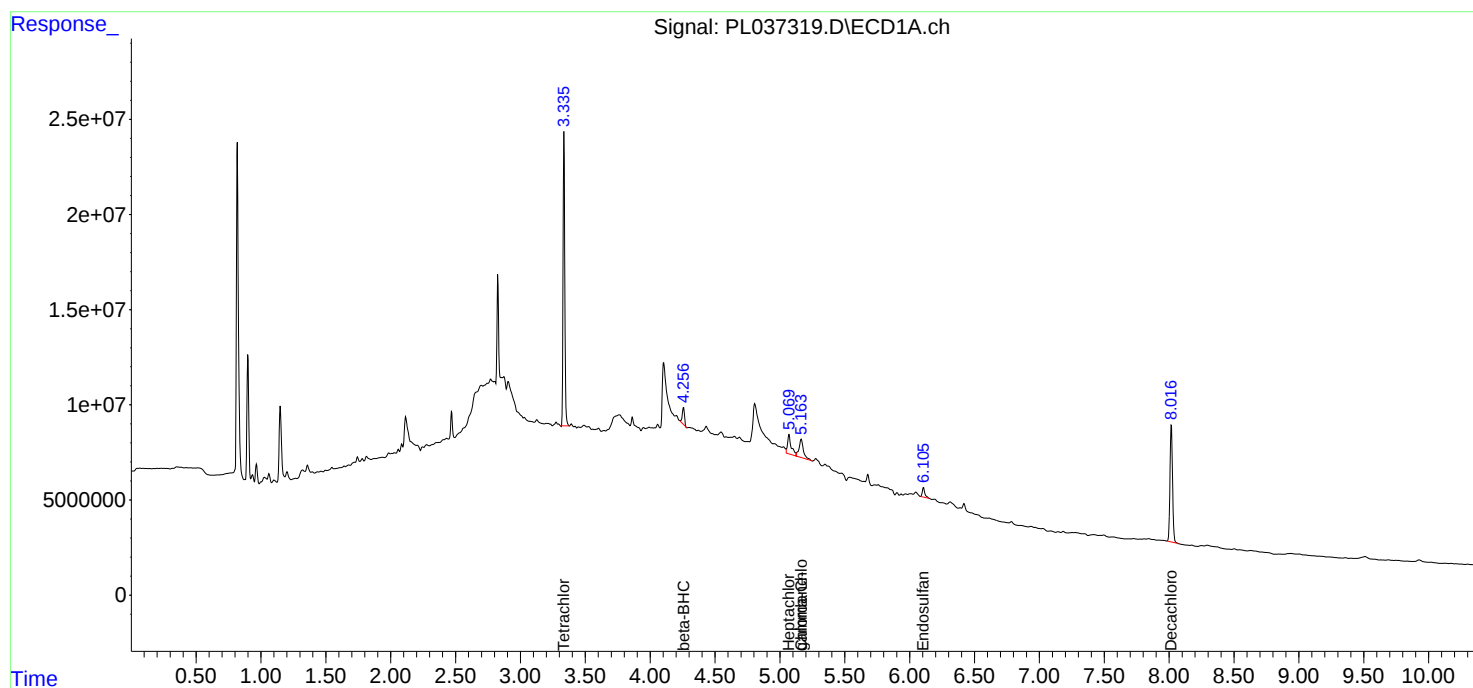


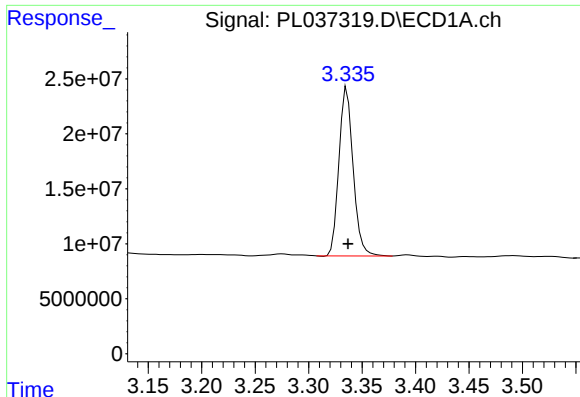

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 141817479
Conc: 17.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

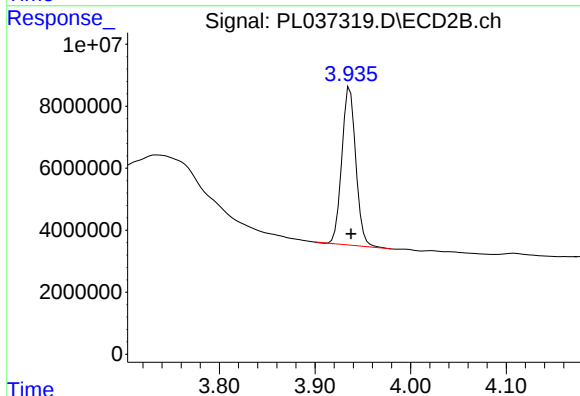


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.001 min
Response: 51738817
Conc: 18.70 ng/ml

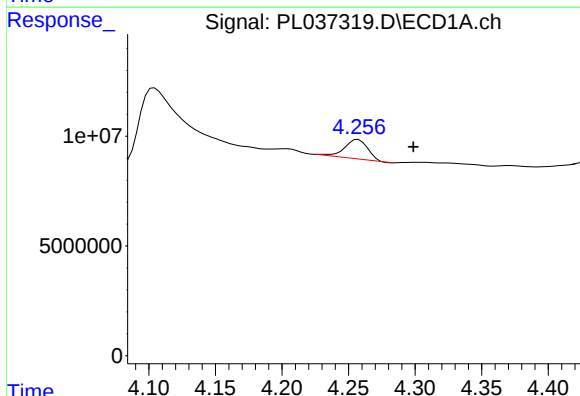


#6 beta-BHC

R.T.: 4.257 min
Delta R.T.: -0.042 min
Response: 10678569
Conc: 2.34 ng/ml

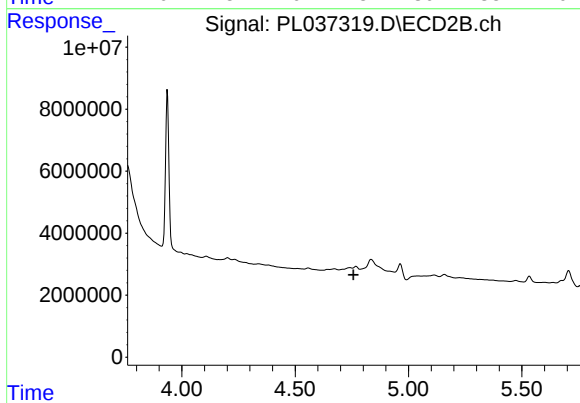

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

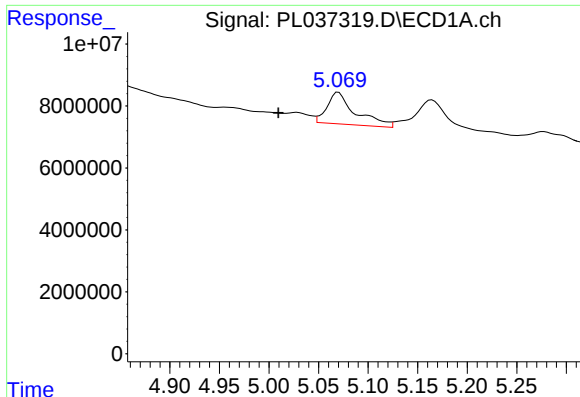

#8 Heptachlor epoxide


R.T.: 5.070 min
Delta R.T.: 0.061 min
Response: 20477310
Conc: 2.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

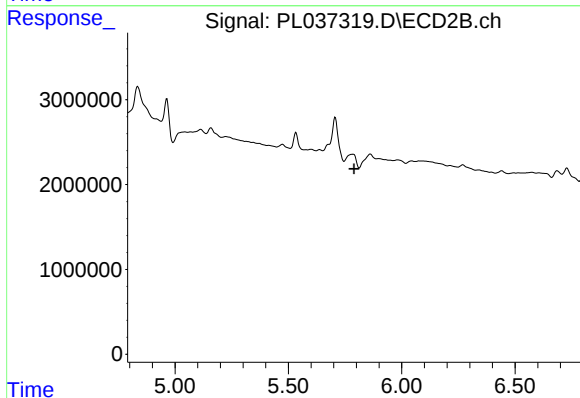


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

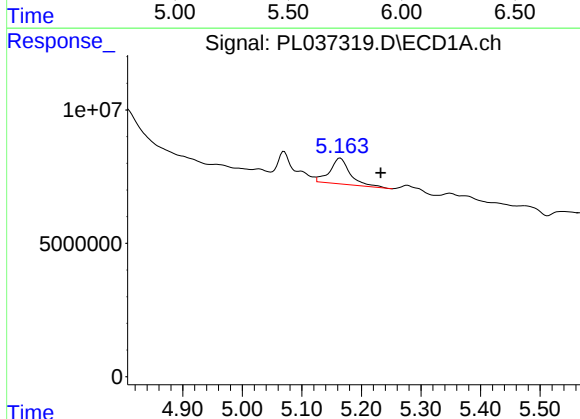


#10 gamma-Chlordane

R.T.: 5.165 min
Delta R.T.: -0.068 min
Response: 23118637
Conc: 2.47 ng/ml

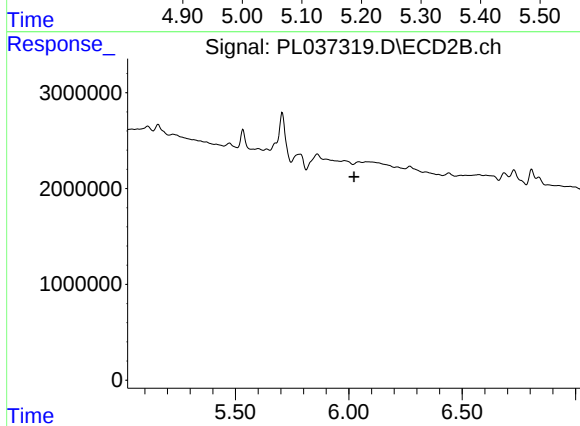

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

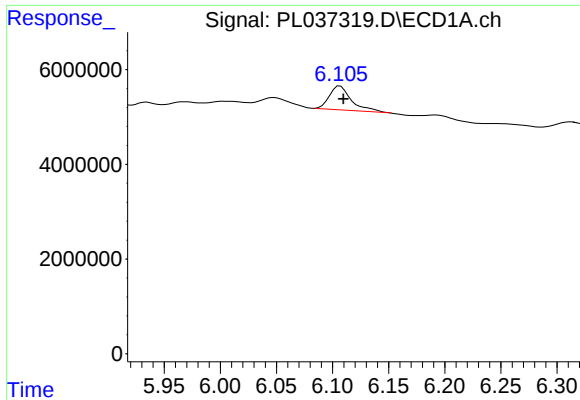

#15 Endosulfan II


R.T.: 6.107 min
Delta R.T.: -0.003 min
Response: 6753134
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

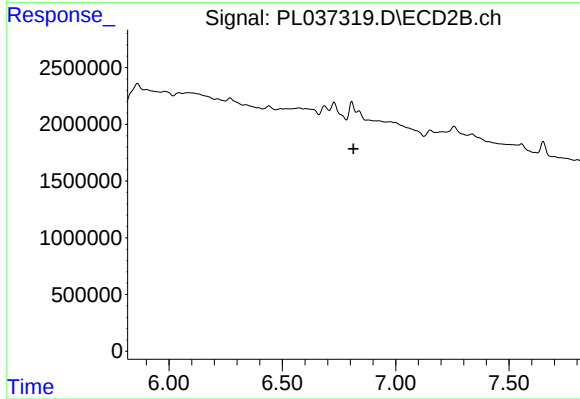


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

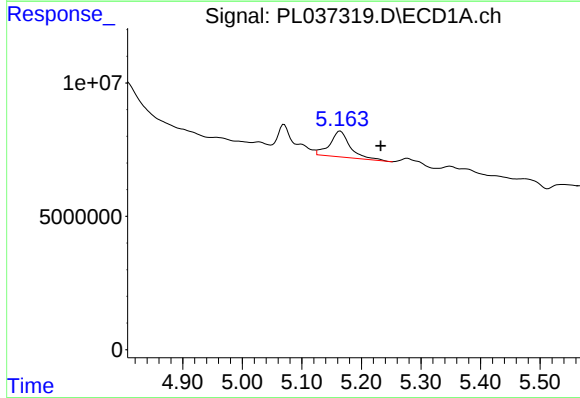


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: -0.068 min
Response: 23118637
Conc: 21.75 ng/ml

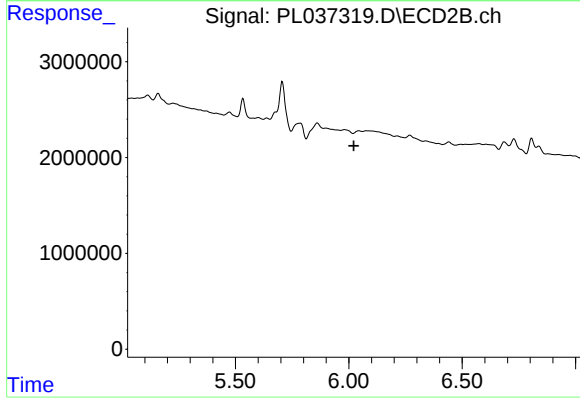

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

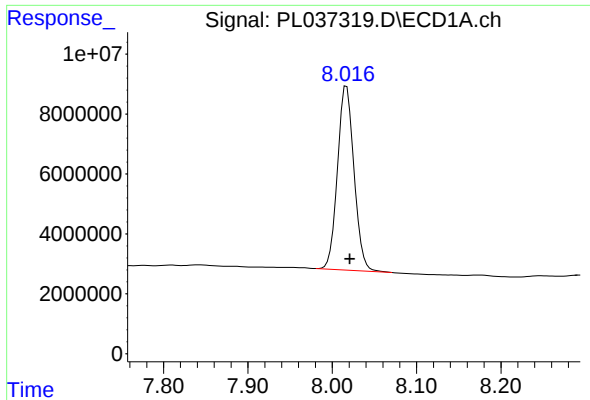

#28 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.004 min
Response: 83742515
Conc: 13.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

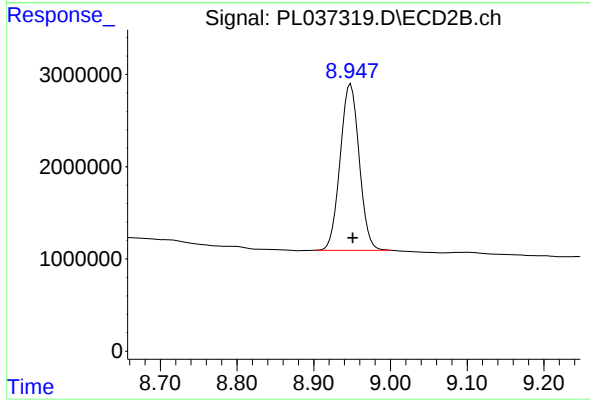

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 31177494
Conc: 15.71 ng/ml