

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 18:27
 Operator : UA\AJ
 Sample : J3622-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:19:47 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	137.5E6	50435260	17.382	18.229
28)	SA Decachlor...	8.018	8.949	82323572	30446457	13.643	15.346
Target Compounds							
2)	A alpha-BHC	3.720f	0.000	11638550	0	0.951	N.D. #
6)	B beta-BHC	4.257f	0.000	8407036	0	1.843	N.D. #
8)	B Heptachlo...	5.072f	0.000	20704573	0	2.210	N.D. #
9)	A Endosulfan I	5.372	0.000	17878834	0	2.113	N.D. #
10)	B gamma-Chl...	5.166f	0.000	36748060	0	3.923	N.D. #
16)	A 4,4'-DDD	5.968	0.000	6018051	0	0.916	N.D. #
17)	MA 4,4'-DDT	6.202	0.000	5889460	0	0.912	N.D. #
25)	Chlordane-3	5.166	0.000	36748060	0	34.573	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 18:27
Operator : UA\AJ
Sample : J3622-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:19:47 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

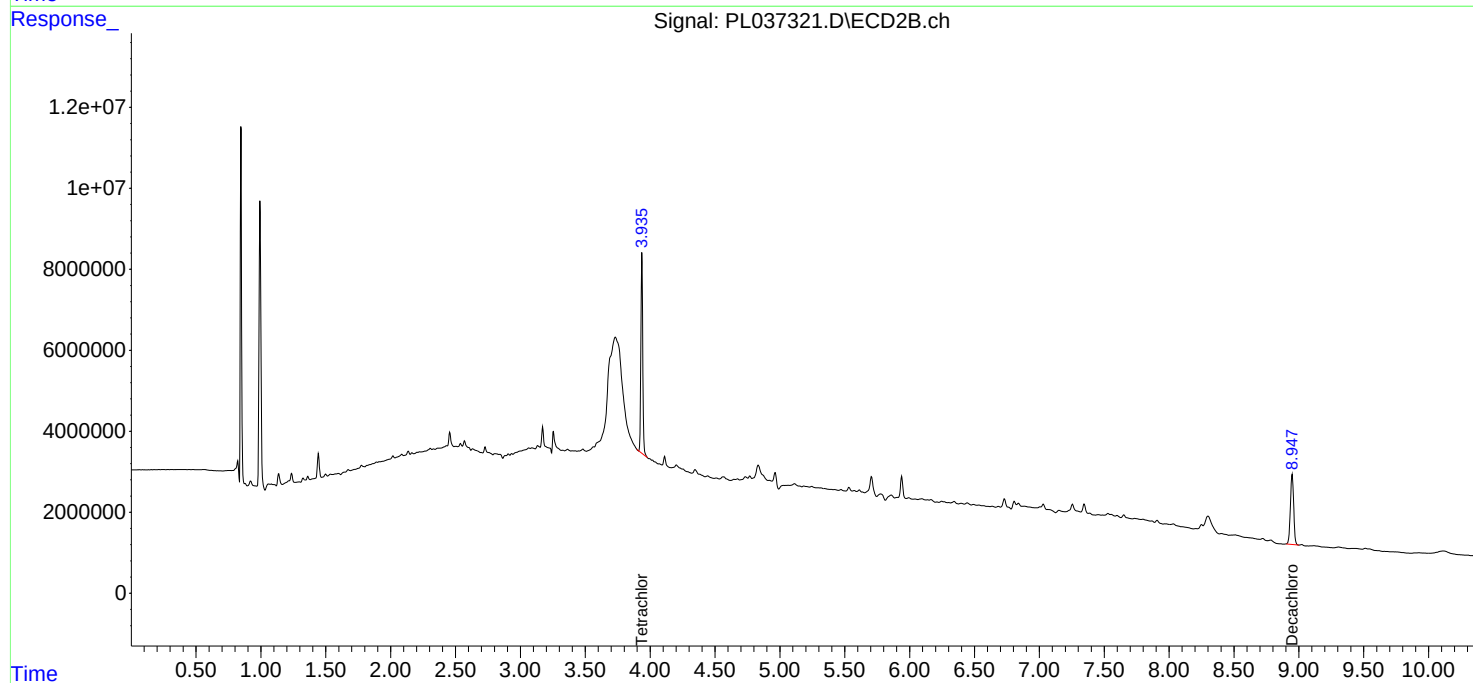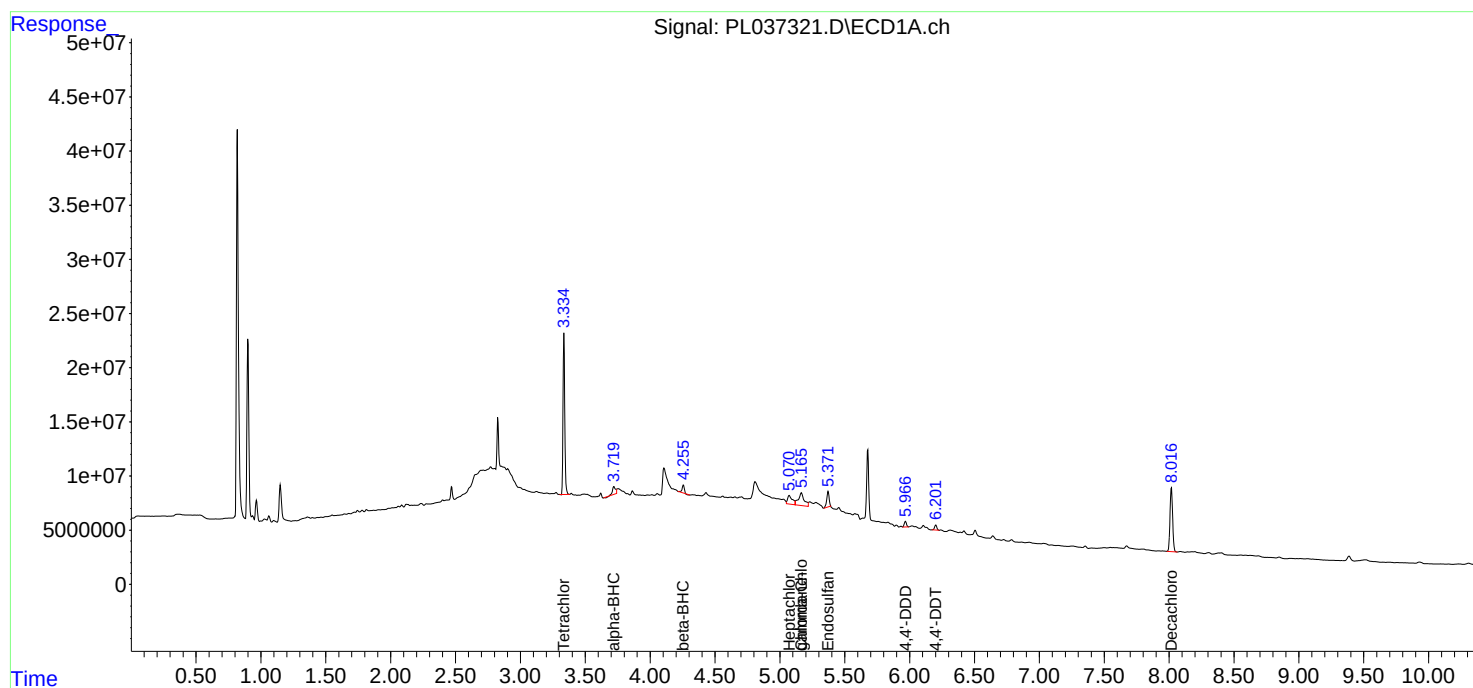


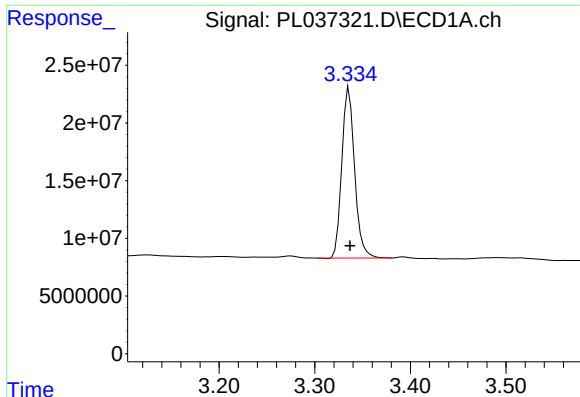

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 137499794
Conc: 17.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

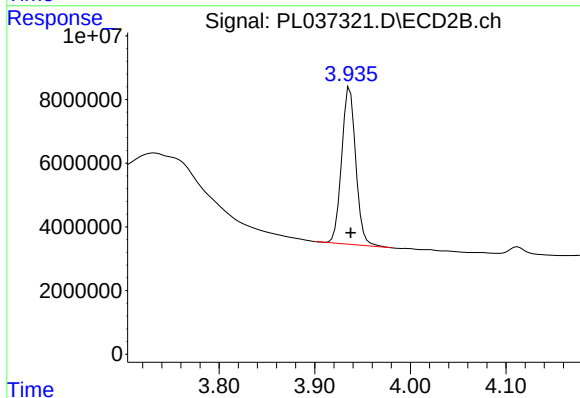


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 50435260
Conc: 18.23 ng/ml

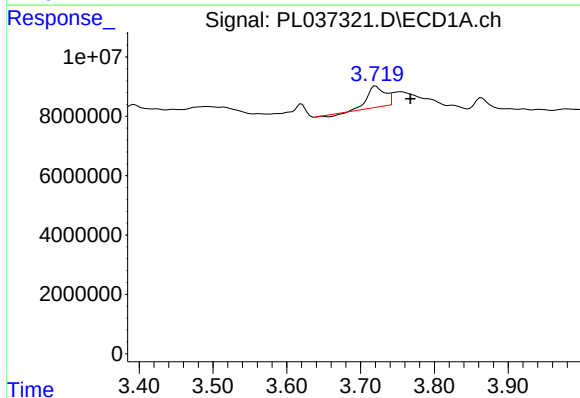


#2 alpha-BHC

R.T.: 3.720 min
Delta R.T.: -0.047 min
Response: 11638550
Conc: 0.95 ng/ml

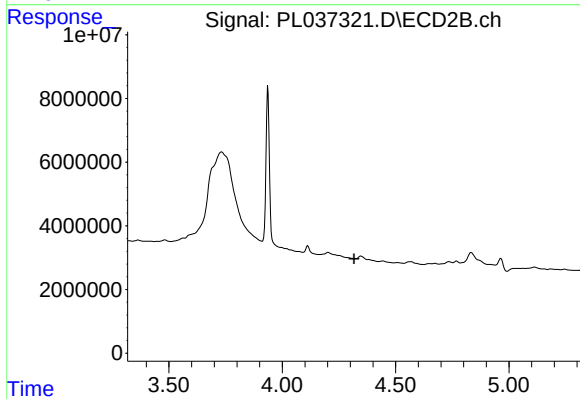

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

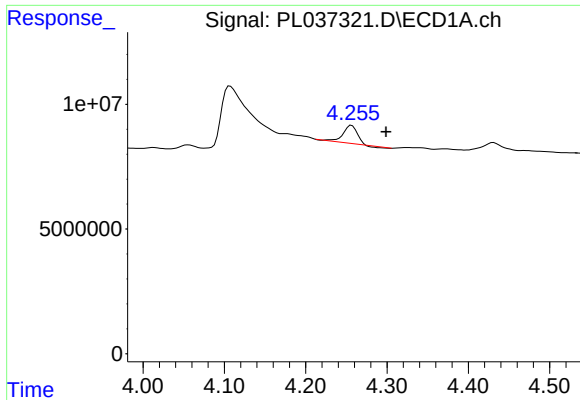

#6 beta-BHC


R.T.: 4.257 min
Delta R.T.: -0.042 min
Response: 8407036
Conc: 1.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

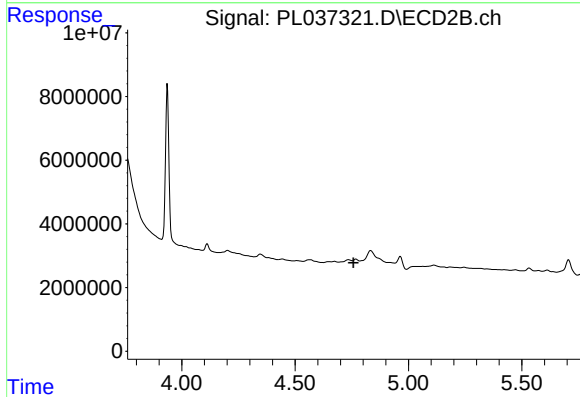


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

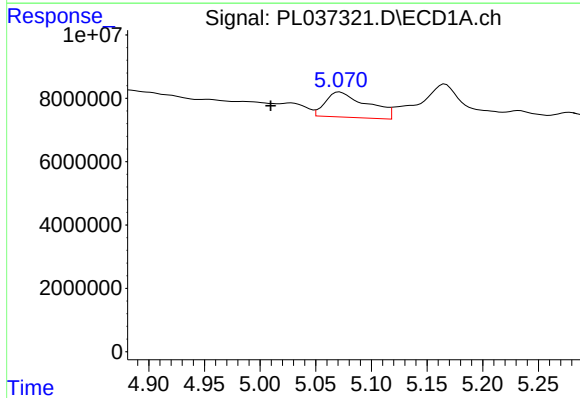


#8 Heptachlor epoxide

R.T.: 5.072 min
Delta R.T.: 0.062 min
Response: 20704573
Conc: 2.21 ng/ml

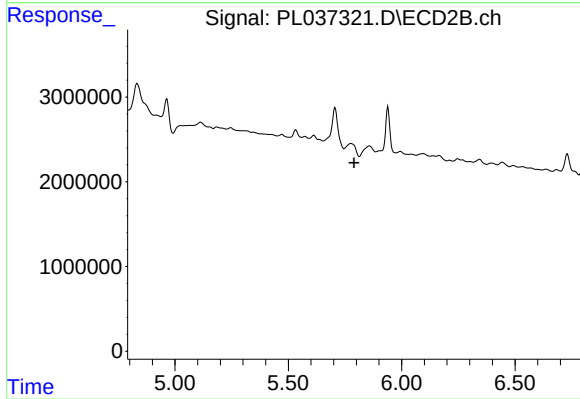

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

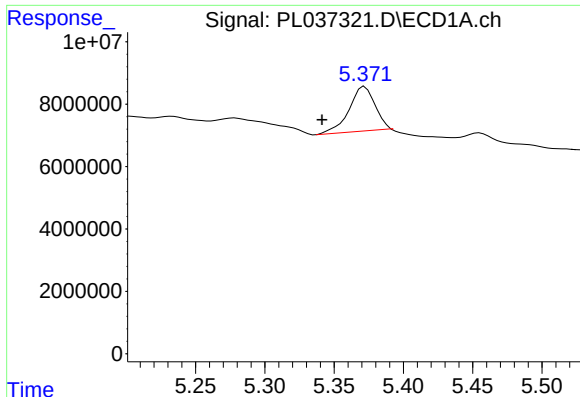

#9 Endosulfan I


R.T.: 5.372 min
Delta R.T.: 0.031 min
Response: 17878834
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

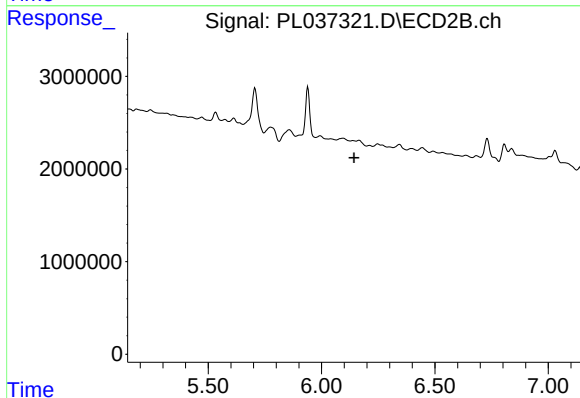


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.144 min
Response: 0
Conc: N.D.

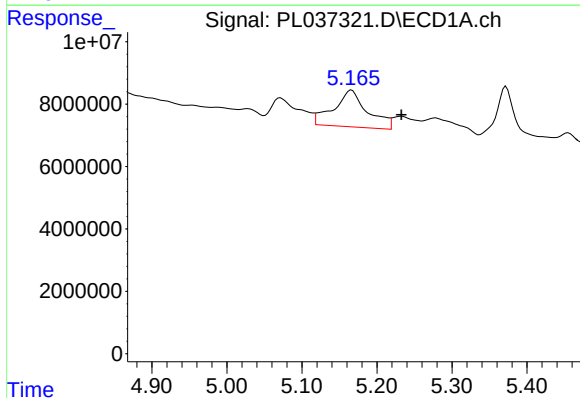


#10 gamma-Chlordane

R.T.: 5.166 min
Delta R.T.: -0.066 min
Response: 36748060
Conc: 3.92 ng/ml

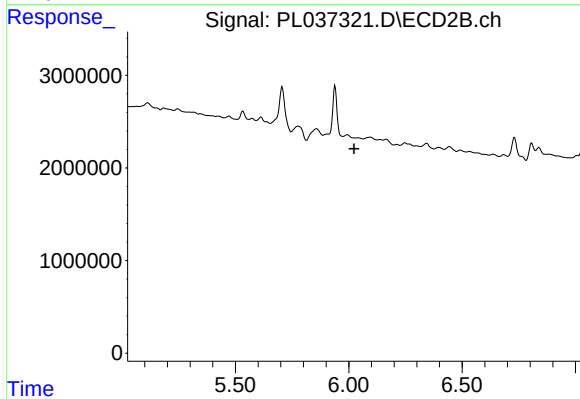

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

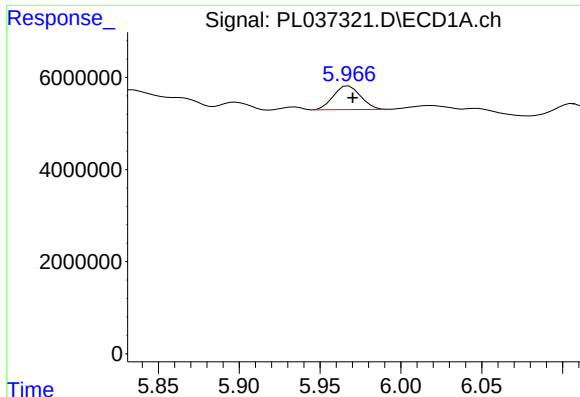

#16 4,4'-DDD


R.T.: 5.968 min
Delta R.T.: -0.002 min
Response: 6018051
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

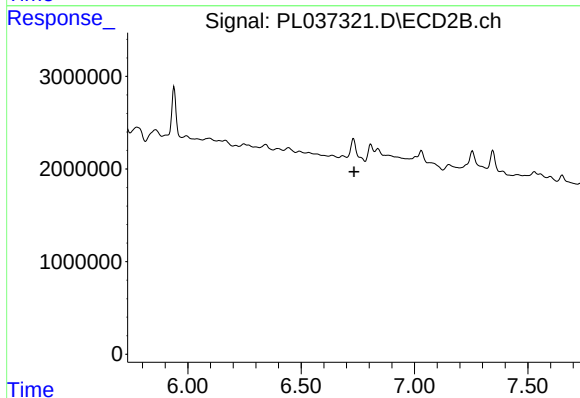


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

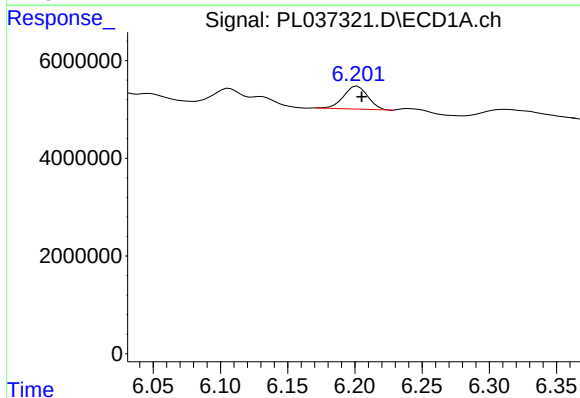


#17 4,4'-DDT

R.T.: 6.202 min
Delta R.T.: -0.003 min
Response: 5889460
Conc: 0.91 ng/ml

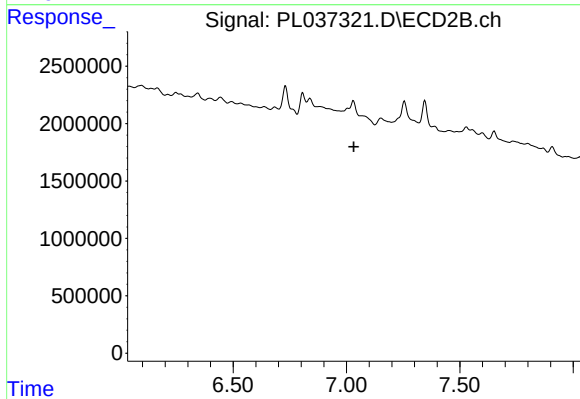

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

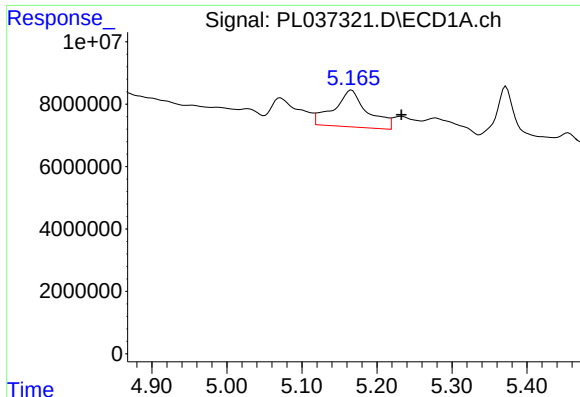

#25 Chlordane-3


R.T.: 5.166 min
Delta R.T.: -0.066 min
Response: 36748060
Conc: 34.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

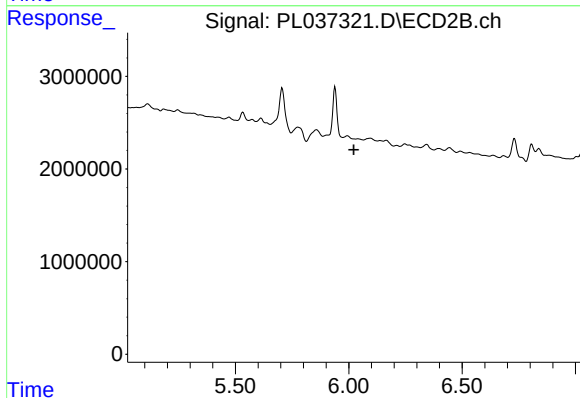


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

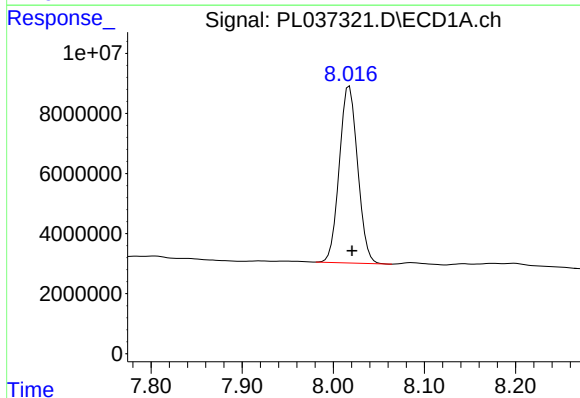

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 82323572
Conc: 13.64 ng/ml

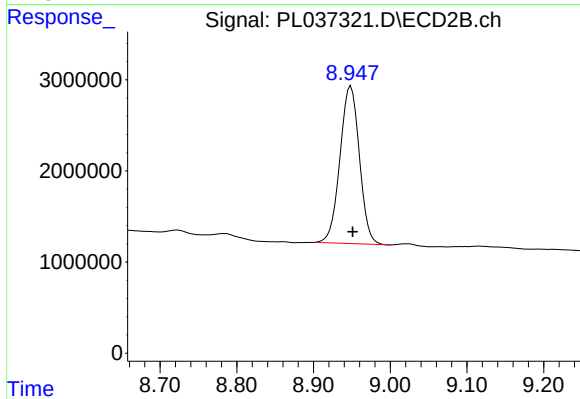

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 30446457
Conc: 15.35 ng/ml