

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 18:55
 Operator : UA\AJ
 Sample : J3665-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:20:25 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	135.8E6	49973587	17.169	18.062
28)	SA Decachlor...	8.018	8.949	69614299	26393900	11.537	13.304
Target Compounds							
6)	B beta-BHC	4.258f	0.000	11452190	0	2.511	N.D. #
8)	B Heptachlo...	5.070f	0.000	17949453	0	1.916	N.D. #
10)	B gamma-Chl...	5.167f	0.000	20196364	0	2.156	N.D. #
25)	Chlordane-3	5.167	0.000	20196364	0	19.001	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 18:55
Operator : UA\AJ
Sample : J3665-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:20:25 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

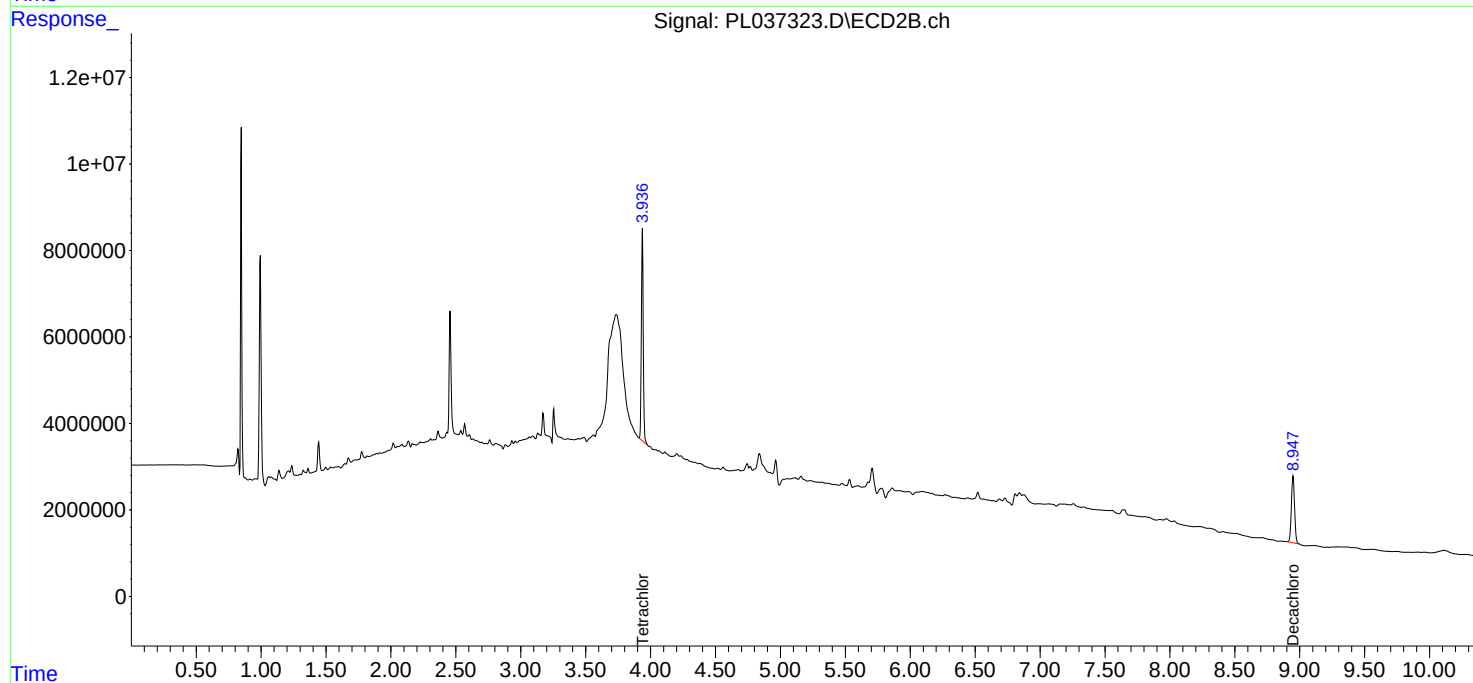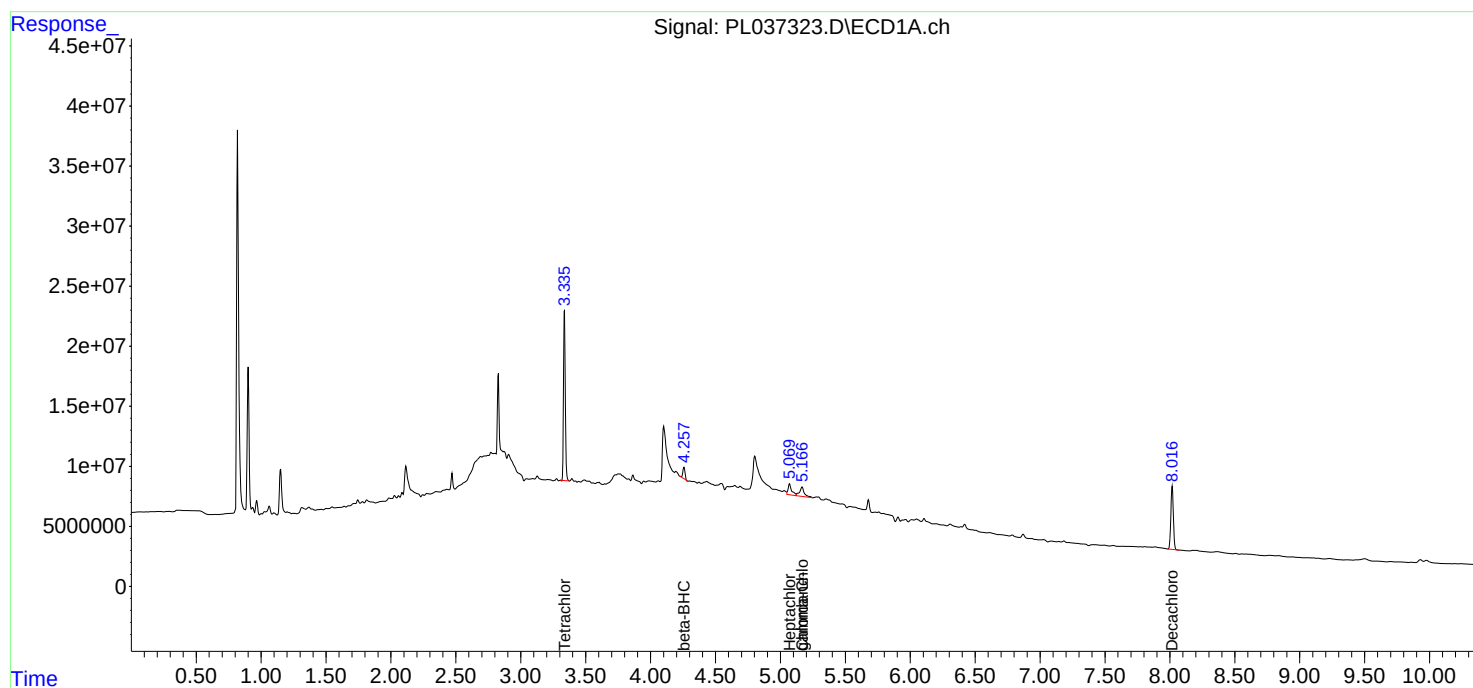


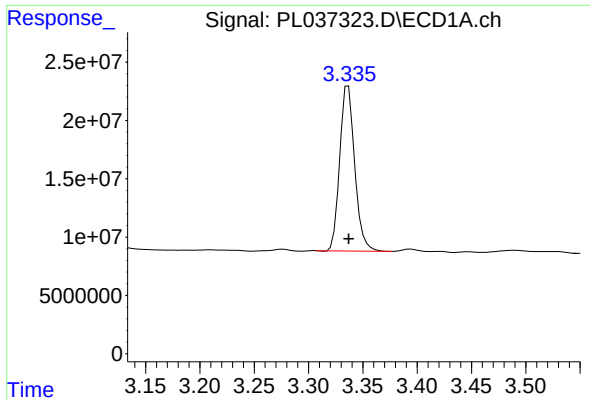

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 135814844
Conc: 17.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

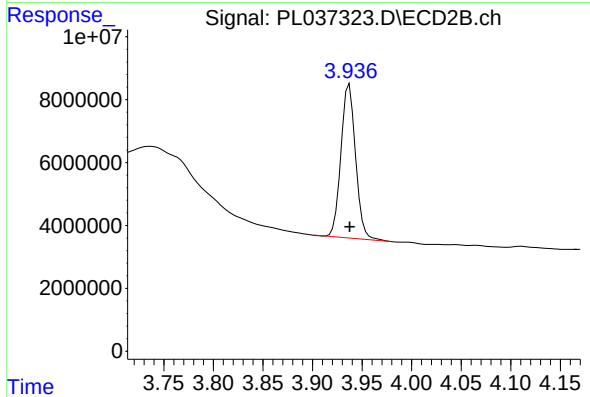


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 49973587
Conc: 18.06 ng/ml

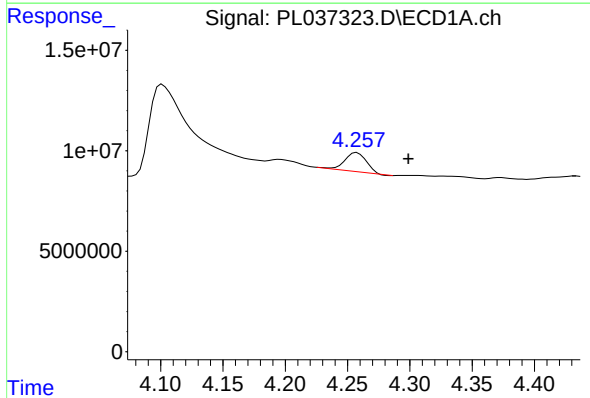


#6 beta-BHC

R.T.: 4.258 min
Delta R.T.: -0.041 min
Response: 11452190
Conc: 2.51 ng/ml

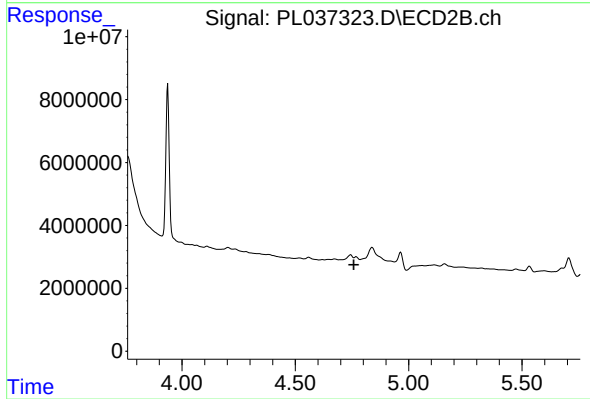

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

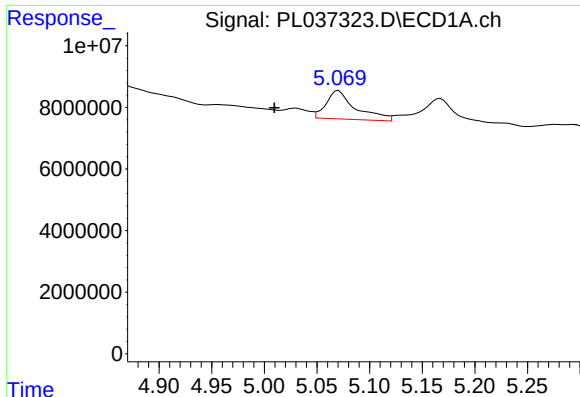

#8 Heptachlor epoxide


R.T.: 5.070 min
Delta R.T.: 0.061 min
Response: 17949453
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

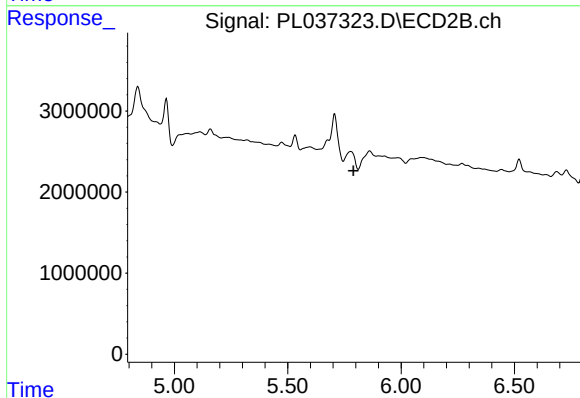


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

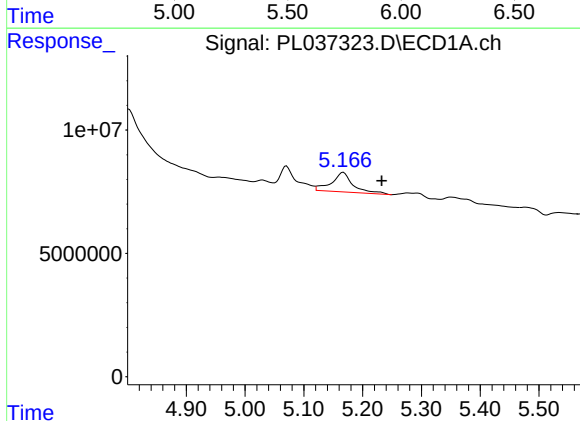


#10 gamma-Chlordane

R.T.: 5.167 min
Delta R.T.: -0.065 min
Response: 20196364
Conc: 2.16 ng/ml

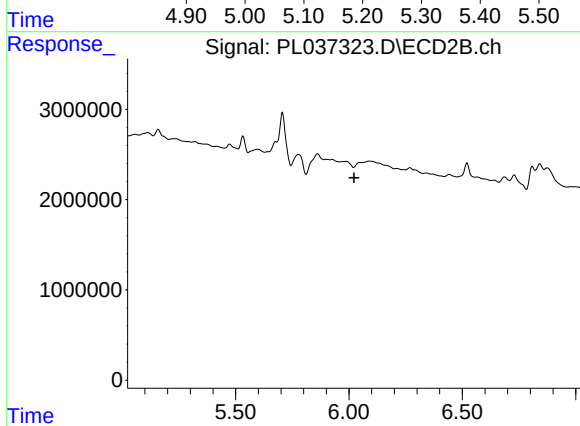

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

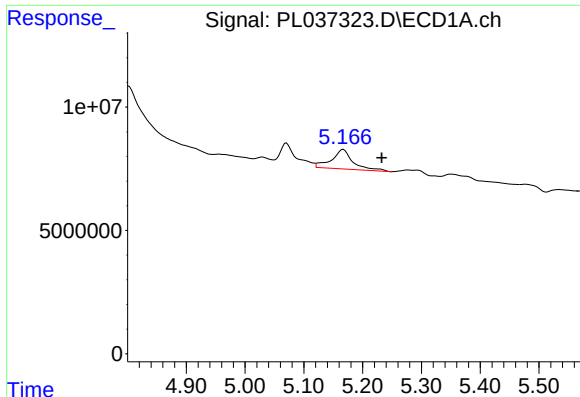

#25 Chlordane-3


R.T.: 5.167 min
Delta R.T.: -0.065 min
Response: 20196364
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

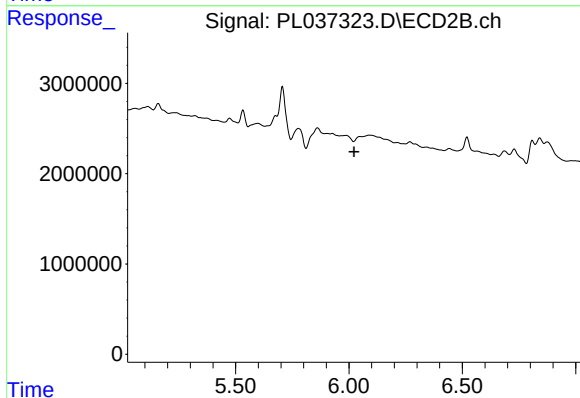


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

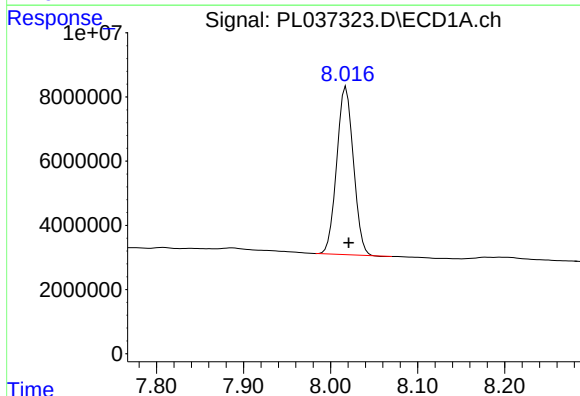

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 69614299
Conc: 11.54 ng/ml

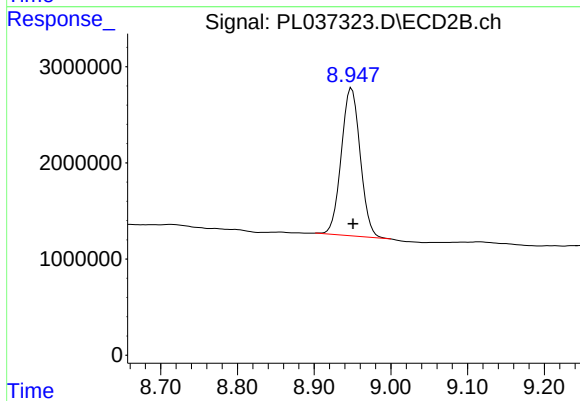

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 26393900
Conc: 13.30 ng/ml