

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 15:37
 Operator : UA\AJ
 Sample : J3642-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-1

Manual Integrations
 APPROVED

ugo
 6/25/2018 1:41:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:15:30 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.935	77514410	25187608	9.799	9.104m
28)	SA Decachlor...	8.017	8.948	47647848	19152751	7.897	9.654
Target Compounds							
12)	B 4,4'-DDE	5.455	6.248	46456747	18580176	5.260m	7.302m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 15:37
Operator : UA\AJ
Sample : J3642-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TEST-PIT-1


Manual Integrations
APPROVED

ugo
6/25/2018 1:41:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:15:30 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

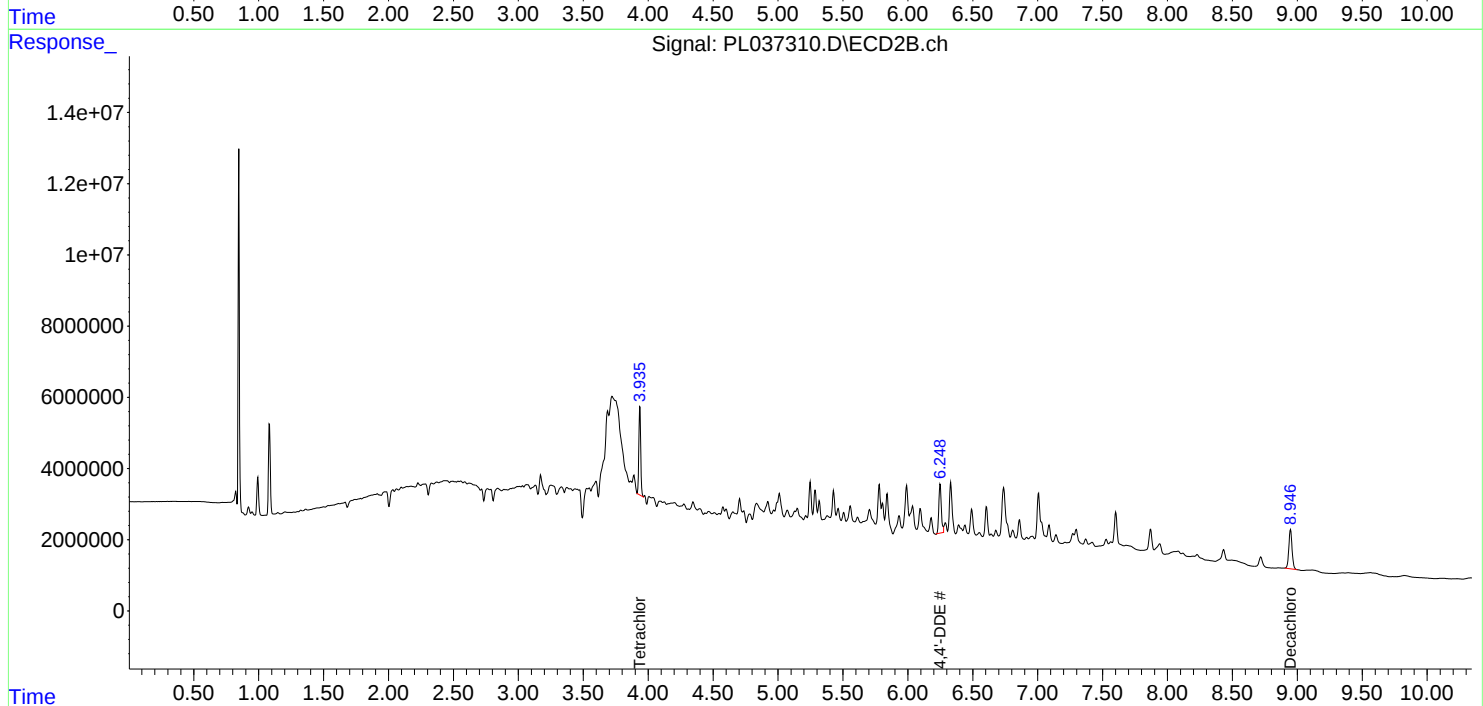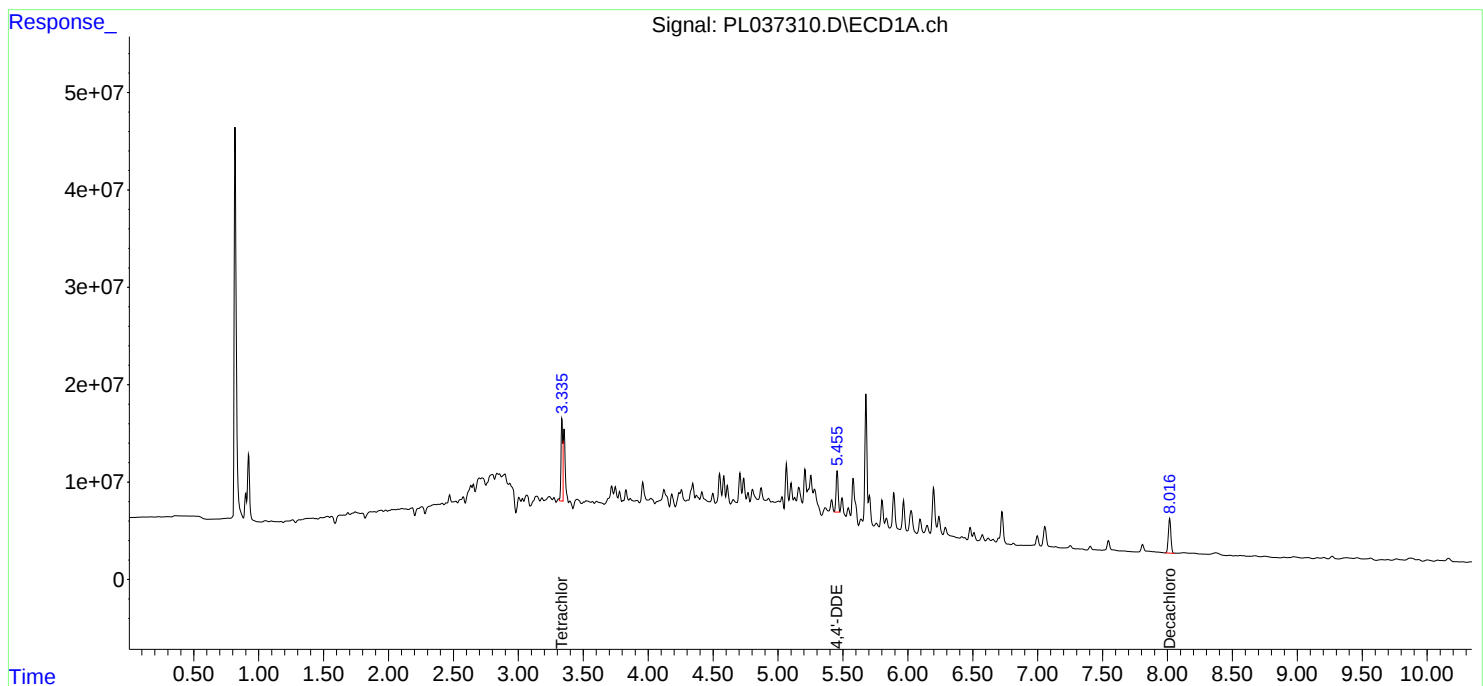

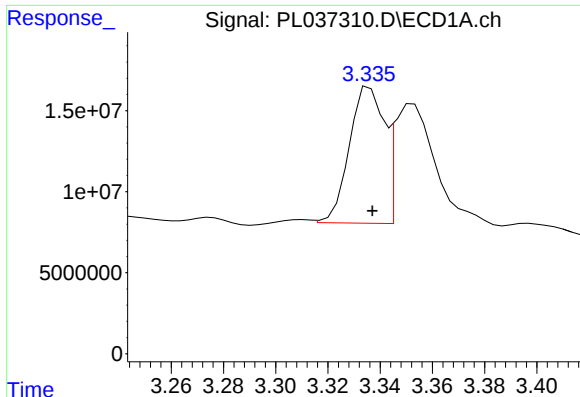


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 77514410
Conc: 9.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1


Manual Integrations
APPROVED

ugo
6/25/2018 1:41:55 PM

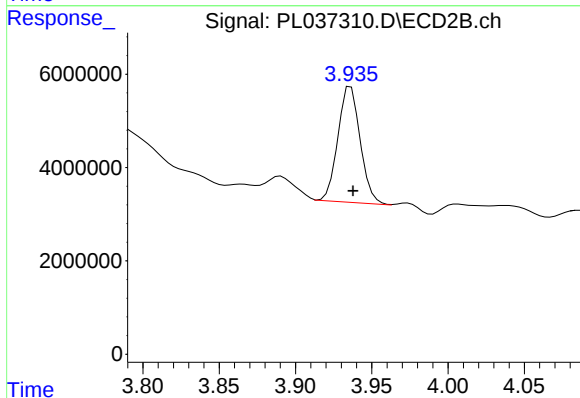


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 25187608
Conc: 9.10 ng/ml m

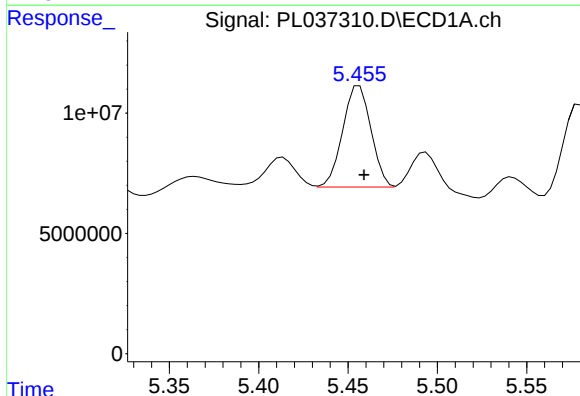


#12 4,4'-DDE

R.T.: 5.455 min
Delta R.T.: -0.004 min
Response: 46456747
Conc: 5.26 ng/ml m

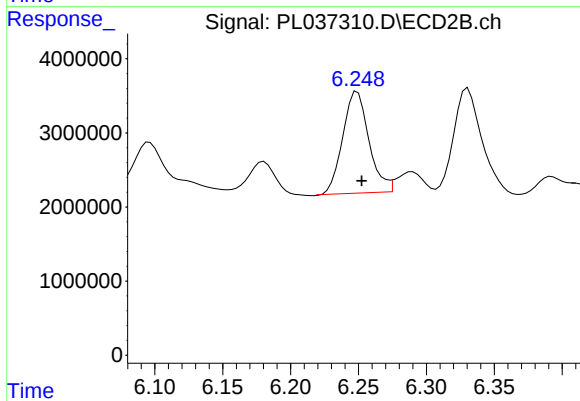

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.005 min
Response: 18580176
Conc: 7.30 ng/ml m

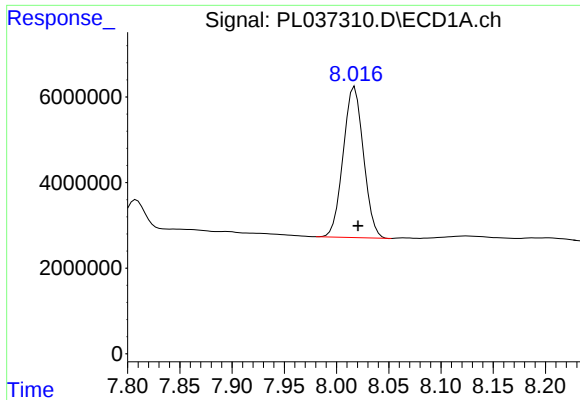


#28 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.003 min
Response: 47647848
Conc: 7.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

Manual Integrations
APPROVED

ugo
6/25/2018 1:41:55 PM

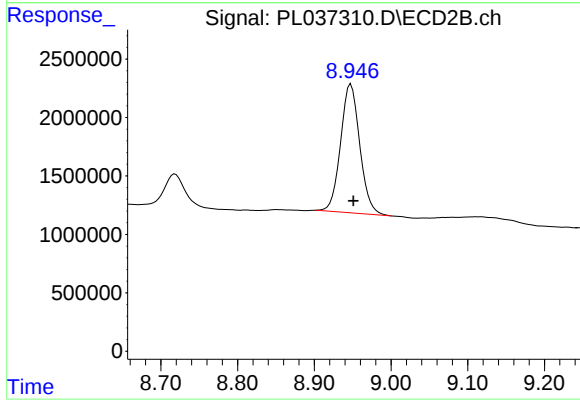

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 19152751
Conc: 9.65 ng/ml