

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 18:41
 Operator : UA\AJ
 Sample : J3622-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-D

Manual Integrations
 APPROVED

ugo
 6/25/2018 1:42:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:20:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	152.2E6	54598422	19.245	19.734
28)	SA Decachlor...	8.018	8.948	97748802	37074391	16.200	18.687
Target Compounds							
16)	A 4,4'-DDD	5.967	6.729	6990006	3979866	1.064m	1.939m#
17)	MA 4,4'-DDT	6.200	7.029	5586993	1395301	0.865m	0.659m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 18:41
Operator : UA\AJ
Sample : J3622-16
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-D


Manual Integrations
APPROVED

ugo
6/25/2018 1:42:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:20:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

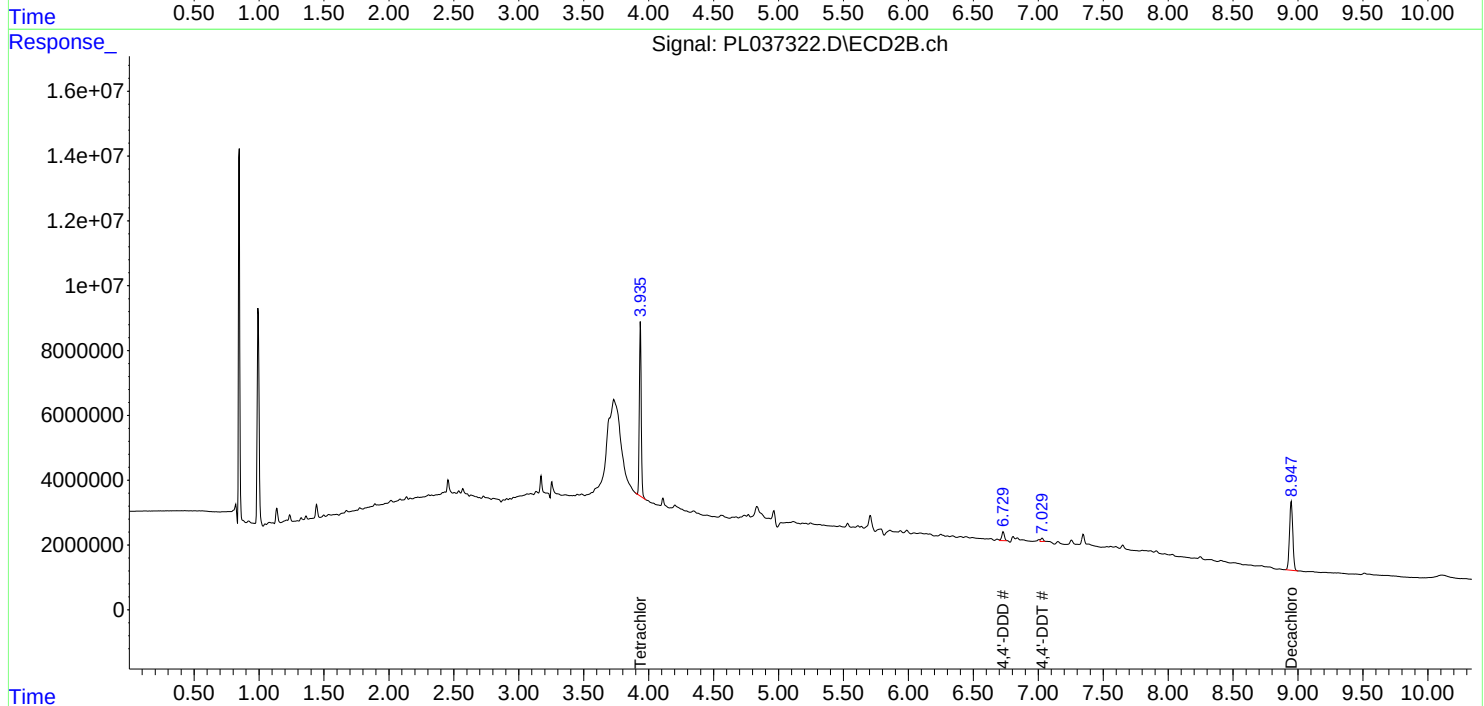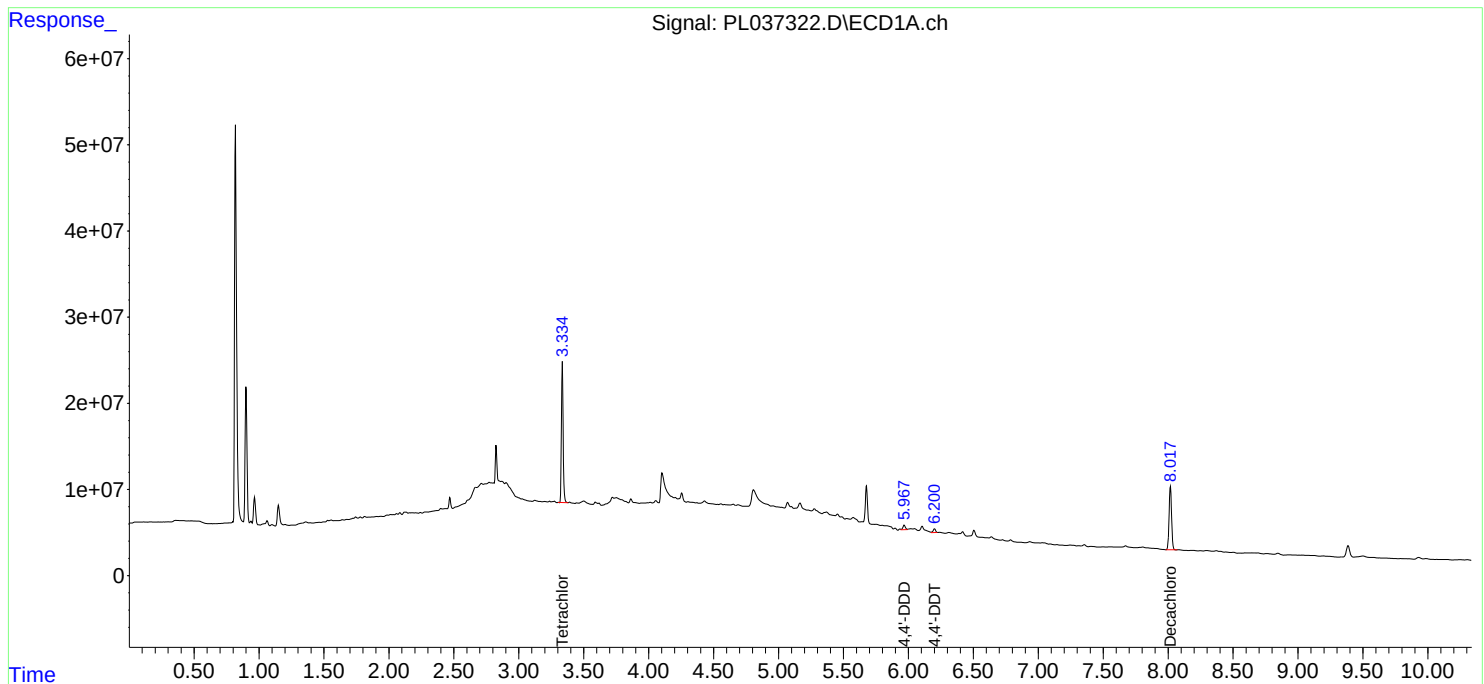

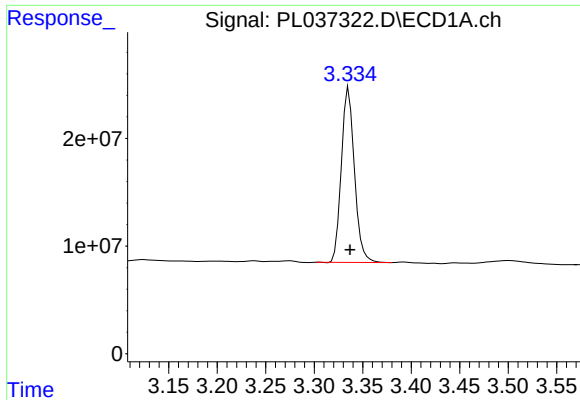


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 152231236
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-D


Manual Integrations
APPROVED

ugo
6/25/2018 1:42:04 PM

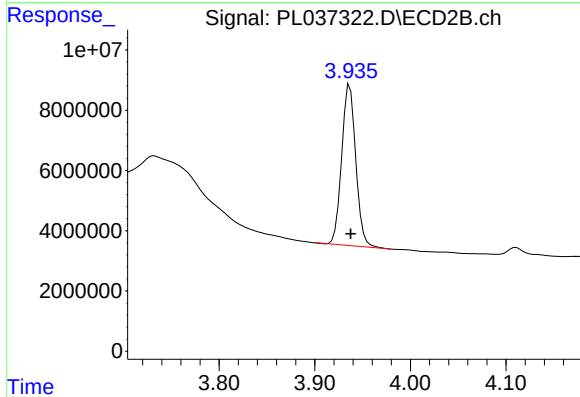


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 54598422
Conc: 19.73 ng/ml

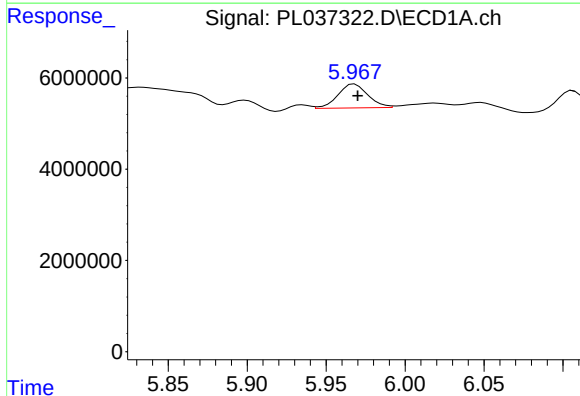


#16 4,4'-DDD

R.T.: 5.967 min
Delta R.T.: -0.004 min
Response: 6990006
Conc: 1.06 ng/ml m

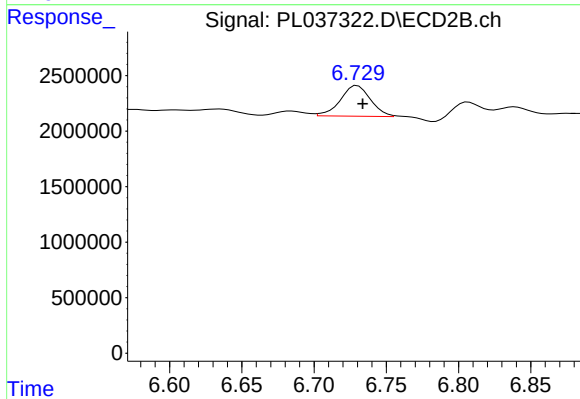

#16 4,4'-DDD

R.T.: 6.729 min
Delta R.T.: -0.005 min
Response: 3979866
Conc: 1.94 ng/ml m

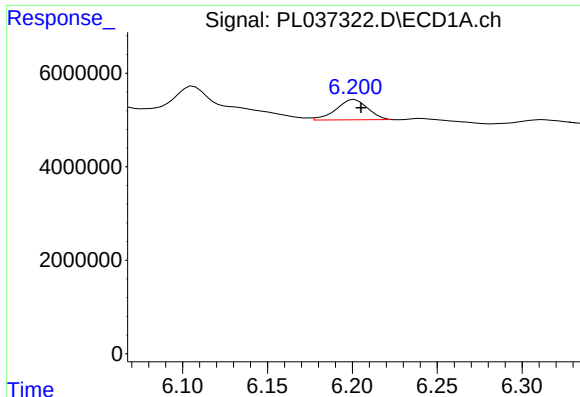


#17 4,4'-DDT

R.T.: 6.200 min
Delta R.T.: -0.005 min
Response: 5586993
Conc: 0.87 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP-D


Manual Integrations
APPROVED

ugo
6/25/2018 1:42:04 PM

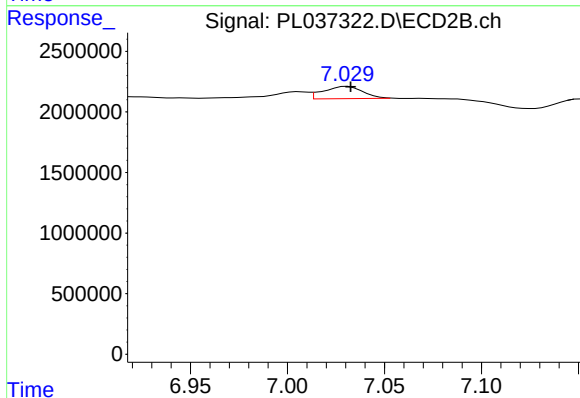


#17 4,4'-DDT

R.T.: 7.029 min
Delta R.T.: -0.003 min
Response: 1395301
Conc: 0.66 ng/ml m

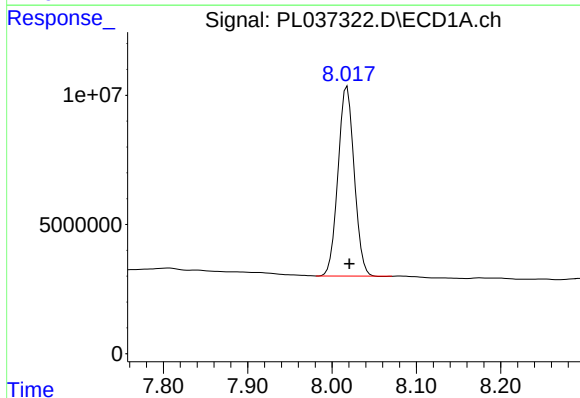

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 97748802
Conc: 16.20 ng/ml

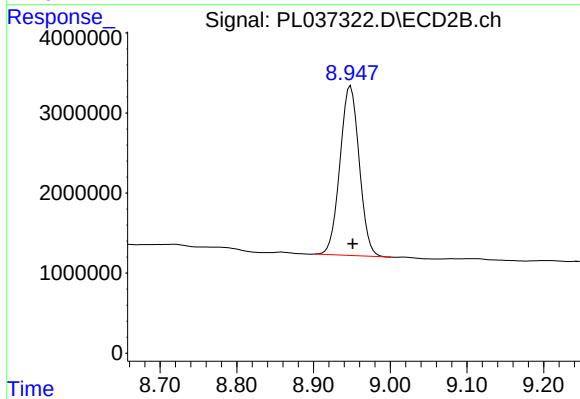

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 37074391
Conc: 18.69 ng/ml