

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
 Data File : PL037324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 19:09
 Operator : UA\AJ
 Sample : J3622-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-A

Manual Integrations
 APPROVED

ugo
 6/25/2018 1:42:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:20:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	137.3E6	49544353	17.358	17.907
28)	SA Decachlor...	8.018	8.949	75460624	27115873	12.506	13.668
Target Compounds							
16)	A 4,4'-DDD	5.967	6.731	4267315	1317010	0.650m	0.642m
17)	MA 4,4'-DDT	6.200	7.029	5814670	1390943	0.901m	0.657m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062218\
Data File : PL037324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 19:09
Operator : UA\AJ
Sample : J3622-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-A


Manual Integrations
APPROVED

ugo
6/25/2018 1:42:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:20:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

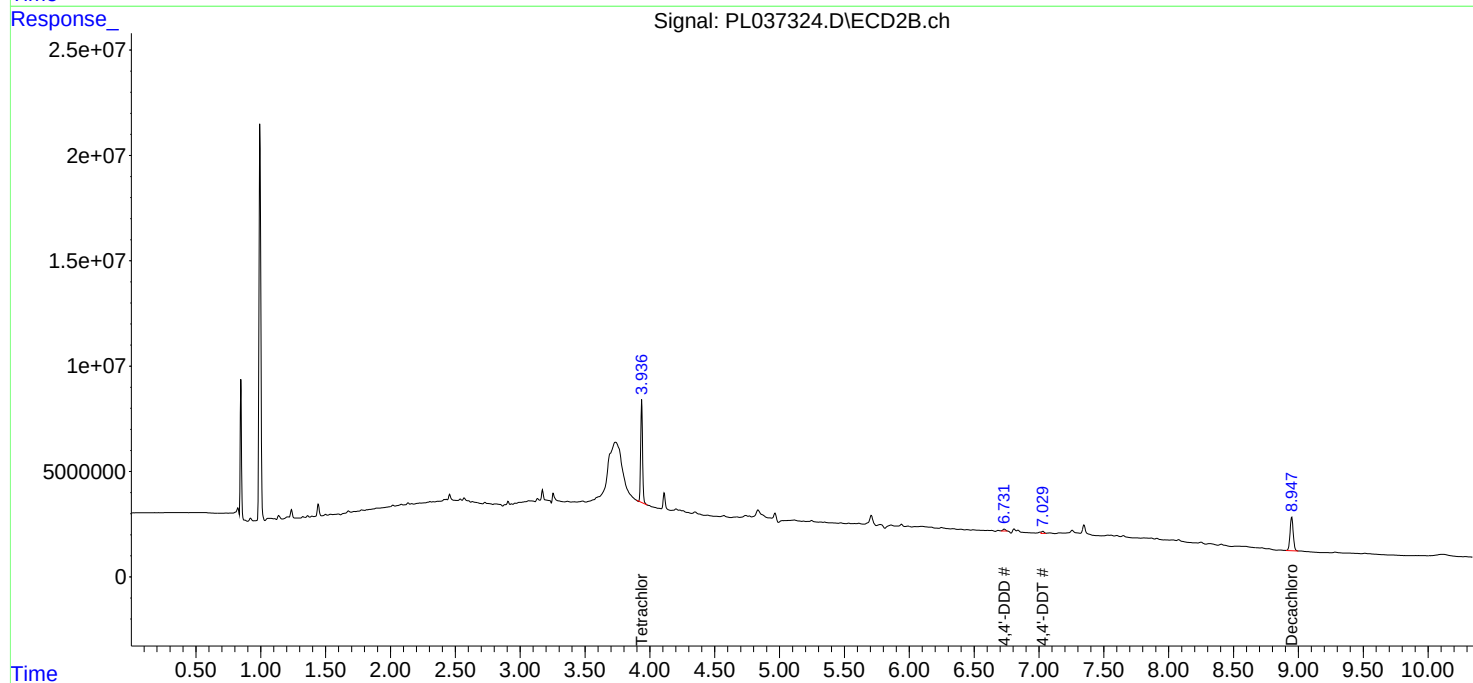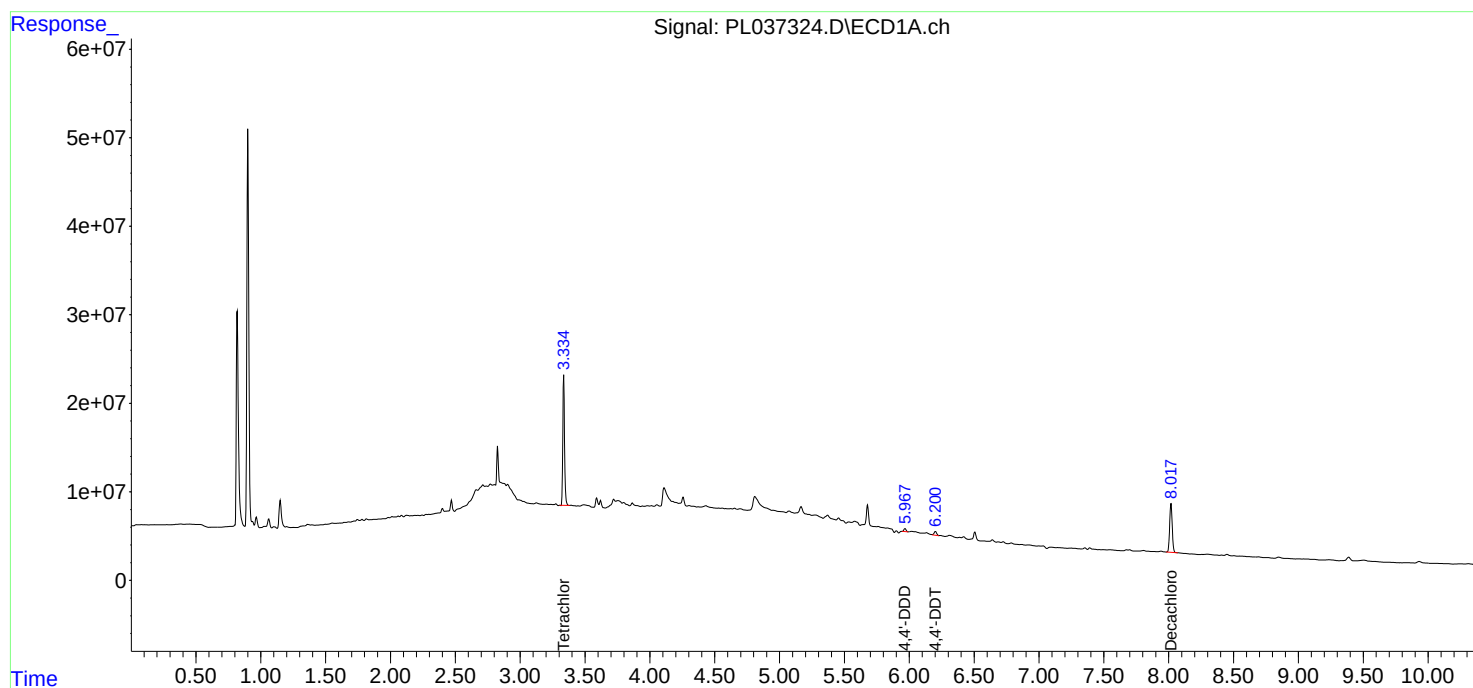

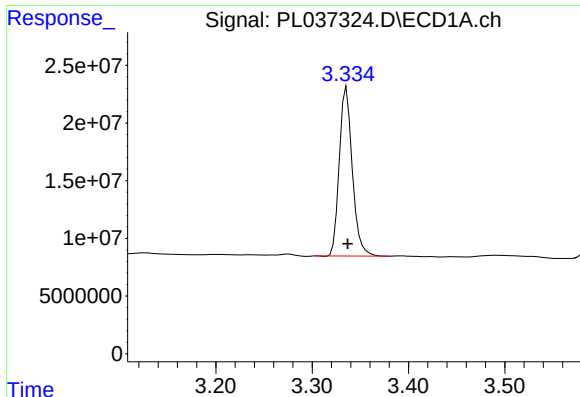


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 137310258
Conc: 17.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-A


Manual Integrations
APPROVED

ugo
6/25/2018 1:42:06 PM

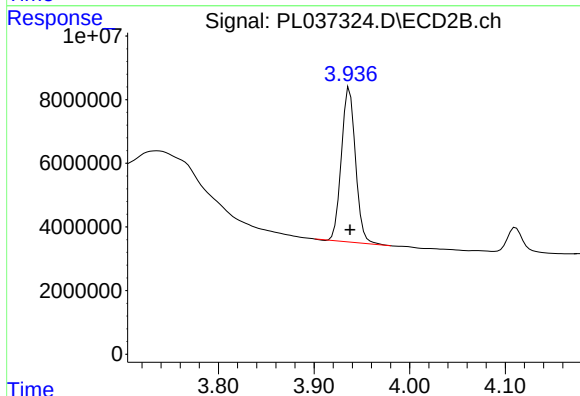


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 49544353
Conc: 17.91 ng/ml

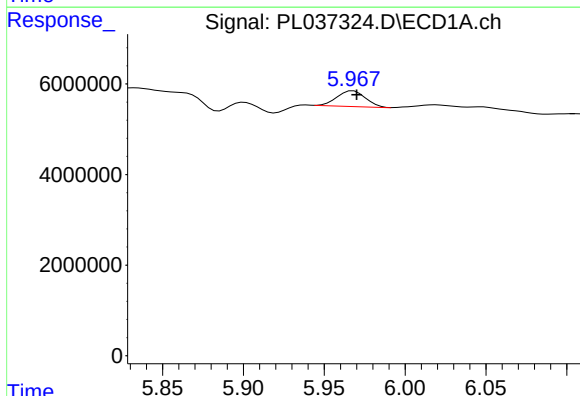


#16 4,4'-DDD

R.T.: 5.967 min
Delta R.T.: -0.004 min
Response: 4267315
Conc: 0.65 ng/ml m

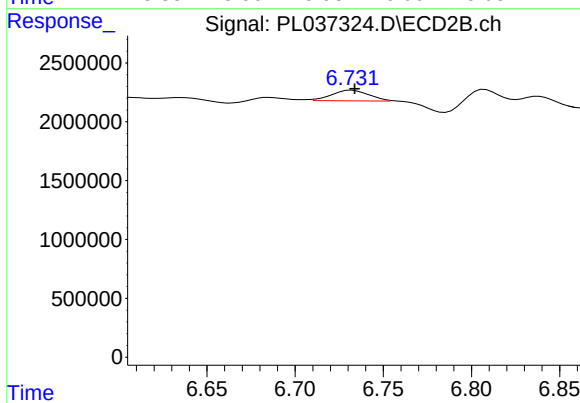

#16 4,4'-DDD

R.T.: 6.731 min
Delta R.T.: -0.003 min
Response: 1317010
Conc: 0.64 ng/ml m

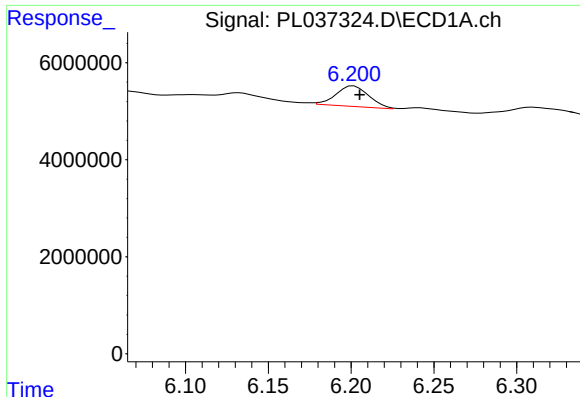


#17 4,4'-DDT

R.T.: 6.200 min
Delta R.T.: -0.005 min
Response: 5814670
Conc: 0.90 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP-A


Manual Integrations
APPROVED

ugo
6/25/2018 1:42:06 PM

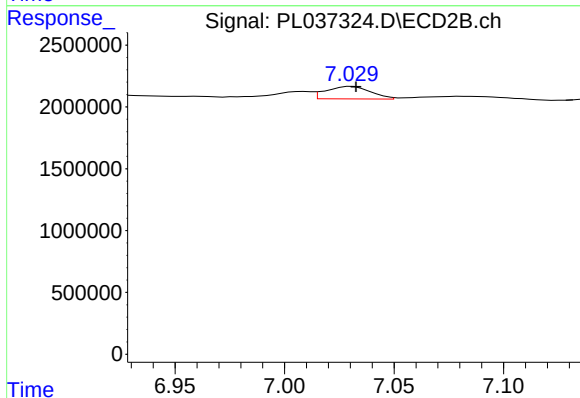


#17 4,4'-DDT

R.T.: 7.029 min
Delta R.T.: -0.003 min
Response: 1390943
Conc: 0.66 ng/ml m

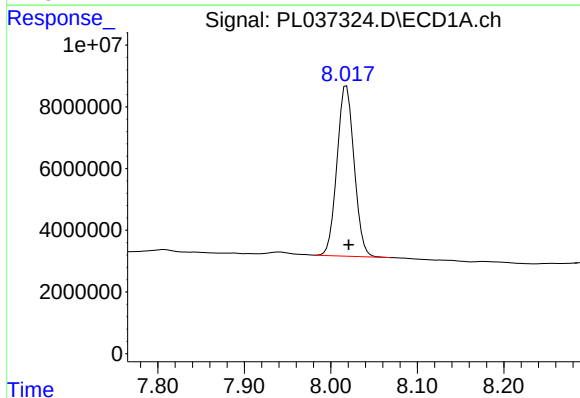

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 75460624
Conc: 12.51 ng/ml

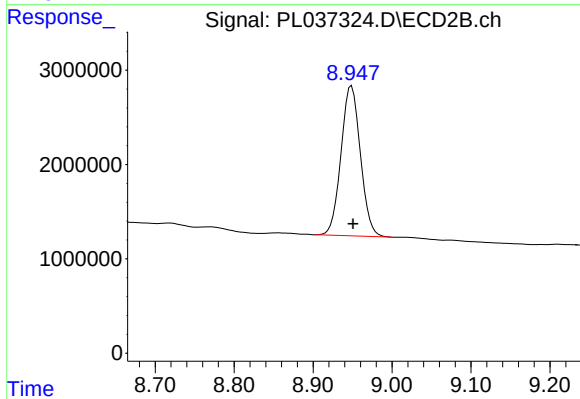

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 27115873
Conc: 13.67 ng/ml