

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 14:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:27:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.531	10641718	18837771	19.356	19.982
28)	SA Decachlor...	10.223	11.431	13895494	20597349	19.607	20.679
Target Compounds							
4)	MA Heptachlor	5.990f	0.000	484515	0	0.642	N.D. #
6)	B beta-BHC	5.990	0.000	484515	0	1.354	N.D. #
7)	B delta-BHC	0.000	7.000f	0	1710107	N.D.	1.455 #
15)	B Endosulfa...	0.000	9.181f	0	525894	N.D.	0.660 #
16)	A 4,4'-DDD	8.033f	0.000	226708	0	0.390	N.D. #
24)	Chlordane-2	6.487	0.000	244214	0	9.120	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 14:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:27:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

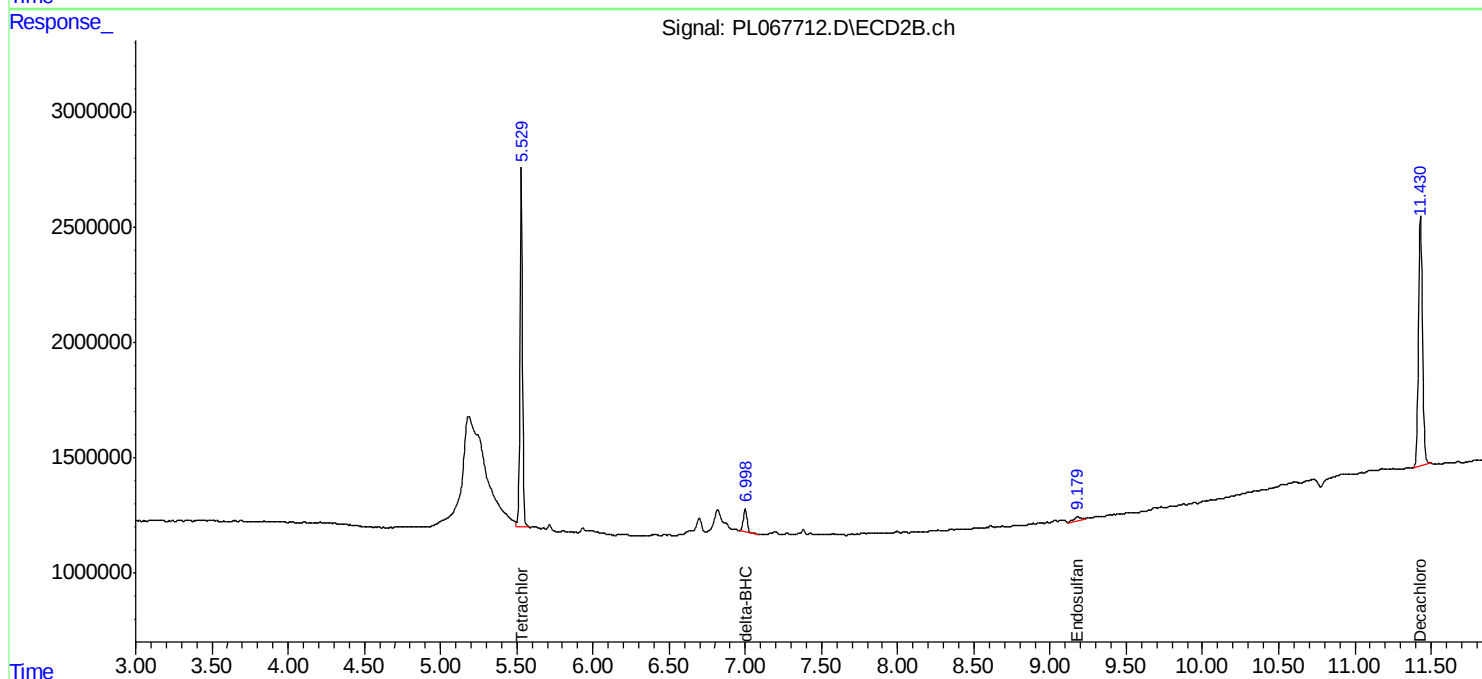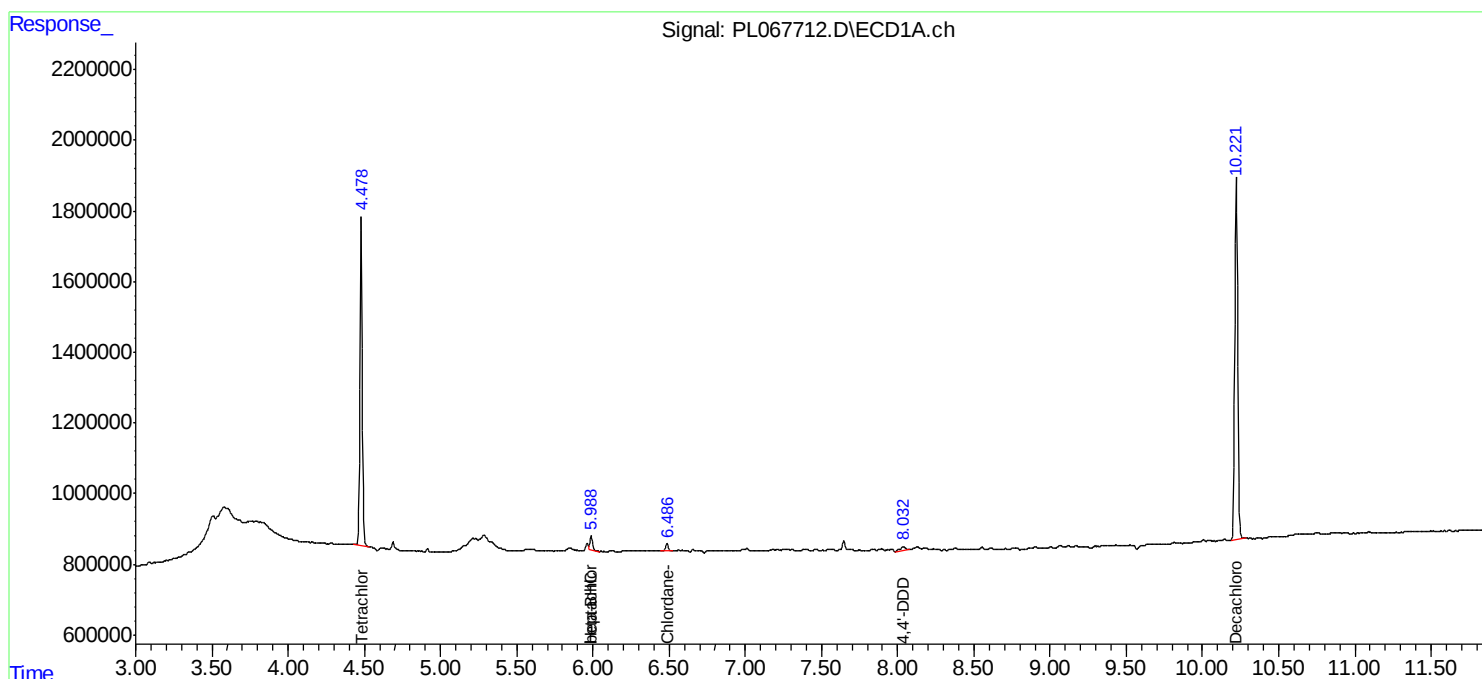


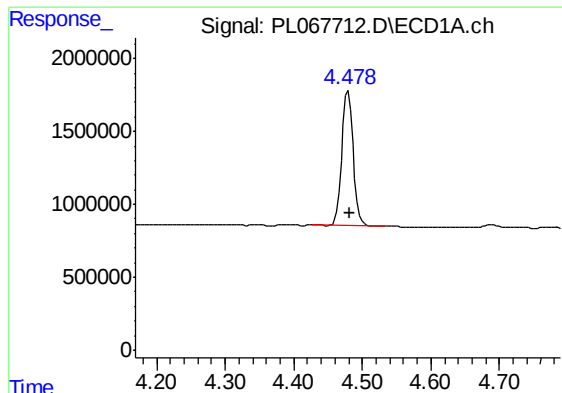

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 10641718
Conc: 19.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

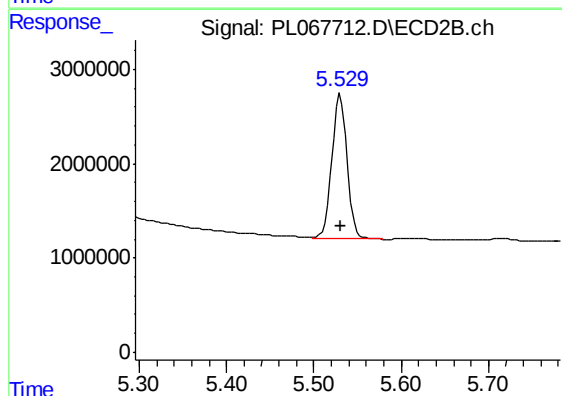


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 18837771
Conc: 19.98 ng/ml

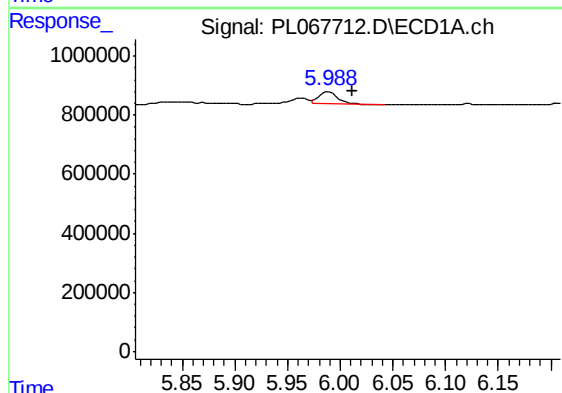


#4 Heptachlor

R.T.: 5.990 min
Delta R.T.: -0.022 min
Response: 484515
Conc: 0.64 ng/ml

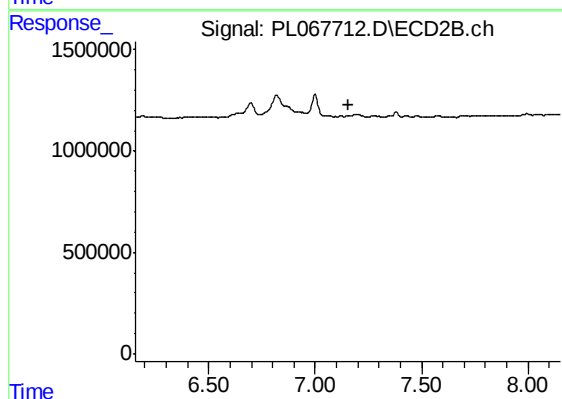

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

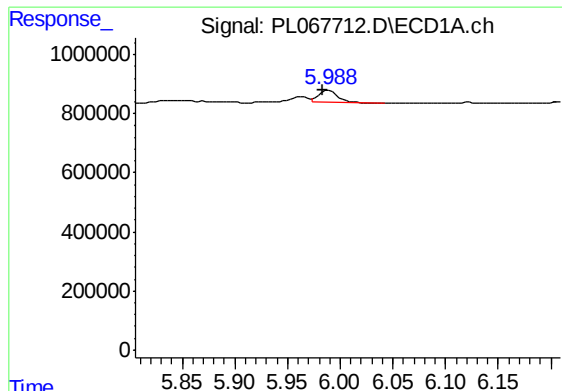

#6 beta-BHC


R.T.: 5.990 min
Delta R.T.: 0.006 min
Response: 484515
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

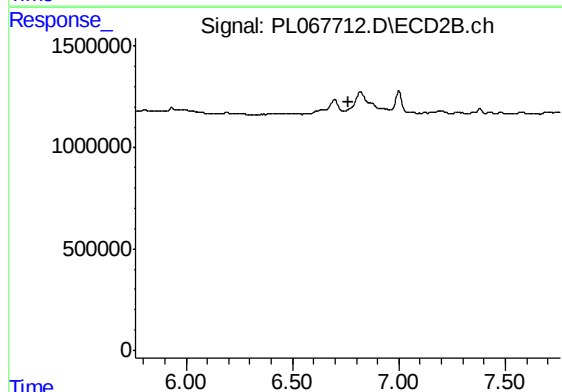


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

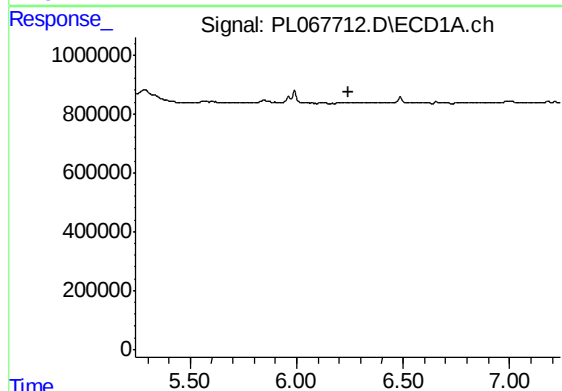


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

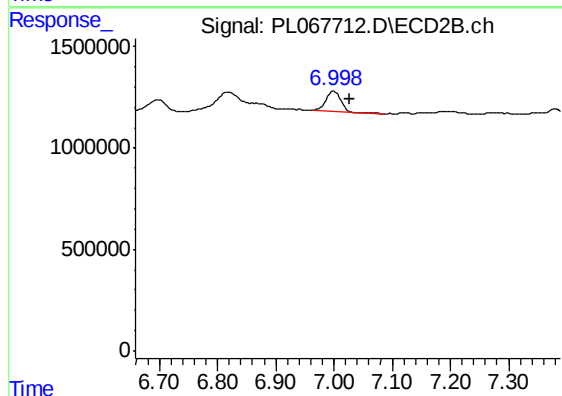

#7 delta-BHC


R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 1710107
Conc: 1.45 ng/ml

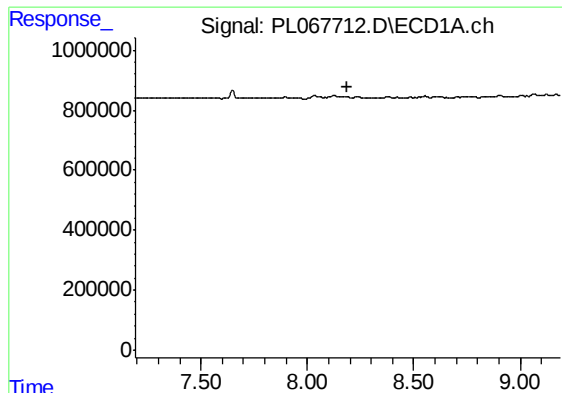

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

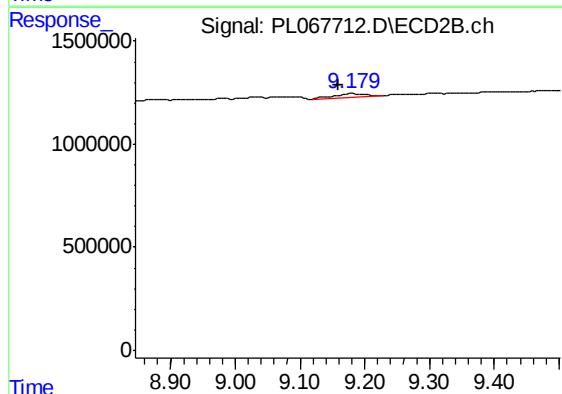


#15 Endosulfan II

R.T.: 9.181 min
Delta R.T.: 0.023 min
Response: 525894
Conc: 0.66 ng/ml

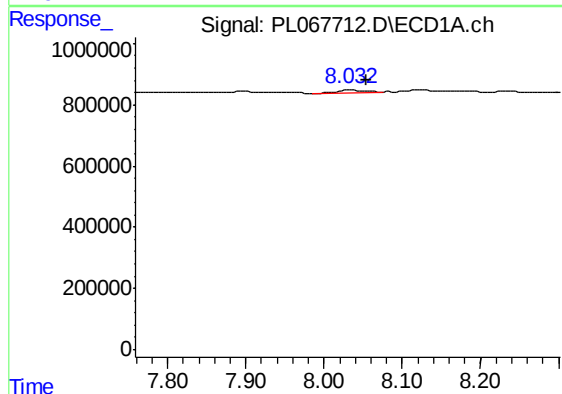


#16 4,4'-DDD

R.T.: 8.033 min
Delta R.T.: -0.022 min
Response: 226708
Conc: 0.39 ng/ml

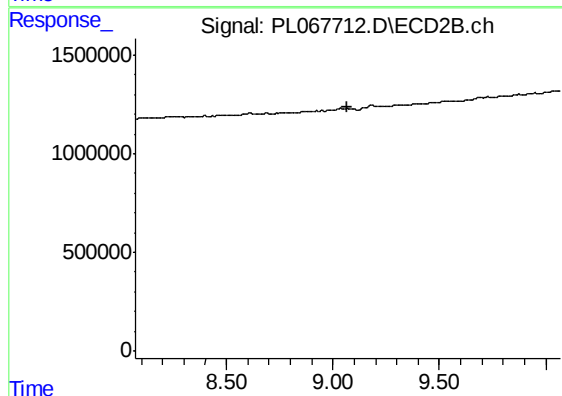

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 9.069 min
Response: 0
Conc: N.D.

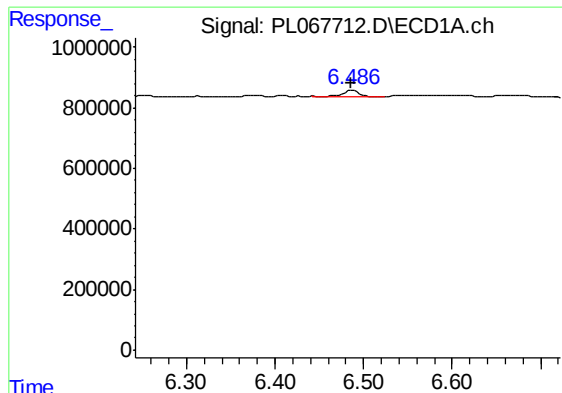

#24 Chlordane-2


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 244214
Conc: 9.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

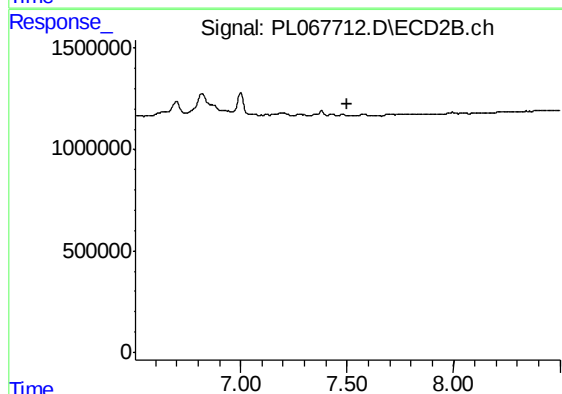


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

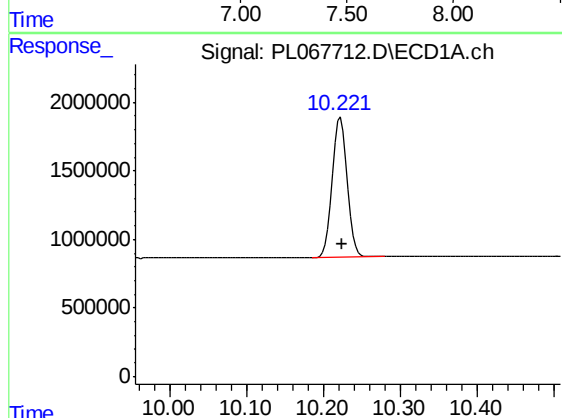

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.002 min
Response: 13895494
Conc: 19.61 ng/ml

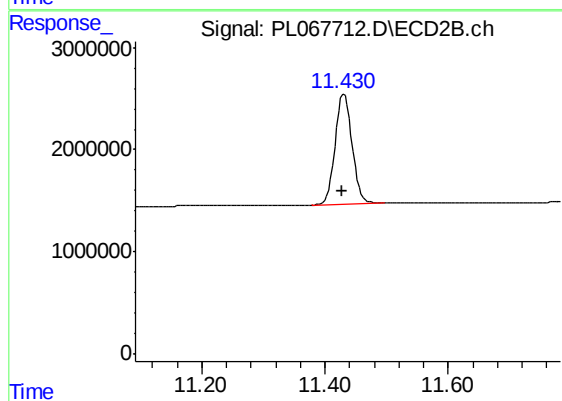

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: 0.002 min
Response: 20597349
Conc: 20.68 ng/ml