

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 19:04
 Operator : AR\AJ
 Sample : M2795-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B2-6-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:35:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.528	7106723	13230986	12.926	14.035
28)	SA Decachlor...	10.219	11.425	8343850	12557601	11.774	12.607
Target Compounds							
6)	B beta-BHC	5.960f	0.000	199100	0	0.556	N.D. #
7)	B delta-BHC	0.000	7.004f	0	886570	N.D.	0.754 #
9)	A Endosulfan I	7.319	0.000	573063	0	0.852	N.D. #
12)	B 4,4'-DDE	7.466	0.000	277330	0	0.417	N.D. #
14)	MA Endrin	7.894f	0.000	198256	0	0.302	N.D. #
15)	B Endosulfa...	0.000	9.177f	0	1392530	N.D.	1.747 #
16)	A 4,4'-DDD	0.000	9.061	0	846504	N.D.	1.190 #
17)	MA 4,4'-DDT	8.307	0.000	206058	0	0.354	N.D. #
23)	Chlordane-1	5.788	0.000	584082	0	31.569	N.D. #
27)	Chlordane-5	0.000	9.213	0	259211	N.D.	8.914 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 19:04
Operator : AR\AJ
Sample : M2795-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
B2-6-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:35:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

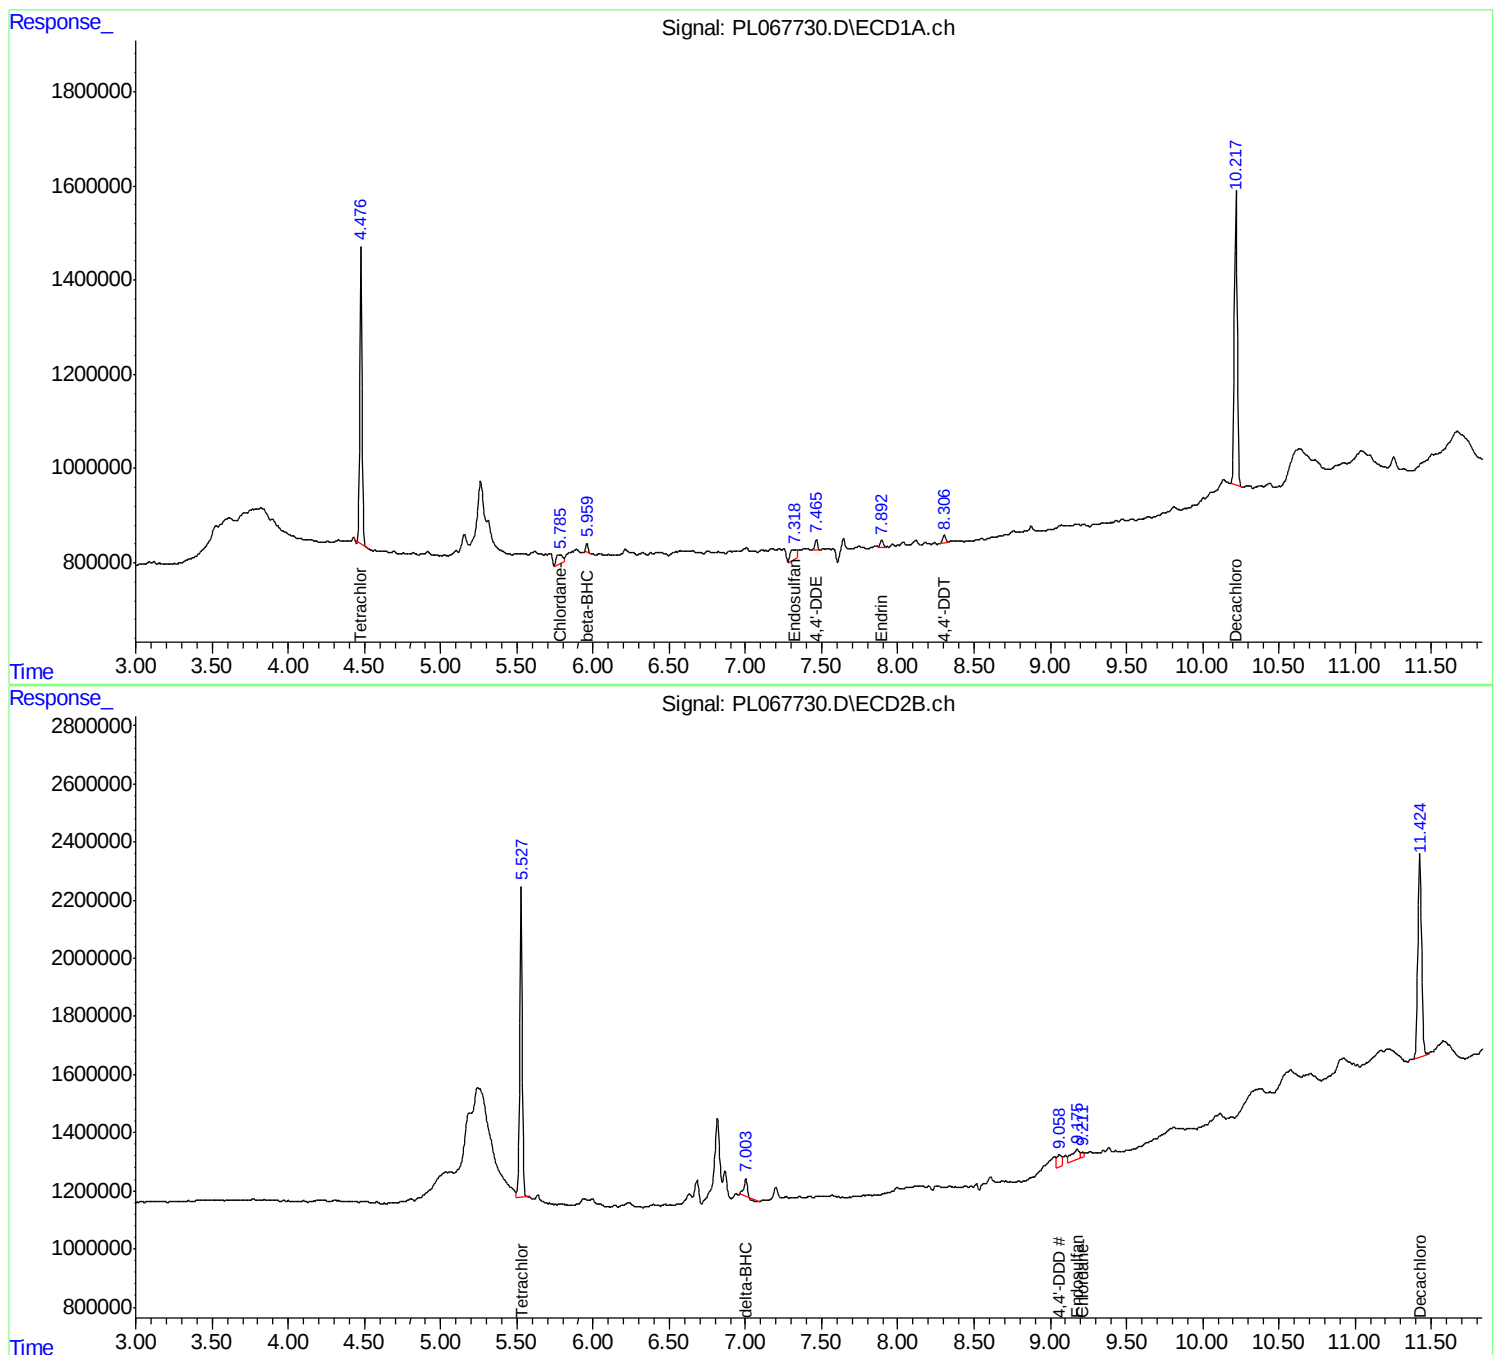


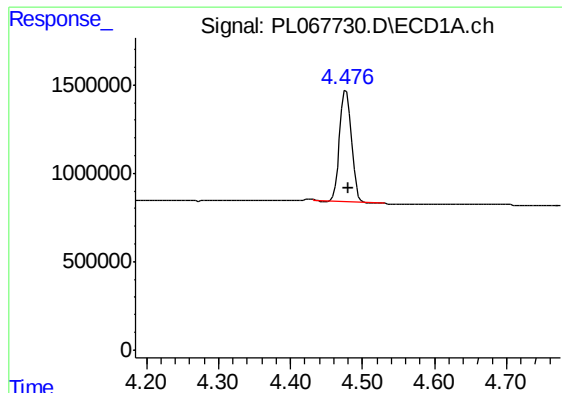

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 7106723
Conc: 12.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
B2-6-8

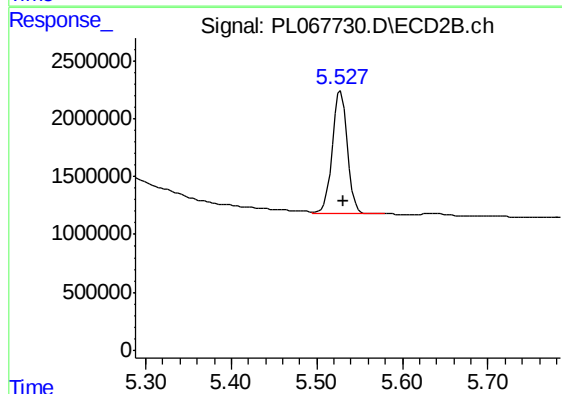


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 13230986
Conc: 14.03 ng/ml

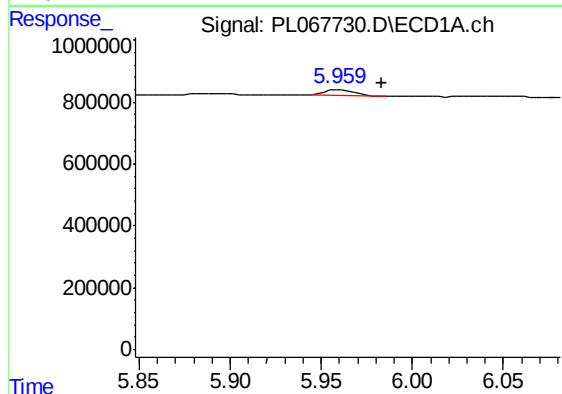


#6 beta-BHC

R.T.: 5.960 min
Delta R.T.: -0.023 min
Response: 199100
Conc: 0.56 ng/ml

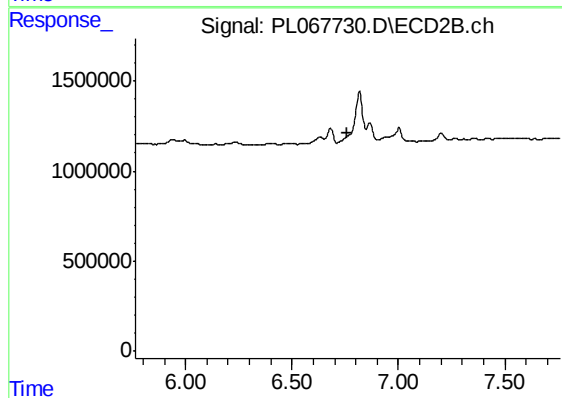

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

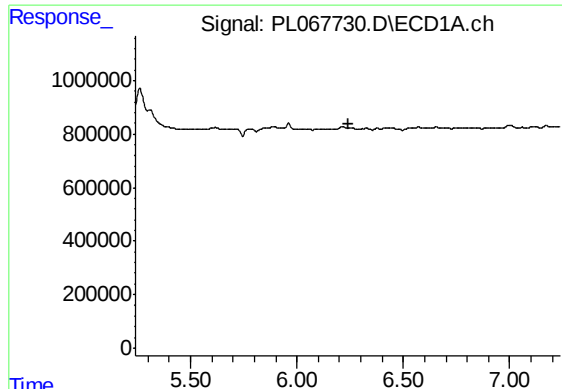

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B2-6-8

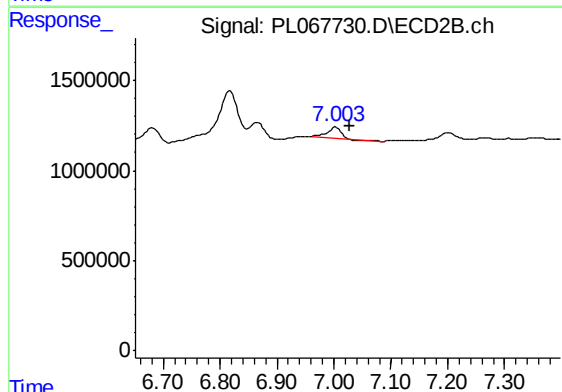


#7 delta-BHC

R.T.: 7.004 min
Delta R.T.: -0.024 min
Response: 886570
Conc: 0.75 ng/ml

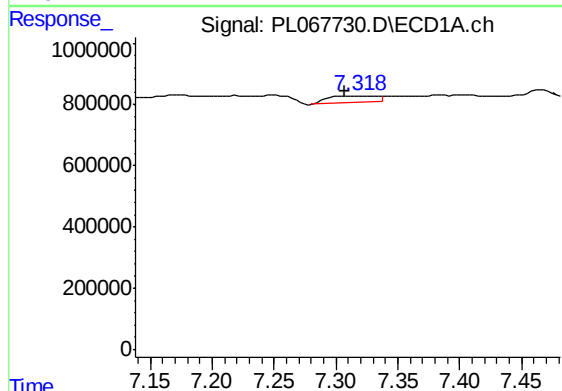


#9 Endosulfan I

R.T.: 7.319 min
Delta R.T.: 0.013 min
Response: 573063
Conc: 0.85 ng/ml

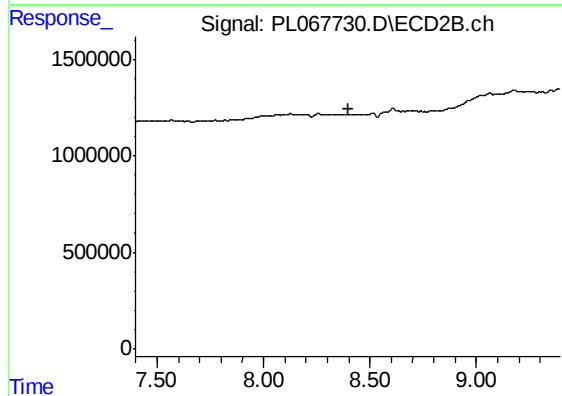

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 8.397 min
Response: 0
Conc: N.D.

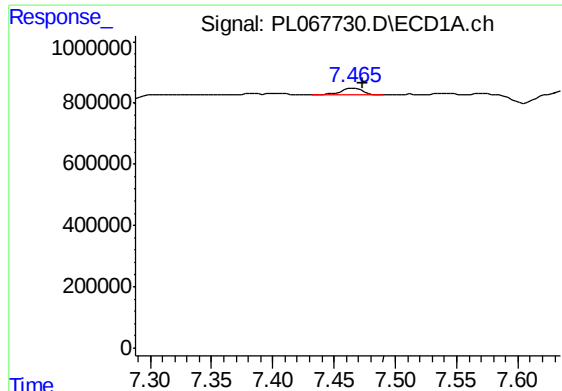

#12 4,4'-DDE


R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 277330
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
B2-6-8

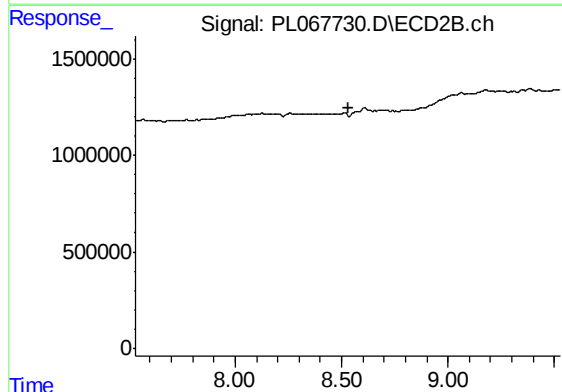


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

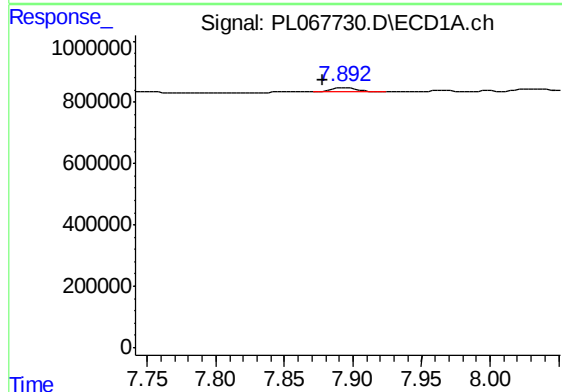


#14 Endrin

R.T.: 7.894 min
Delta R.T.: 0.016 min
Response: 198256
Conc: 0.30 ng/ml

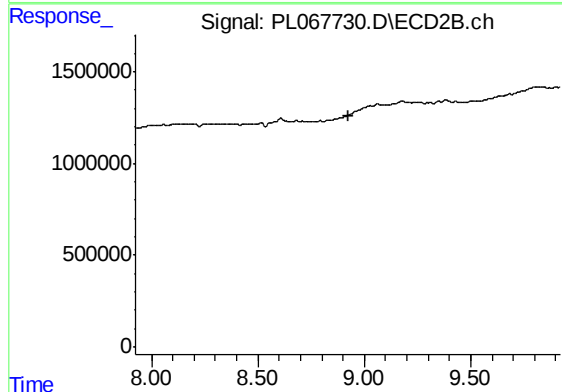

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

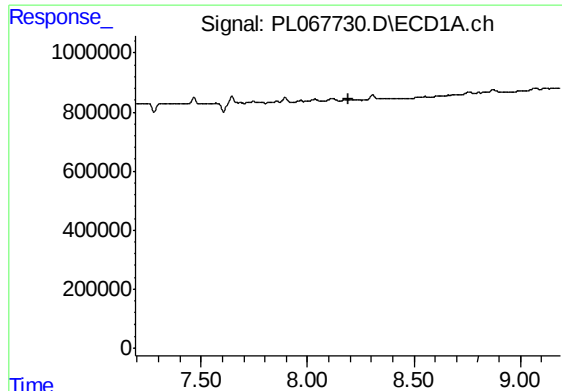

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B2-6-8

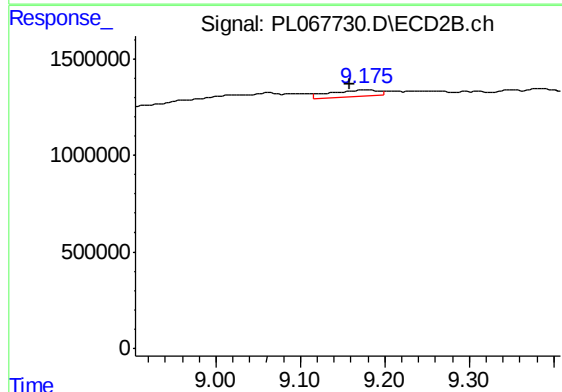


#15 Endosulfan II

R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 1392530
Conc: 1.75 ng/ml

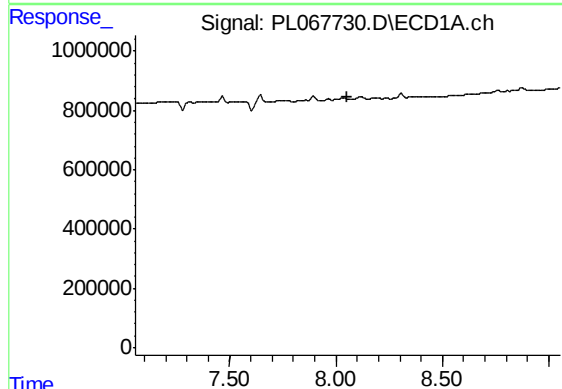


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.055 min
Response: 0
Conc: N.D.

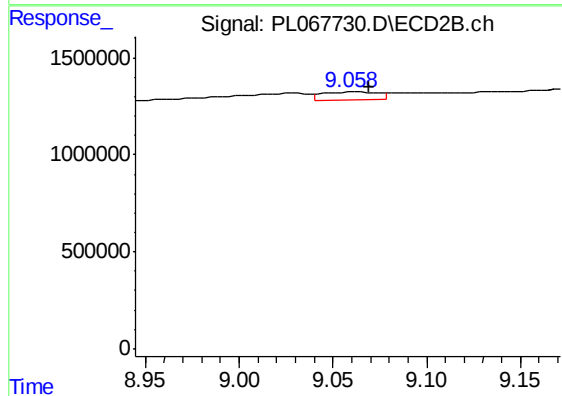

#16 4,4'-DDD


R.T.: 9.061 min
Delta R.T.: -0.008 min
Response: 846504
Conc: 1.19 ng/ml

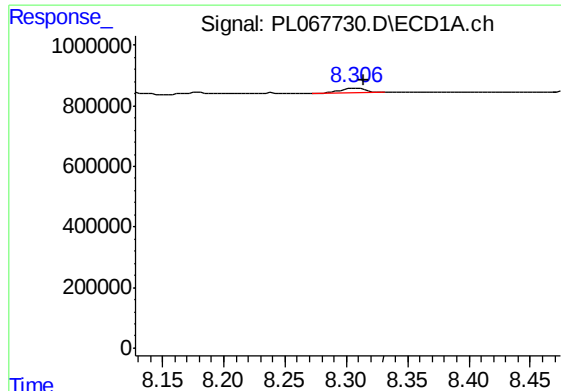

#17 4,4'-DDT


R.T.: 8.307 min
Delta R.T.: -0.007 min
Response: 206058
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
B2-6-8

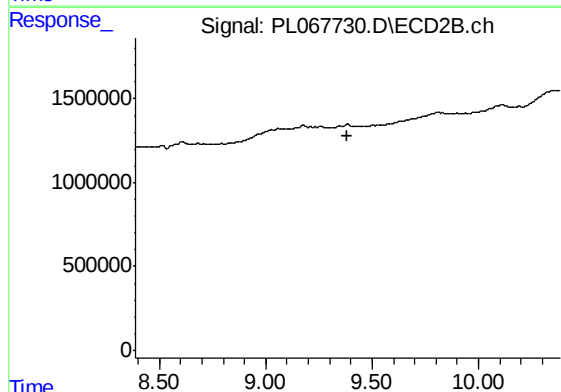


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.386 min
Response: 0
Conc: N.D.

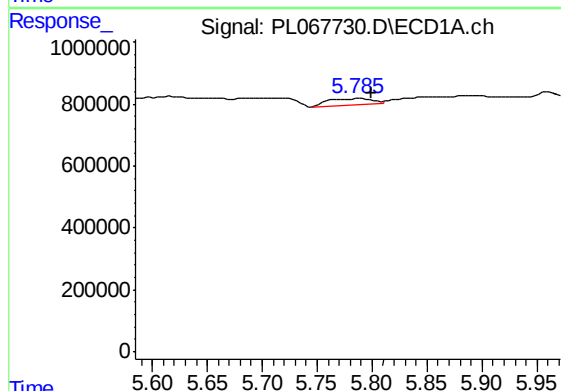


#23 Chlordane-1

R.T.: 5.788 min
Delta R.T.: -0.012 min
Response: 584082
Conc: 31.57 ng/ml

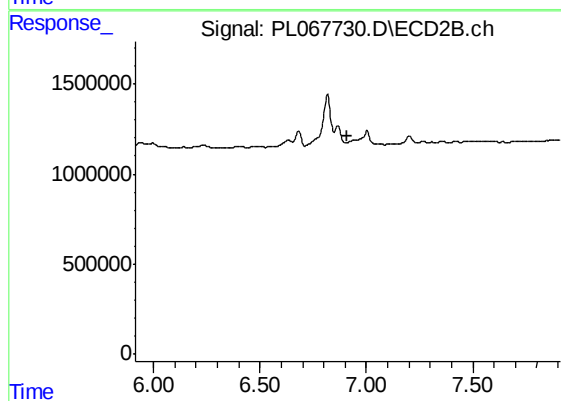

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

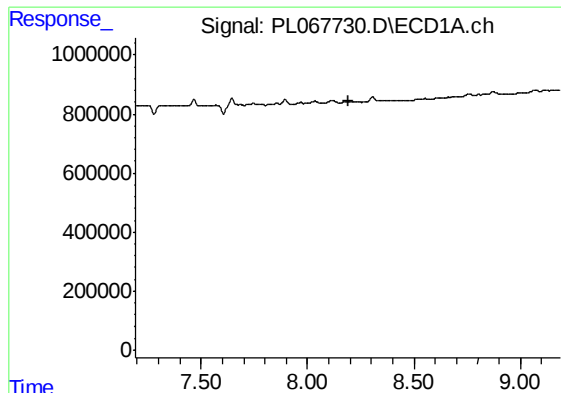

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B2-6-8

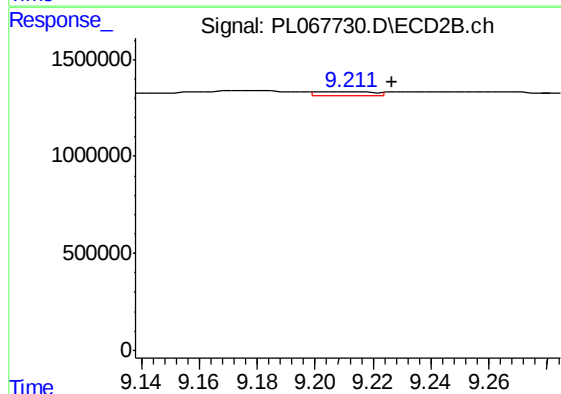


#27 Chlordane-5

R.T.: 9.213 min
Delta R.T.: -0.014 min
Response: 259211
Conc: 8.91 ng/ml

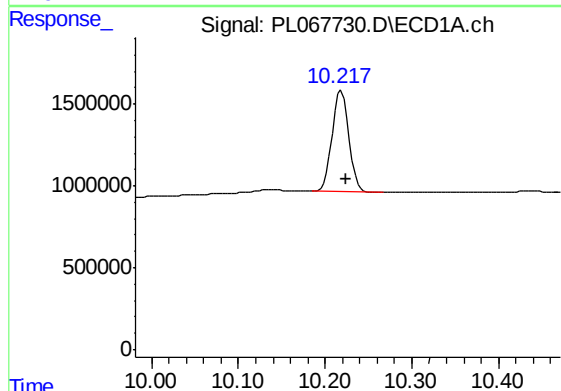

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 8343850
Conc: 11.77 ng/ml

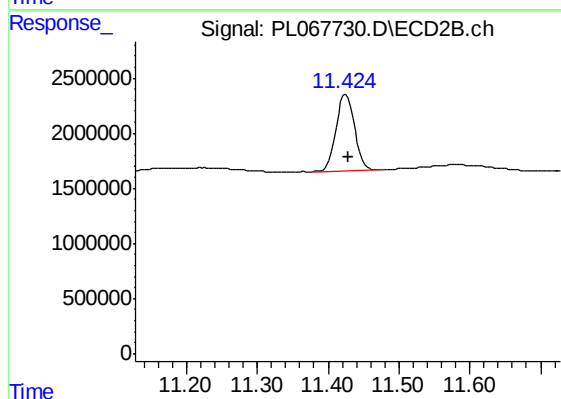

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 12557601
Conc: 12.61 ng/ml