

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 19:20
 Operator : AR\AJ
 Sample : M2795-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B3-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:35:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.528	2811512	5085776	5.114	5.395
28)	SA Decachlor...	10.218	11.425	4898696	7927654	6.912	7.959
Target Compounds							
2)	A alpha-BHC	5.162f	0.000	233176	0	0.317	N.D. #
7)	B delta-BHC	0.000	7.002f	0	929278	N.D.	0.791 #
11)	B alpha-Chl...	0.000	8.339	0	171218	N.D.	0.170 #
15)	B Endosulfa...	0.000	9.178f	0	441868	N.D.	0.554 #
16)	A 4,4'-DDD	0.000	9.094f	0	740085	N.D.	1.041 #
22)	Mirex	9.298	0.000	144020	0	0.229	N.D. #
23)	Chlordane-1	5.792	0.000	695081	0	37.568	N.D. #
26)	Chlordane-4	0.000	8.339	0	171218	N.D.	1.056 #
27)	Chlordane-5	0.000	9.219	0	46333	N.D.	1.593 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 19:20
Operator : AR\AJ
Sample : M2795-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
B3-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:35:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

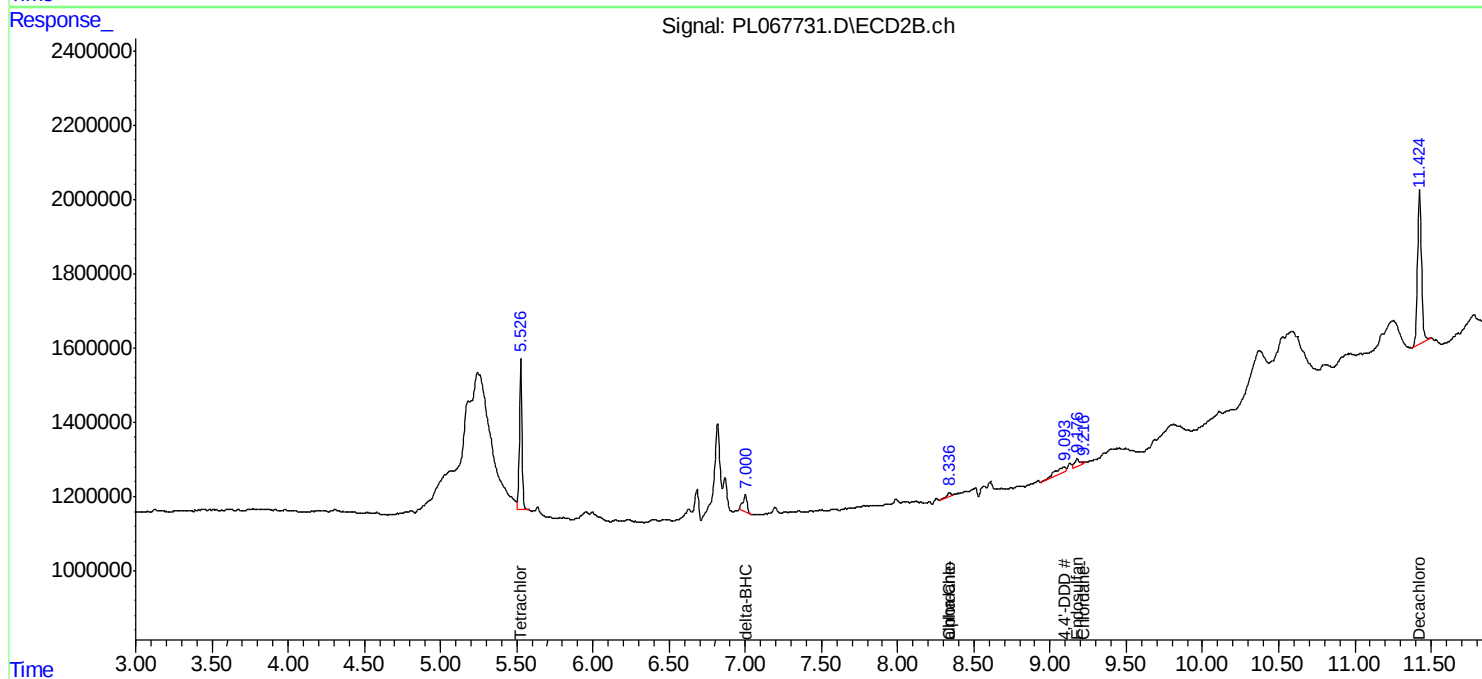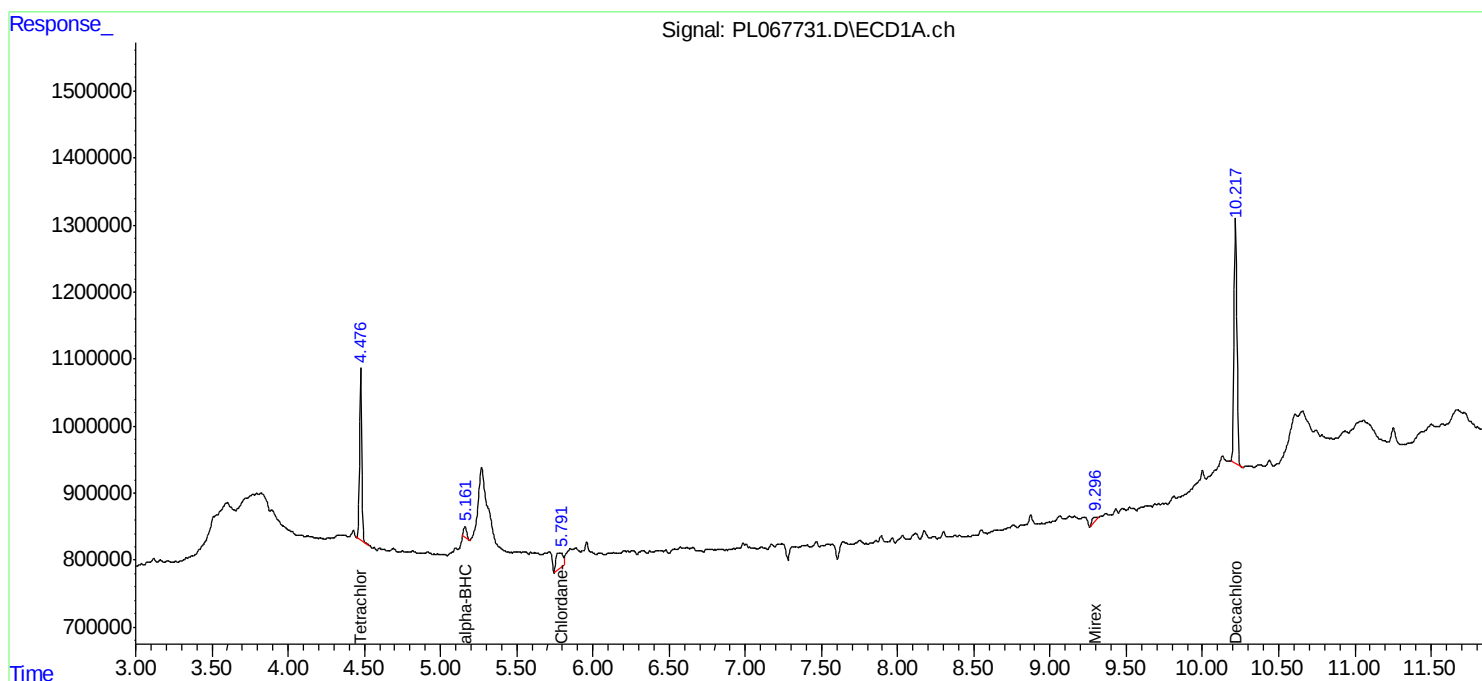


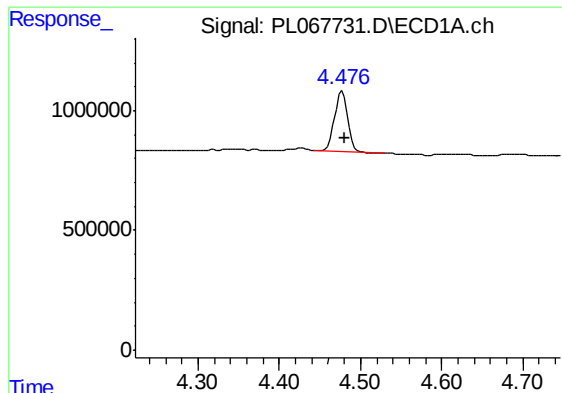

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 2811512
Conc: 5.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
B3-0-2

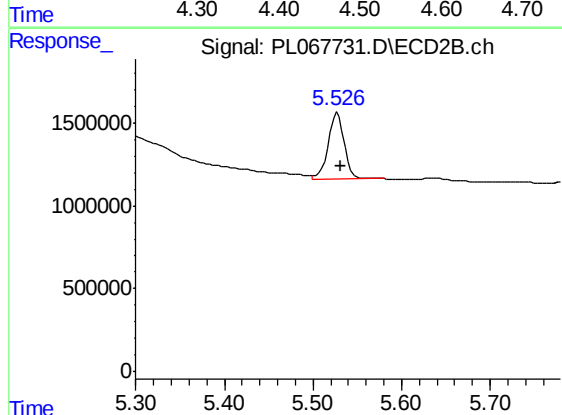


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 5085776
Conc: 5.39 ng/ml

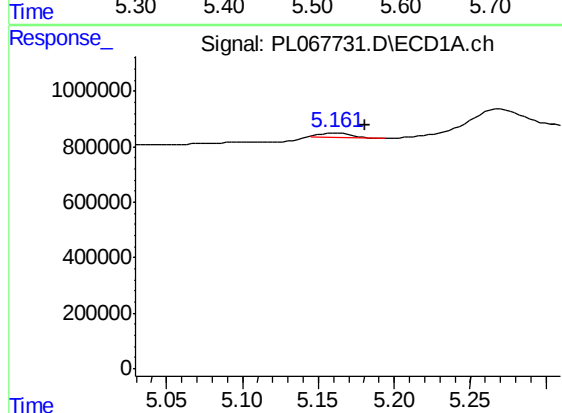


#2 alpha-BHC

R.T.: 5.162 min
Delta R.T.: -0.018 min
Response: 233176
Conc: 0.32 ng/ml

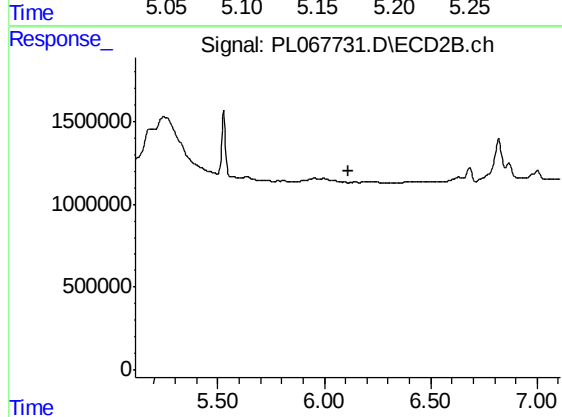

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

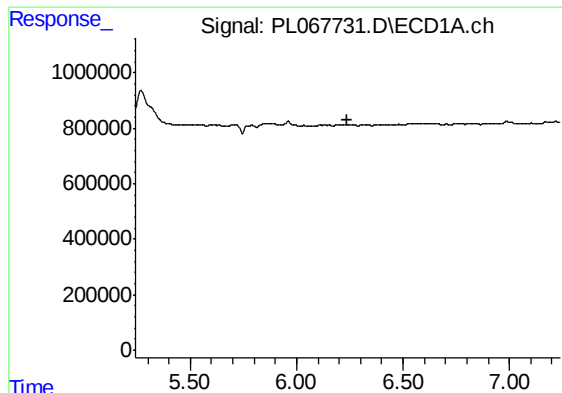

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B3-0-2

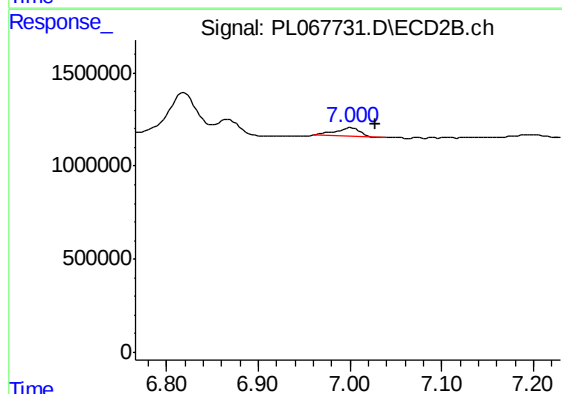


#7 delta-BHC

R.T.: 7.002 min
Delta R.T.: -0.026 min
Response: 929278
Conc: 0.79 ng/ml

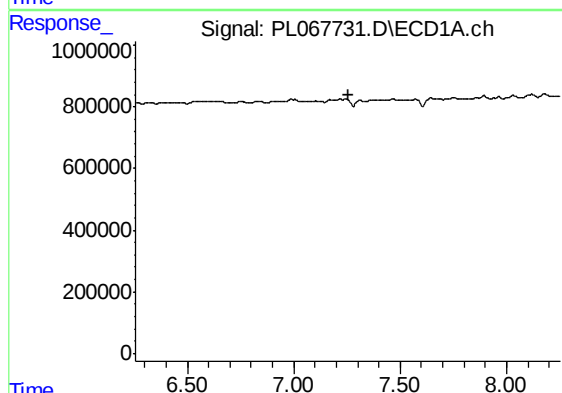


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

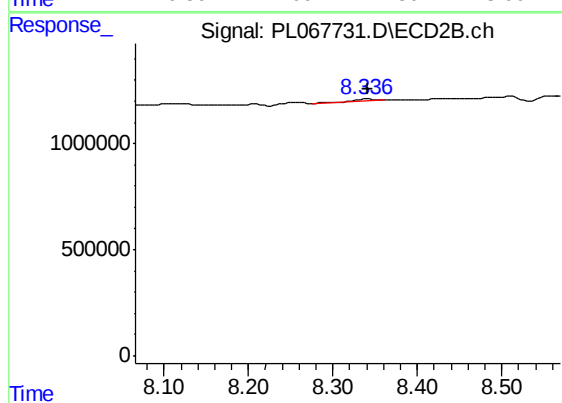

#11 alpha-Chlordane


R.T.: 8.339 min
Delta R.T.: -0.003 min
Response: 171218
Conc: 0.17 ng/ml

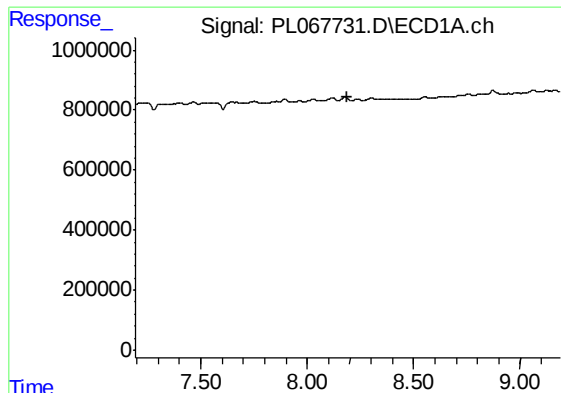

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B3-0-2

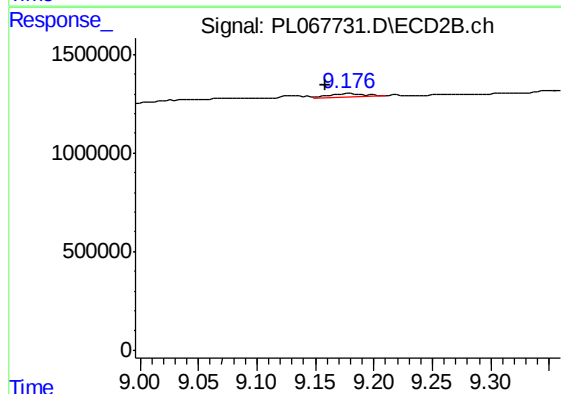


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.020 min
Response: 441868
Conc: 0.55 ng/ml

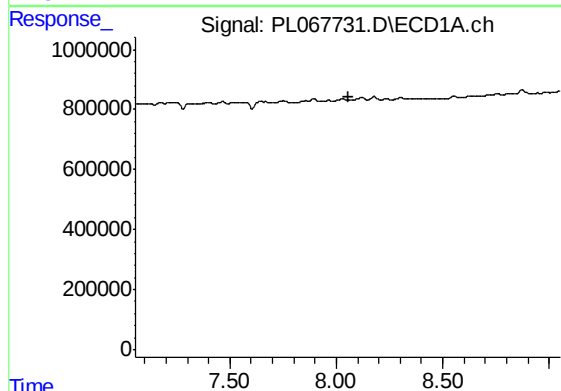


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.055 min
Response: 0
Conc: N.D.

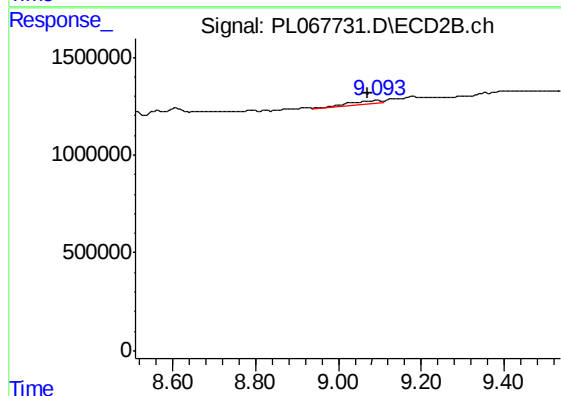

#16 4,4'-DDD


R.T.: 9.094 min
Delta R.T.: 0.025 min
Response: 740085
Conc: 1.04 ng/ml

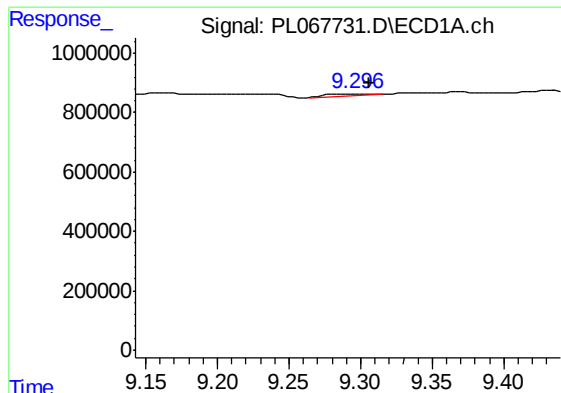

#22 Mirex


R.T.: 9.298 min
Delta R.T.: -0.008 min
Response: 144020
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
B3-0-2

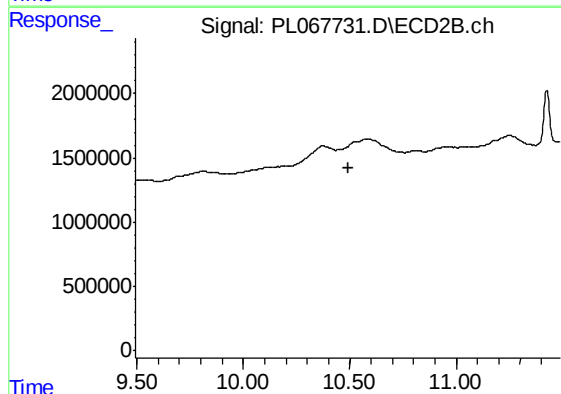


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

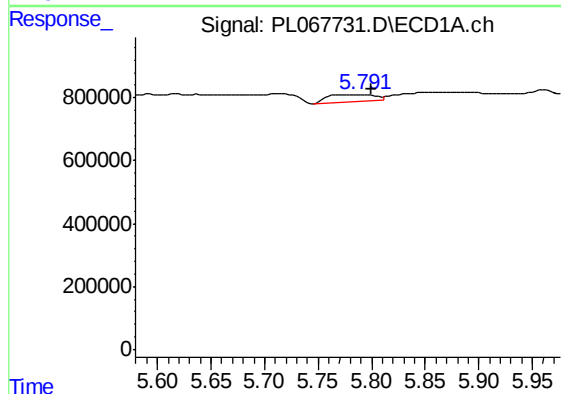


#23 Chlordane-1

R.T.: 5.792 min
Delta R.T.: -0.008 min
Response: 695081
Conc: 37.57 ng/ml

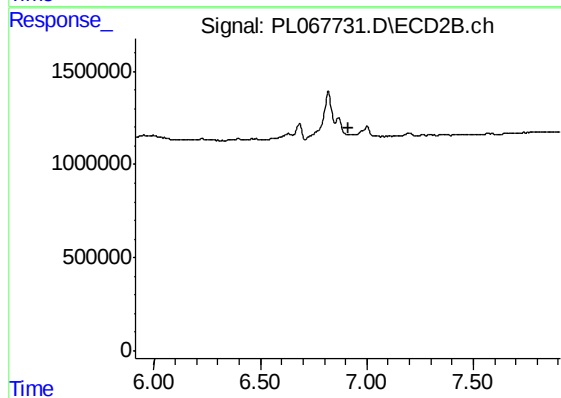

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

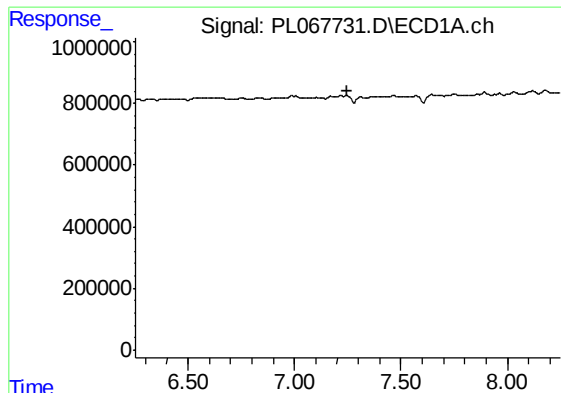

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B3-0-2

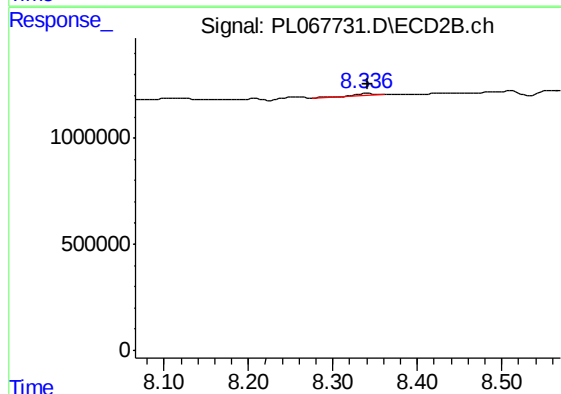


#26 Chlordane-4

R.T.: 8.339 min
Delta R.T.: -0.002 min
Response: 171218
Conc: 1.06 ng/ml

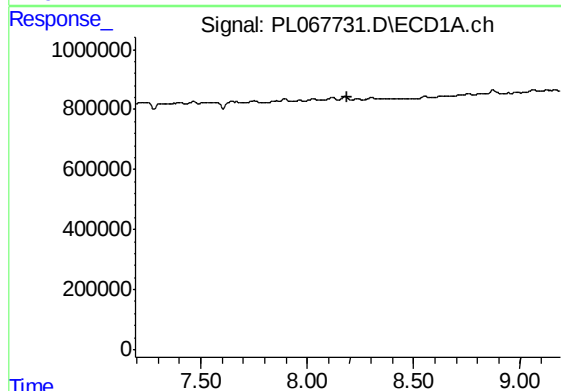


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 8.191 min
Response: 0
Conc: N.D.

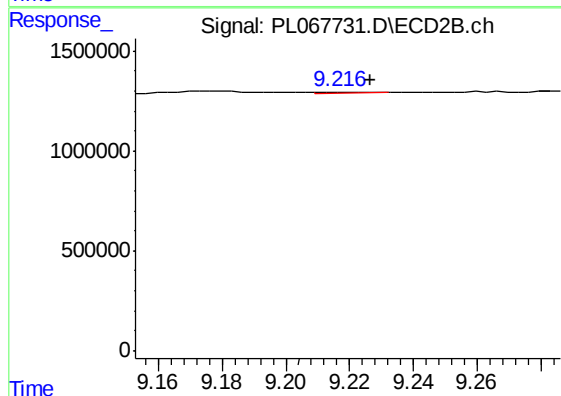

#27 Chlordane-5


R.T.: 9.219 min
Delta R.T.: -0.008 min
Response: 46333
Conc: 1.59 ng/ml

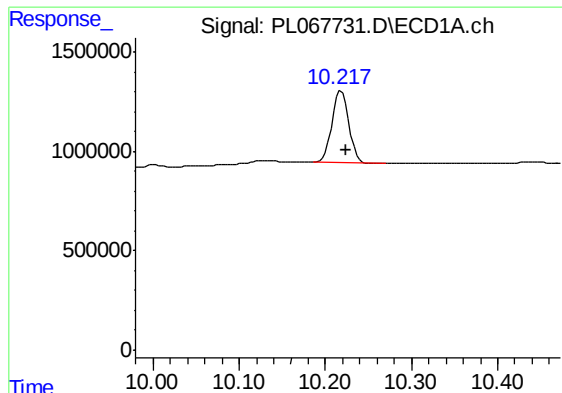

#28 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.006 min
Response: 4898696
Conc: 6.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
B3-0-2

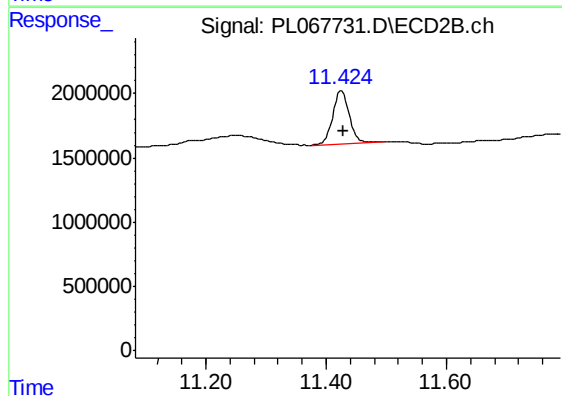

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 7927654
Conc: 7.96 ng/ml