

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 21:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:37:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.528	10816315	19685600	19.674	20.881
28)	SA Decachlor...	10.216	11.424	13599911	20453224	19.190	20.534
Target Compounds							
3)	MA gamma-BHC...	5.613	0.000	493919	0	0.659	N.D. #
4)	MA Heptachlor	5.985f	0.000	482408	0	0.640	N.D. #
6)	B beta-BHC	5.985	0.000	482408	0	1.348	N.D. #
14)	MA Endrin	7.891	0.000	162798	0	0.248	N.D. #
15)	B Endosulfa...	0.000	9.180f	0	59930	N.D.	0.075 #
21)	B Endrin ke...	9.120	0.000	171760	0	0.226	N.D. #
23)	Chlordane-1	0.000	6.938f	0	333839	N.D.	11.822 #
24)	Chlordane-2	6.483	0.000	303454	0	11.332	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 21:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:37:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

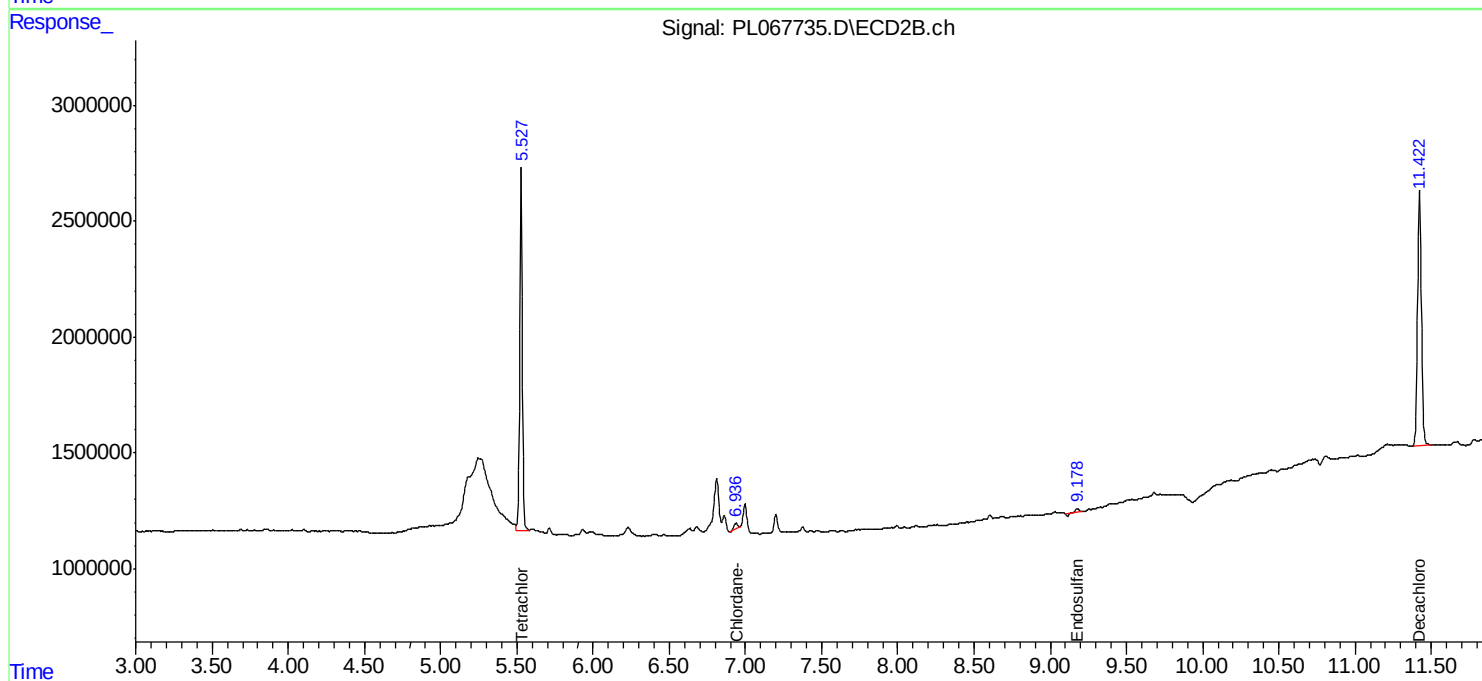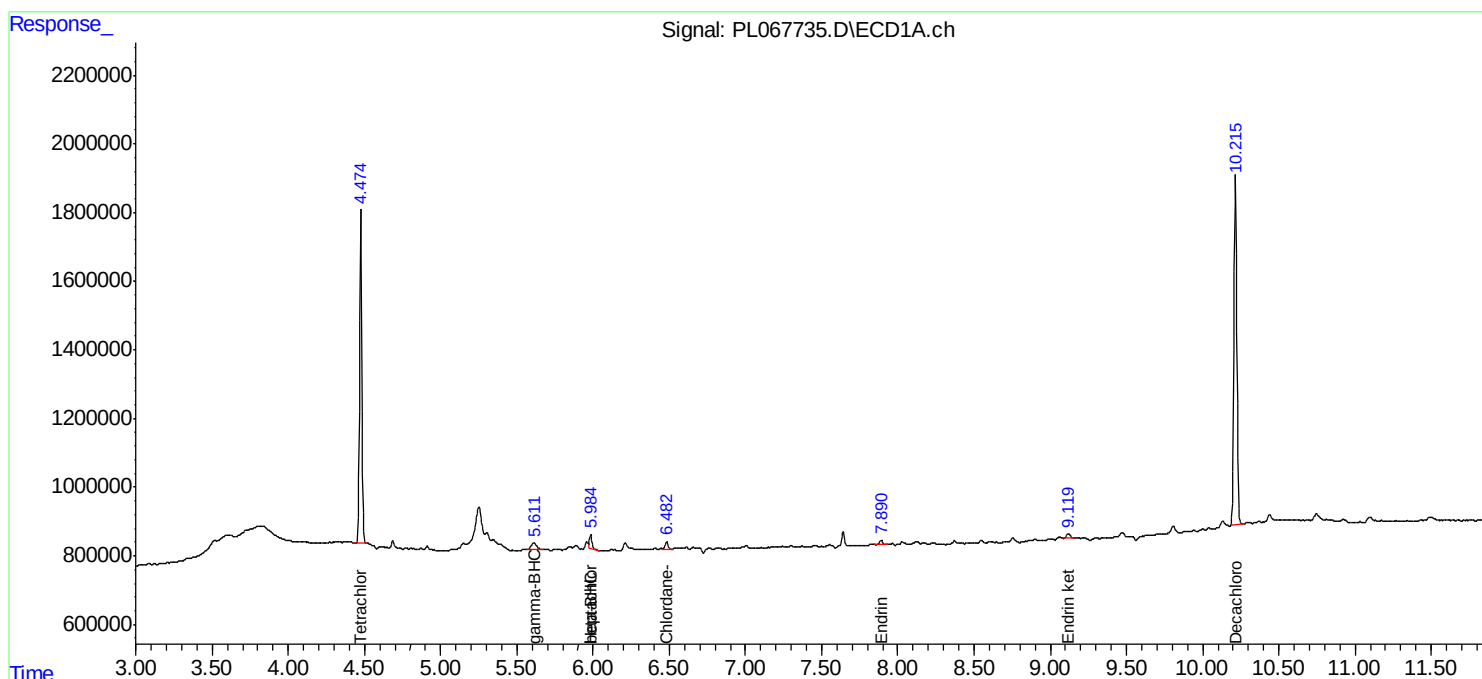


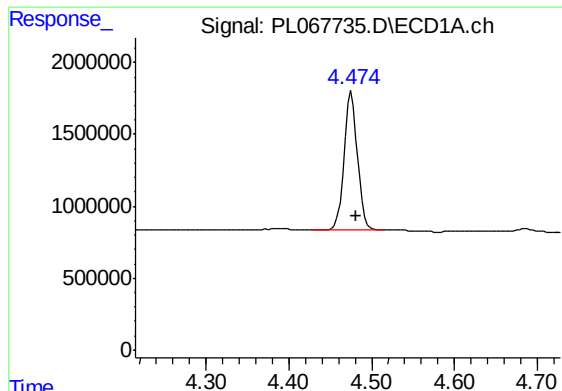

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 10816315
Conc: 19.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

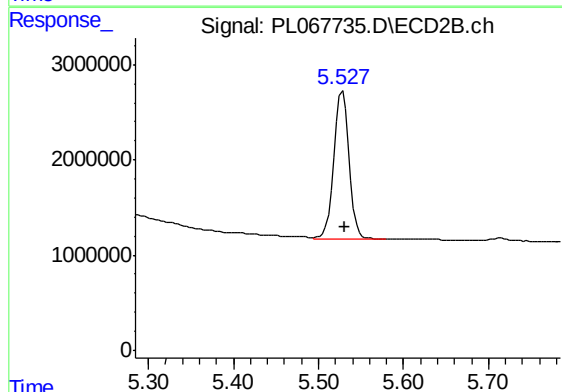


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 19685600
Conc: 20.88 ng/ml

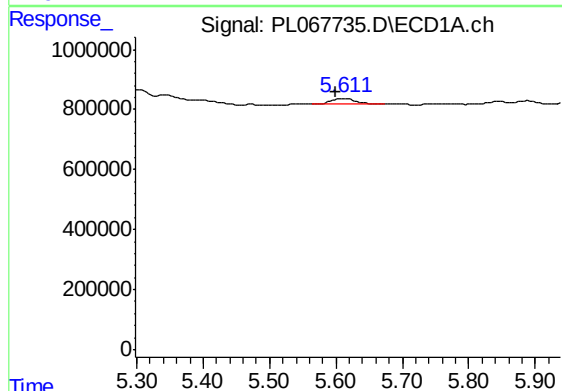


#3 gamma-BHC (Lindane)

R.T.: 5.613 min
Delta R.T.: 0.012 min
Response: 493919
Conc: 0.66 ng/ml

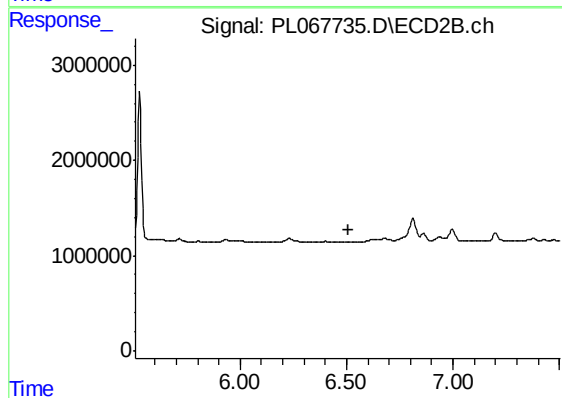

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

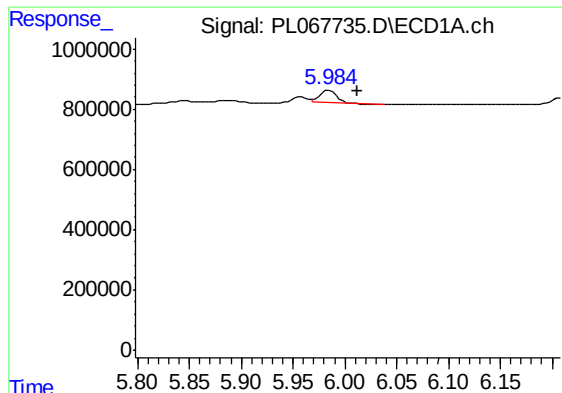

#4 Heptachlor


R.T.: 5.985 min
Delta R.T.: -0.027 min
Response: 482408
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

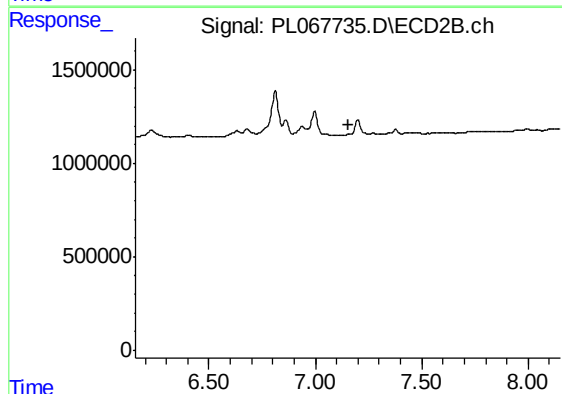


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

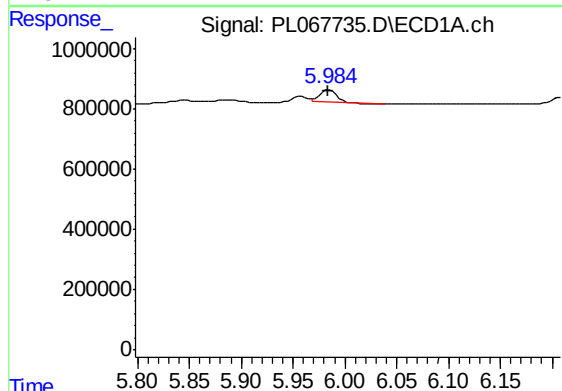


#6 beta-BHC

R.T.: 5.985 min
Delta R.T.: 0.002 min
Response: 482408
Conc: 1.35 ng/ml

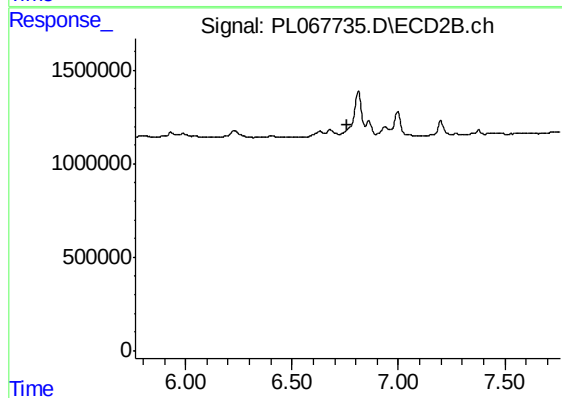

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

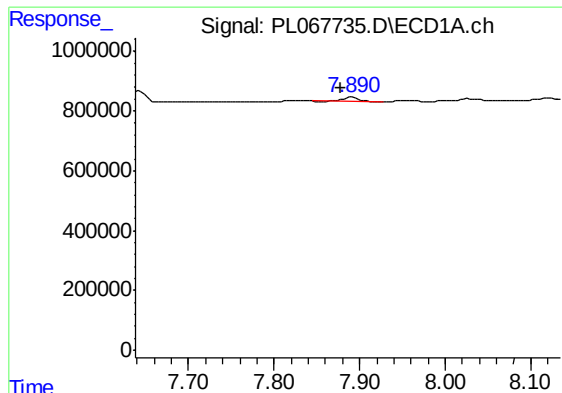

#14 Endrin


R.T.: 7.891 min
Delta R.T.: 0.013 min
Response: 162798
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

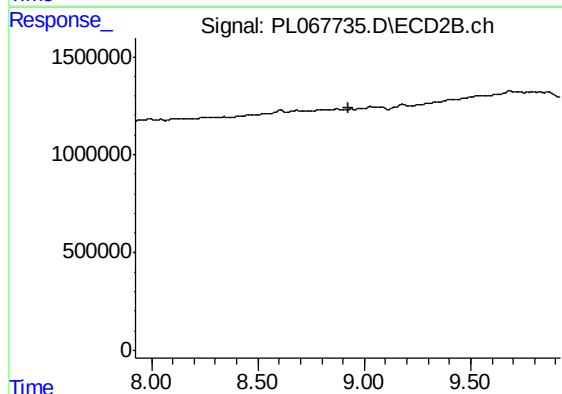


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

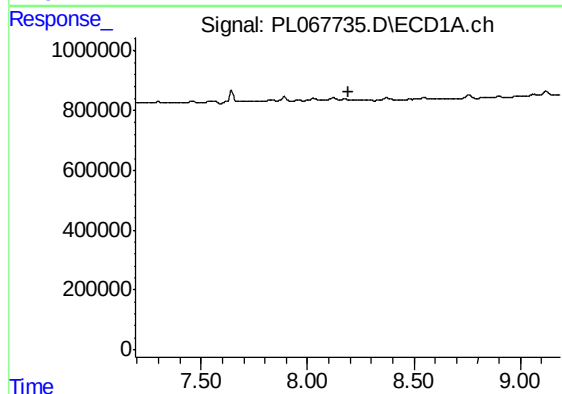


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

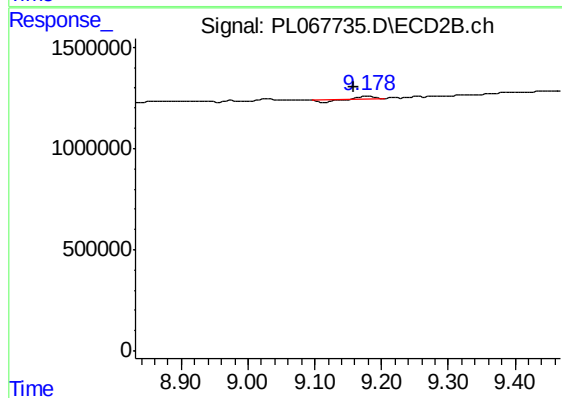

#15 Endosulfan II


R.T.: 9.180 min
Delta R.T.: 0.022 min
Response: 59930
Conc: 0.08 ng/ml

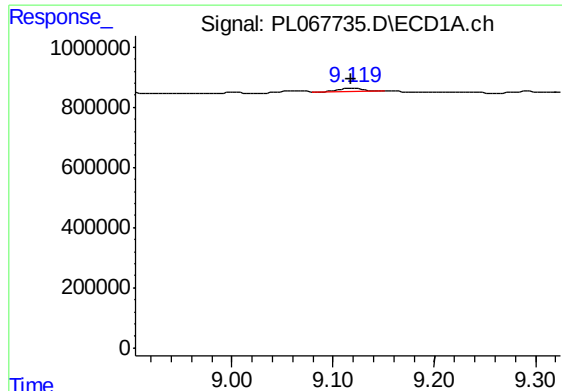

#21 Endrin ketone


R.T.: 9.120 min
Delta R.T.: 0.003 min
Response: 171760
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

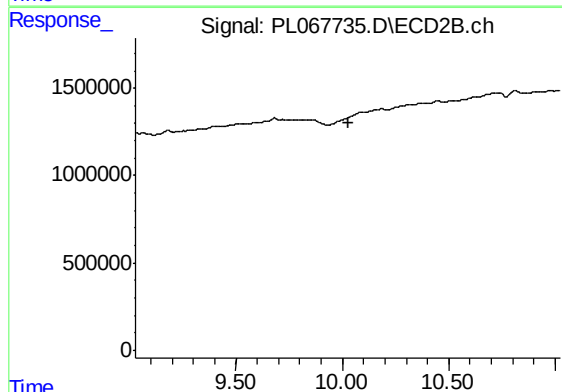


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

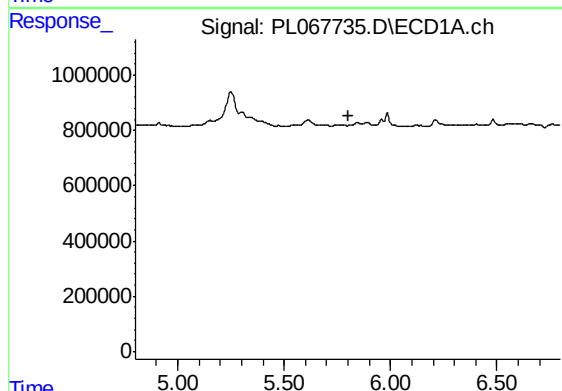


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.800 min
Response: 0
Conc: N.D.

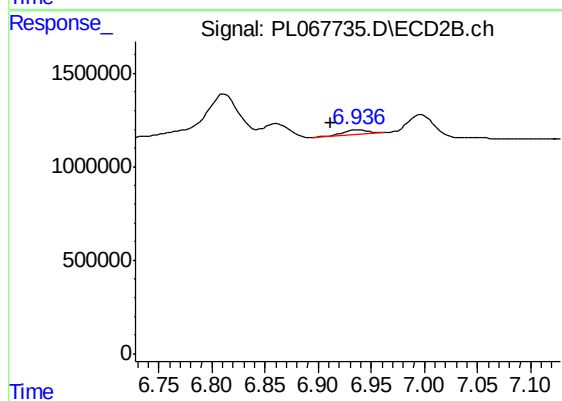

#23 Chlordane-1


R.T.: 6.938 min
Delta R.T.: 0.026 min
Response: 333839
Conc: 11.82 ng/ml

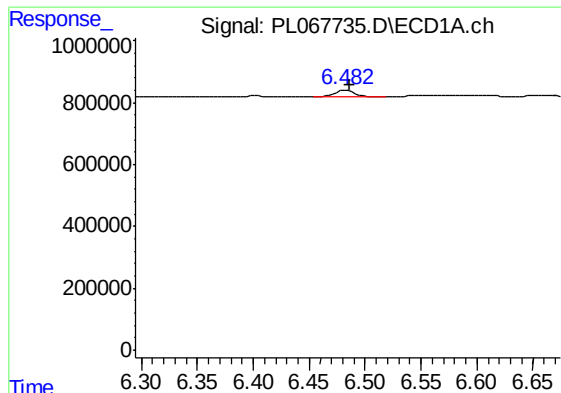

#24 Chlordane-2


R.T.: 6.483 min
Delta R.T.: -0.003 min
Response: 303454
Conc: 11.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

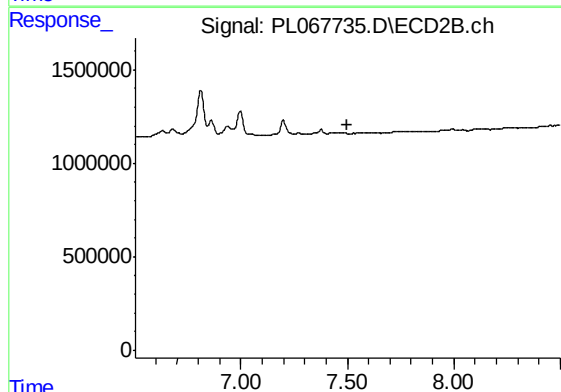


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

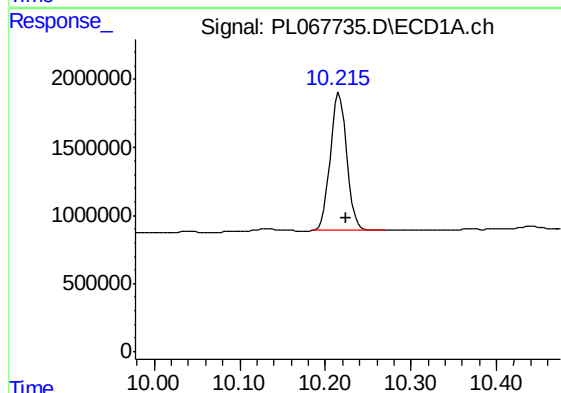

#28 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.008 min
Response: 13599911
Conc: 19.19 ng/ml

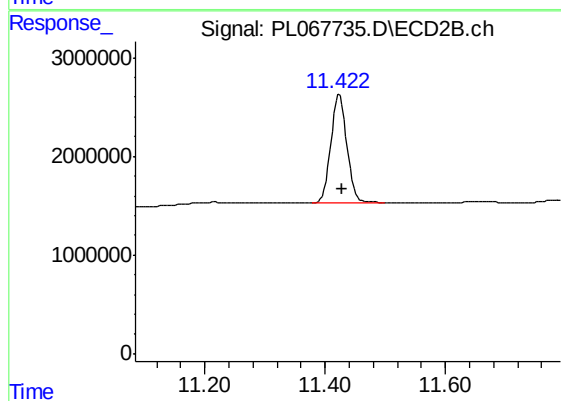

#28 Decachlorobiphenyl

R.T.: 11.424 min
Delta R.T.: -0.005 min
Response: 20453224
Conc: 20.53 ng/ml