

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 10:40
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 17:38:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.483	5.524	30400990	49989332	55.296	53.026
28)	SA Decachlor...	10.227	11.429	35590028	50603657	50.220	50.804
Target Compounds							
23)	Chlordane-1	5.802	6.907	9842241	16775046	531.959	594.059
24)	Chlordane-2	6.489	7.499	13968076	19469278	521.620	534.193
25)	Chlordane-3	7.186	8.257	36040797	69426465	536.396	518.735
26)	Chlordane-4	7.253	8.338	38691207	83719856	529.446	516.469
27)	Chlordane-5	8.194	9.225	11416804	15072198	521.814	518.343



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 10:40
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 17:38:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

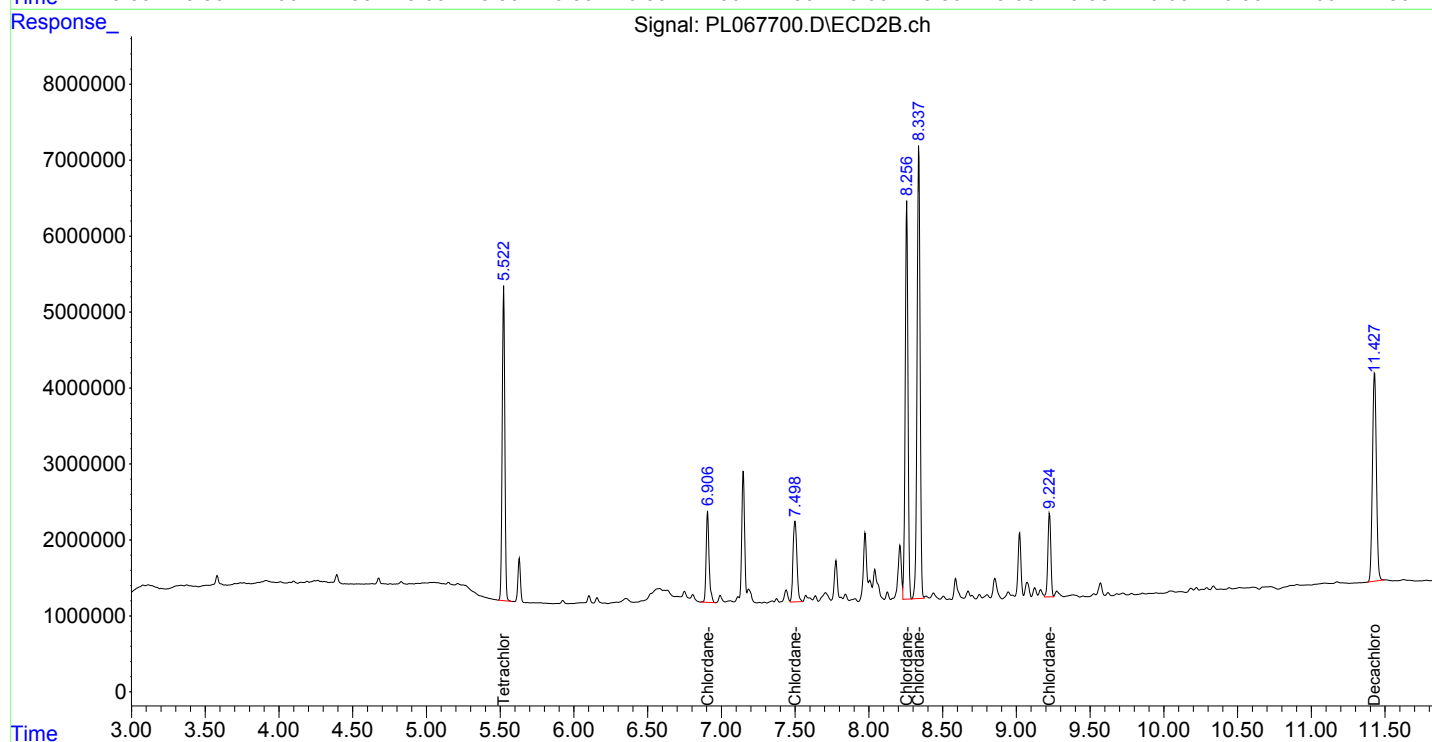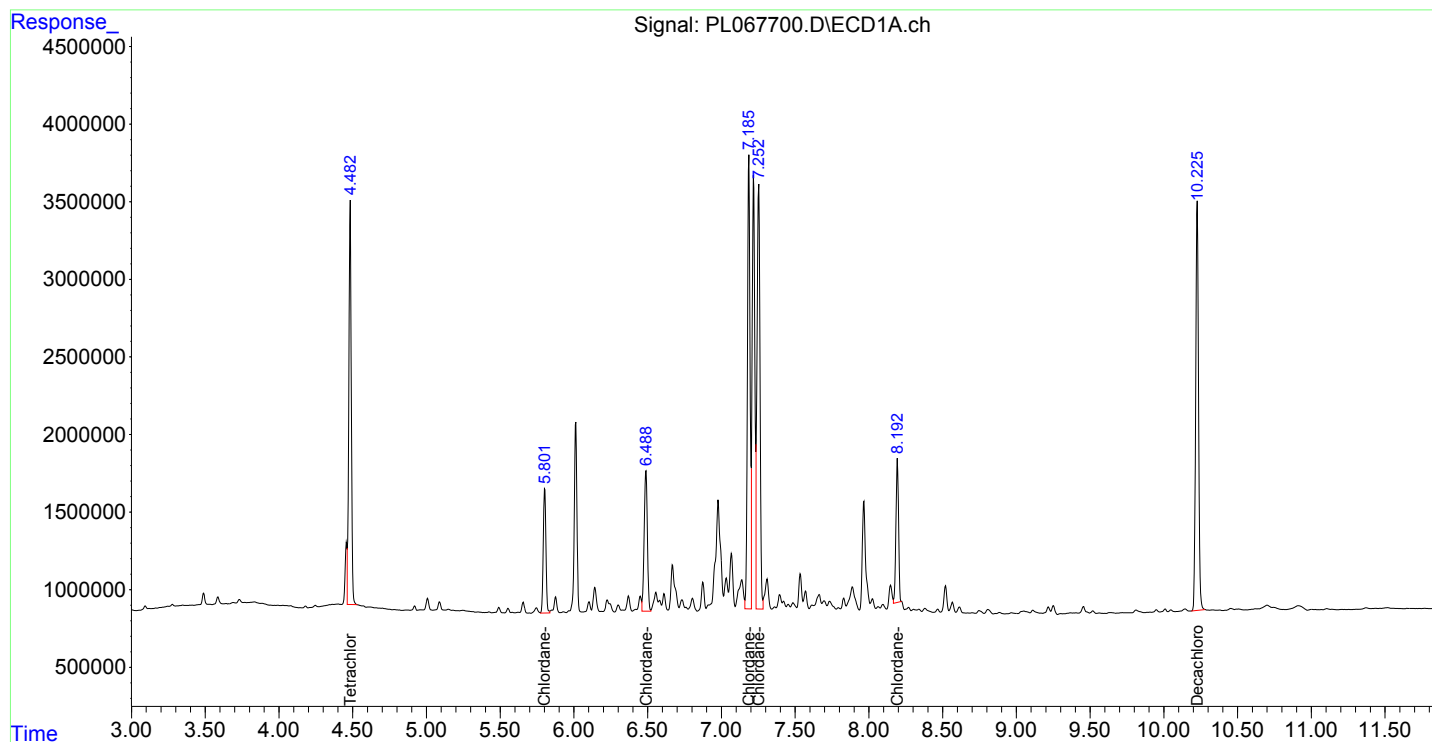


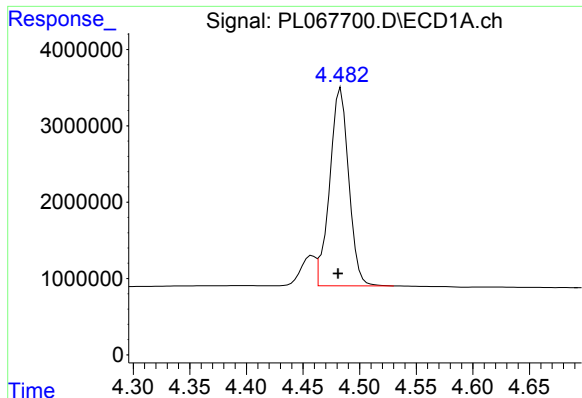

#1 Tetrachloro-m-xylene


R.T.: 4.483 min
Delta R.T.: 0.002 min
Response: 30400990
Conc: 55.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

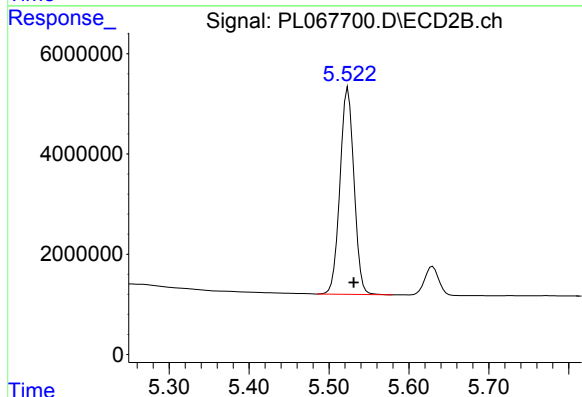


#1 Tetrachloro-m-xylene

R.T.: 5.524 min
Delta R.T.: -0.007 min
Response: 49989332
Conc: 53.03 ng/ml

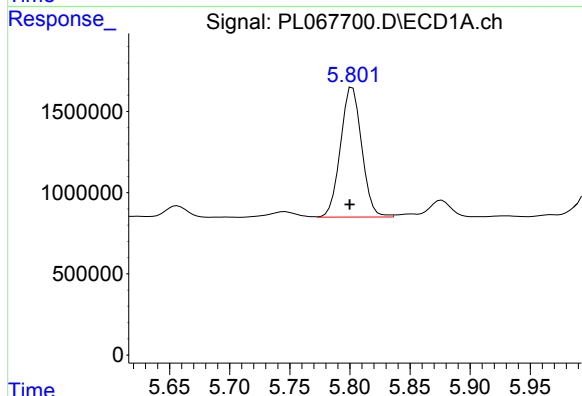


#23 Chlordane-1

R.T.: 5.802 min
Delta R.T.: 0.002 min
Response: 9842241
Conc: 531.96 ng/ml

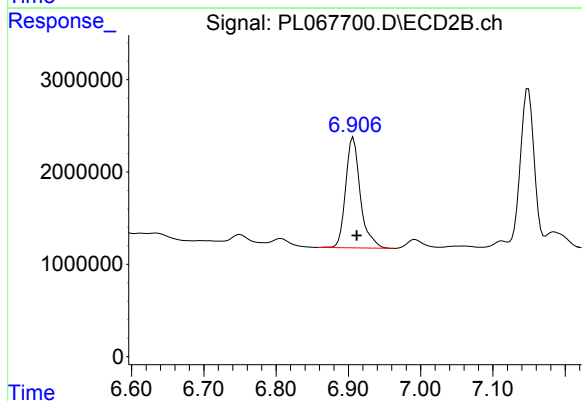

#23 Chlordane-1


R.T.: 6.907 min
Delta R.T.: -0.005 min
Response: 16775046
Conc: 594.06 ng/ml

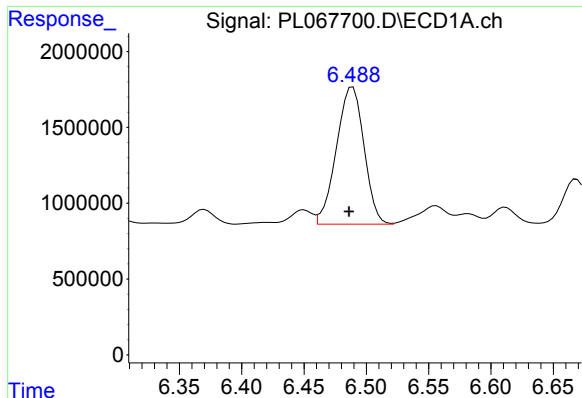

#24 Chlordane-2


R.T.: 6.489 min
Delta R.T.: 0.003 min
Response: 13968076
Conc: 521.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

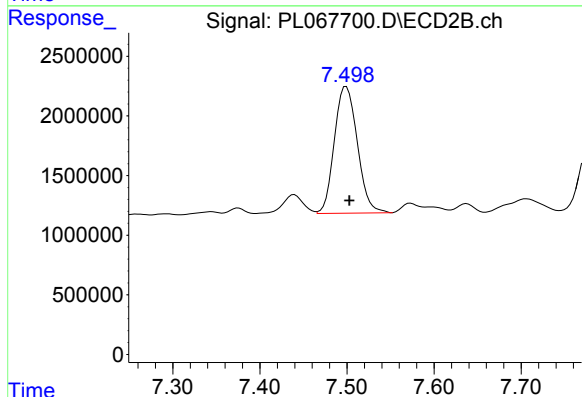


#24 Chlordane-2

R.T.: 7.499 min
Delta R.T.: -0.003 min
Response: 19469278
Conc: 534.19 ng/ml

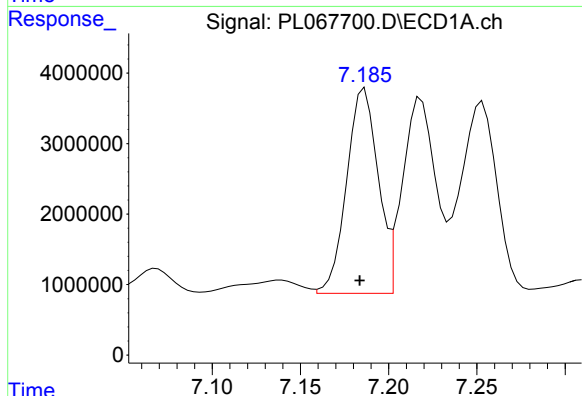


#25 Chlordane-3

R.T.: 7.186 min
Delta R.T.: 0.003 min
Response: 36040797
Conc: 536.40 ng/ml

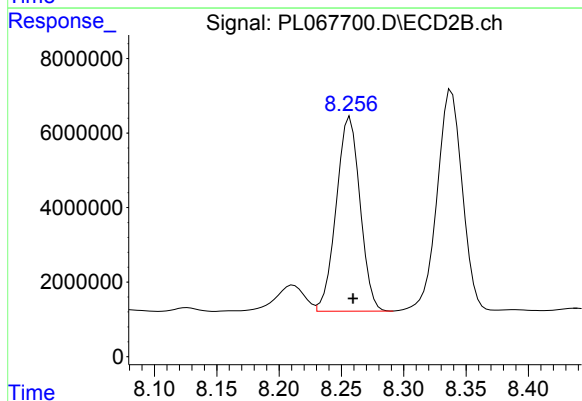

#25 Chlordane-3


R.T.: 8.257 min
Delta R.T.: -0.002 min
Response: 69426465
Conc: 518.74 ng/ml

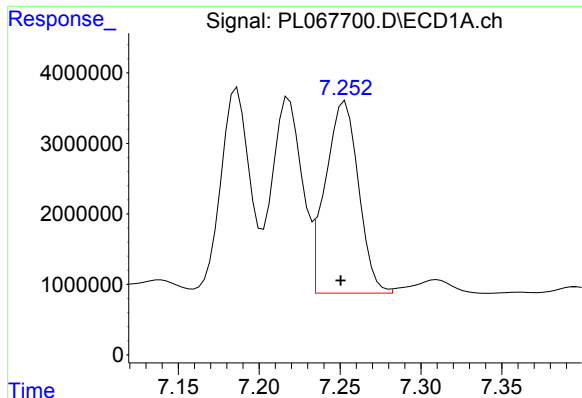

#26 Chlordane-4


R.T.: 7.253 min
Delta R.T.: 0.003 min
Response: 38691207
Conc: 529.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

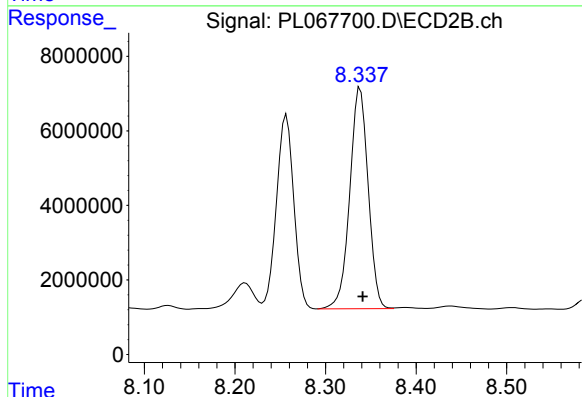


#26 Chlordane-4

R.T.: 8.338 min
Delta R.T.: -0.003 min
Response: 83719856
Conc: 516.47 ng/ml

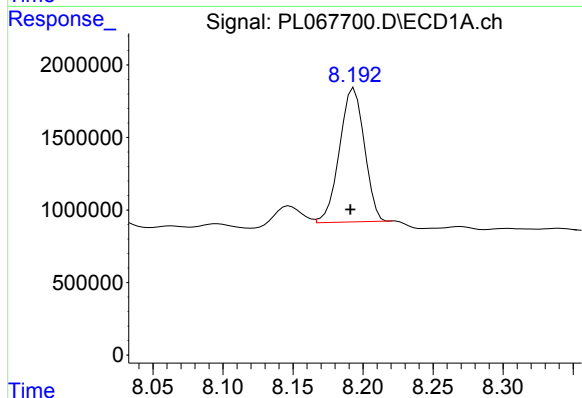


#27 Chlordane-5

R.T.: 8.194 min
Delta R.T.: 0.003 min
Response: 11416804
Conc: 521.81 ng/ml

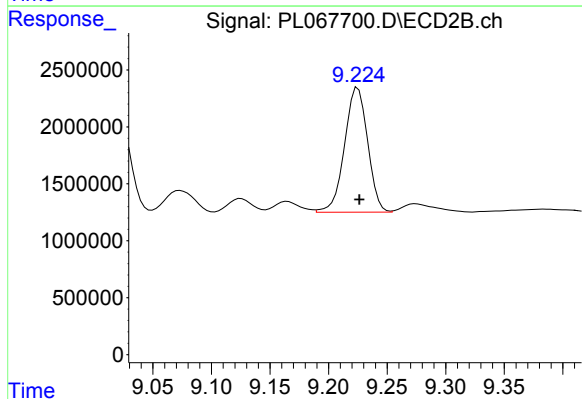

#27 Chlordane-5


R.T.: 9.225 min
Delta R.T.: -0.001 min
Response: 15072198
Conc: 518.34 ng/ml

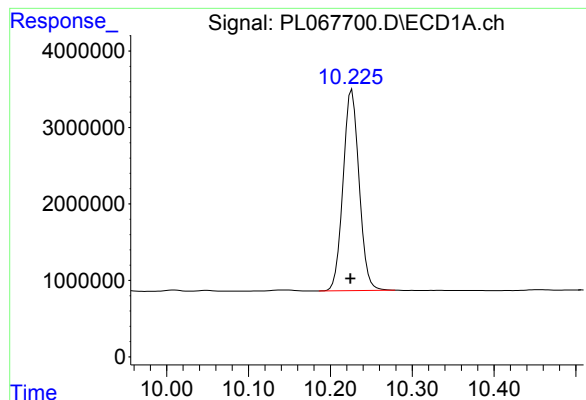

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: 0.002 min
Response: 35590028
Conc: 50.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

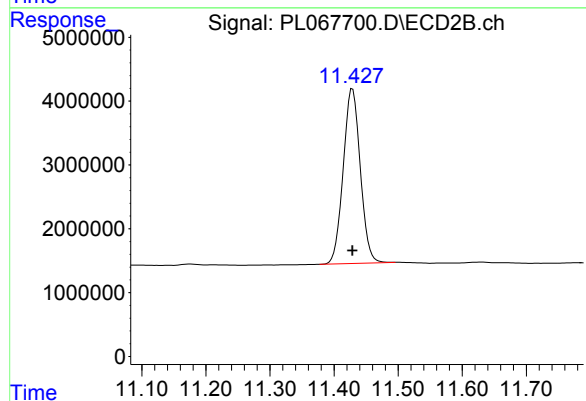

#28 Decachlorobiphenyl

R.T.: 11.429 min
Delta R.T.: 0.000 min
Response: 50603657
Conc: 50.80 ng/ml