

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 12:04
 Operator : AR\AJ
 Sample : PB137245BS
 Misc : CHLOR BS
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:24:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.528	11766383	21527961	21.402m	22.836
28)	SA Decachlor...	10.220	11.426	14905027	22368902	21.032	22.457
Target Compounds							
23)	Chlordane-1	5.797	6.909	4032627	6184305	217.958	219.006
24)	Chlordane-2	6.483	7.500	6501040	8006685	242.773	219.685
25)	Chlordane-3	7.180	8.257	13722425	27596539	204.231	206.194
26)	Chlordane-4	7.247	8.339	14975182	33724246	204.919	208.045
27)	Chlordane-5	8.188	9.225	4608254	5945609	210.624	204.473

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 PB137245BS

Manual Integrations
 APPROVED

Ankita
 6/23/2021 10:17:13 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 12:04
Operator : AR\AJ
Sample : PB137245BS
Misc : CHLOR BS
ALS Vial : 10 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:24:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampled :
PB137245BS

Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:13 AM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

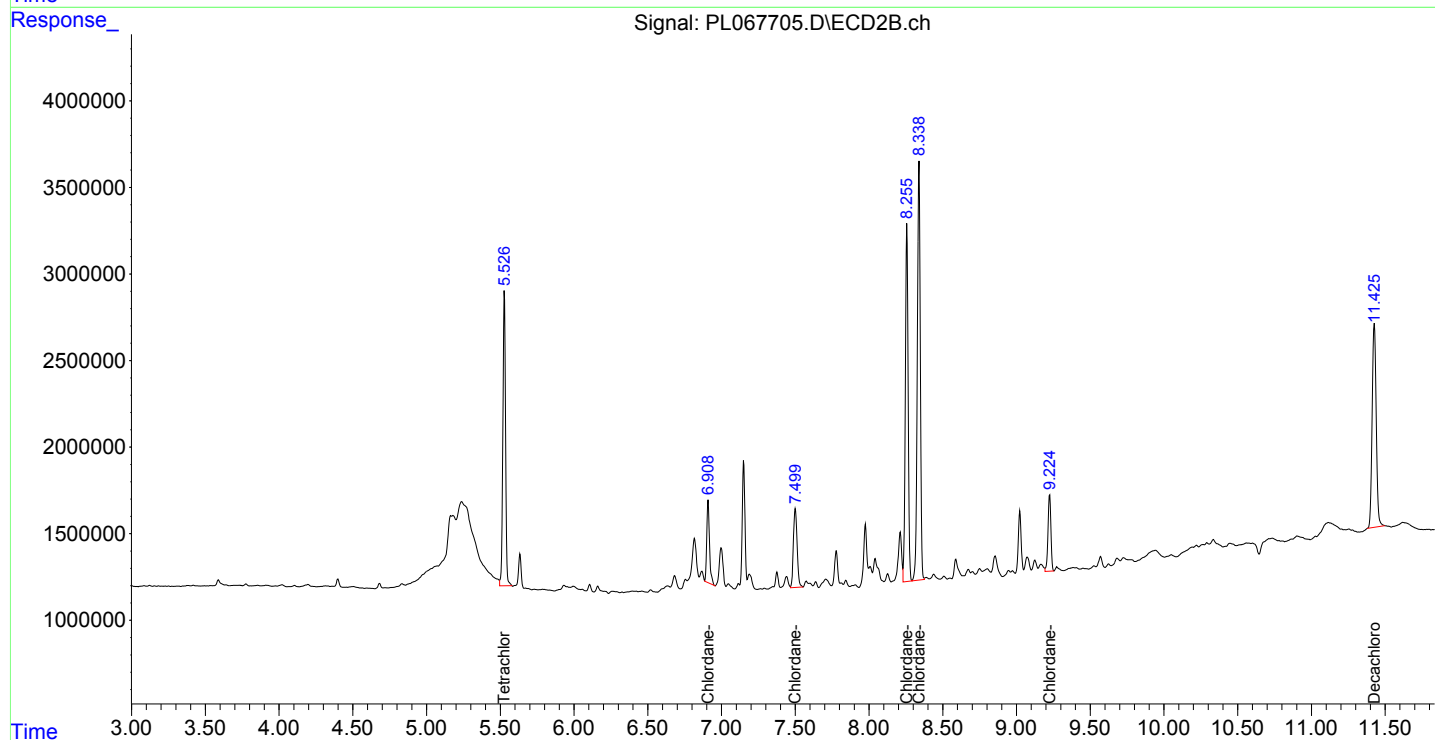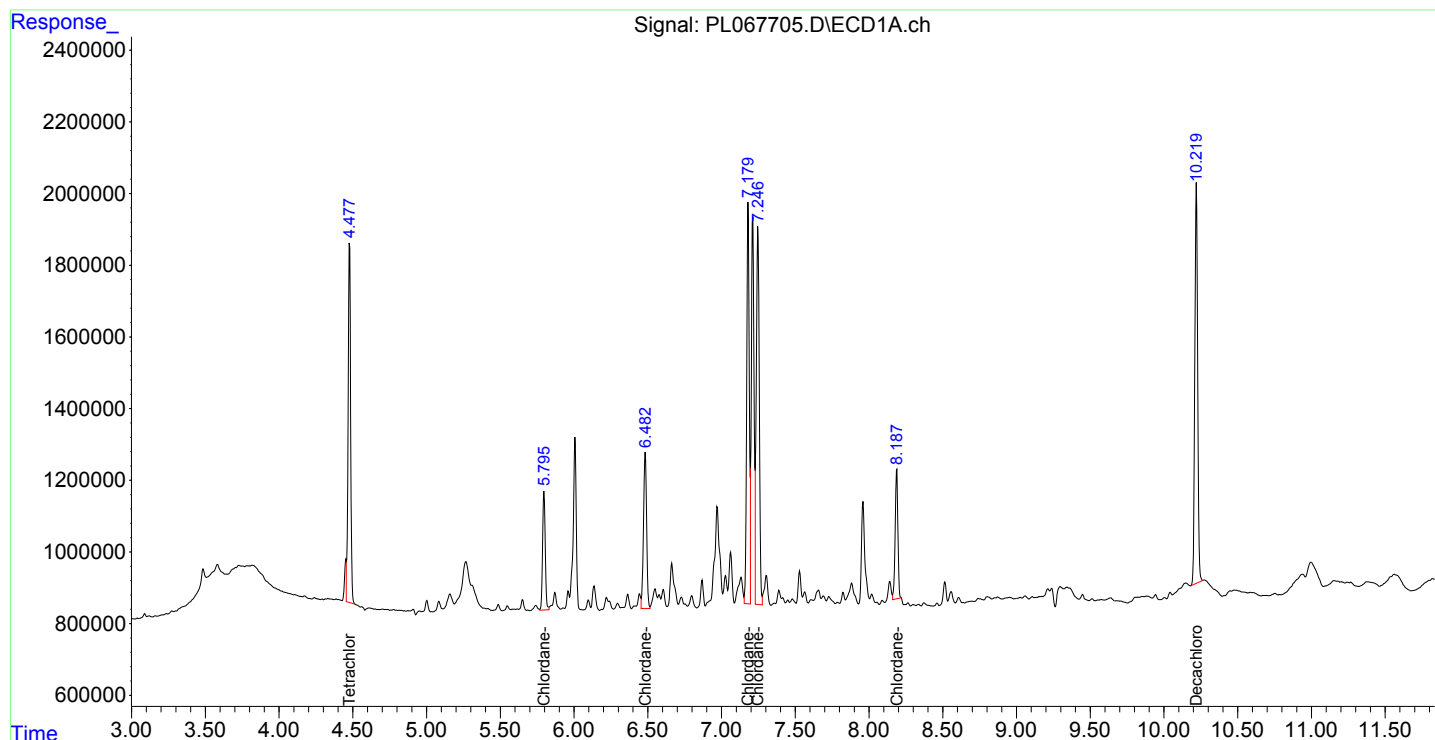

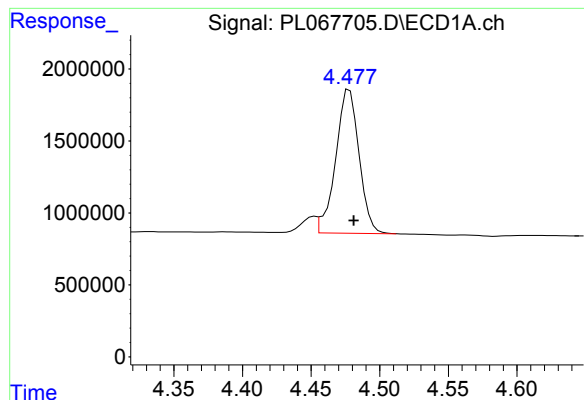


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 11766383
Conc: 21.40 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PB137245BS


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:13 AM

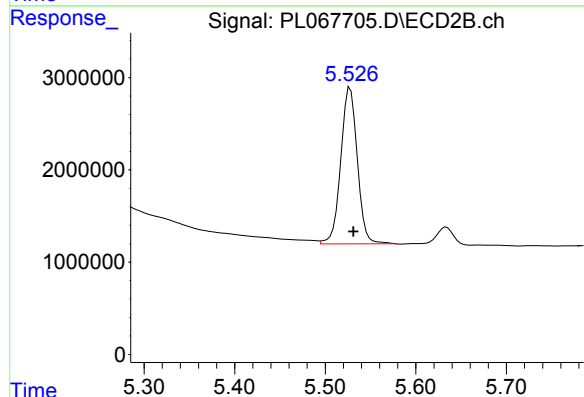


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 21527961
Conc: 22.84 ng/ml

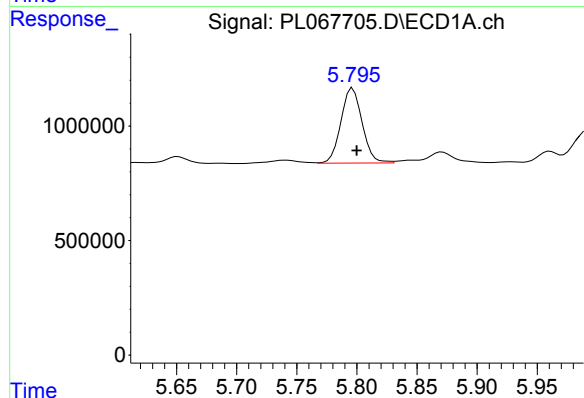


#23 Chlordane-1

R.T.: 5.797 min
Delta R.T.: -0.003 min
Response: 4032627
Conc: 217.96 ng/ml

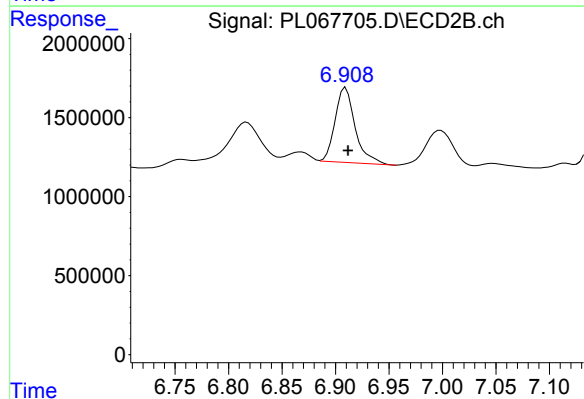

#23 Chlordane-1

R.T.: 6.909 min
Delta R.T.: -0.002 min
Response: 6184305
Conc: 219.01 ng/ml

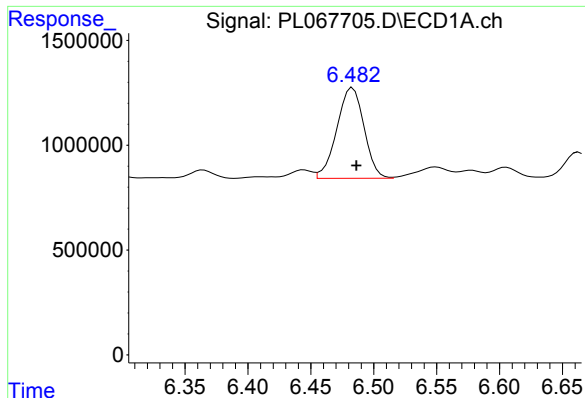


#24 Chlordane-2

R.T.: 6.483 min
Delta R.T.: -0.003 min
Response: 6501040
Conc: 242.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137245BS


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:13 AM

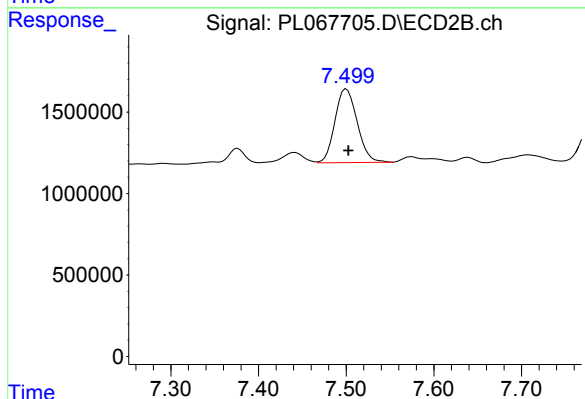


#24 Chlordane-2

R.T.: 7.500 min
Delta R.T.: -0.002 min
Response: 8006685
Conc: 219.69 ng/ml

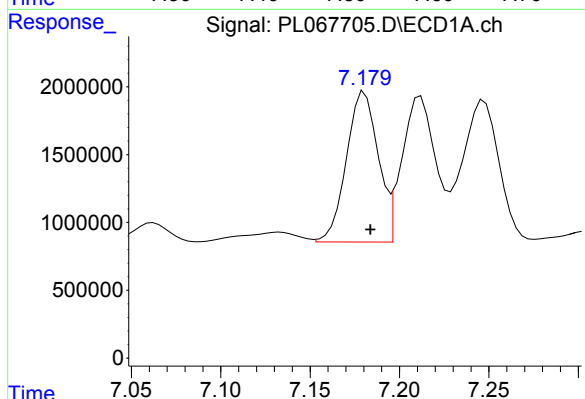


#25 Chlordane-3

R.T.: 7.180 min
Delta R.T.: -0.003 min
Response: 13722425
Conc: 204.23 ng/ml

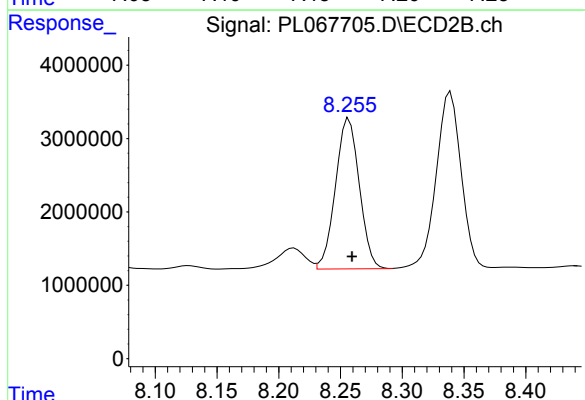

#25 Chlordane-3

R.T.: 8.257 min
Delta R.T.: -0.002 min
Response: 27596539
Conc: 206.19 ng/ml

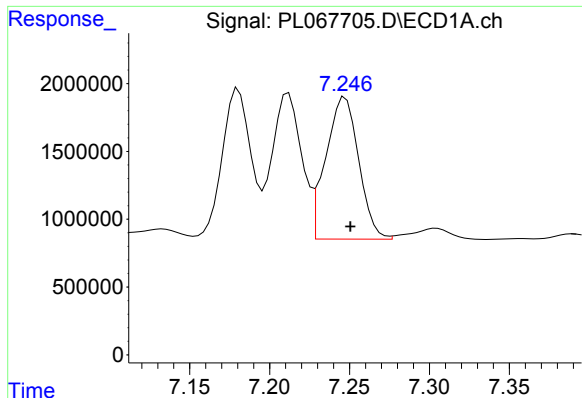


#26 Chlordane-4

R.T.: 7.247 min
Delta R.T.: -0.003 min
Response: 14975182
Conc: 204.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137245BS


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:13 AM

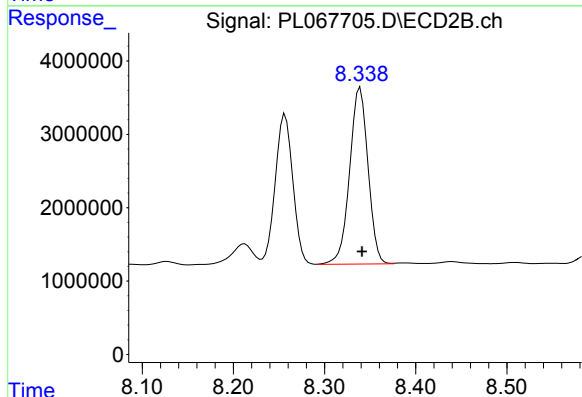


#26 Chlordane-4

R.T.: 8.339 min
Delta R.T.: -0.002 min
Response: 33724246
Conc: 208.05 ng/ml

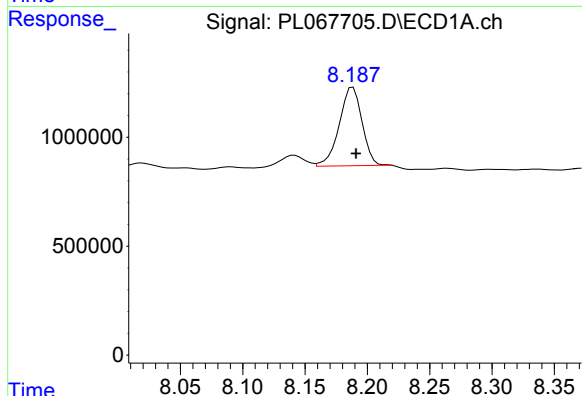


#27 Chlordane-5

R.T.: 8.188 min
Delta R.T.: -0.003 min
Response: 4608254
Conc: 210.62 ng/ml

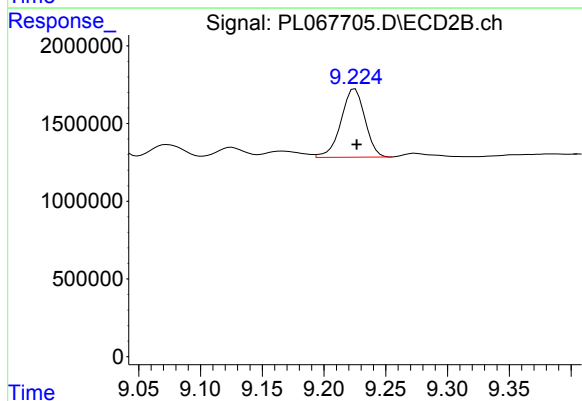

#27 Chlordane-5


R.T.: 9.225 min
Delta R.T.: -0.001 min
Response: 5945609
Conc: 204.47 ng/ml

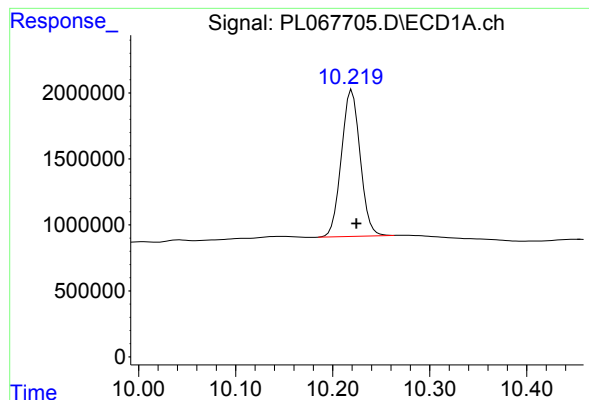

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 14905027
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137245BS

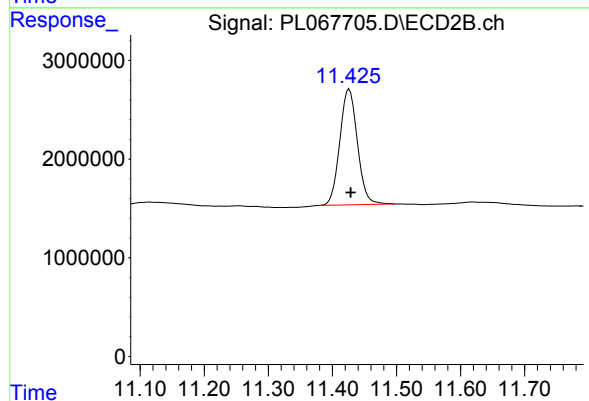

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.002 min
Response: 22368902
Conc: 22.46 ng/ml

Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:13 AM