

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 12:41
 Operator : AR\AJ
 Sample : PB137195BS
 Misc : CHLOR BS
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:25:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.528	11699711	21191250	21.281m	22.479
28)	SA Decachlor...	10.220	11.426	15049329	21545095	21.236	21.630
Target Compounds							
23)	Chlordane-1	5.797	6.909	3922211	5885283	211.990	208.417
24)	Chlordane-2	6.484	7.501	6412357	7925006	239.461	217.444
25)	Chlordane-3	7.180	8.258	13503366	27496892	200.971	205.449
26)	Chlordane-4	7.247	8.340	14760064	33550310	201.975	206.972
27)	Chlordane-5	8.188	9.226	4635025	6045664	211.847	207.914

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 PB137195BS

Manual Integrations
 APPROVED

Ankita
 6/23/2021 10:17:16 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 12:41
Operator : AR\AJ
Sample : PB137195BS
Misc : CHLOR BS
ALS Vial : 12 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:25:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampled :
PB137195BS

Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:16 AM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

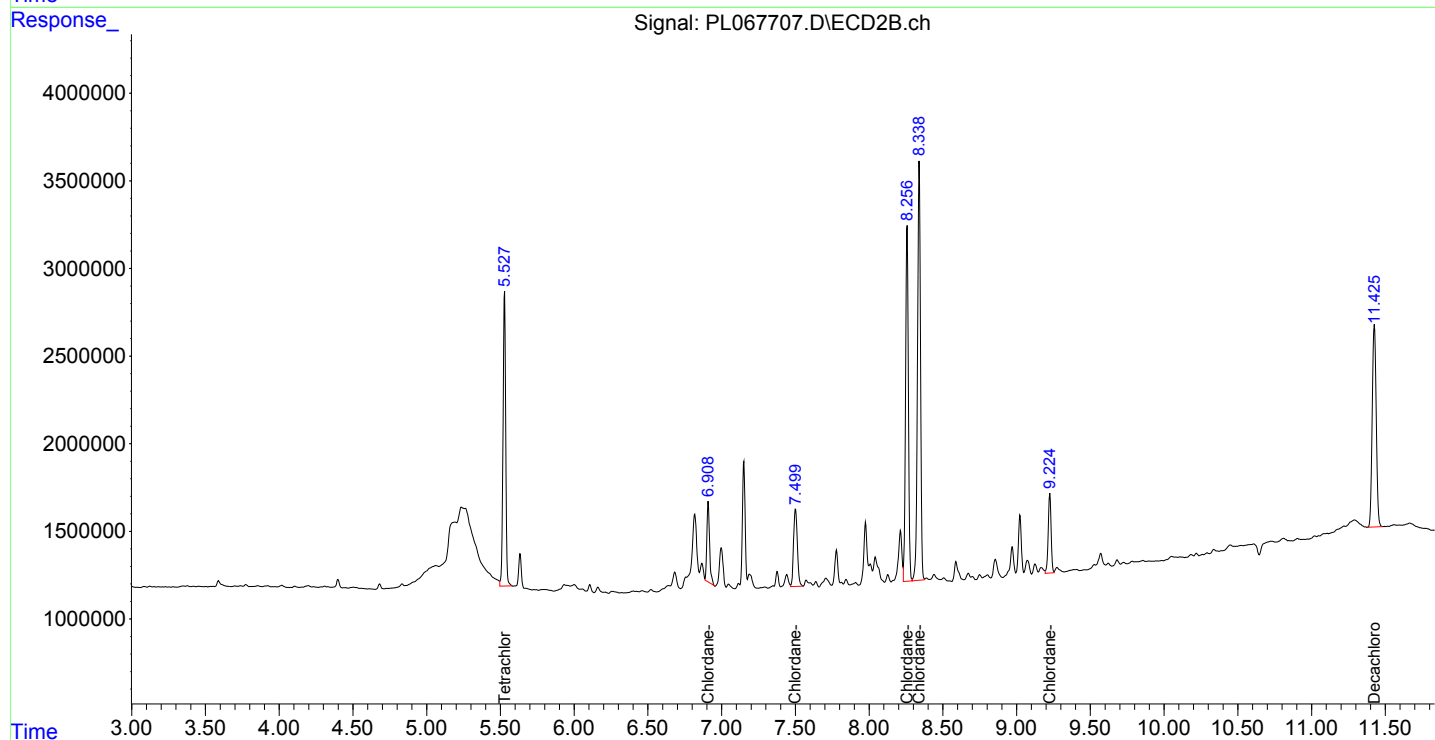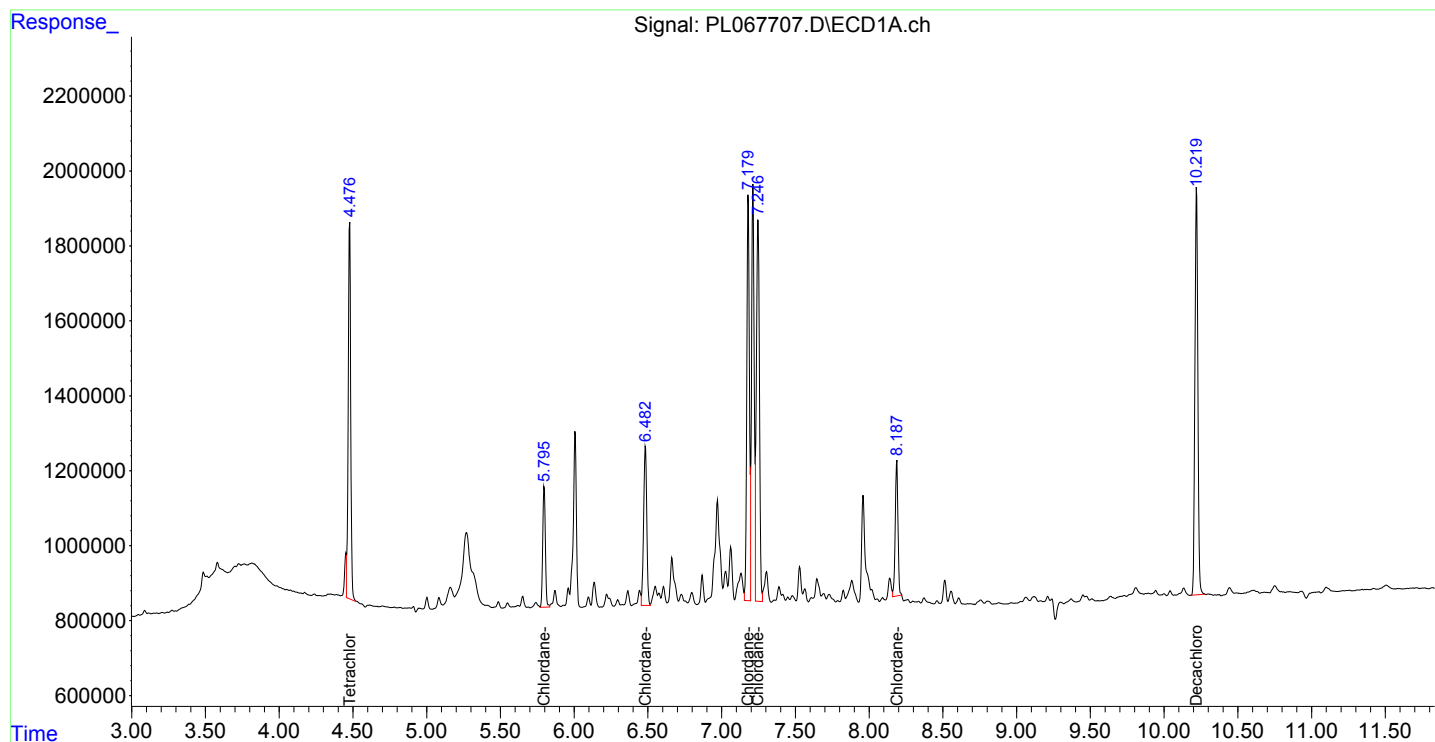

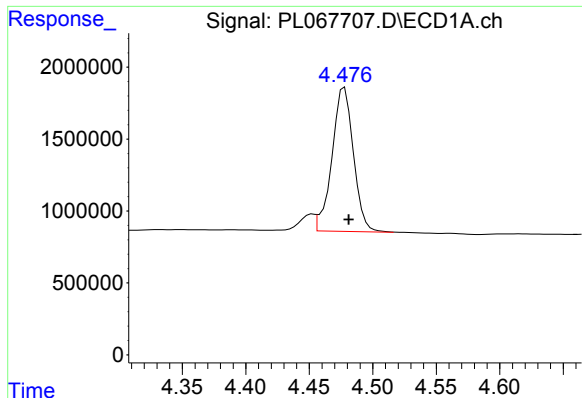


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 11699711
Conc: 21.28 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PB137195BS


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:16 AM

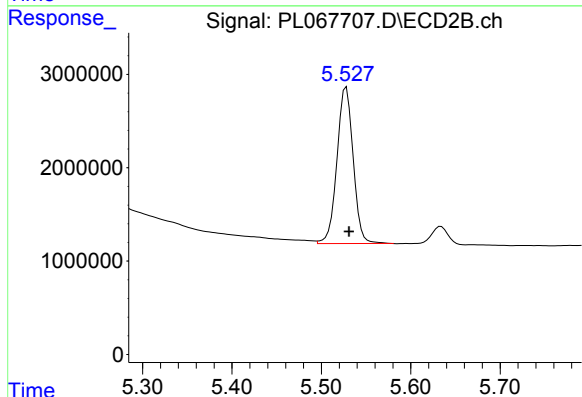


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 21191250
Conc: 22.48 ng/ml

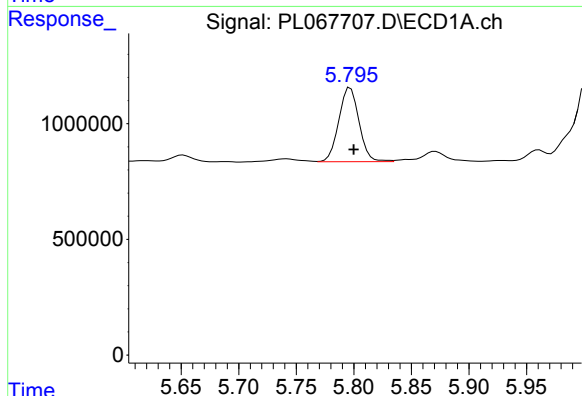


#23 Chlordane-1

R.T.: 5.797 min
Delta R.T.: -0.003 min
Response: 3922211
Conc: 211.99 ng/ml

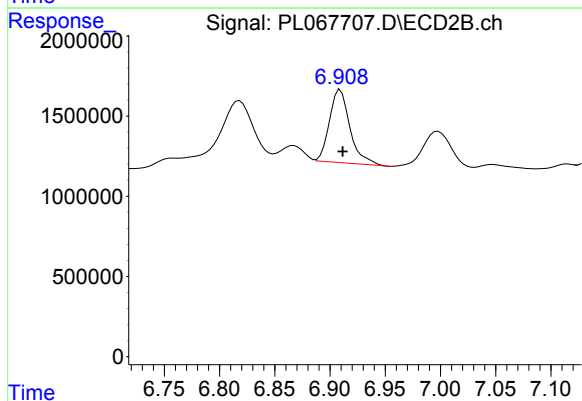

#23 Chlordane-1

R.T.: 6.909 min
Delta R.T.: -0.002 min
Response: 5885283
Conc: 208.42 ng/ml

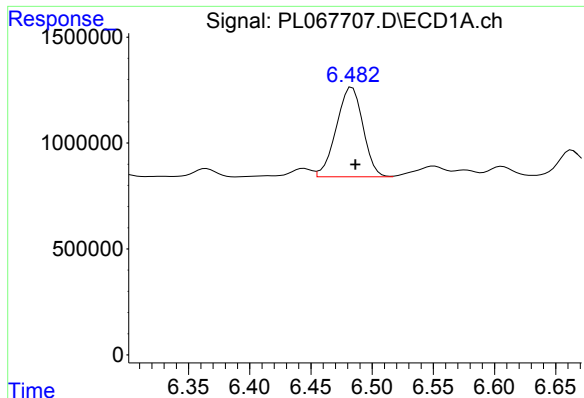


#24 Chlordane-2

R.T.: 6.484 min
Delta R.T.: -0.003 min
Response: 6412357
Conc: 239.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137195BS


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:16 AM

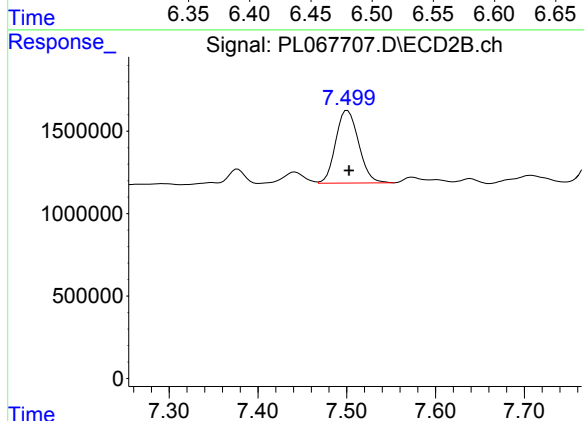


#24 Chlordane-2

R.T.: 7.501 min
Delta R.T.: -0.002 min
Response: 7925006
Conc: 217.44 ng/ml

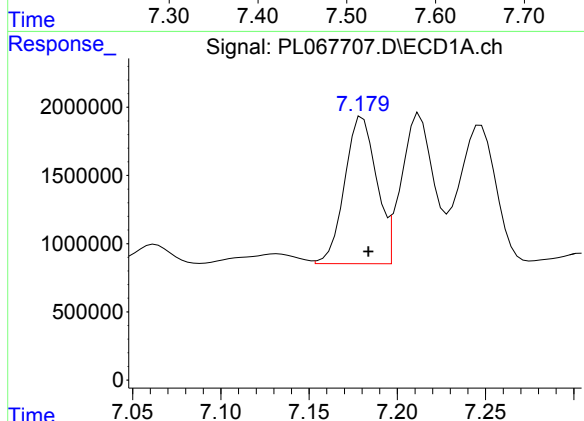


#25 Chlordane-3

R.T.: 7.180 min
Delta R.T.: -0.003 min
Response: 13503366
Conc: 200.97 ng/ml

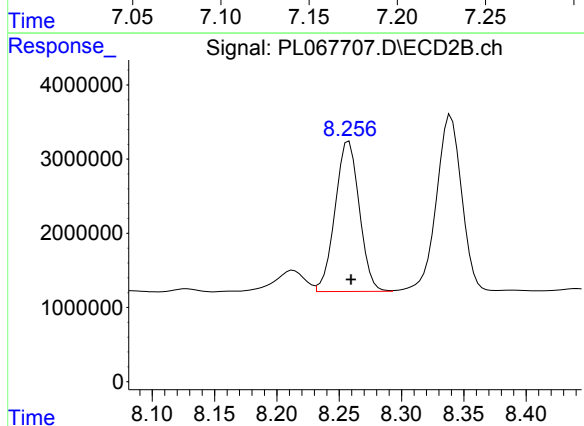

#25 Chlordane-3

R.T.: 8.258 min
Delta R.T.: -0.002 min
Response: 27496892
Conc: 205.45 ng/ml

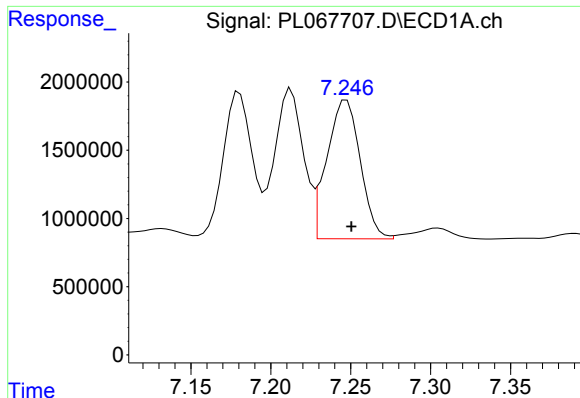


#26 Chlordane-4

R.T.: 7.247 min
Delta R.T.: -0.003 min
Response: 14760064
Conc: 201.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137195BS


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:16 AM

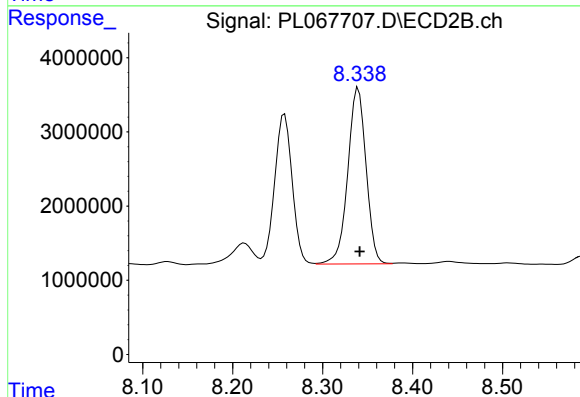


#26 Chlordane-4

R.T.: 8.340 min
Delta R.T.: -0.002 min
Response: 33550310
Conc: 206.97 ng/ml

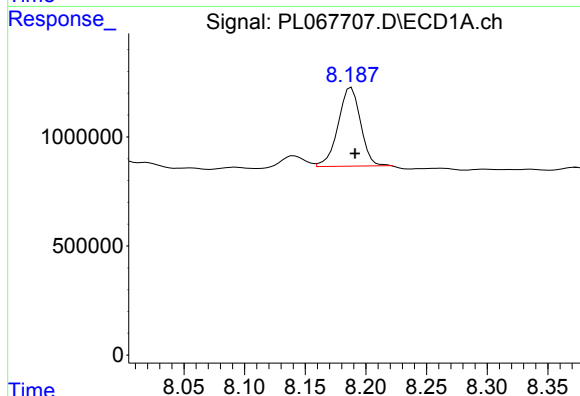


#27 Chlordane-5

R.T.: 8.188 min
Delta R.T.: -0.003 min
Response: 4635025
Conc: 211.85 ng/ml

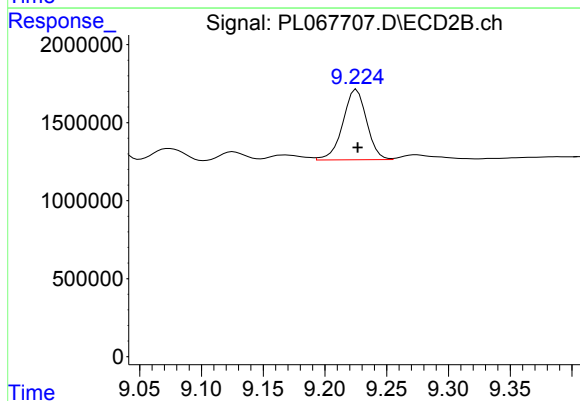

#27 Chlordane-5


R.T.: 9.226 min
Delta R.T.: 0.000 min
Response: 6045664
Conc: 207.91 ng/ml

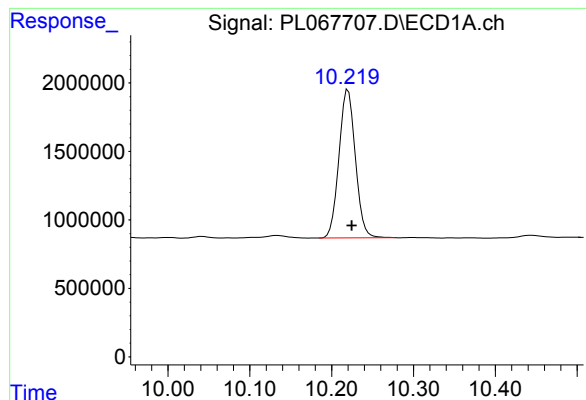

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 15049329
Conc: 21.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137195BS

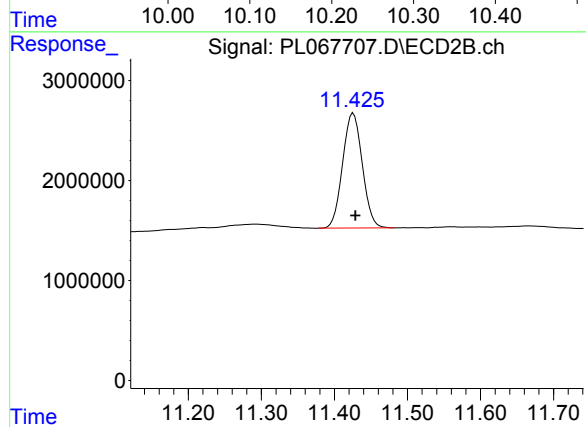

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 21545095
Conc: 21.63 ng/ml

Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:16 AM