

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 13:48
 Operator : AR\AJ
 Sample : M2762-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:27:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	5.530	11472262	19728533	20.867m	20.927
28) SA Decachlor...	10.223	11.432	14414090	21556143	20.339	21.641

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 WC_AQUEOUS_DBD

Manual Integrations
 APPROVED

Ankita
 6/23/2021 10:17:20 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 13:48
Operator : AR\AJ
Sample : M2762-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:27:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampleId :
WC_AQUEOUS_DBD

Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:20 AM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

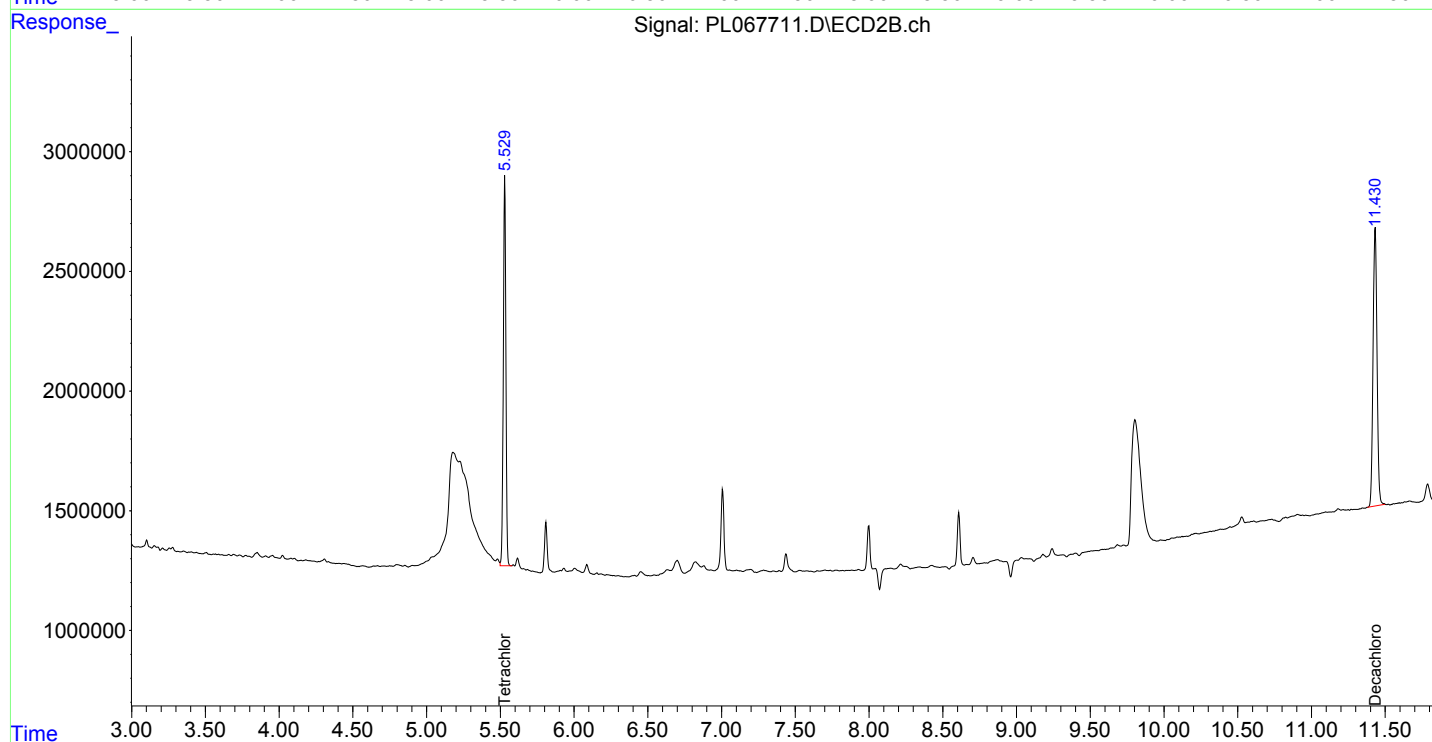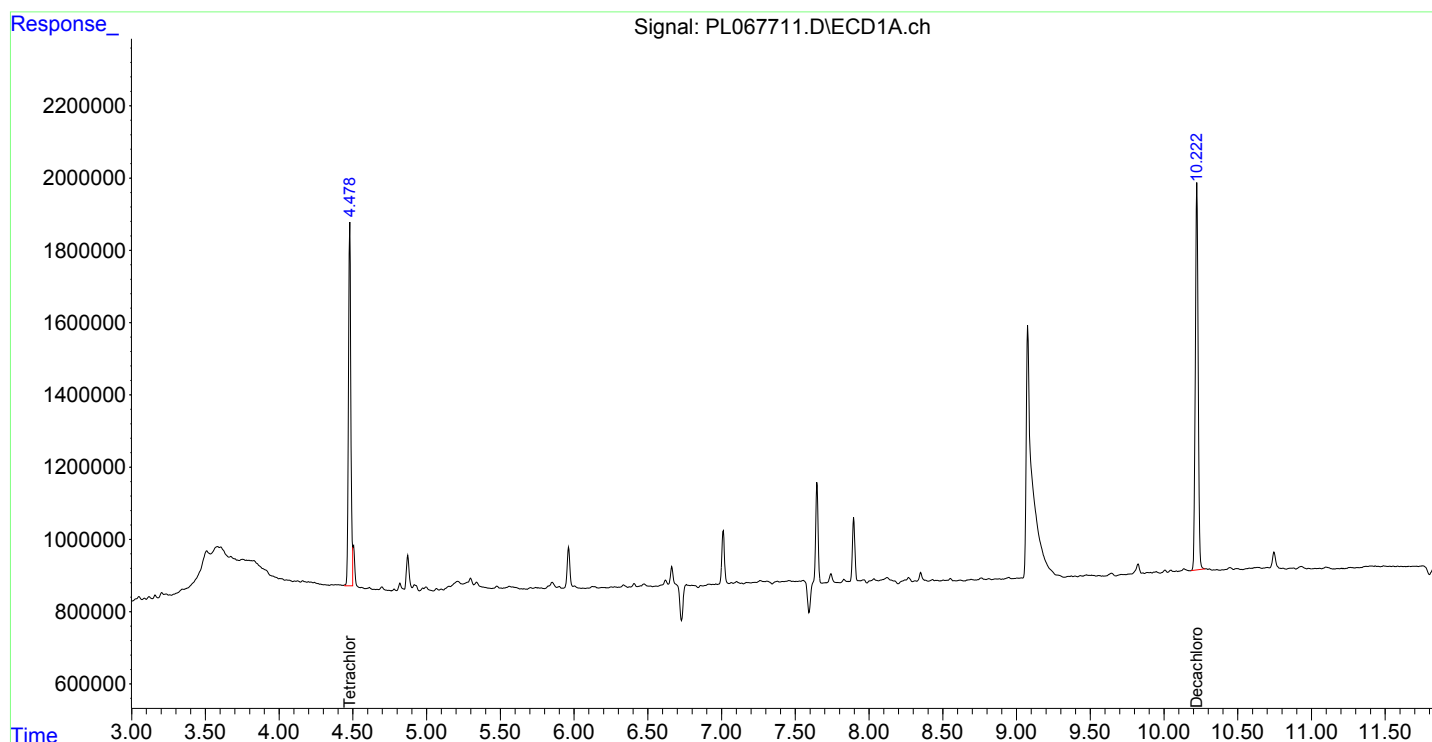

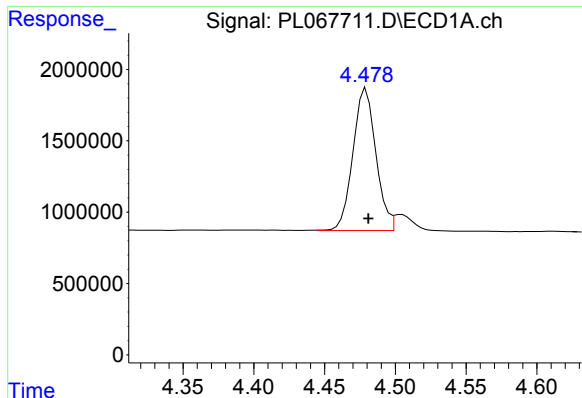


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11472262
Conc: 20.87 ng/ml m

Instrument :
ECD_L
ClientSampleId :
WC_AQUEOUS_DBD


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:20 AM

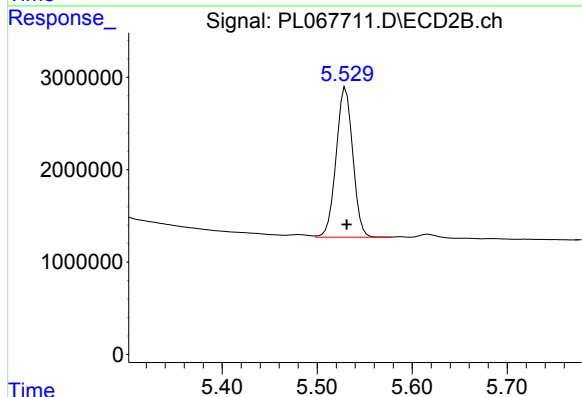


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 19728533
Conc: 20.93 ng/ml

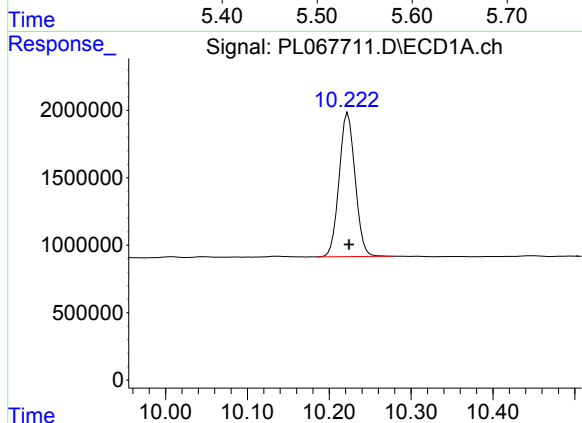

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.001 min
Response: 14414090
Conc: 20.34 ng/ml

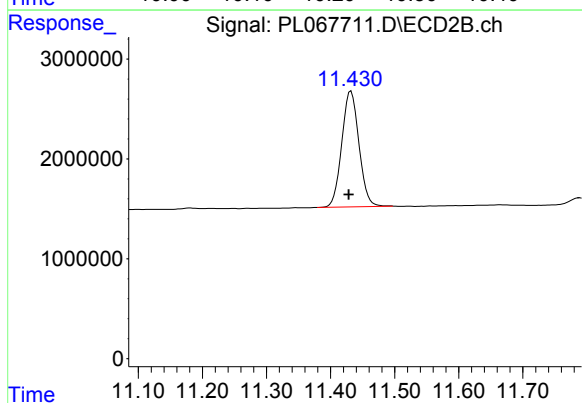

#28 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: 0.003 min
Response: 21556143
Conc: 21.64 ng/ml