

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
 Data File : PL067724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 17:24
 Operator : AR\AJ
 Sample : M2790-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:32:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	5.528	4056745	7338580	7.379	7.784
28) SA Decachlor...	10.218	11.425	6142209	10040747	8.667	10.080
Target Compounds						
12) B 4,4'-DDE	7.466	8.522	1112652	788777	1.672	0.871 #
17) MA 4,4'-DDT	8.306	9.380	827993	769743	1.423	1.050m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-062121

Manual Integrations
 APPROVED

Ankita
 6/23/2021 10:17:31 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062221\
Data File : PL067724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 17:24
Operator : AR\AJ
Sample : M2790-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:32:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation



Instrument :
ECD_L


ClientSampled :
SU-04-062121

Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:31 AM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

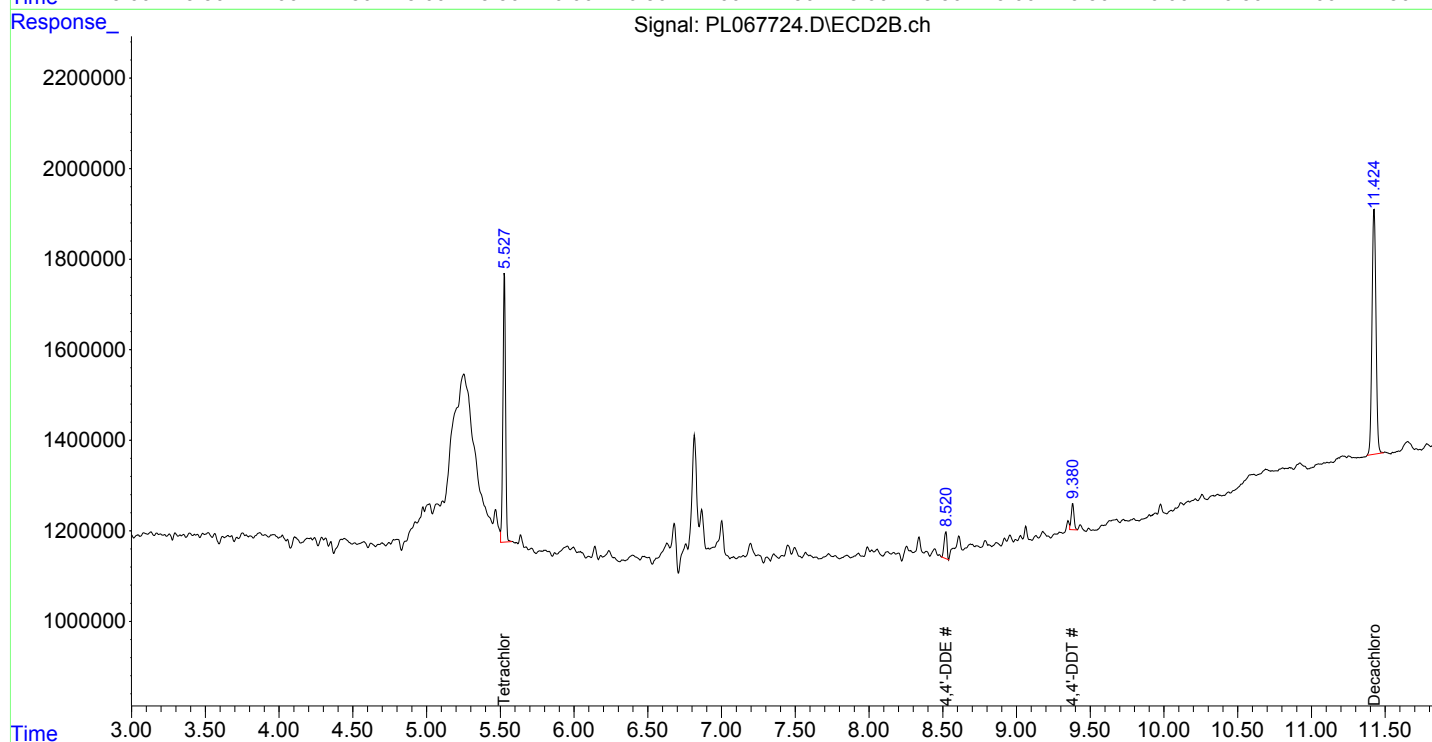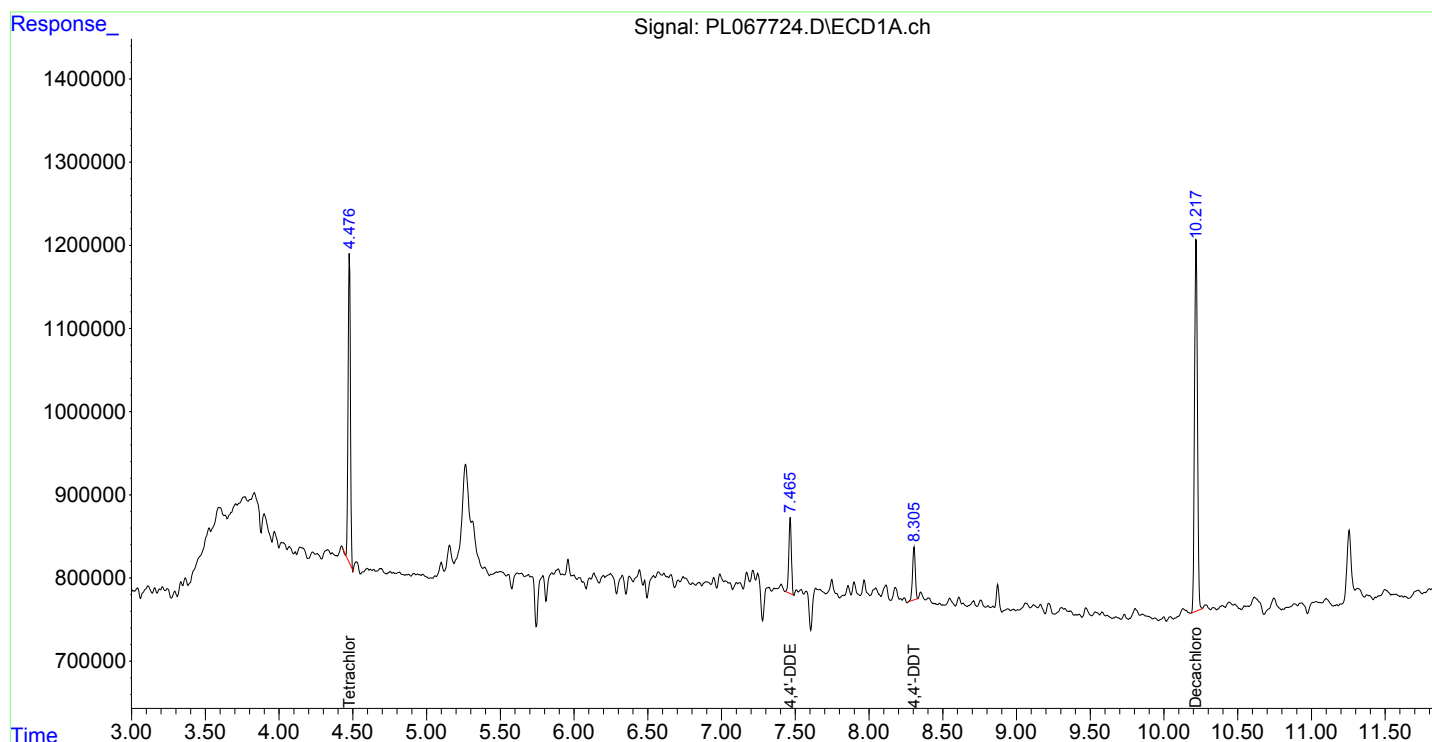

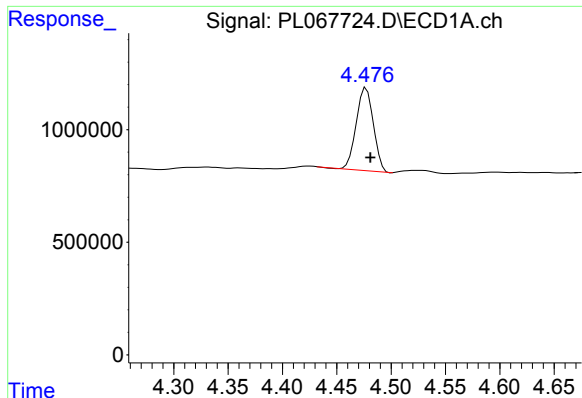


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 4056745
Conc: 7.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-062121


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:31 AM

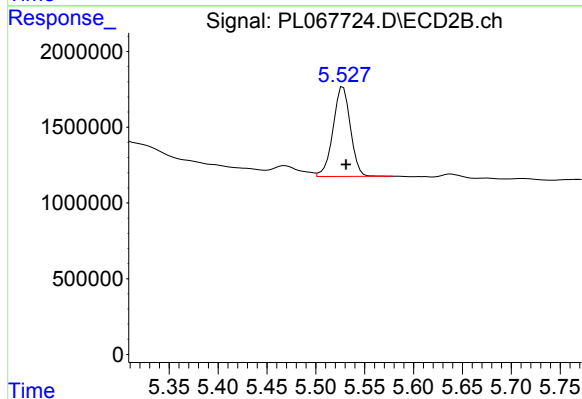


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 7338580
Conc: 7.78 ng/ml

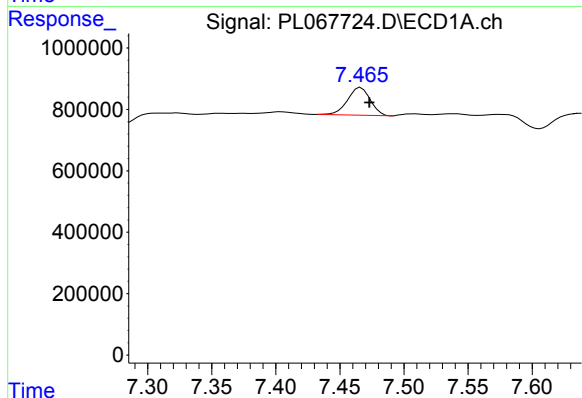


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 1112652
Conc: 1.67 ng/ml

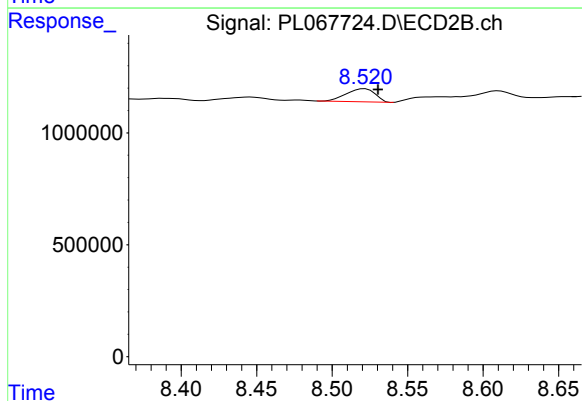

#12 4,4'-DDE

R.T.: 8.522 min
Delta R.T.: -0.009 min
Response: 788777
Conc: 0.87 ng/ml

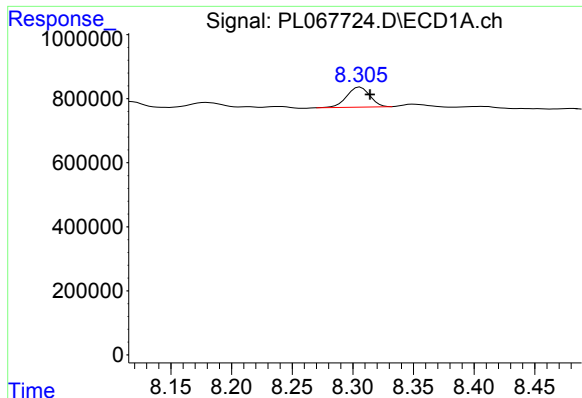


#17 4,4'-DDT

R.T.: 8.306 min
Delta R.T.: -0.008 min
Response: 827993
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-062121


Manual Integrations
APPROVED

Ankita
6/23/2021 10:17:31 AM

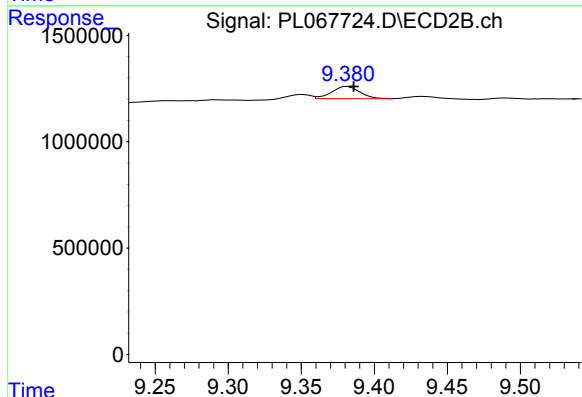


#17 4,4'-DDT

R.T.: 9.380 min
Delta R.T.: -0.006 min
Response: 769743
Conc: 1.05 ng/ml m

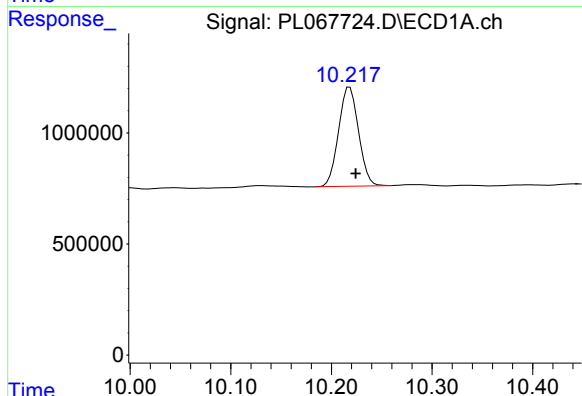

#28 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.006 min
Response: 6142209
Conc: 8.67 ng/ml

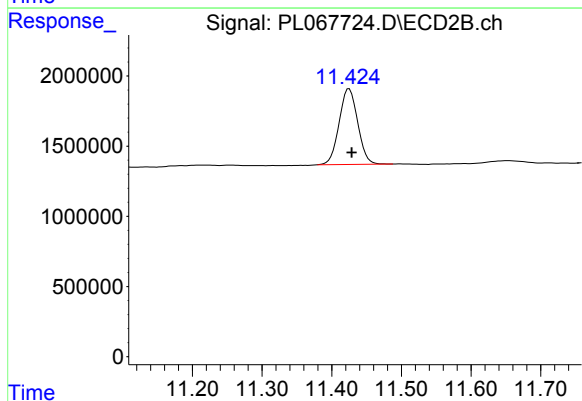

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.004 min
Response: 10040747
Conc: 10.08 ng/ml