

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062318\
 Data File : PL037341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2018 15:09
 Operator : UA\AJ
 Sample : J3570-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:38:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.938	122.1E6	40362496	15.437	14.589
28)	SA Decachlor...	8.019	8.950	88859274	31807704	14.726	16.033
Target Compounds							
2)	A alpha-BHC	3.756	0.000	7670673	0	0.627	N.D. #
3)	MA gamma-BHC...	4.059	0.000	9728819	0	0.943	N.D. #
6)	B beta-BHC	4.259f	0.000	26913279	0	5.901	N.D. #
7)	B delta-BHC	0.000	4.965	0	8922036	N.D.	3.164 #
10)	B gamma-Chl...	5.165f	0.000	19817508	0	2.116	N.D. #
15)	B Endosulfa...	6.051f	0.000	13174881	0	1.792	N.D. #
23)	Chlordane-1	4.114	4.965	14688224	8922036	47.836	74.251 #
25)	Chlordane-3	5.165	0.000	19817508	0	18.644	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062318\
Data File : PL037341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2018 15:09
Operator : UA\AJ
Sample : J3570-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:38:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

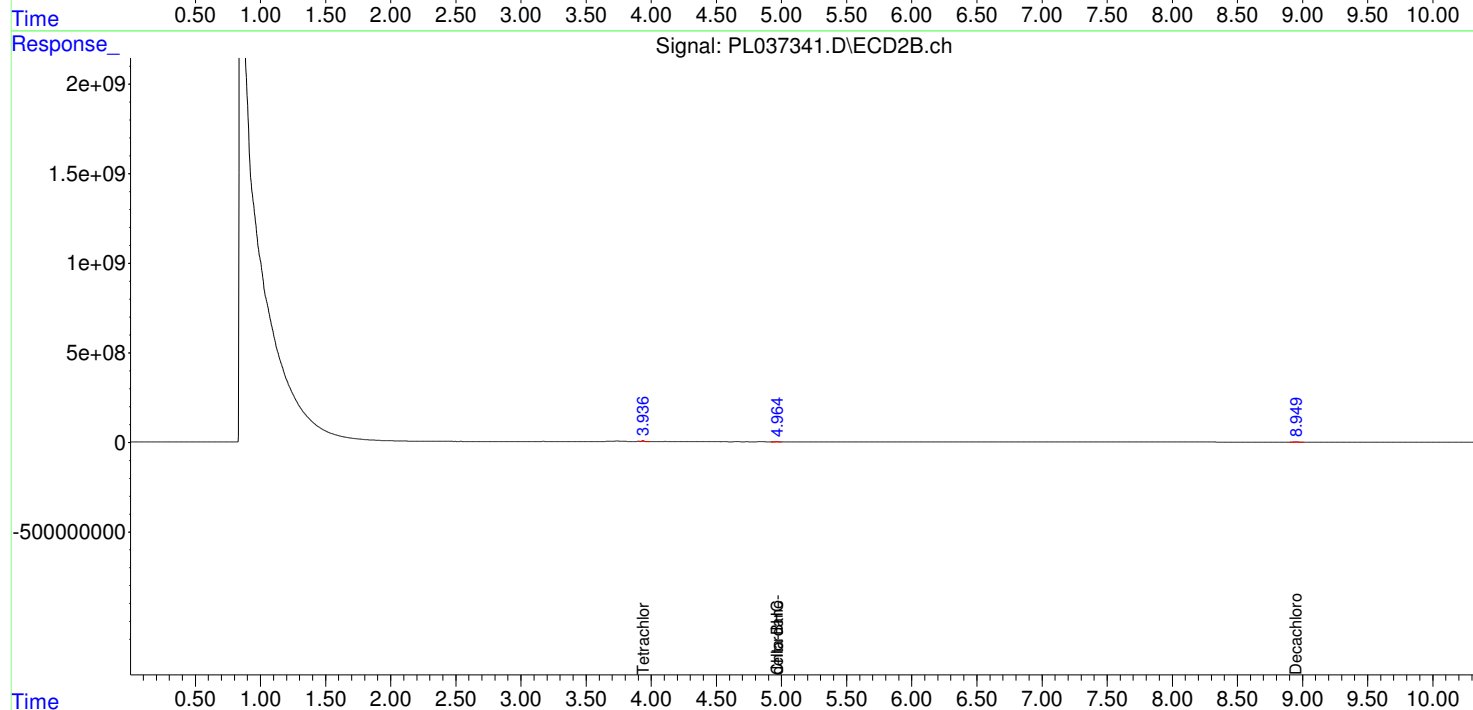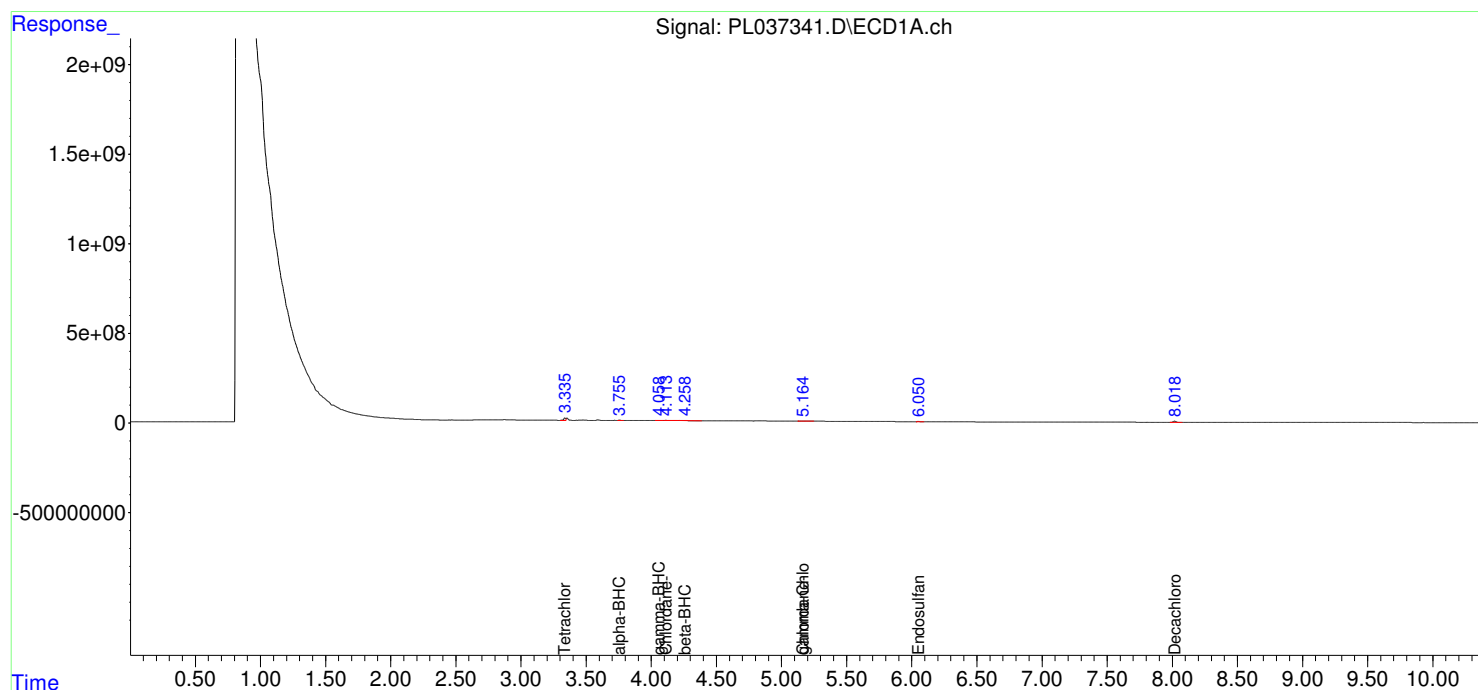


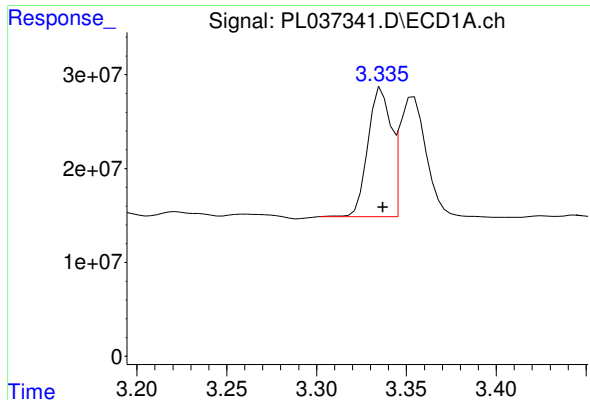

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 122108124
Conc: 15.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

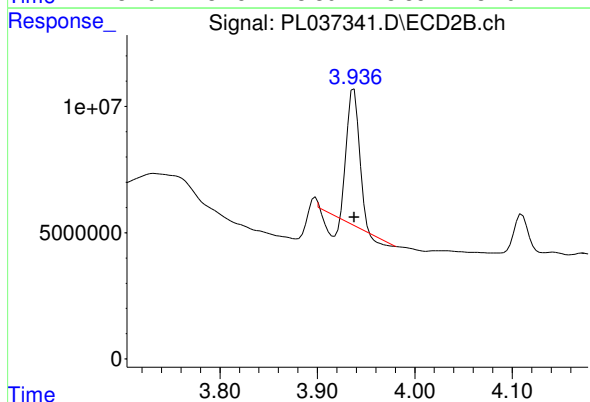


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 40362496
Conc: 14.59 ng/ml

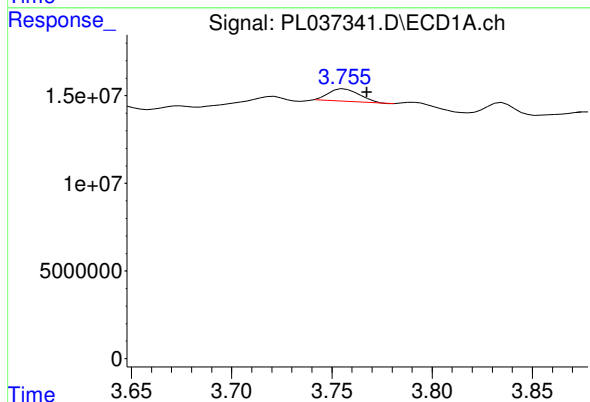


#2 alpha-BHC

R.T.: 3.756 min
Delta R.T.: -0.011 min
Response: 7670673
Conc: 0.63 ng/ml

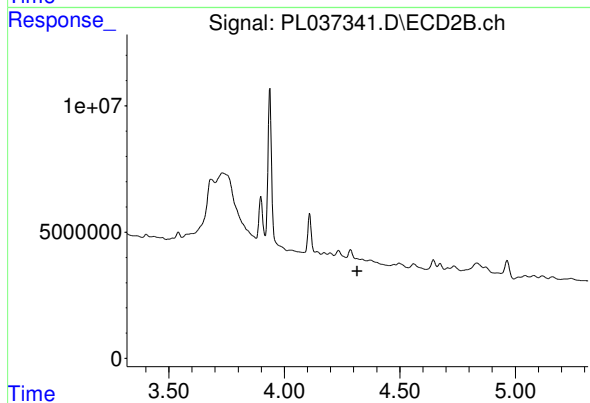

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.317 min
Response: 0
Conc: N.D.

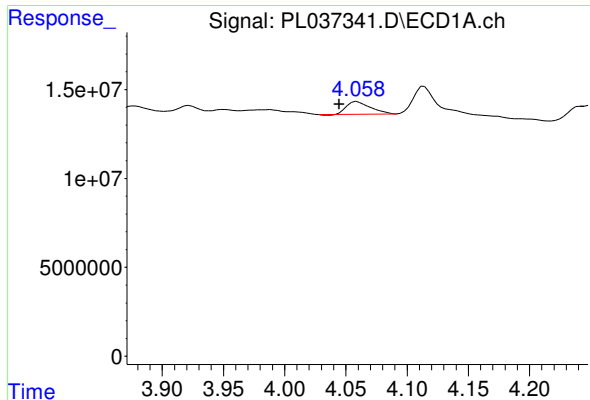

#3 gamma-BHC (Lindane)


R.T.: 4.059 min
Delta R.T.: 0.015 min
Response: 9728819
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

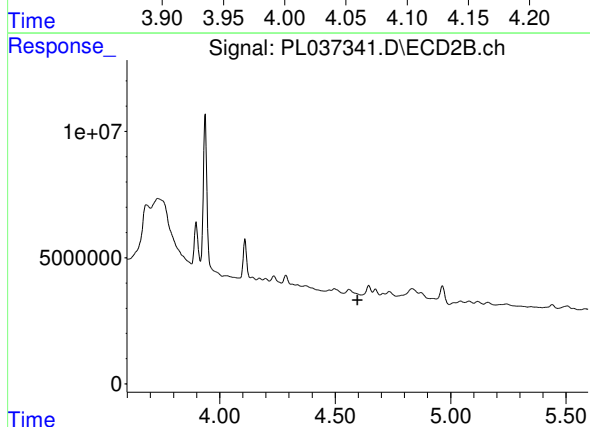


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

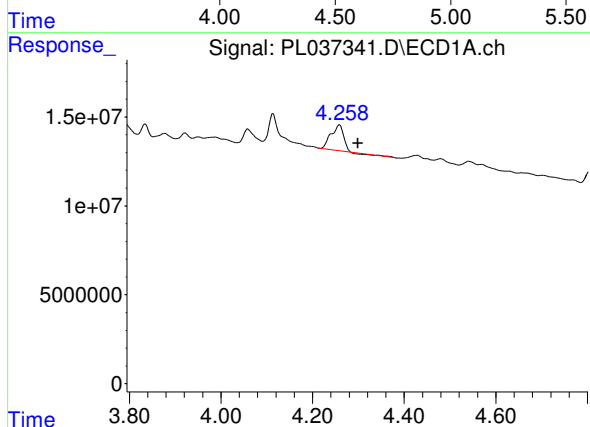


#6 beta-BHC

R.T.: 4.259 min
Delta R.T.: -0.040 min
Response: 26913279
Conc: 5.90 ng/ml

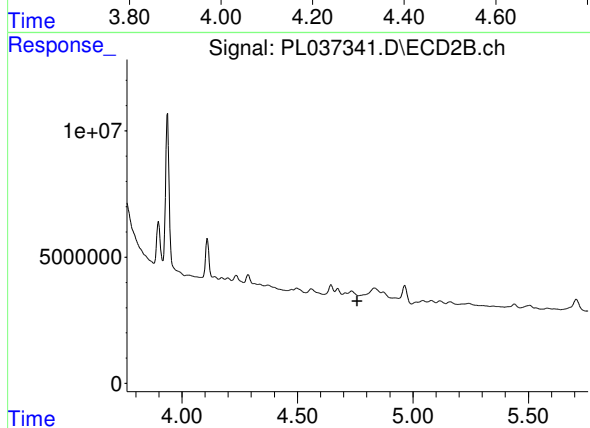

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

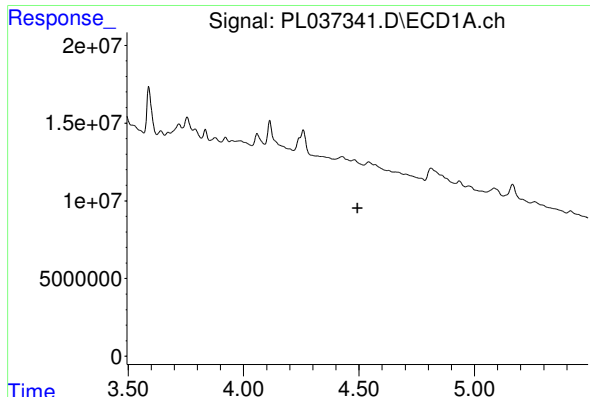

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

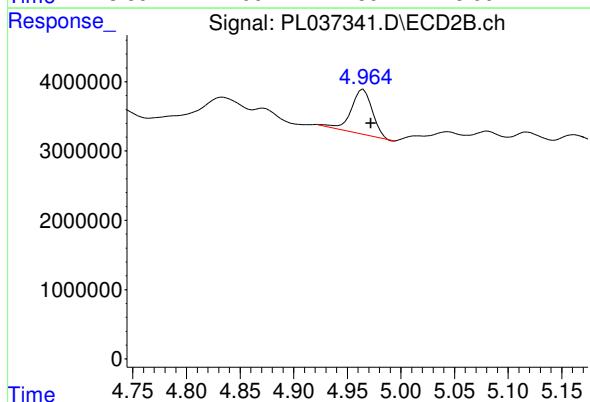


#7 delta-BHC

R.T.: 4.965 min
Delta R.T.: -0.007 min
Response: 8922036
Conc: 3.16 ng/ml

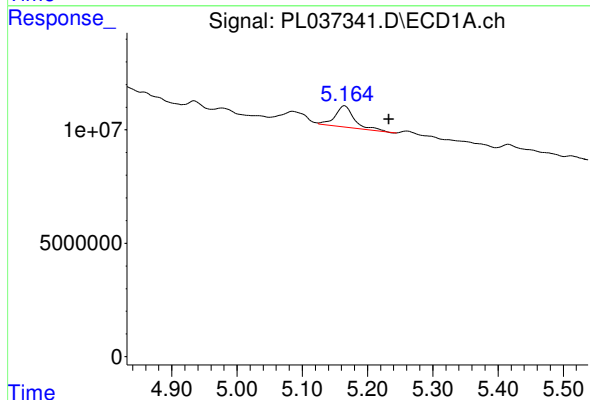


#10 gamma-Chlordane

R.T.: 5.165 min
Delta R.T.: -0.007 min
Response: 19817508
Conc: 2.12 ng/ml

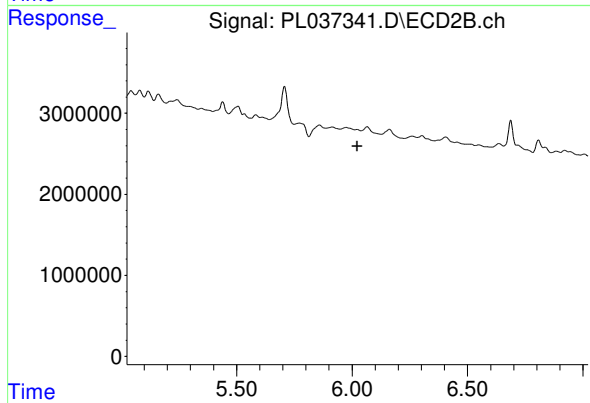

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

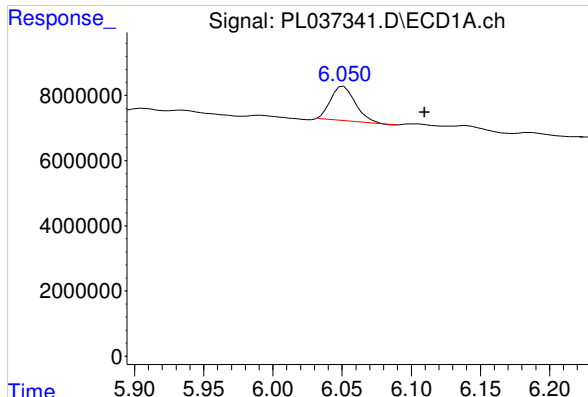

#15 Endosulfan II


R.T.: 6.051 min
Delta R.T.: -0.059 min
Response: 13174881
Conc: 1.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

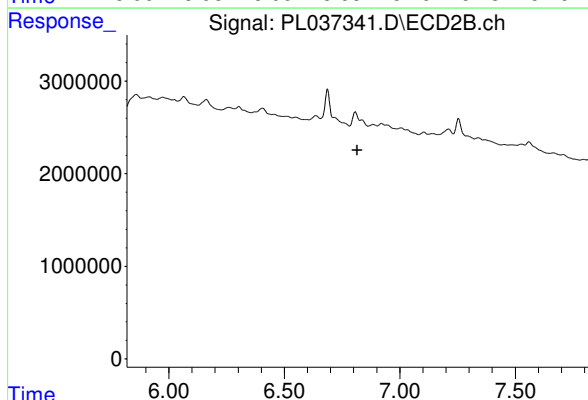


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.814 min
Response: 0
Conc: N.D.

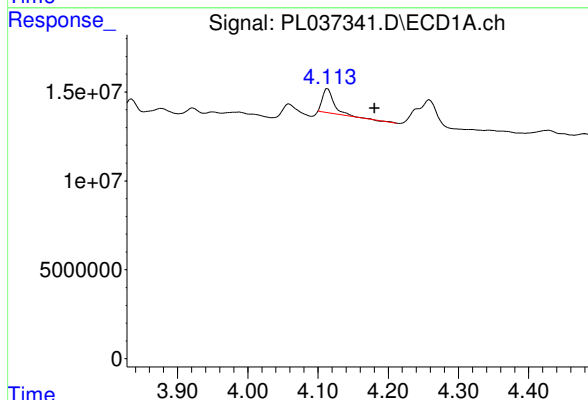


#23 Chlordane-1

R.T.: 4.114 min
Delta R.T.: -0.067 min
Response: 14688224
Conc: 47.84 ng/ml

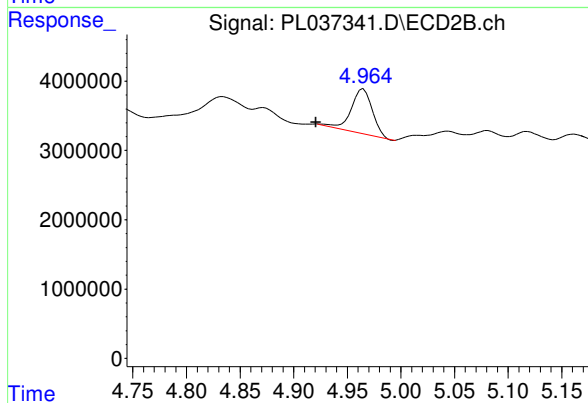

#23 Chlordane-1


R.T.: 4.965 min
Delta R.T.: 0.044 min
Response: 8922036
Conc: 74.25 ng/ml

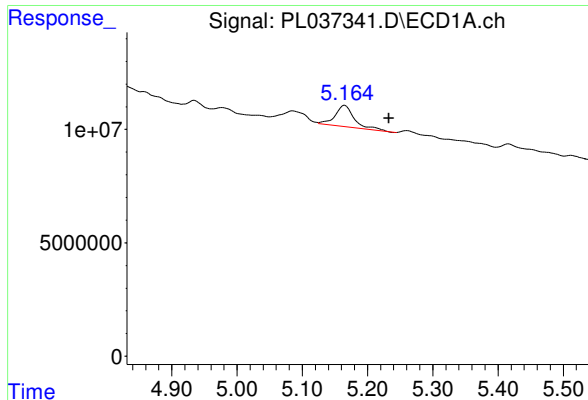

#25 Chlordane-3


R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 19817508
Conc: 18.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

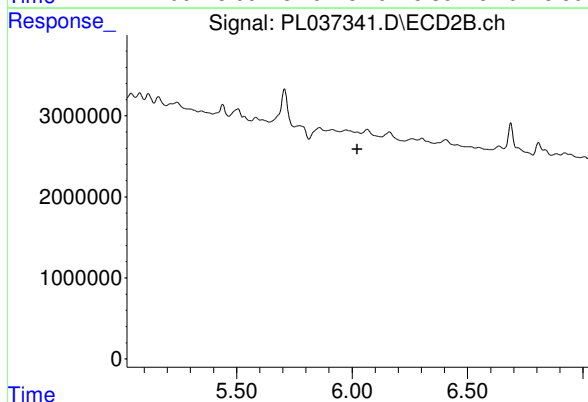


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

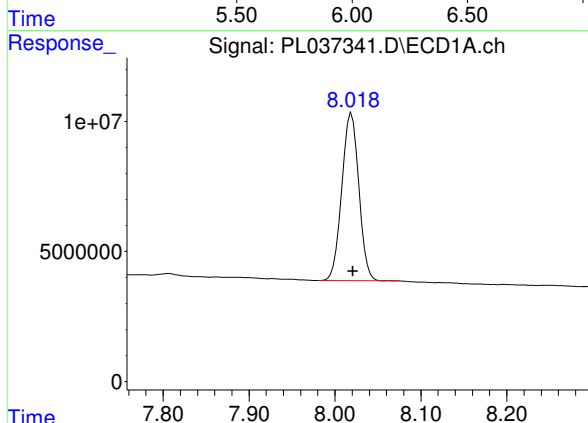

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.001 min
Response: 88859274
Conc: 14.73 ng/ml

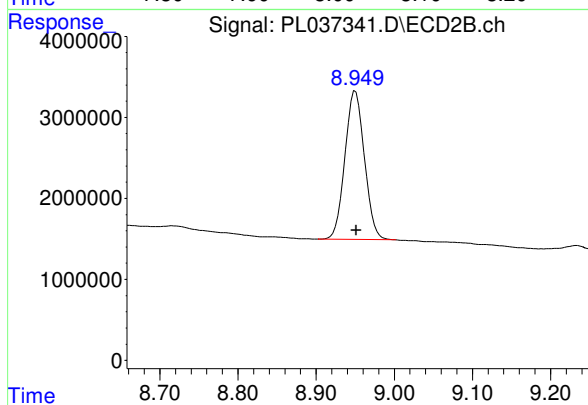

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 31807704
Conc: 16.03 ng/ml