

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062318\
 Data File : PL037340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2018 14:55
 Operator : UA\AJ
 Sample : J3627-35
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GROUND-WATER

Manual Integrations
 APPROVED

ugo
 6/25/2018 1:43:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:37:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.937	120.9E6	46053454	15.285m	16.645
28)	SA Decachlor...	8.018	8.950	81661928	30026929	13.534	15.135

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062318\
Data File : PL037340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2018 14:55
Operator : UA\AJ
Sample : J3627-35
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

ugo
6/25/2018 1:43:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:37:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

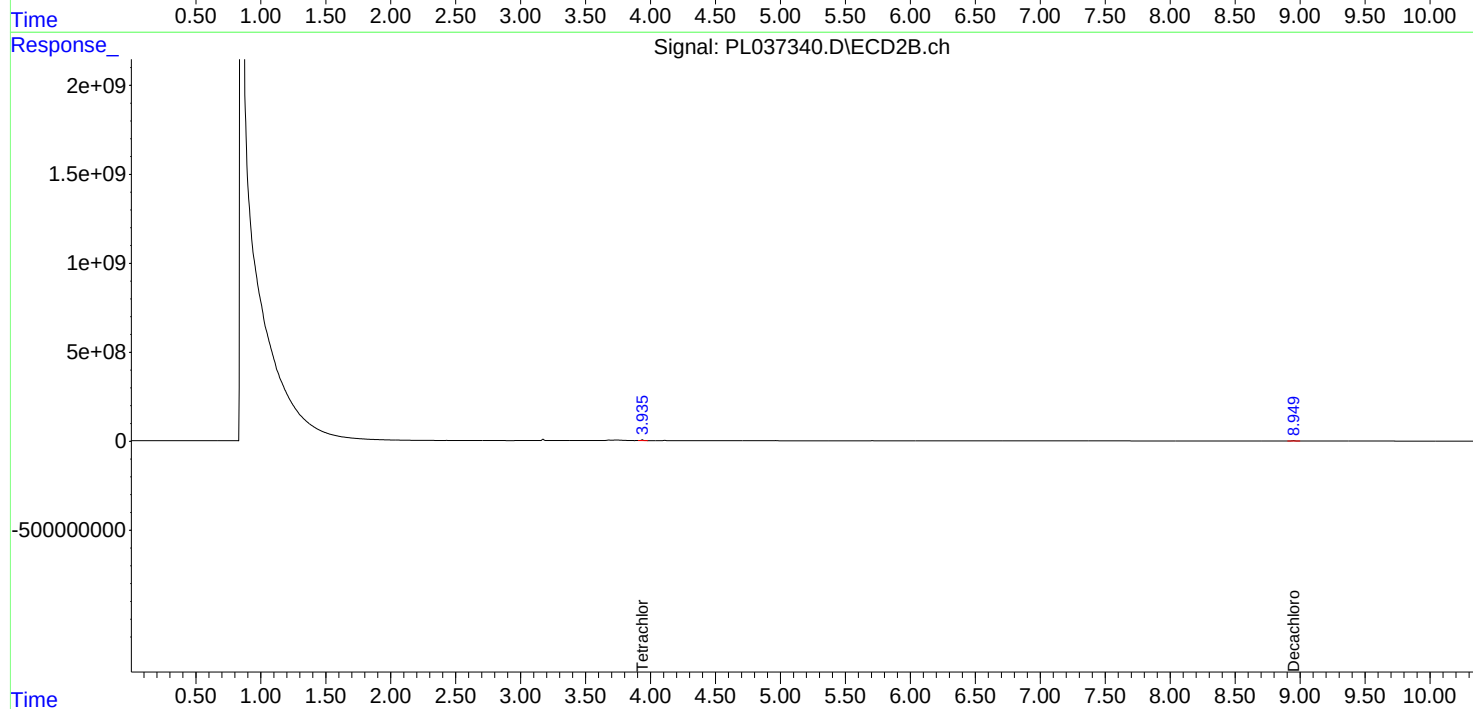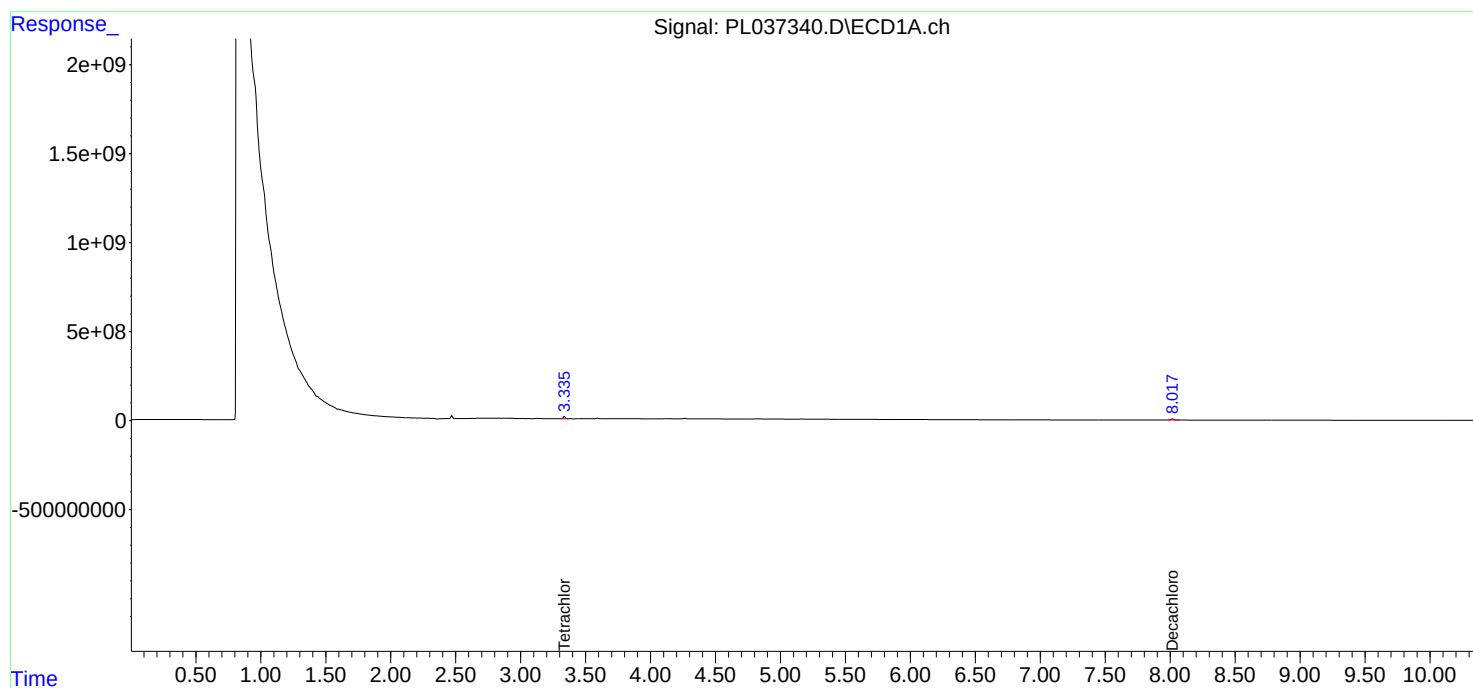

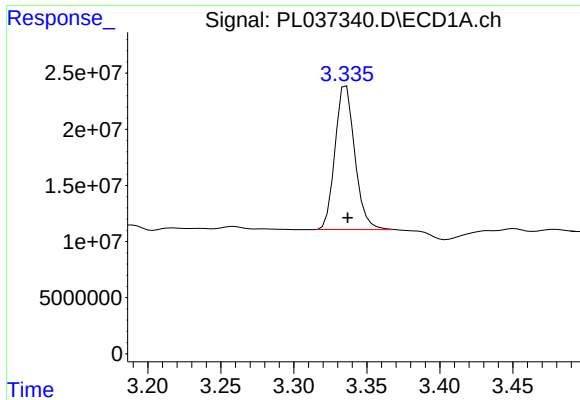


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 120906035
Conc: 15.28 ng/ml m

Instrument :
ECD_L
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

ugo
6/25/2018 1:43:58 PM

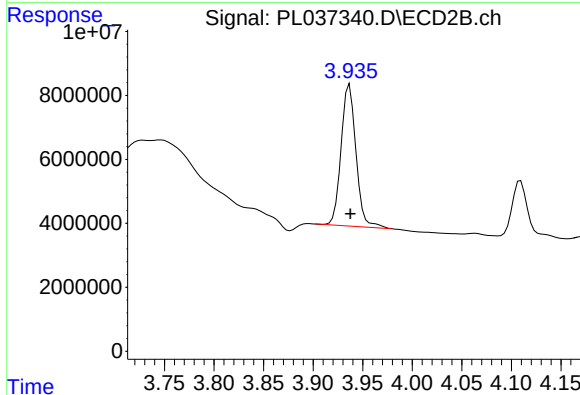


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 46053454
Conc: 16.65 ng/ml

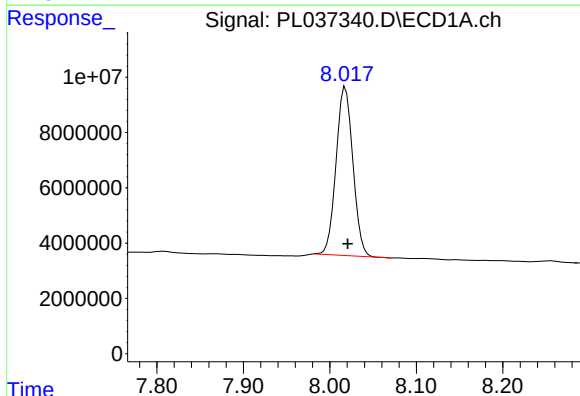

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 81661928
Conc: 13.53 ng/ml

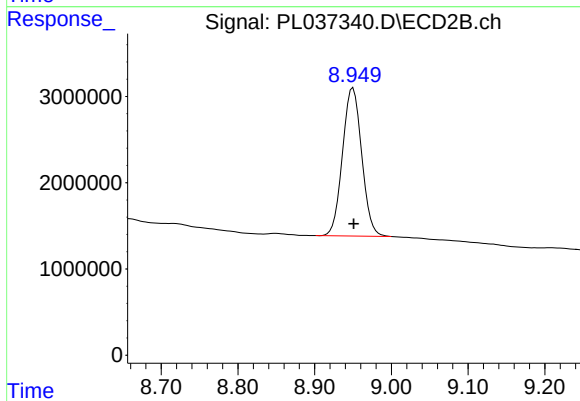

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 30026929
Conc: 15.13 ng/ml