

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
 Data File : PL067765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 18:14
 Operator : AR\AJ
 Sample : M2795-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:49:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	10355666	18888448	18.836	20.036
28)	SA Decachlor...	10.219	11.424	13081164	19542740	18.458	19.620
Target Compounds							
2)	A alpha-BHC	5.206f	0.000	80745	0	0.110	N.D. #
5)	MB Aldrin	6.337	0.000	212780	0	0.289	N.D. #
7)	B delta-BHC	0.000	6.999f	0	1393084	N.D.	1.185 #
11)	B alpha-Chl...	7.251	0.000	196303	0	0.268	N.D. #
15)	B Endosulfa...	0.000	9.179f	0	668399	N.D.	0.838 #
16)	A 4,4'-DDD	8.031f	0.000	168517	0	0.290	N.D. #
18)	B Endrin al...	0.000	9.320f	0	166402	N.D.	0.261 #
21)	B Endrin ke...	9.142f	10.050f	-8456	249240	N.D.	0.275
26)	Chlordane-4	7.251	0.000	196303	0	2.686	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
Data File : PL067765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:14
Operator : AR\AJ
Sample : M2795-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:49:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

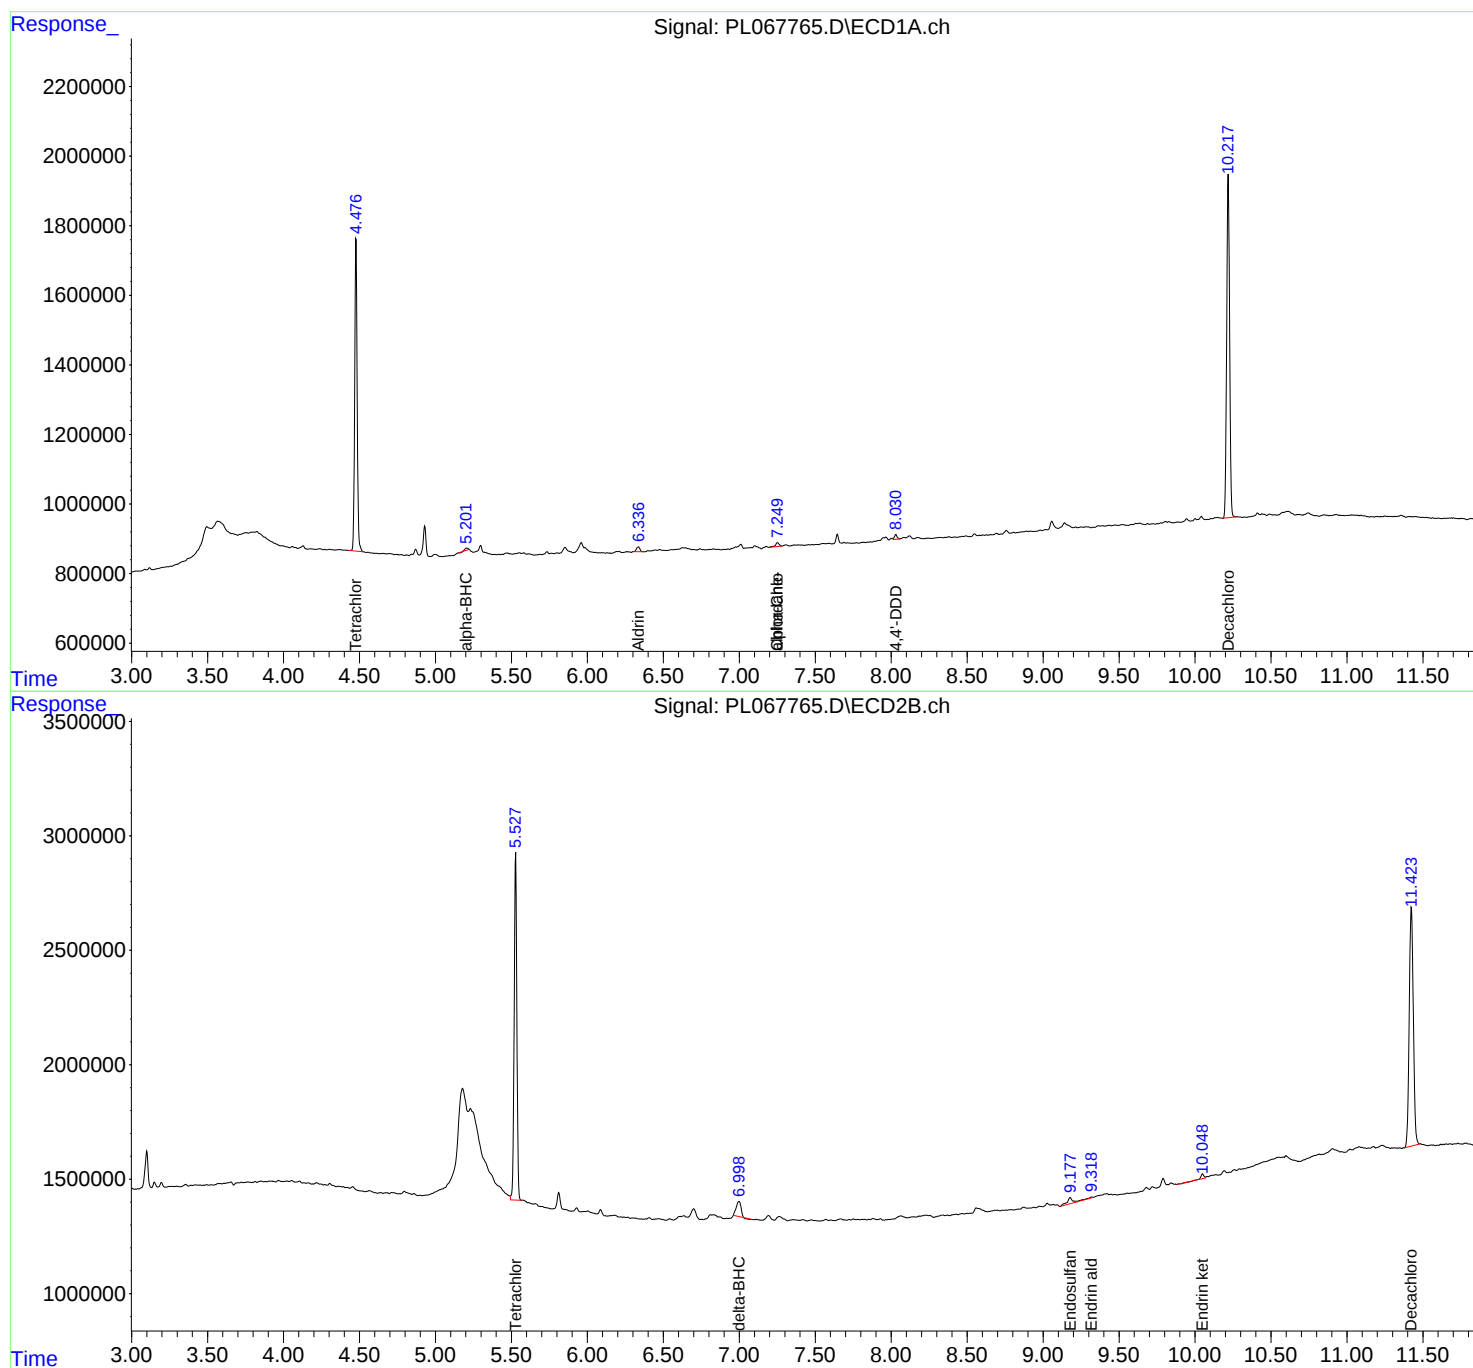


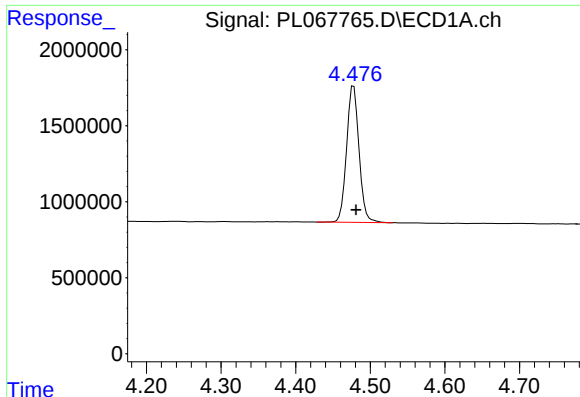

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10355666
Conc: 18.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

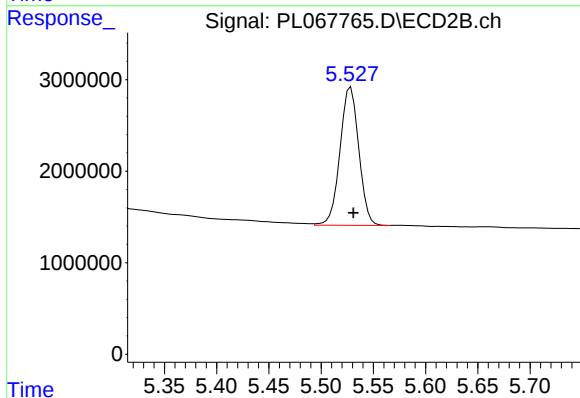


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 18888448
Conc: 20.04 ng/ml

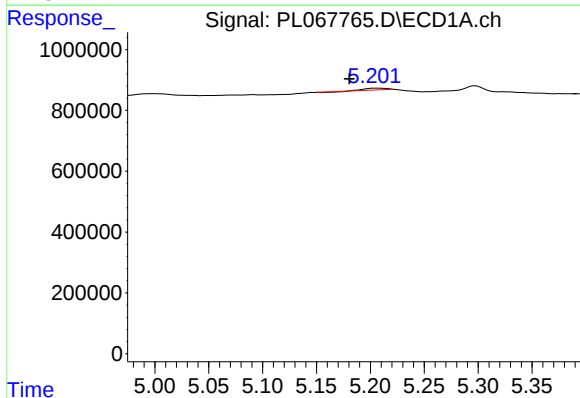


#2 alpha-BHC

R.T.: 5.206 min
Delta R.T.: 0.025 min
Response: 80745
Conc: 0.11 ng/ml

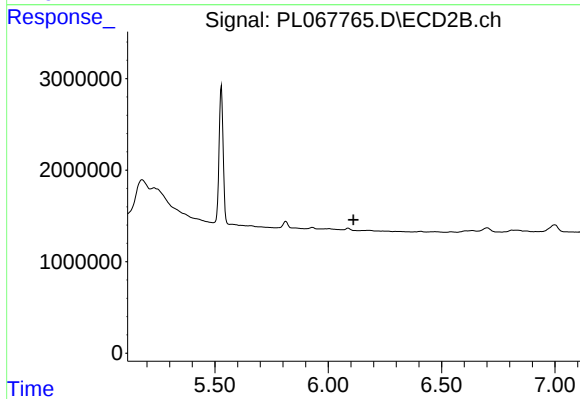

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

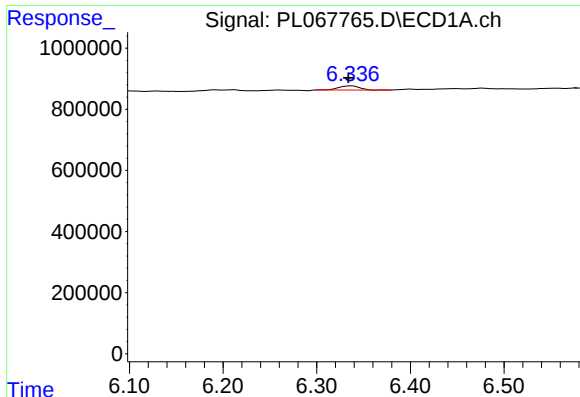

#5 Aldrin


R.T.: 6.337 min
Delta R.T.: 0.003 min
Response: 212780
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

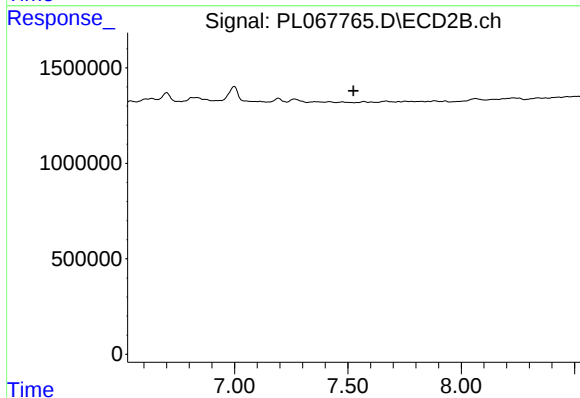


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

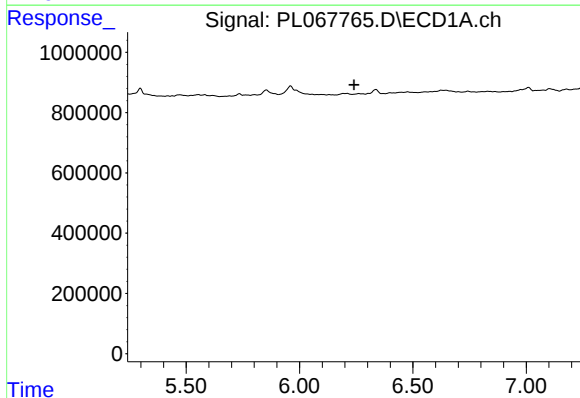


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

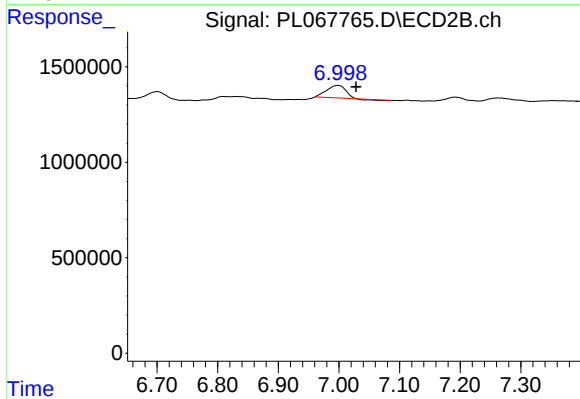

#7 delta-BHC


R.T.: 6.999 min
Delta R.T.: -0.029 min
Response: 1393084
Conc: 1.19 ng/ml

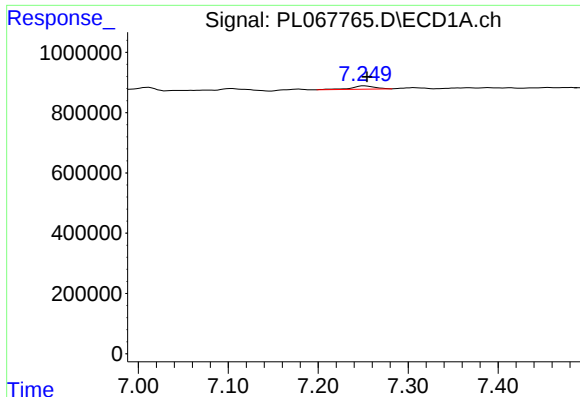

#11 alpha-Chlordane


R.T.: 7.251 min
Delta R.T.: -0.003 min
Response: 196303
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

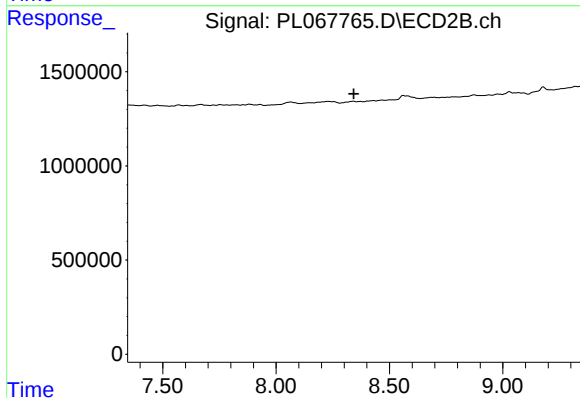


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

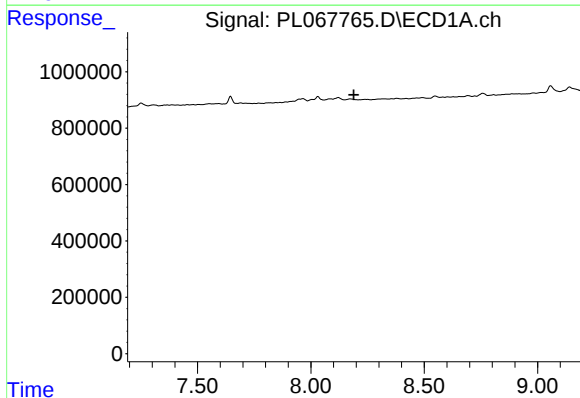


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

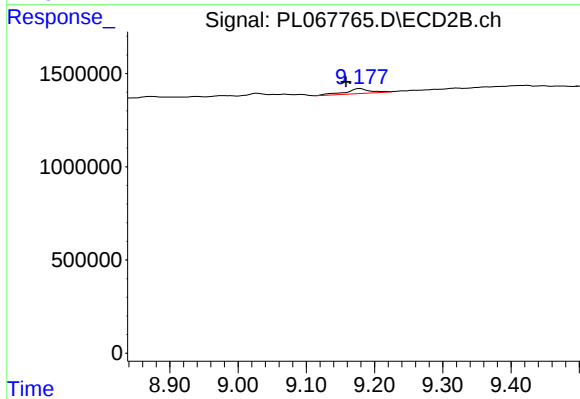

#15 Endosulfan II


R.T.: 9.179 min
Delta R.T.: 0.020 min
Response: 668399
Conc: 0.84 ng/ml

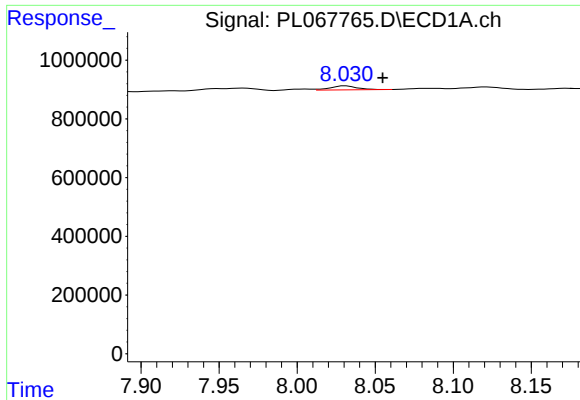

#16 4,4'-DDD


R.T.: 8.031 min
Delta R.T.: -0.023 min
Response: 168517
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

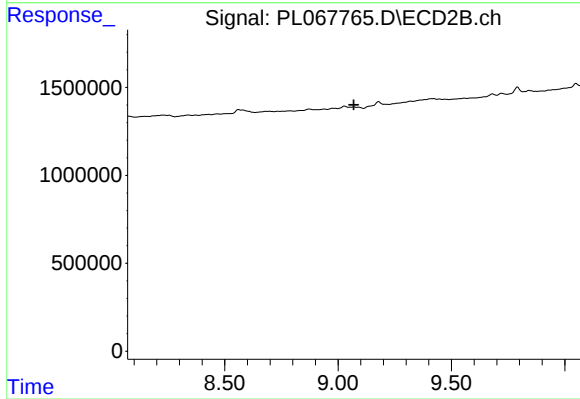


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

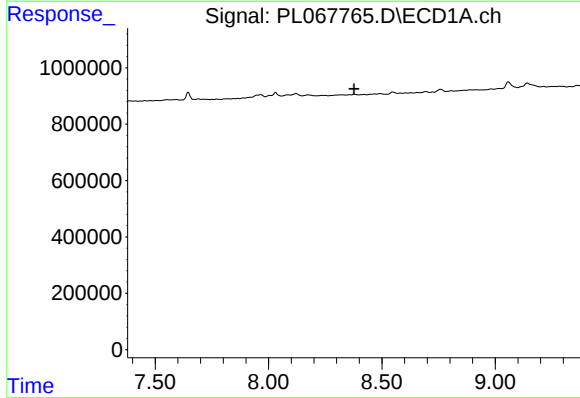


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.377 min
Response: 0
Conc: N.D.

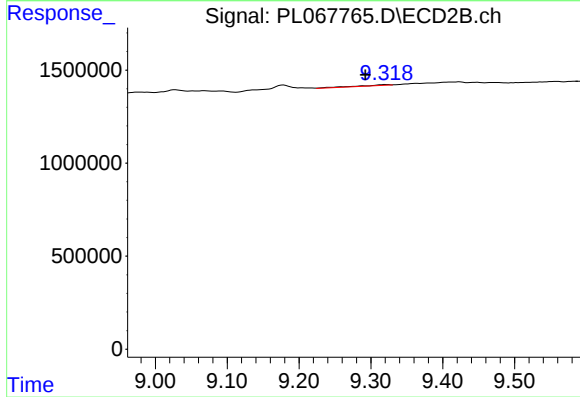

#18 Endrin aldehyde


R.T.: 9.320 min
Delta R.T.: 0.027 min
Response: 166402
Conc: 0.26 ng/ml

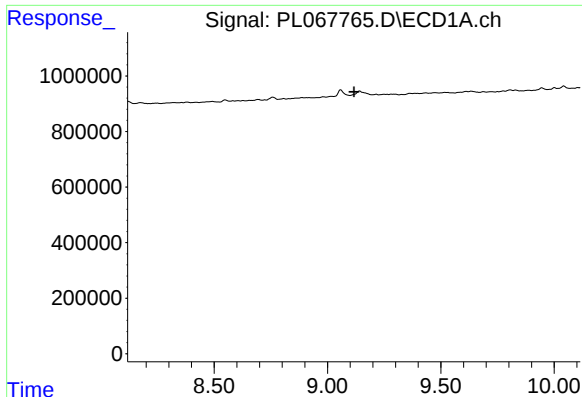

#21 Endrin ketone


R.T.: 9.142 min
Delta R.T.: 0.025 min
Response: -8456
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

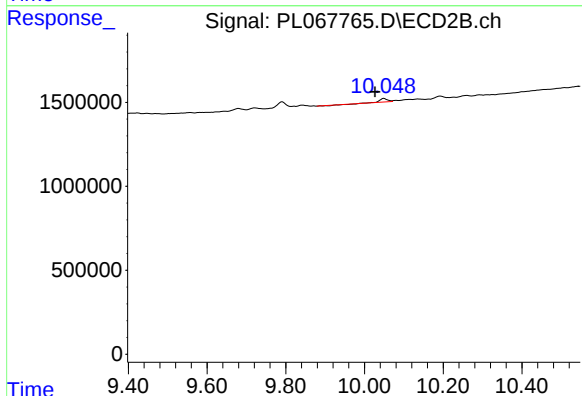


#21 Endrin ketone

R.T.: 10.050 min
Delta R.T.: 0.023 min
Response: 249240
Conc: 0.27 ng/ml

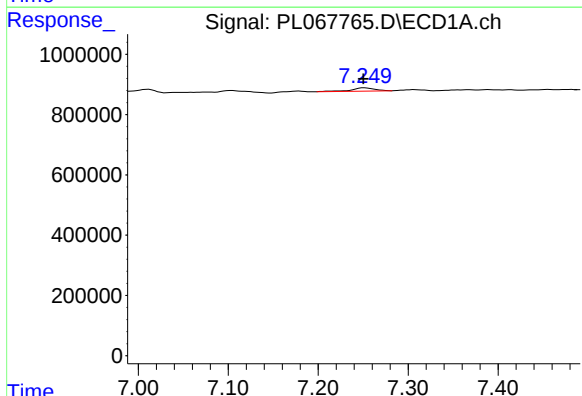


#26 Chlordane-4

R.T.: 7.251 min
Delta R.T.: 0.000 min
Response: 196303
Conc: 2.69 ng/ml

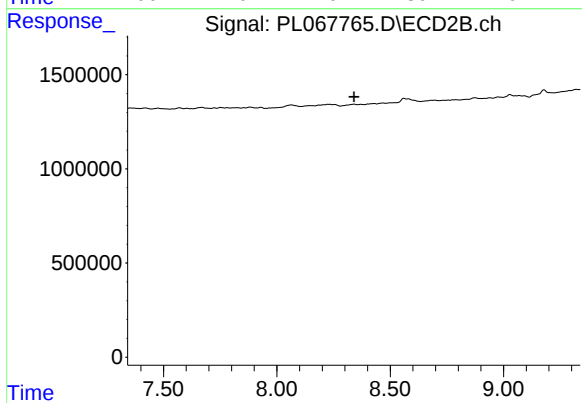

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.341 min
Response: 0
Conc: N.D.

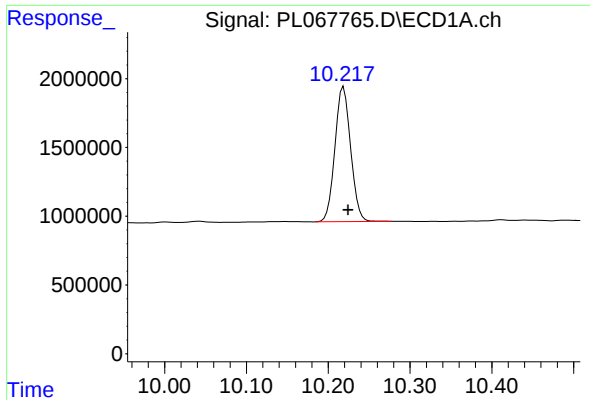

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 13081164
Conc: 18.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

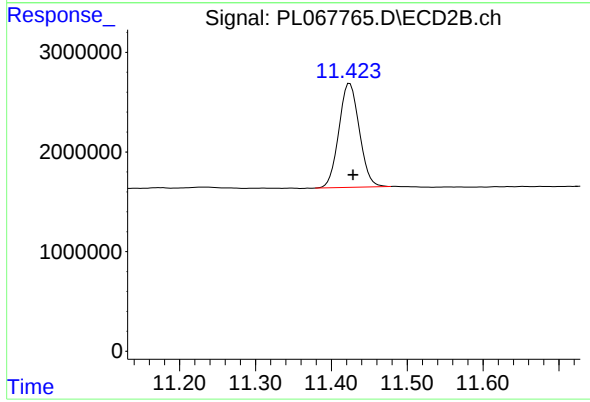

#28 Decachlorobiphenyl

R.T.: 11.424 min
Delta R.T.: -0.004 min
Response: 19542740
Conc: 19.62 ng/ml