

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
 Data File : PL067742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 10:28
 Operator : AR\AJ
 Sample : M2764-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PHC-250EM-001RE

Manual Integrations
 APPROVED

Ankita
 6/24/2021 12:58:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:42:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.484	5.529	5054386	9245388	9.193m	9.807
28)	SA Decachlor...	10.225	11.430	25051265	36434825	35.349	36.579

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
Data File : PL067742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 10:28
Operator : AR\AJ
Sample : M2764-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PHC-250EM-001RE


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:42:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

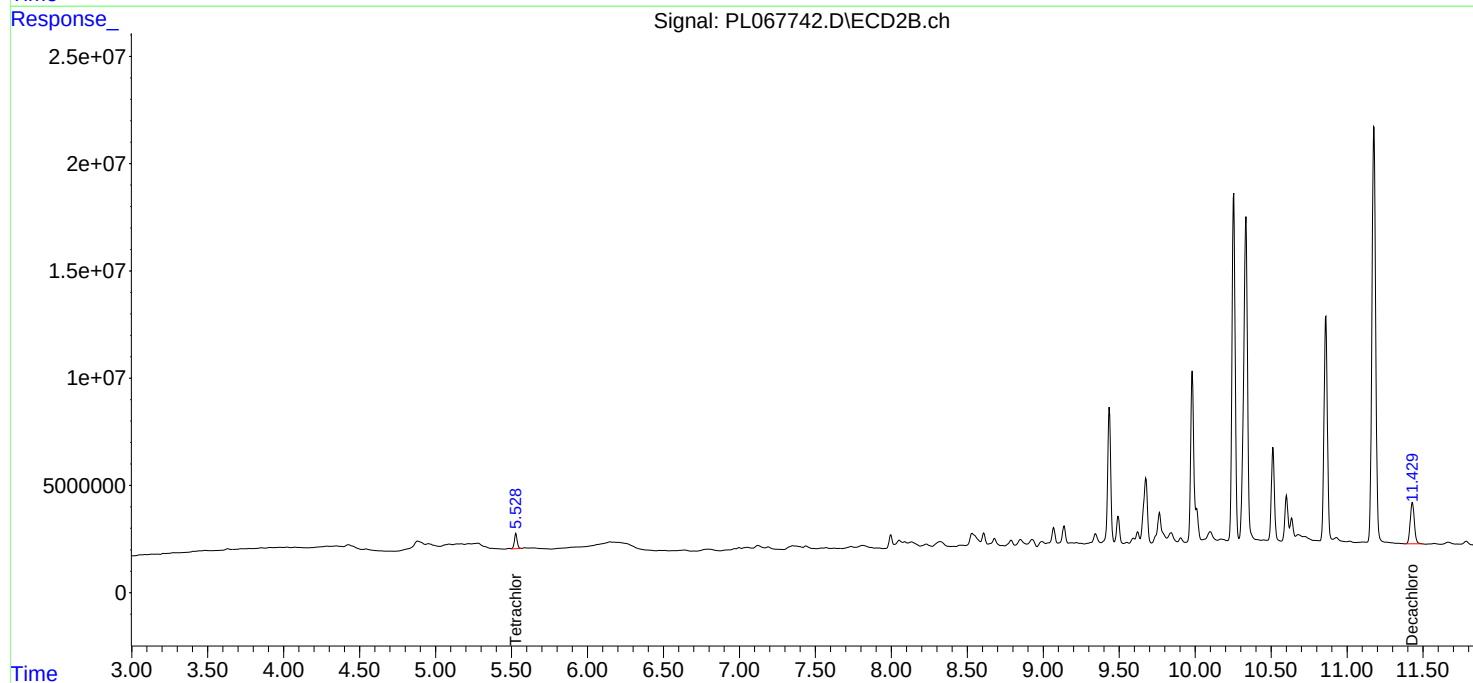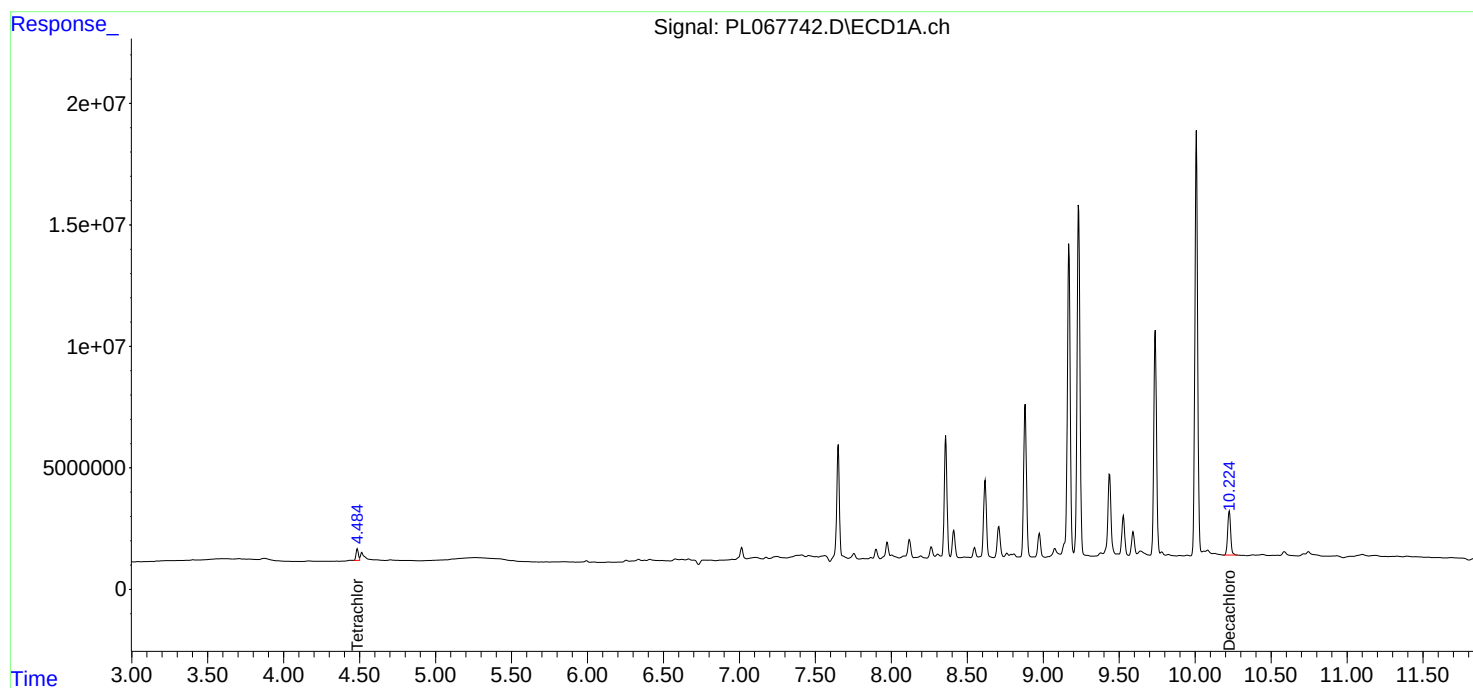

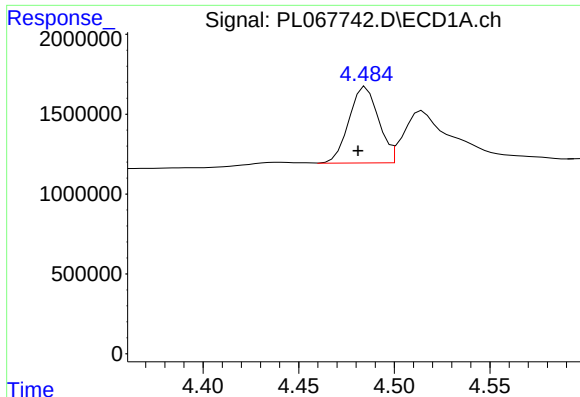


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: 0.003 min
Response: 5054386
Conc: 9.19 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PHC-250EM-001RE


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:39 PM

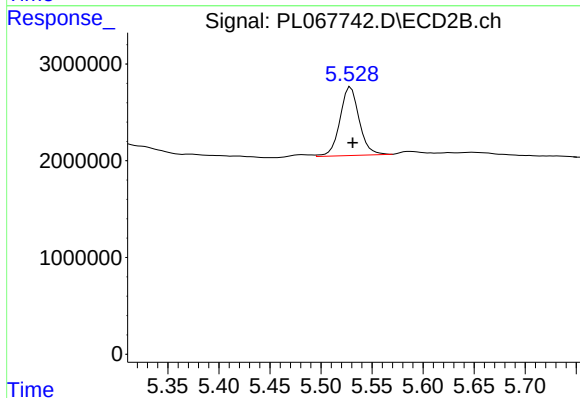


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 9245388
Conc: 9.81 ng/ml

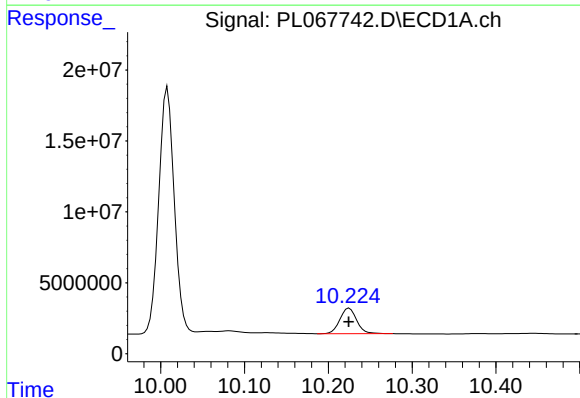

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 25051265
Conc: 35.35 ng/ml

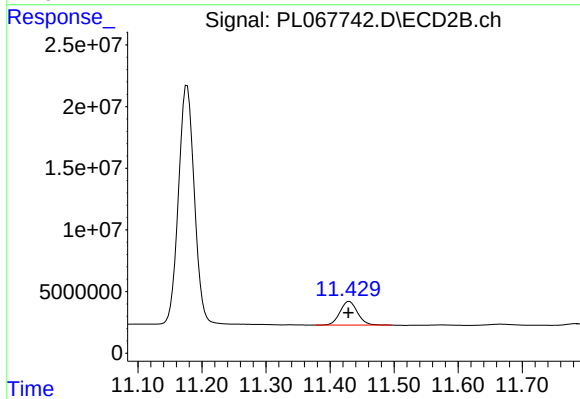

#28 Decachlorobiphenyl

R.T.: 11.430 min
Delta R.T.: 0.002 min
Response: 36434825
Conc: 36.58 ng/ml