

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
 Data File : PL067744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 11:01
 Operator : AR\AJ
 Sample : M2800-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BORING-ADDITION

Manual Integrations
 APPROVED

Ankita
 6/24/2021 12:58:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:43:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.546f	10089676	16610804	18.352	17.620
28)	SA Decachlor...	10.221	11.445f	12553318	17091896	17.714	17.160
Target Compounds							
10)	B gamma-Chl...	7.182	8.275	2913536	3895463	4.019	3.858
11)	B alpha-Chl...	7.249	8.356	5106259	9972071	6.975m	9.877m#
12)	B 4,4'-DDE	7.479	8.526	997790	1002417	1.500	1.107m#
15)	B Endosulfa...	8.189	9.154	1829711	847961	2.971	1.064 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
Data File : PL067744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 11:01
Operator : AR\AJ
Sample : M2800-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BORING-ADDITION


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:43:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

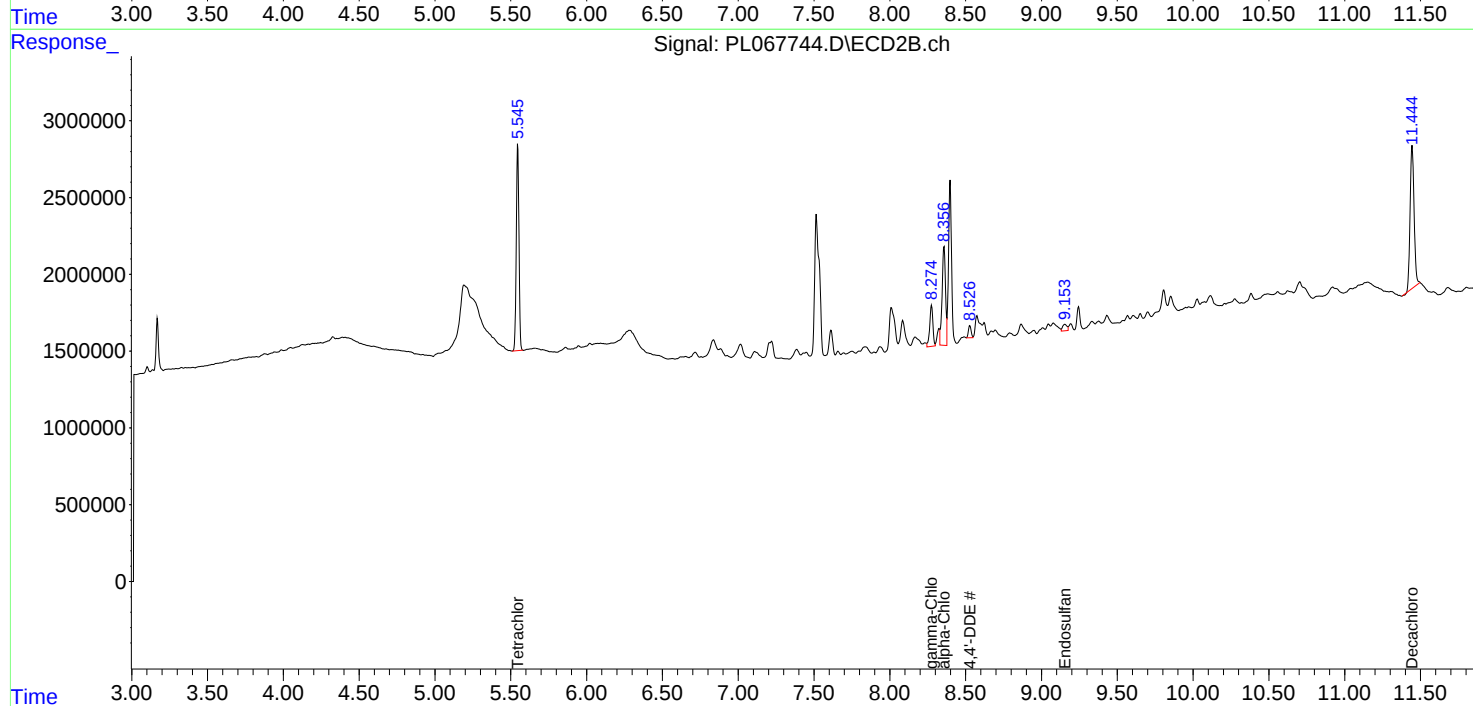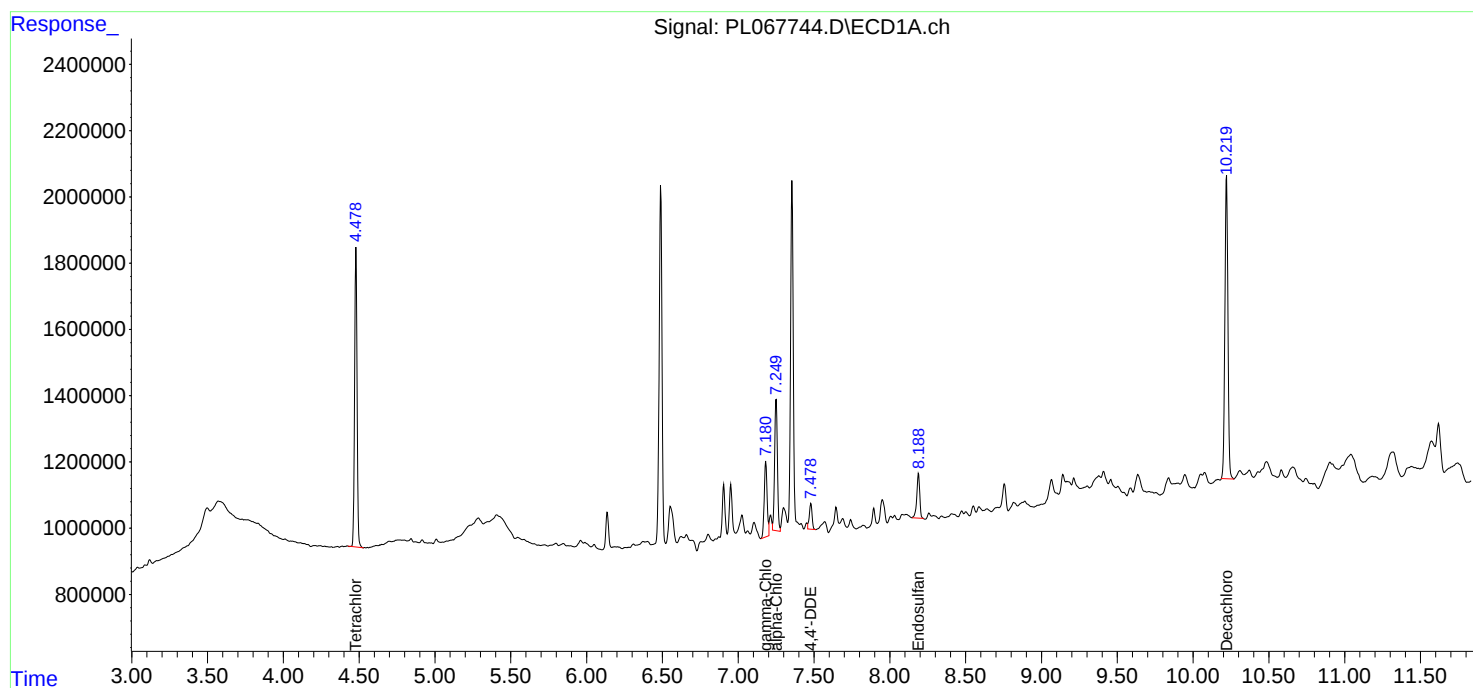

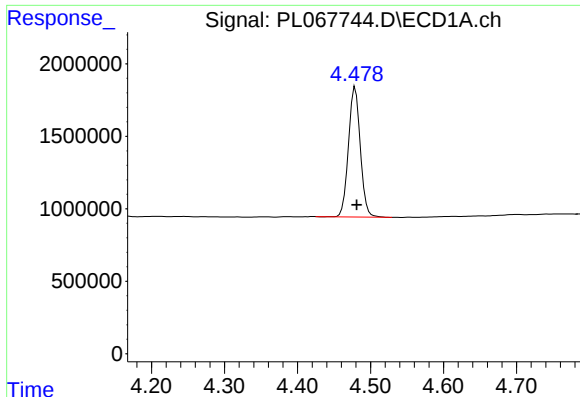


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 10089676
Conc: 18.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORING-ADDITION


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:15 PM

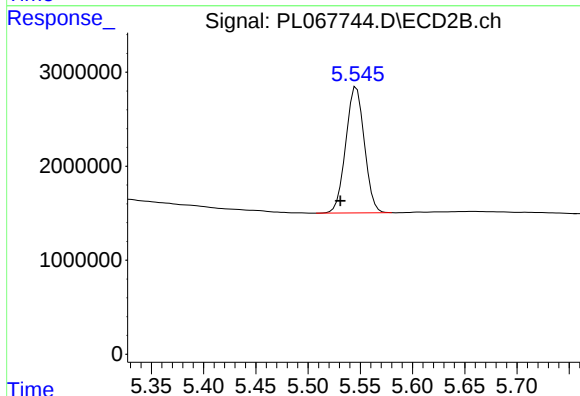


#1 Tetrachloro-m-xylene

R.T.: 5.546 min
Delta R.T.: 0.015 min
Response: 16610804
Conc: 17.62 ng/ml

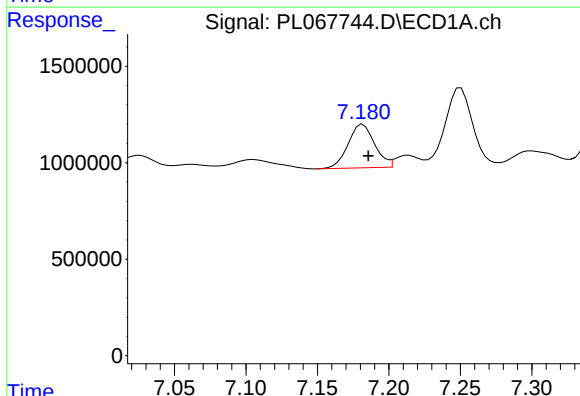


#10 gamma-Chlordane

R.T.: 7.182 min
Delta R.T.: -0.004 min
Response: 2913536
Conc: 4.02 ng/ml

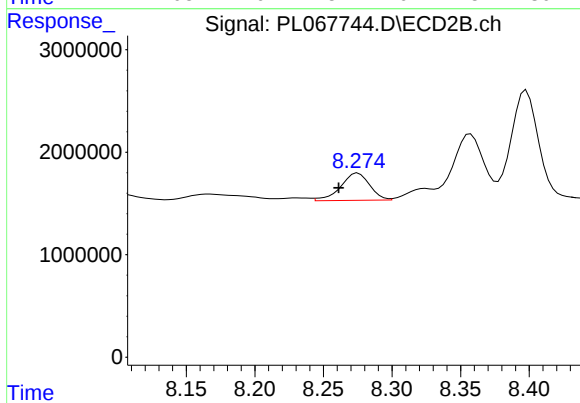

#10 gamma-Chlordane

R.T.: 8.275 min
Delta R.T.: 0.014 min
Response: 3895463
Conc: 3.86 ng/ml

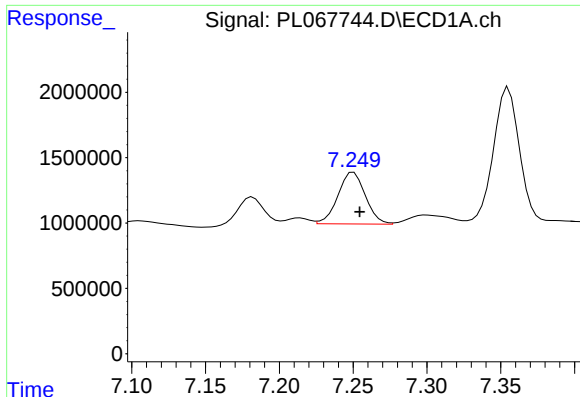


#11 alpha-Chlordane

R.T.: 7.249 min
Delta R.T.: -0.006 min
Response: 5106259
Conc: 6.97 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BORING-ADDITION


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:15 PM

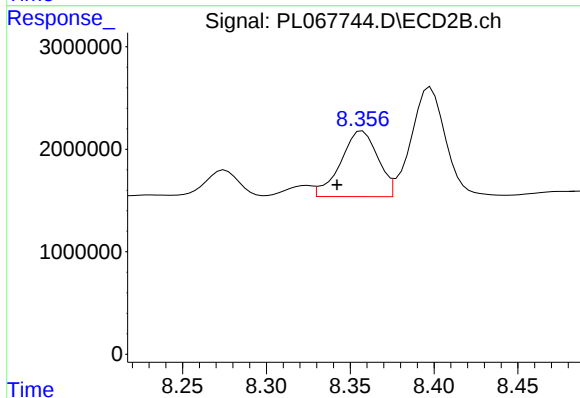


#11 alpha-Chlordane

R.T.: 8.356 min
Delta R.T.: 0.014 min
Response: 9972071
Conc: 9.88 ng/ml m

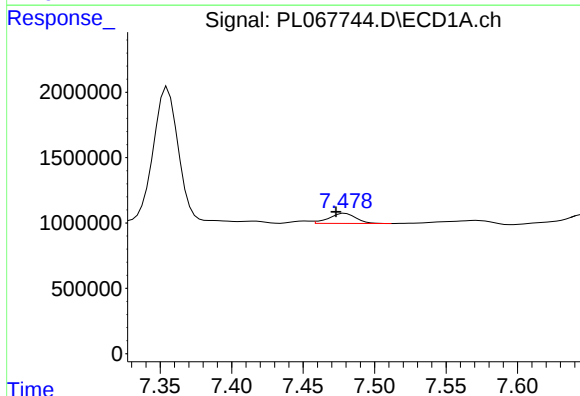


#12 4,4'-DDE

R.T.: 7.479 min
Delta R.T.: 0.006 min
Response: 997790
Conc: 1.50 ng/ml

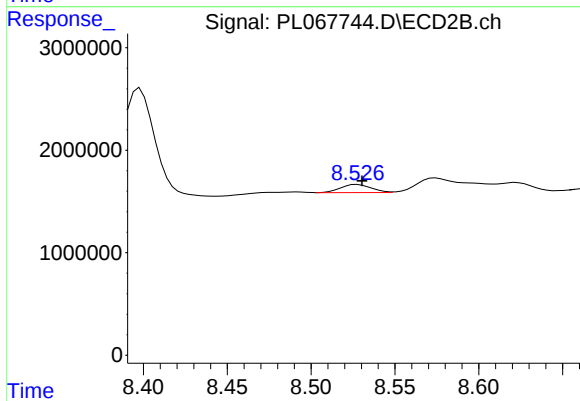

#12 4,4'-DDE

R.T.: 8.526 min
Delta R.T.: -0.004 min
Response: 1002417
Conc: 1.11 ng/ml m

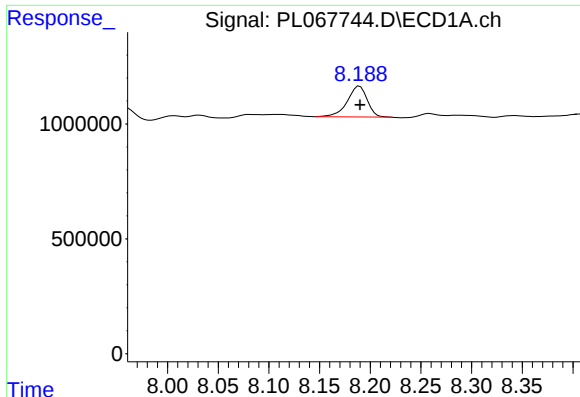


#15 Endosulfan II

R.T.: 8.189 min
Delta R.T.: 0.000 min
Response: 1829711
Conc: 2.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORING-ADDITION


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:15 PM

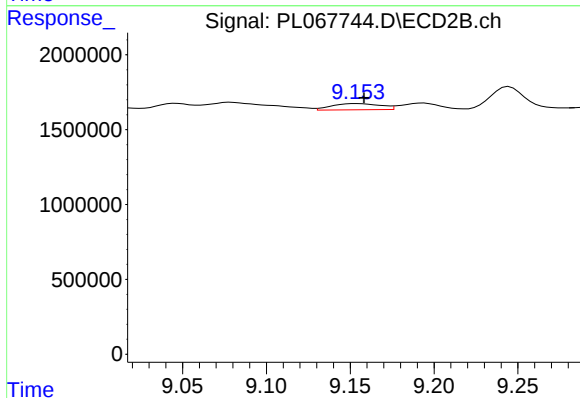


#15 Endosulfan II

R.T.: 9.154 min
Delta R.T.: -0.004 min
Response: 847961
Conc: 1.06 ng/ml

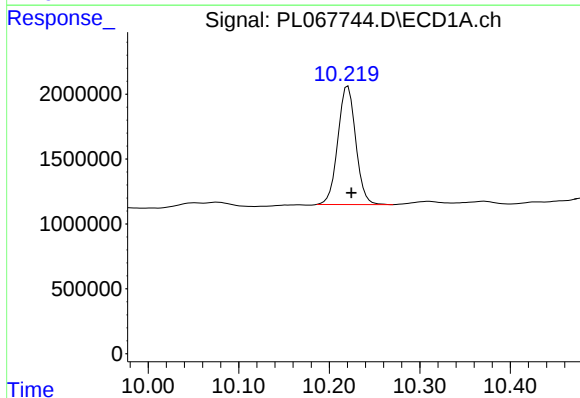

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 12553318
Conc: 17.71 ng/ml

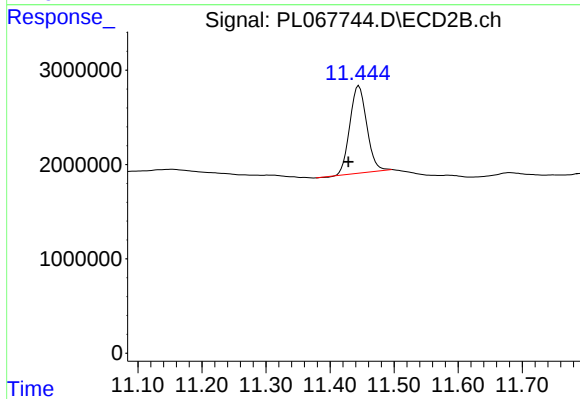

#28 Decachlorobiphenyl

R.T.: 11.445 min
Delta R.T.: 0.016 min
Response: 17091896
Conc: 17.16 ng/ml