

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
 Data File : PL067751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 13:34
 Operator : AR\AJ
 Sample : M2811-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-04-062221

Manual Integrations
 APPROVED

Ankita
 6/24/2021 4:19:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:45:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	5494032	9391986	9.993m	9.963
28)	SA Decachlor...	10.220	11.428	8389726	12839367	11.838	12.890
Target Compounds							
10)	B gamma-Chl...	7.180	8.258	786714	841014	1.085	0.833m
11)	B alpha-Chl...	7.250	8.341	1423009	2754618	1.944	2.728 #
12)	B 4,4'-DDE	7.473	8.522	355588	513504	0.534	0.567m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
Data File : PL067751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 13:34
Operator : AR\AJ
Sample : M2811-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-04-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 4:19:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:45:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

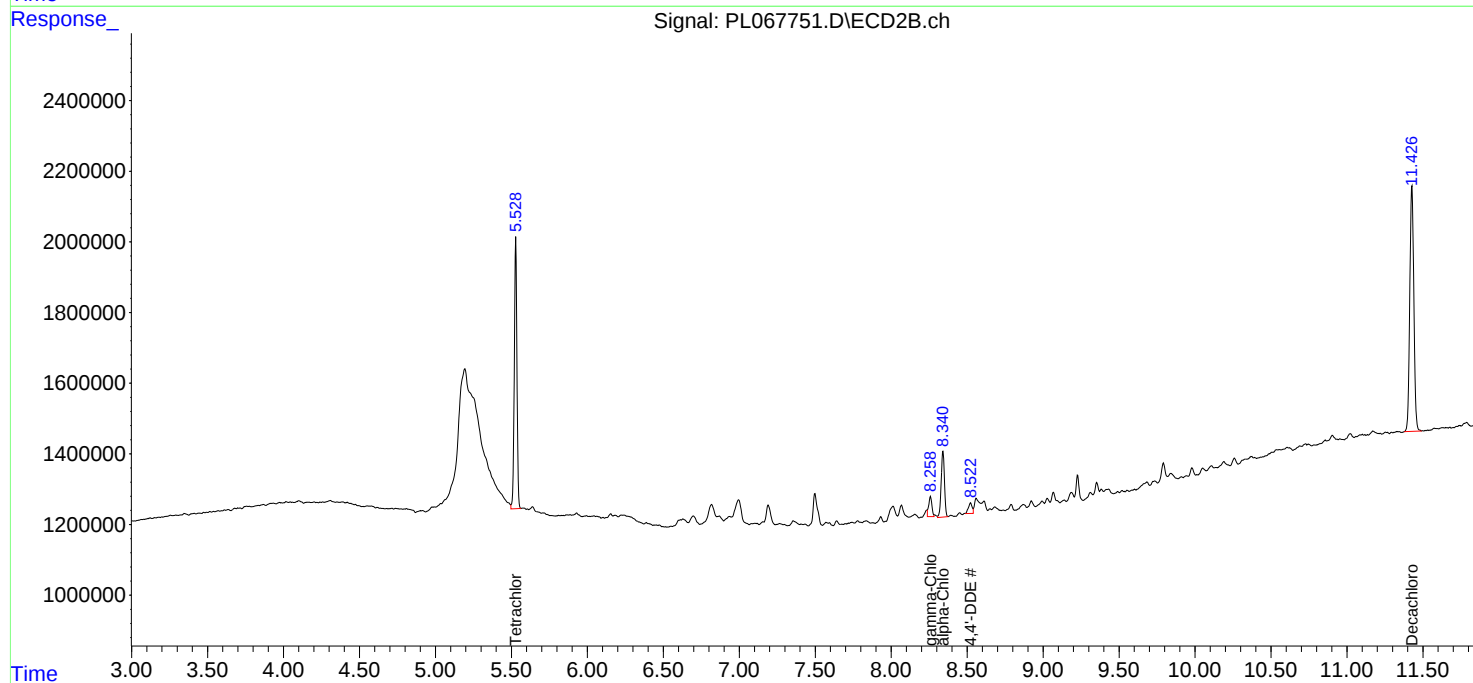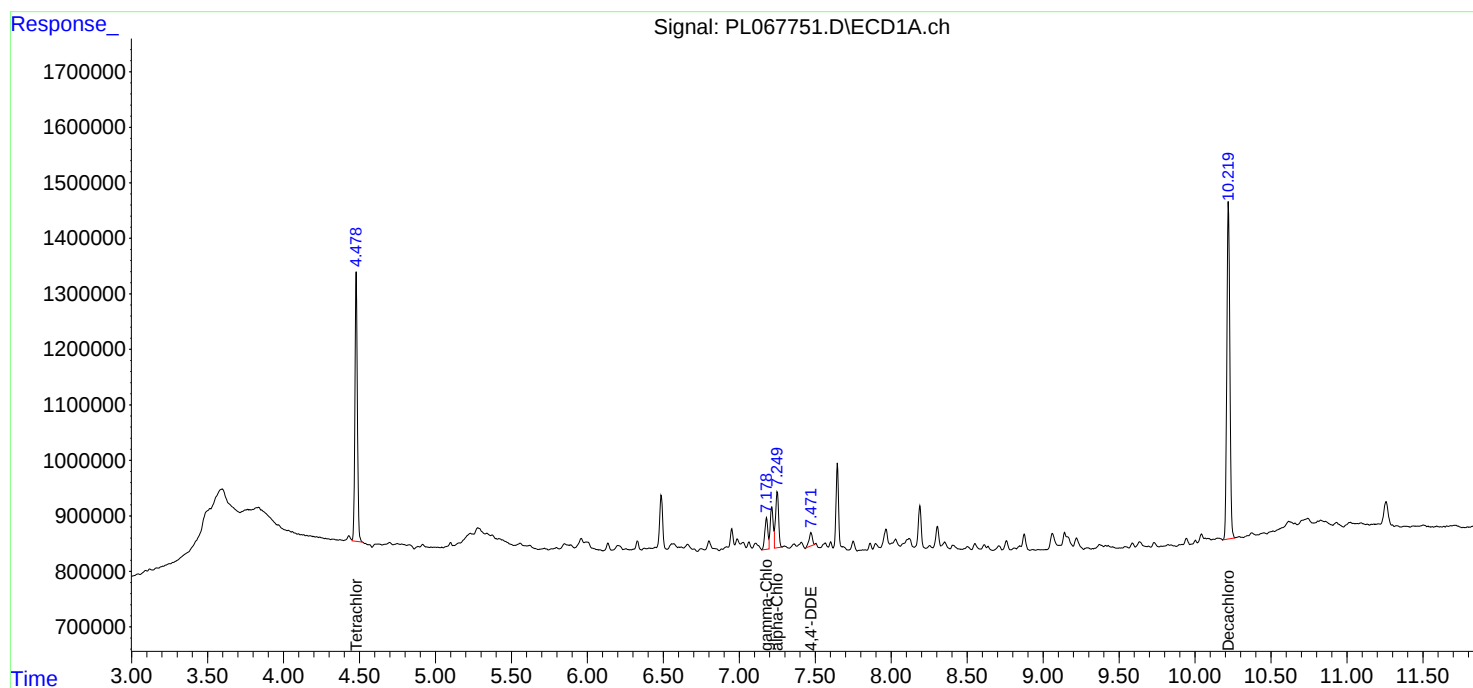

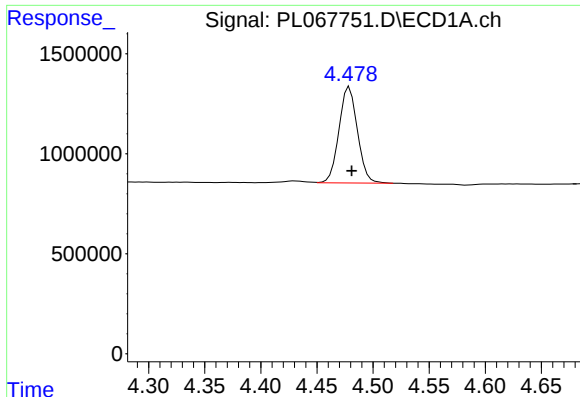


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 5494032
Conc: 9.99 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HR-04-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 4:19:53 PM

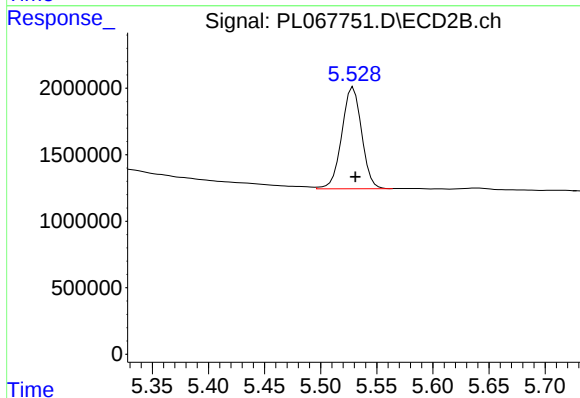


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 9391986
Conc: 9.96 ng/ml

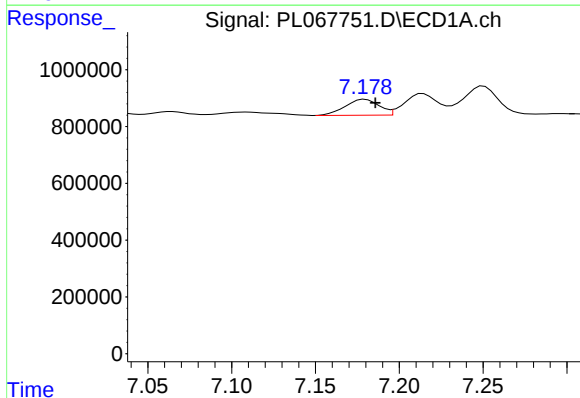


#10 gamma-Chlordane

R.T.: 7.180 min
Delta R.T.: -0.006 min
Response: 786714
Conc: 1.09 ng/ml

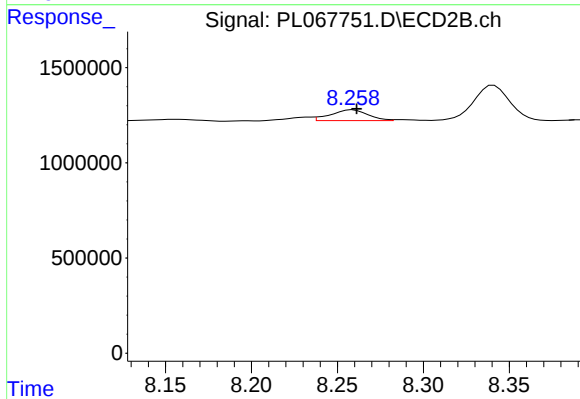

#10 gamma-Chlordane

R.T.: 8.258 min
Delta R.T.: -0.004 min
Response: 841014
Conc: 0.83 ng/ml m

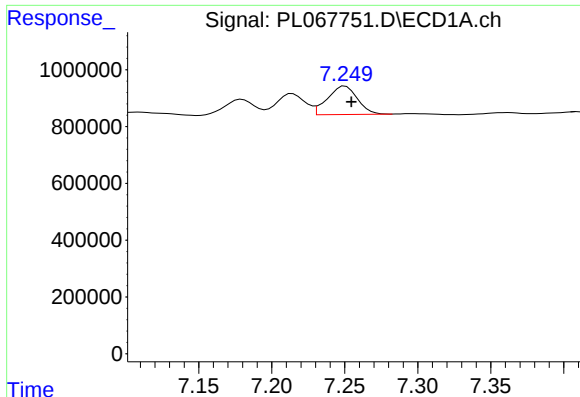


#11 alpha-Chlordane

R.T.: 7.250 min
Delta R.T.: -0.004 min
Response: 1423009
Conc: 1.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 4:19:53 PM

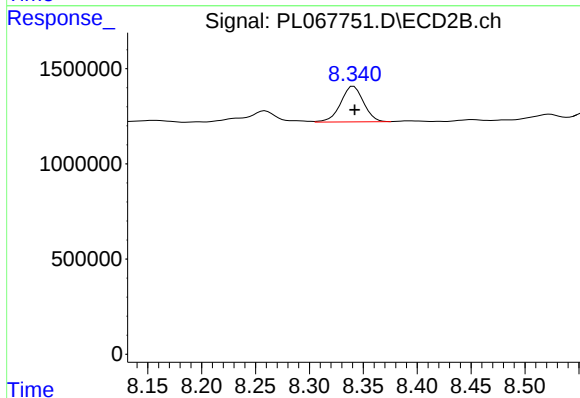


#11 alpha-Chlordane

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 2754618
Conc: 2.73 ng/ml

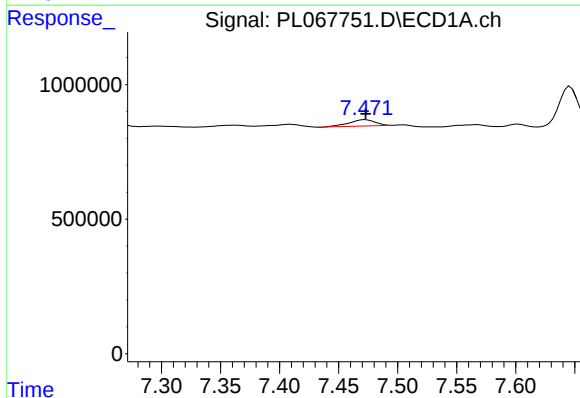


#12 4,4'-DDE

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 355588
Conc: 0.53 ng/ml

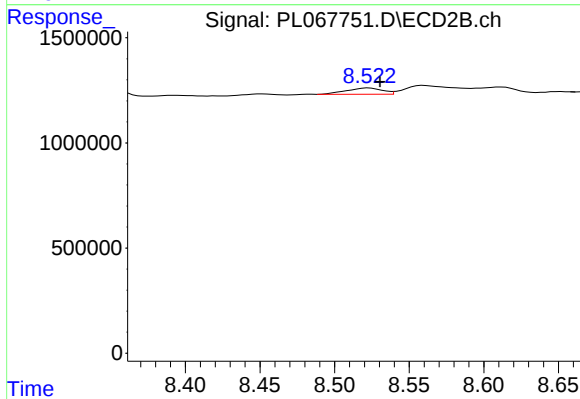

#12 4,4'-DDE

R.T.: 8.522 min
Delta R.T.: -0.009 min
Response: 513504
Conc: 0.57 ng/ml m

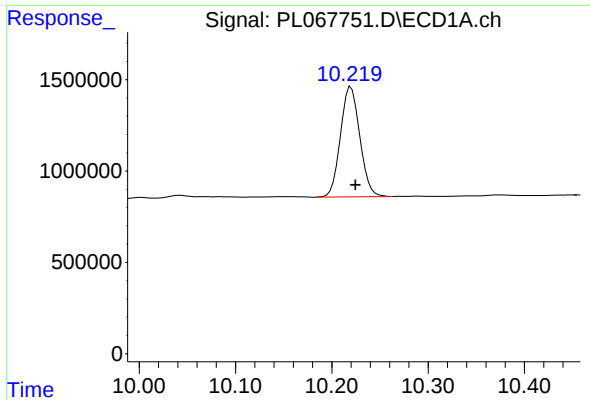


#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 8389726
Conc: 11.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-062221

Manual Integrations
APPROVED

Ankita
6/24/2021 4:19:53 PM

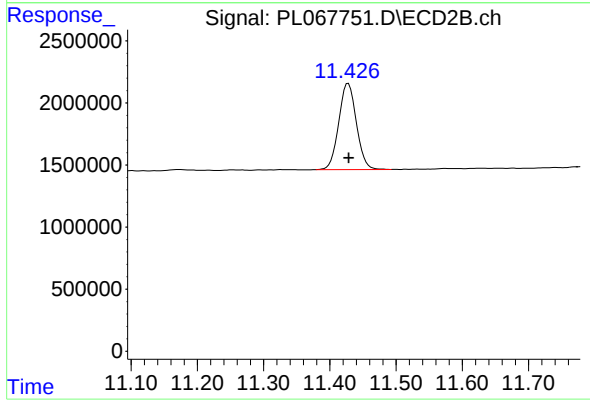

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 12839367
Conc: 12.89 ng/ml