

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
 Data File : PL067752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 13:51
 Operator : AR\AJ
 Sample : M2812-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 356-349

Manual Integrations
 APPROVED

Ankita
 6/24/2021 12:58:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:46:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.472	5.523	9056626	35012190	16.473m	37.139 #
28)	SA Decachlor...	10.220	11.429	7121582	10181120	10.049	10.221

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
Data File : PL067752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 13:51
Operator : AR\AJ
Sample : M2812-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
356-349


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:46:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

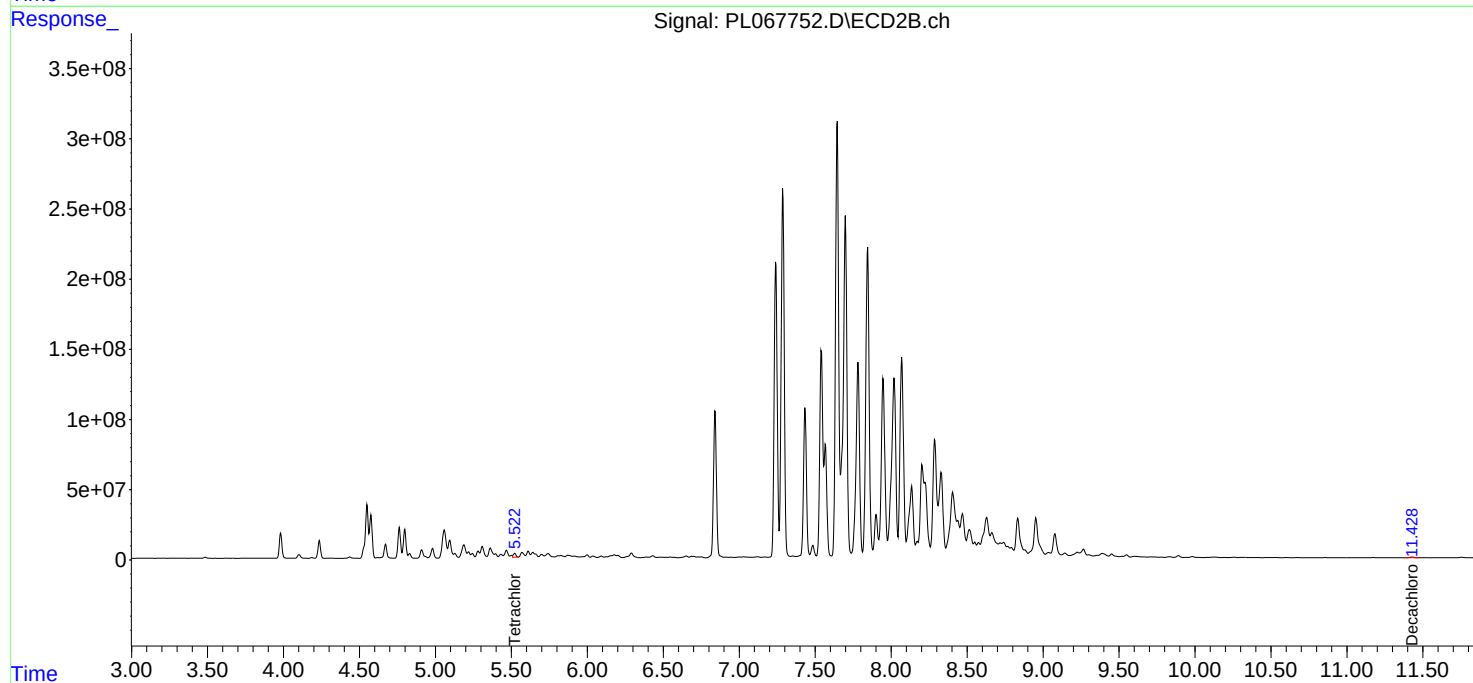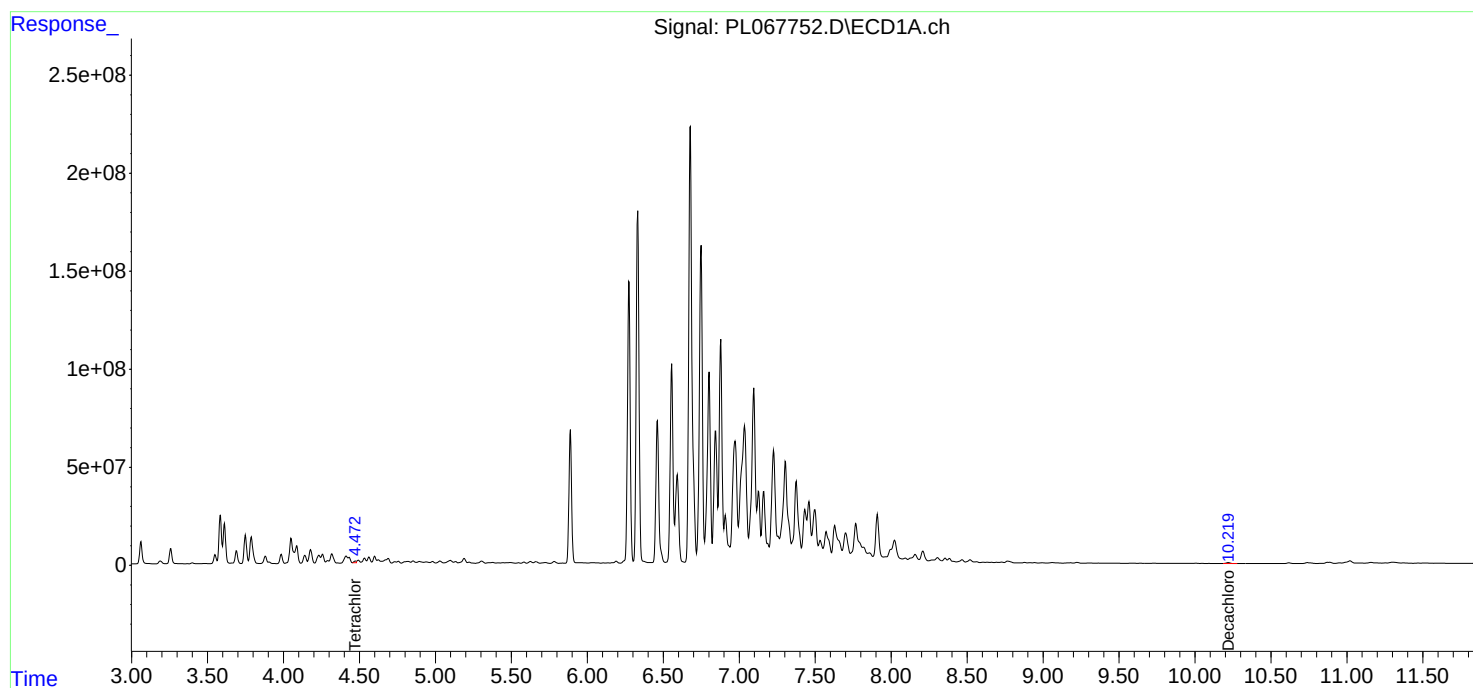

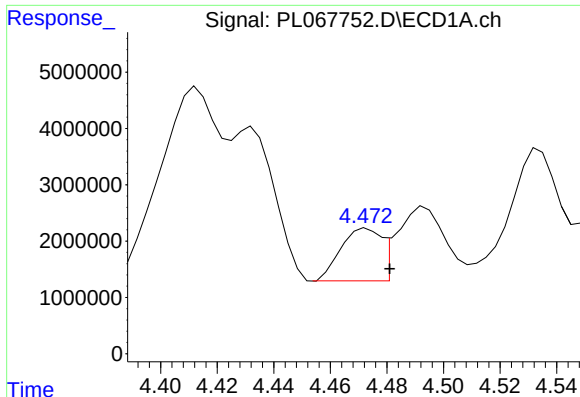


#1 Tetrachloro-m-xylene

R.T.: 4.472 min
Delta R.T.: -0.009 min
Response: 9056626
Conc: 16.47 ng/ml m

Instrument :
ECD_L
ClientSampleId :
356-349


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:21 PM

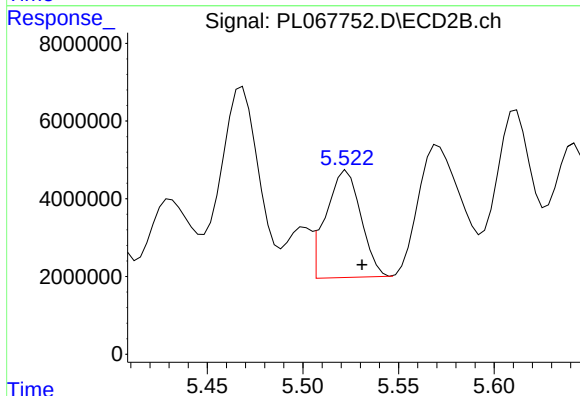


#1 Tetrachloro-m-xylene

R.T.: 5.523 min
Delta R.T.: -0.008 min
Response: 35012190
Conc: 37.14 ng/ml

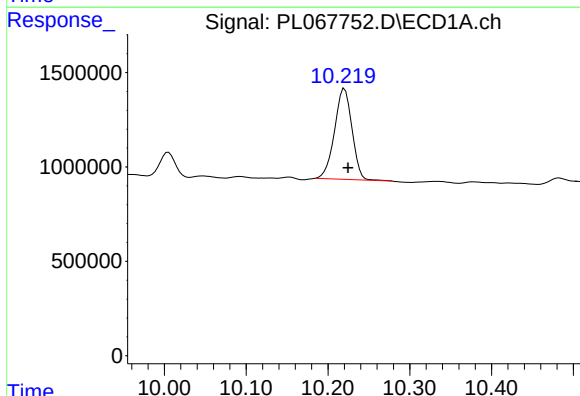

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 7121582
Conc: 10.05 ng/ml

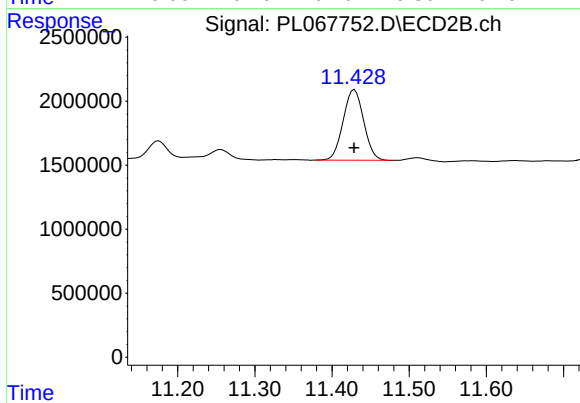

#28 Decachlorobiphenyl

R.T.: 11.429 min
Delta R.T.: 0.000 min
Response: 10181120
Conc: 10.22 ng/ml