

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
 Data File : PL067757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 15:13
 Operator : AR\AJ
 Sample : M2816-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-062221

Manual Integrations
 APPROVED

Ankita
 6/24/2021 12:58:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:47:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	5.529	4726197	8425293	8.596m	8.937
28) SA Decachlor...	10.220	11.427	6389057	9425042	9.015	9.462
Target Compounds						
11) B alpha-Chl...	7.244	8.342	1196756	1986823	1.635	1.968
12) B 4,4'-DDE	7.467	8.525	803808	1947587	1.208m	2.150 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062321\
Data File : PL067757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 15:13
Operator : AR\AJ
Sample : M2816-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:47:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

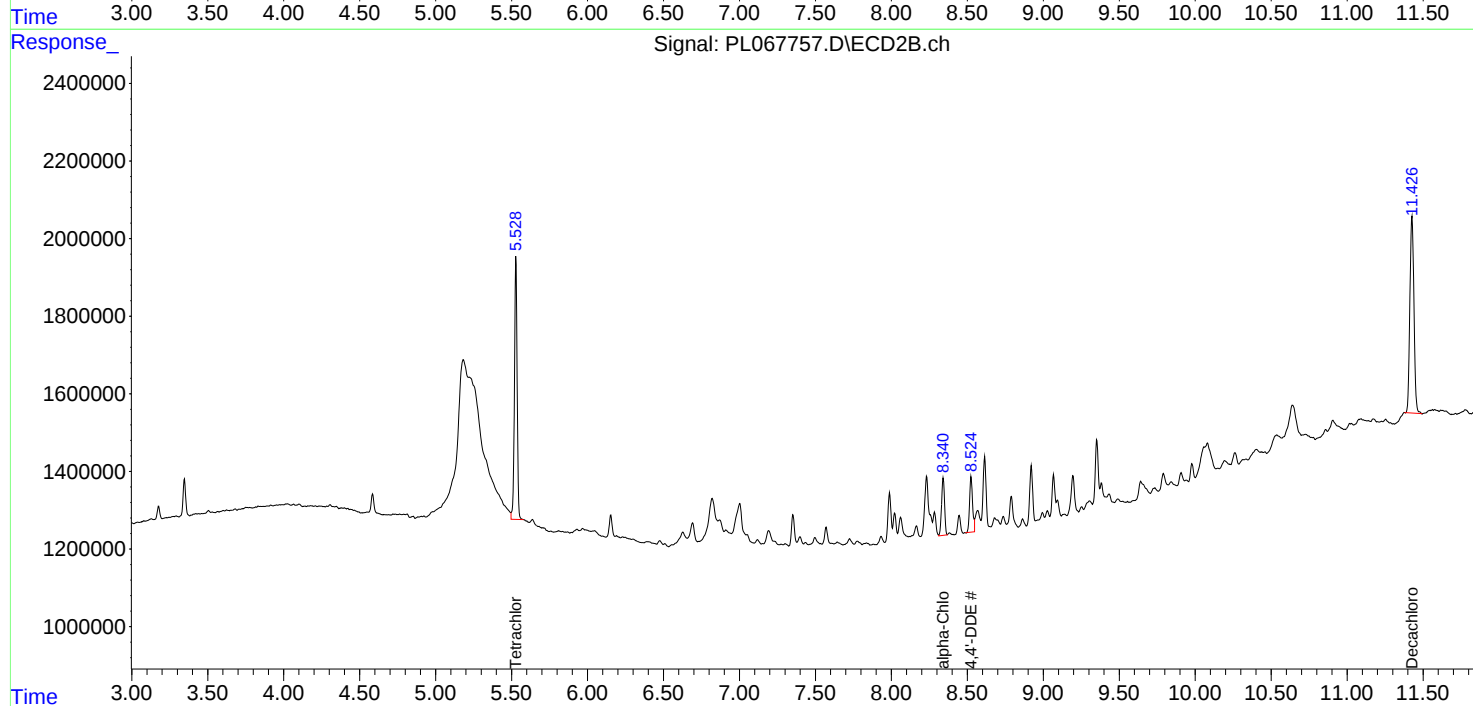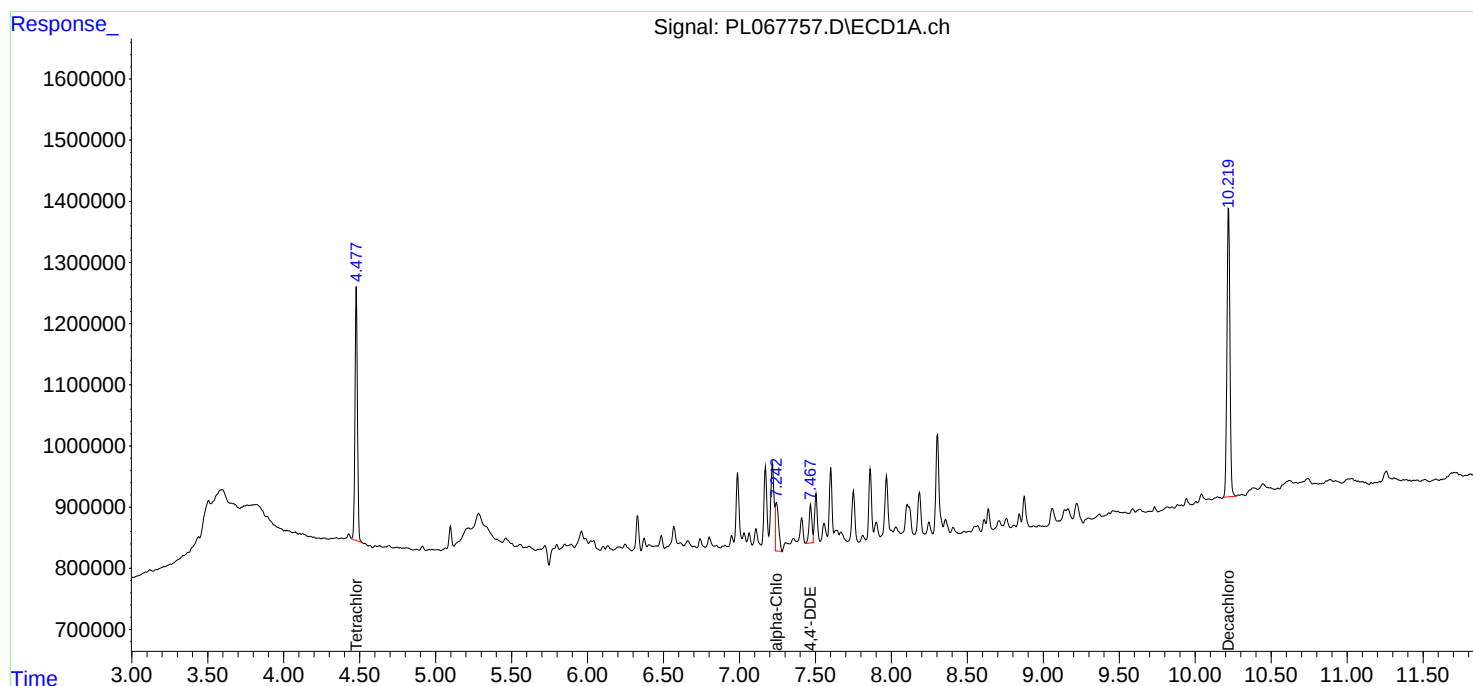

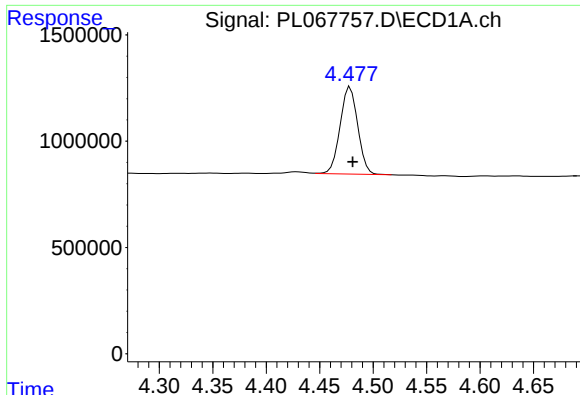


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 4726197
Conc: 8.60 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:29 PM

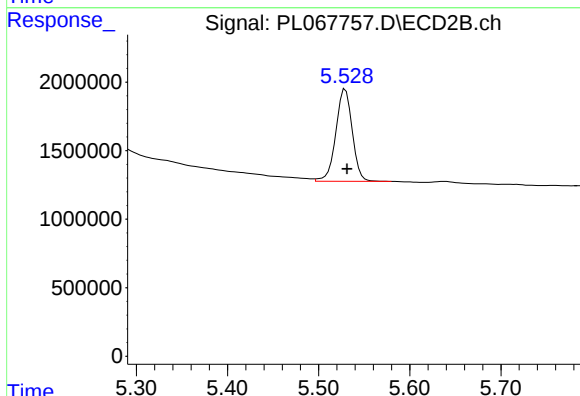


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 8425293
Conc: 8.94 ng/ml

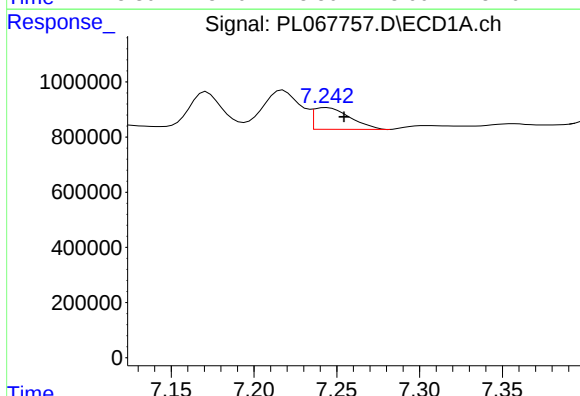


#11 alpha-Chlordane

R.T.: 7.244 min
Delta R.T.: -0.011 min
Response: 1196756
Conc: 1.63 ng/ml

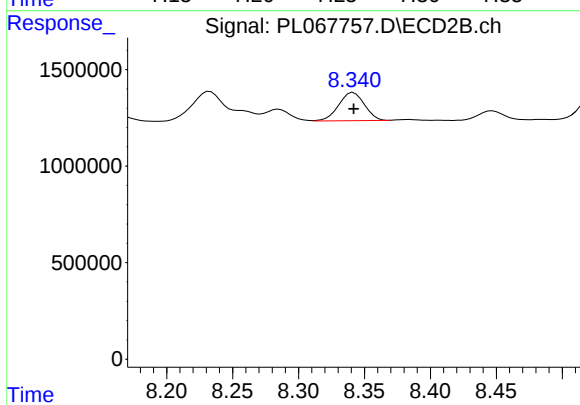

#11 alpha-Chlordane

R.T.: 8.342 min
Delta R.T.: 0.000 min
Response: 1986823
Conc: 1.97 ng/ml

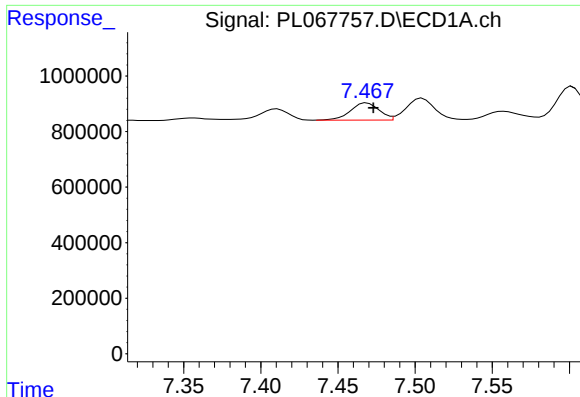


#12 4,4'-DDE

R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 803808
Conc: 1.21 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 12:58:29 PM

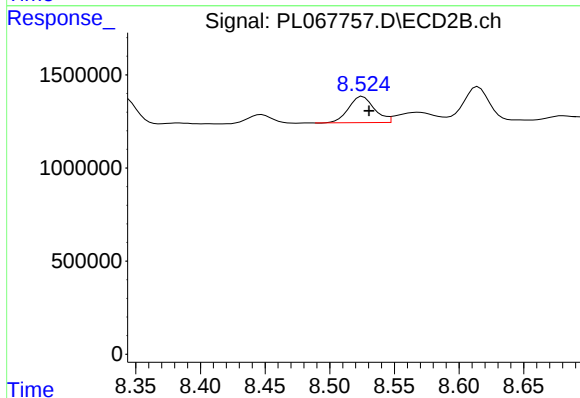


#12 4,4'-DDE

R.T.: 8.525 min
Delta R.T.: -0.005 min
Response: 1947587
Conc: 2.15 ng/ml

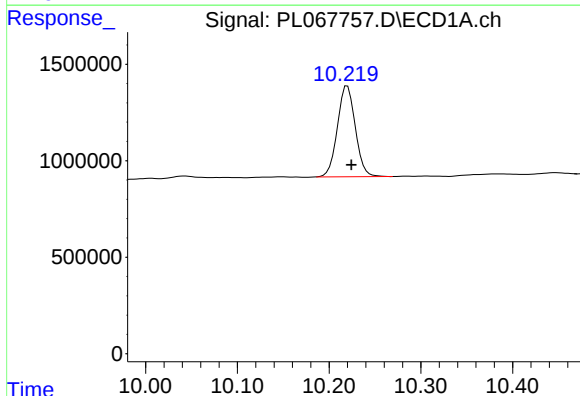

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 6389057
Conc: 9.02 ng/ml

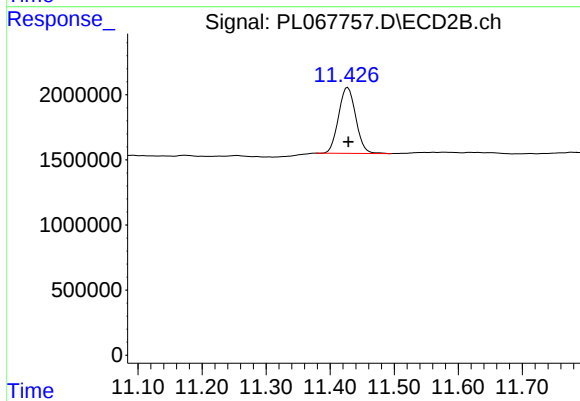

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.001 min
Response: 9425042
Conc: 9.46 ng/ml