

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 17:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 02:20:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.634	15204342	37849097	20.103	19.956
28)	SA Decachlor...	11.634	10.375	13623079	32719027	21.649	21.303
Target Compounds							
4)	MA Heptachlor	0.000	6.138f	0	154760	N.D.	0.068 #
6)	B beta-BHC	0.000	6.138	0	154760	N.D.	0.148 #
7)	B delta-BHC	7.119f	6.398	686548	425793	0.879	0.188 #
8)	B Heptachlo...	0.000	7.059	0	291816	N.D.	0.152 #
11)	B alpha-Chl...	0.000	7.385f	0	274872	N.D.	0.144 #
13)	MA Dieldrin	0.000	7.748	0	146163	N.D.	0.081 #
14)	MA Endrin	0.000	8.060f	0	395278	N.D.	0.260 #
15)	B Endosulfa...	9.301	0.000	269317	0	0.424	N.D. #
19)	B Endosulfa...	0.000	8.764	0	205914	N.D.	0.134 #
21)	B Endrin ke...	10.183f	0.000	498312	0	0.691	N.D. #
24)	Chlordane-2	0.000	6.629	0	387426	N.D.	5.572 #
26)	Chlordane-4	0.000	7.385f	0	274872	N.D.	1.458 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 17:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 02:20:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

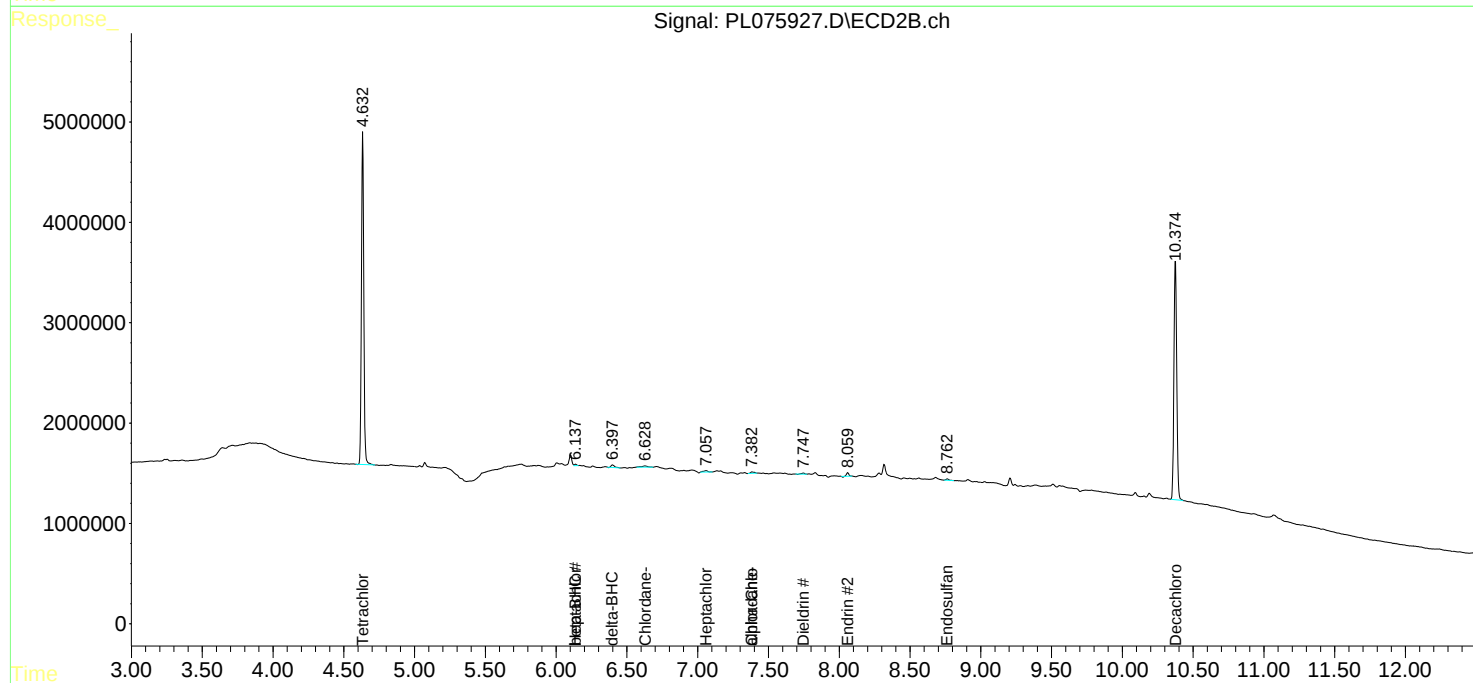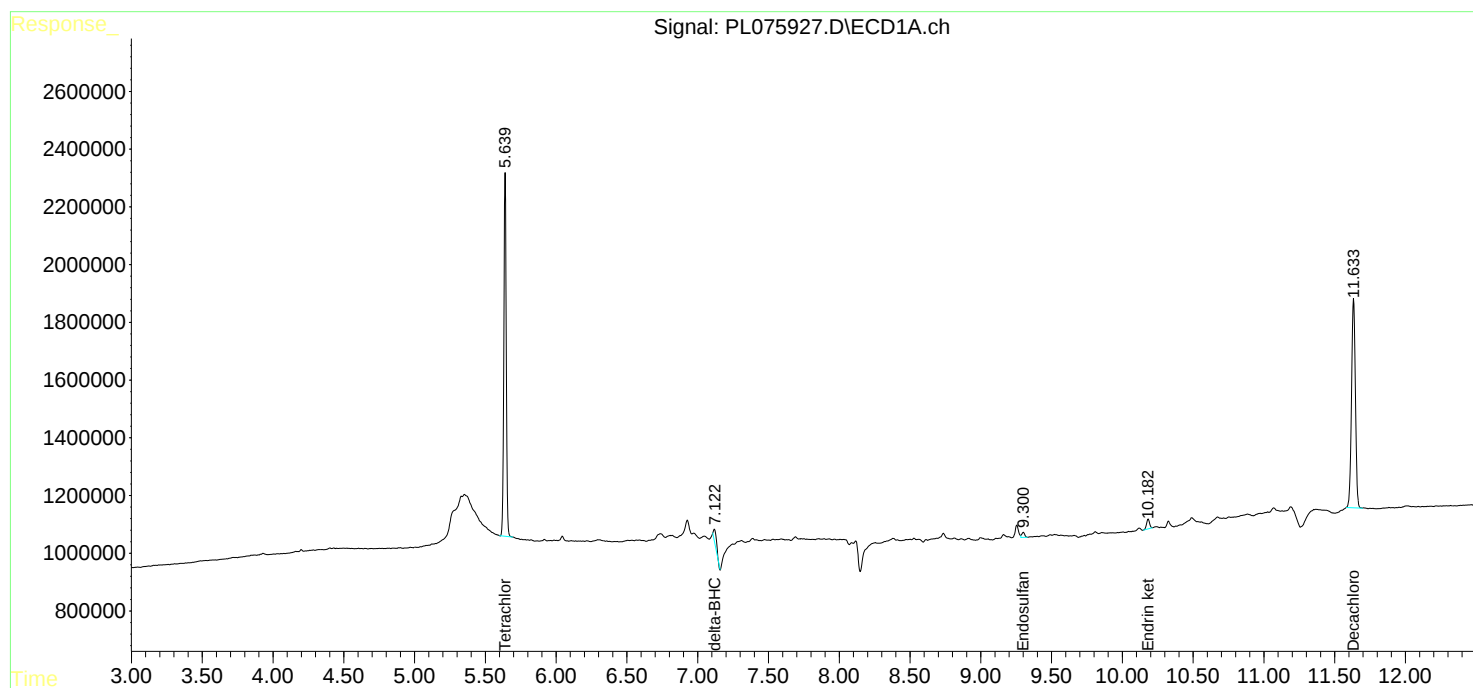


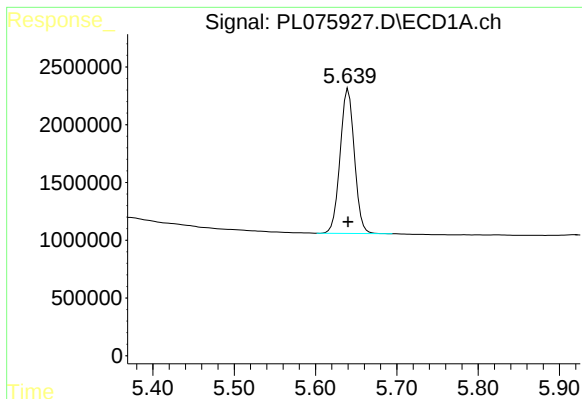

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 15204342
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

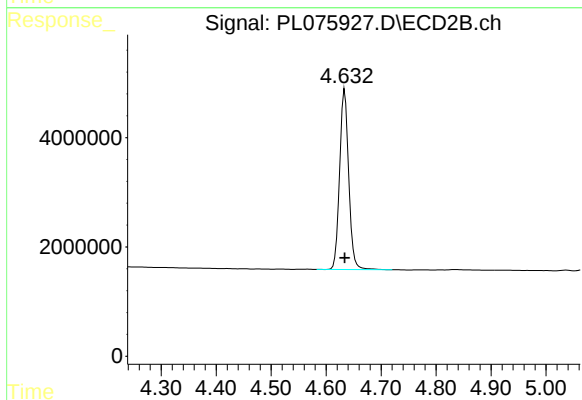


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 37849097
Conc: 19.96 ng/ml

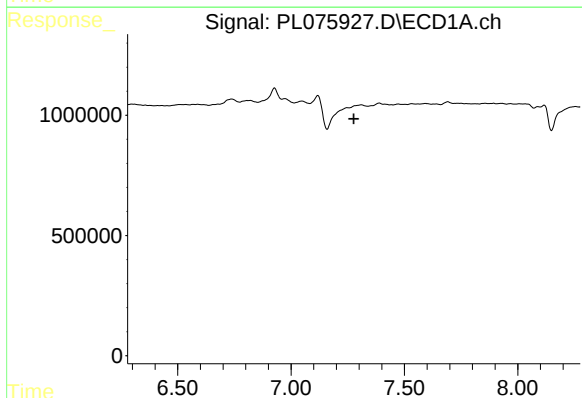


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.277 min
Response: 0
Conc: N.D.

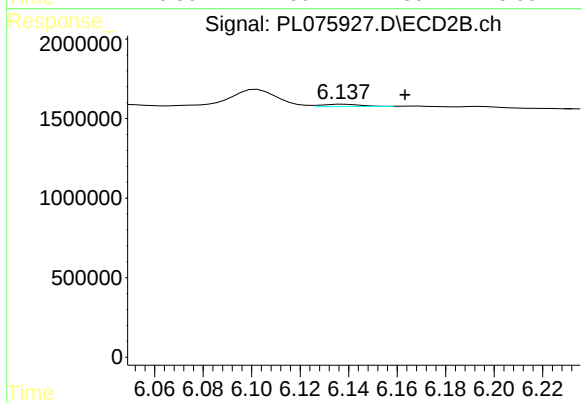

#4 Heptachlor


R.T.: 6.138 min
Delta R.T.: -0.025 min
Response: 154760
Conc: 0.07 ng/ml

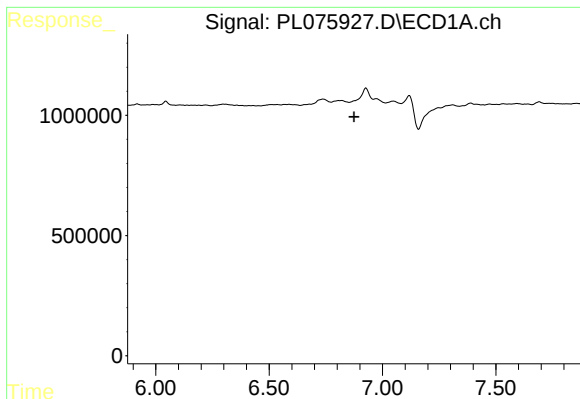

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.875 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

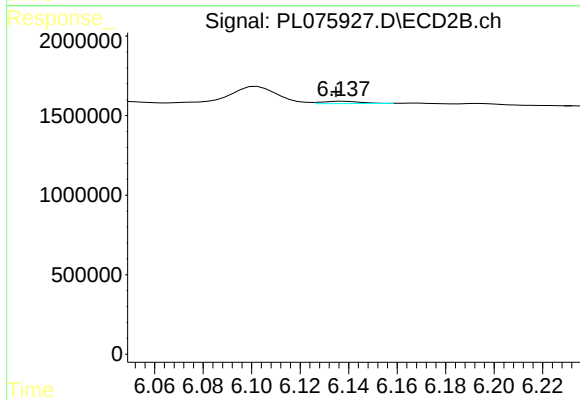


#6 beta-BHC

R.T.: 6.138 min
Delta R.T.: 0.003 min
Response: 154760
Conc: 0.15 ng/ml

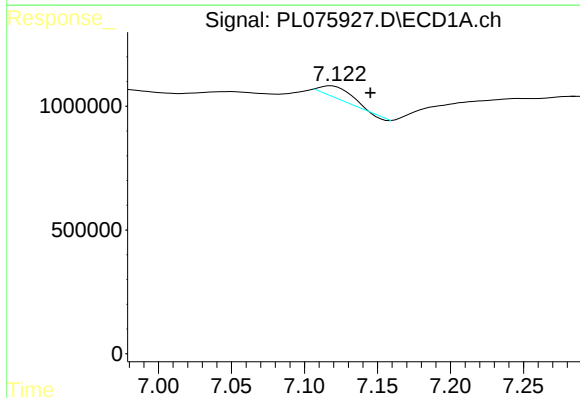


#7 delta-BHC

R.T.: 7.119 min
Delta R.T.: -0.027 min
Response: 686548
Conc: 0.88 ng/ml

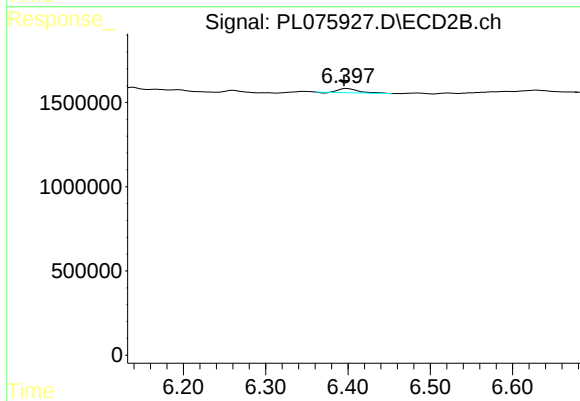

#7 delta-BHC


R.T.: 6.398 min
Delta R.T.: 0.003 min
Response: 425793
Conc: 0.19 ng/ml

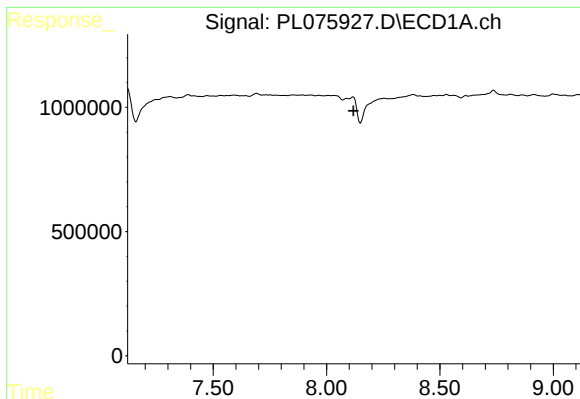

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 8.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

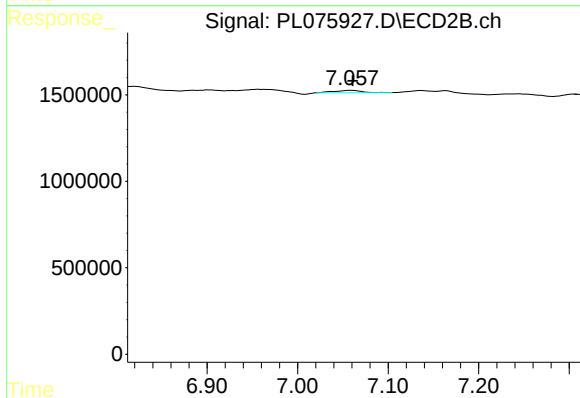


#8 Heptachlor epoxide

R.T.: 7.059 min
Delta R.T.: -0.002 min
Response: 291816
Conc: 0.15 ng/ml

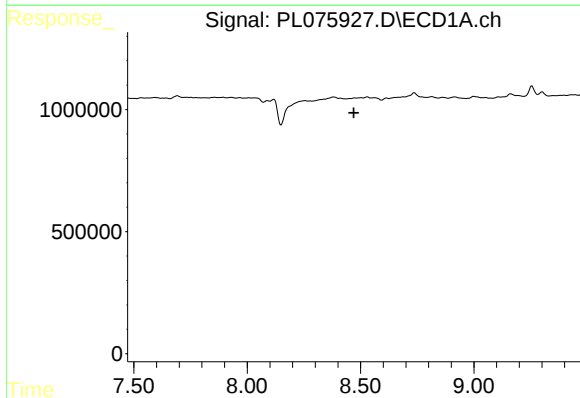


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

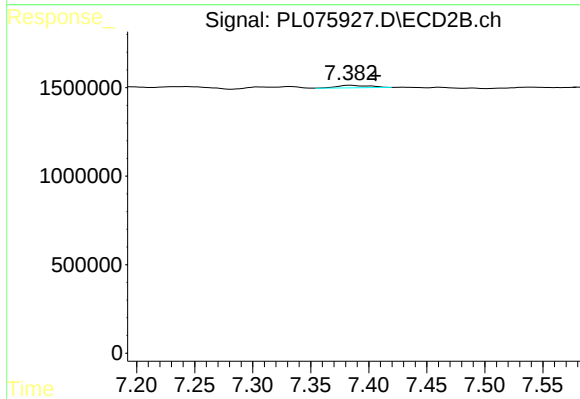

#11 alpha-Chlordane


R.T.: 7.385 min
Delta R.T.: -0.022 min
Response: 274872
Conc: 0.14 ng/ml

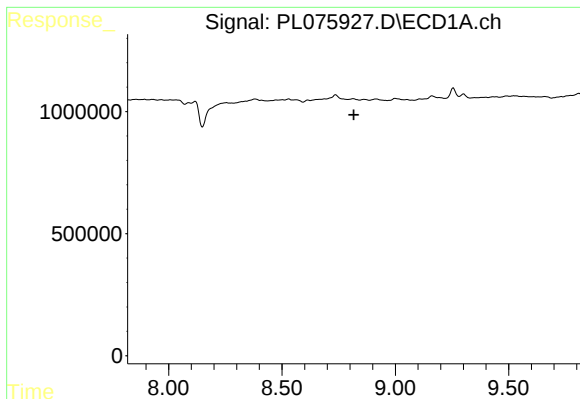

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

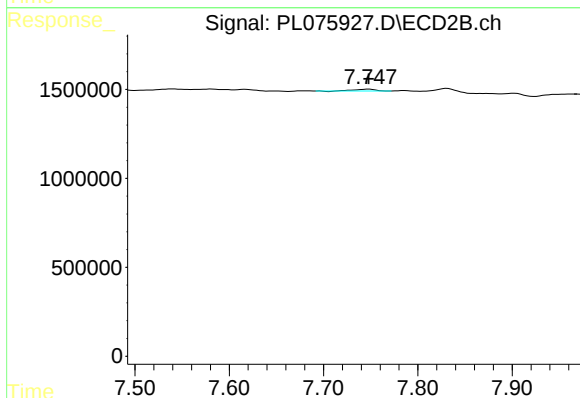


#13 Dieldrin

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 146163
Conc: 0.08 ng/ml

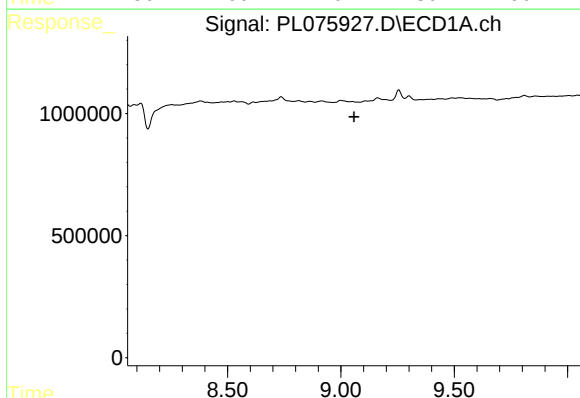


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

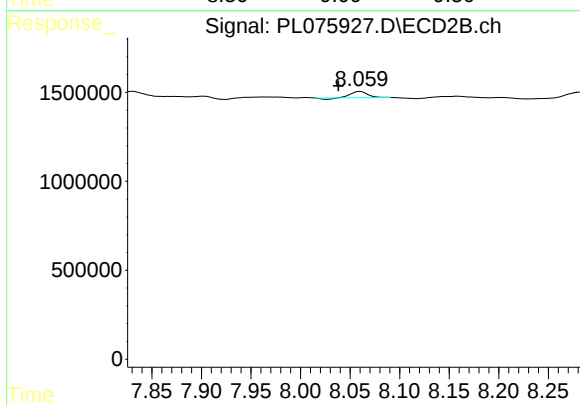

#14 Endrin


R.T.: 8.060 min
Delta R.T.: 0.022 min
Response: 395278
Conc: 0.26 ng/ml

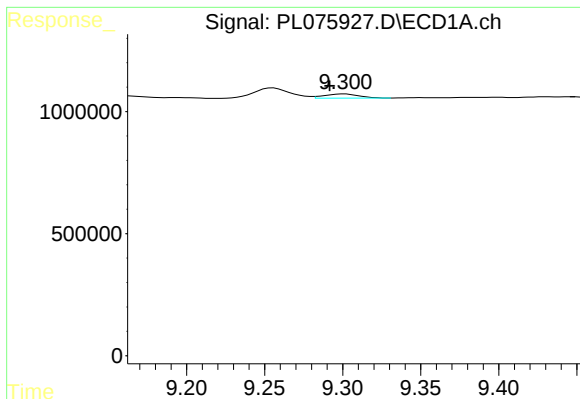

#15 Endosulfan II


R.T.: 9.301 min
Delta R.T.: 0.010 min
Response: 269317
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

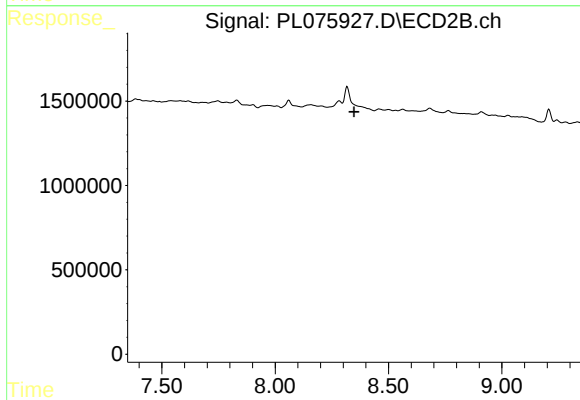


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

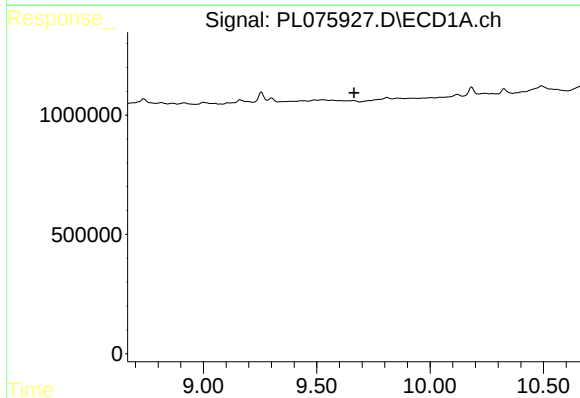


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.665 min
Response: 0
Conc: N.D.

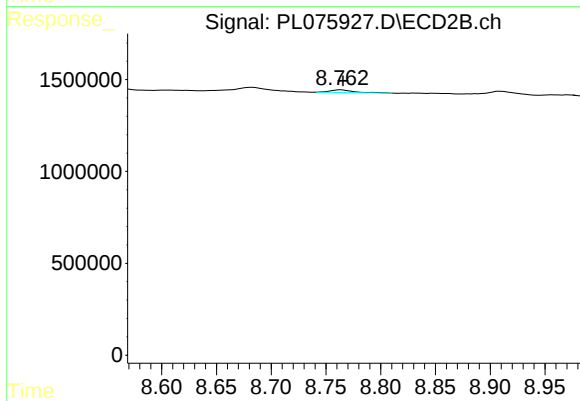

#19 Endosulfan Sulfate


R.T.: 8.764 min
Delta R.T.: -0.002 min
Response: 205914
Conc: 0.13 ng/ml

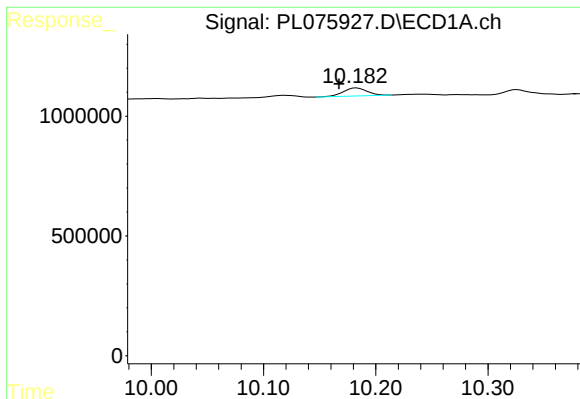

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.016 min
Response: 498312
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

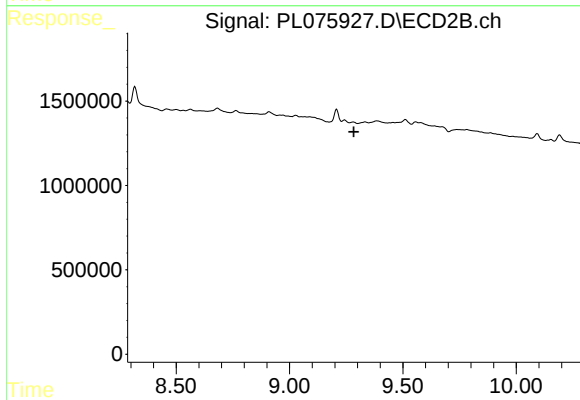


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

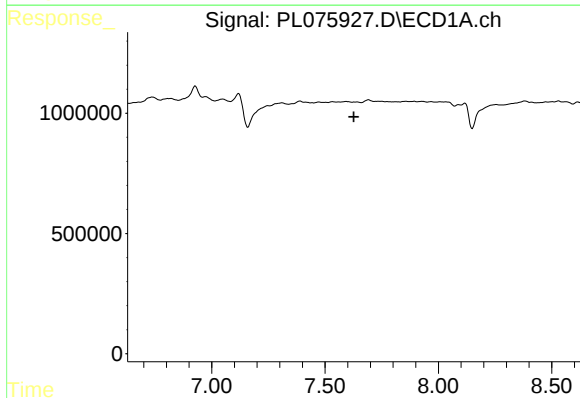


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.627 min
Response: 0
Conc: N.D.

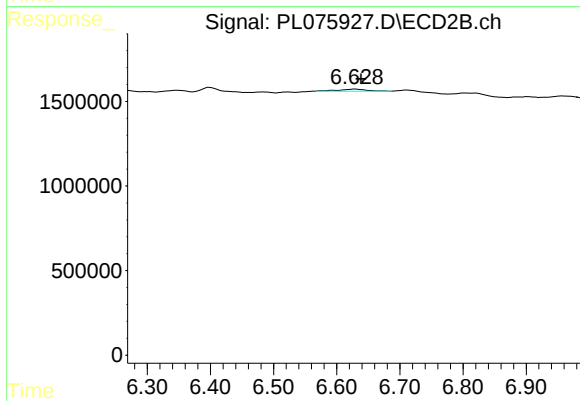

#24 Chlordane-2


R.T.: 6.629 min
Delta R.T.: -0.009 min
Response: 387426
Conc: 5.57 ng/ml

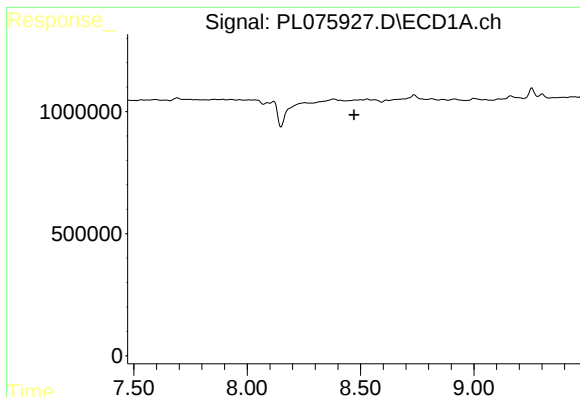

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

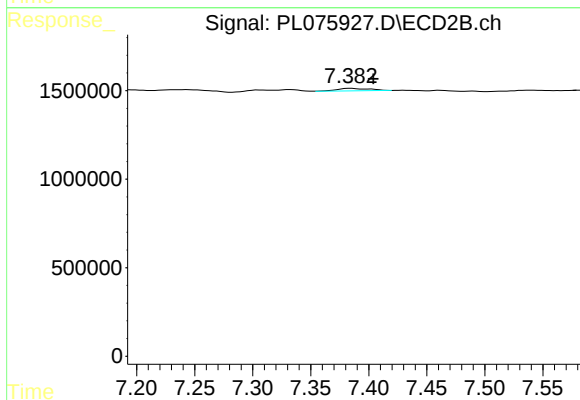


#26 Chlordane-4

R.T.: 7.385 min
Delta R.T.: -0.020 min
Response: 274872
Conc: 1.46 ng/ml

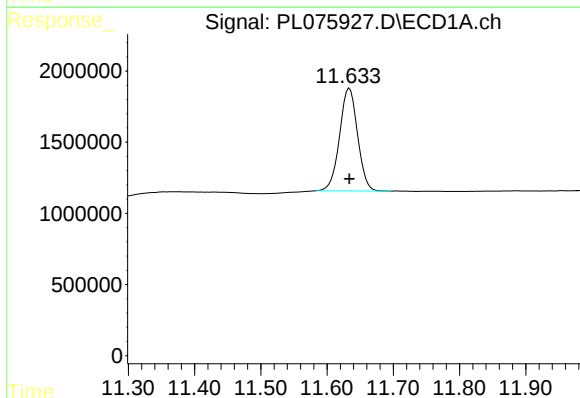

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 13623079
Conc: 21.65 ng/ml

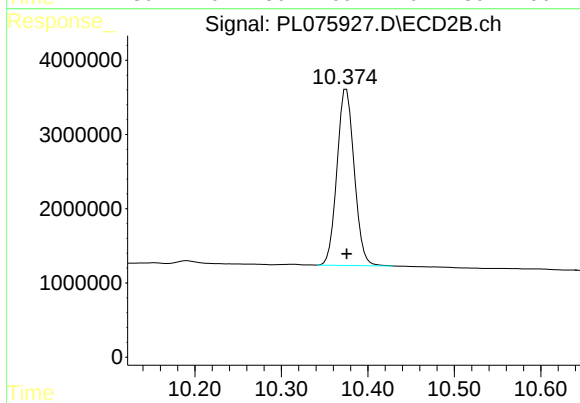

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 32719027
Conc: 21.30 ng/ml