



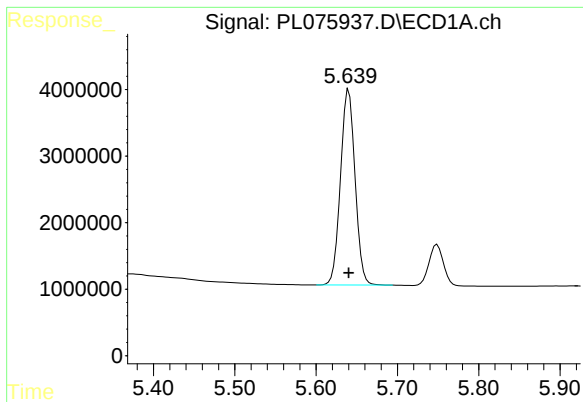

#1 Tetrachloro-m-xylene

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 36520963
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

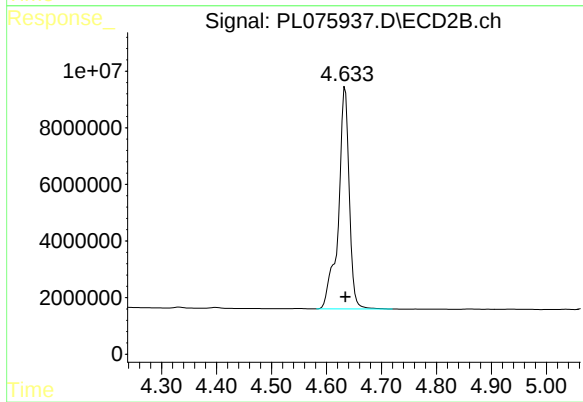

#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 107940942
Conc: 50.00 ng/ml