

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
 Data File : PL075948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 23:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 05:12:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.634	15263865	37964265	20.182	20.017
28)	SA Decachlor...	11.632	10.375	13895601	33989192	22.082	22.130
Target Compounds							
7)	B delta-BHC	7.120f	6.400	672435	604588	0.861	0.268 #
8)	B Heptachlo...	8.121	7.058	1181842	395970	1.484	0.206 #
10)	B gamma-Chl...	0.000	7.336	0	300306	N.D.	0.156 #
11)	B alpha-Chl...	0.000	7.383f	0	328707	N.D.	0.172 #
14)	MA Endrin	0.000	8.061f	0	279241	N.D.	0.184 #
15)	B Endosulfa...	9.300	0.000	246103	0	0.388	N.D. #
21)	B Endrin ke...	10.182	0.000	717066	0	0.995	N.D. #
24)	Chlordane-2	0.000	6.654	0	1174072	N.D.	16.885 #
25)	Chlordane-3	0.000	7.336	0	300306	N.D.	1.703 #
26)	Chlordane-4	0.000	7.383f	0	328707	N.D.	1.744 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062322\
Data File : PL075948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 23:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 05:12:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

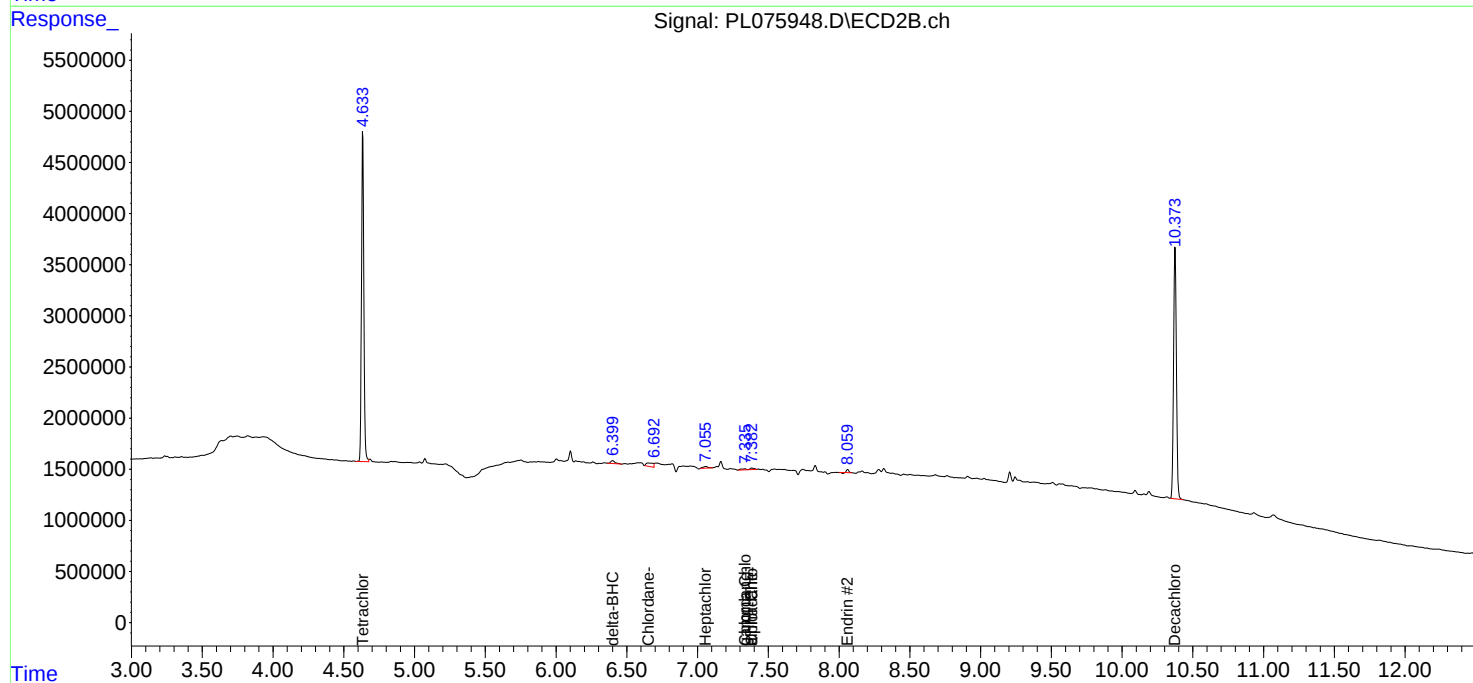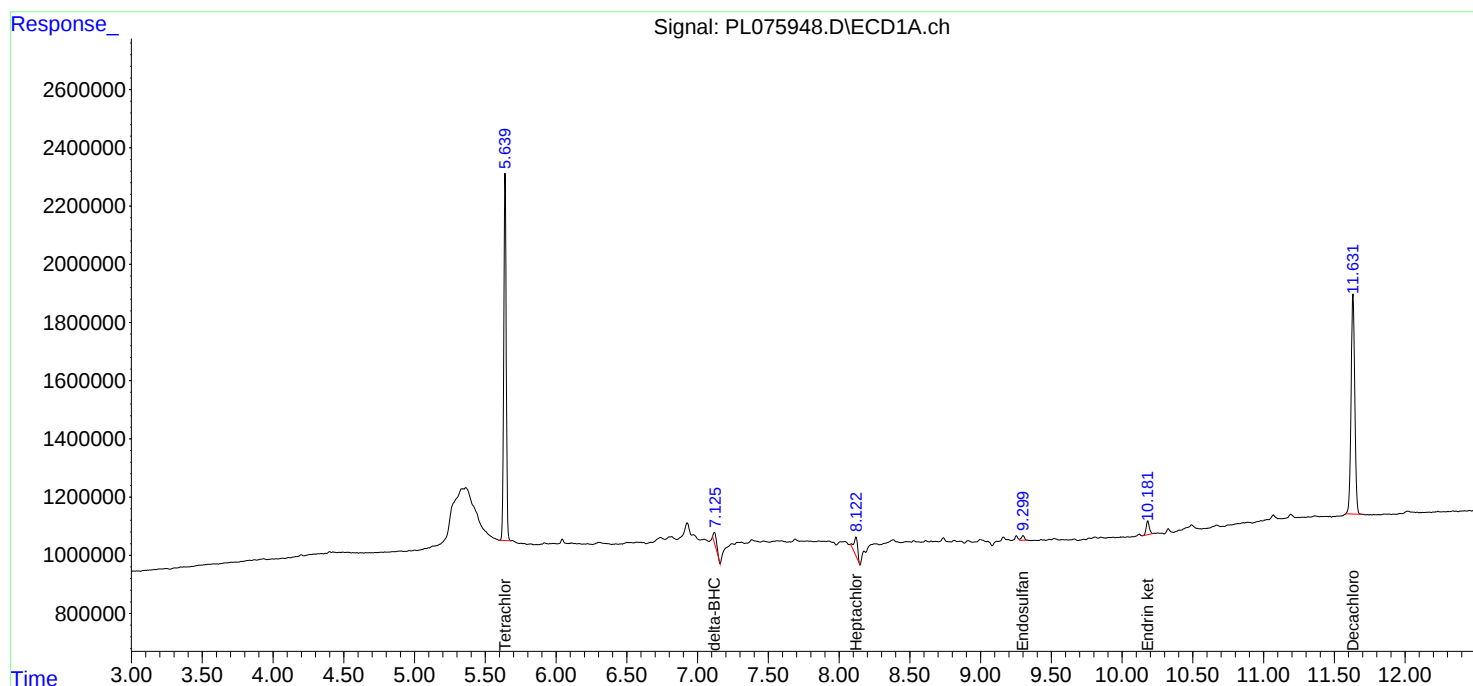


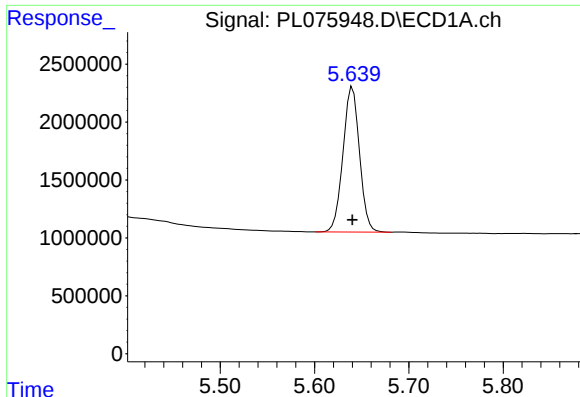

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 15263865
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

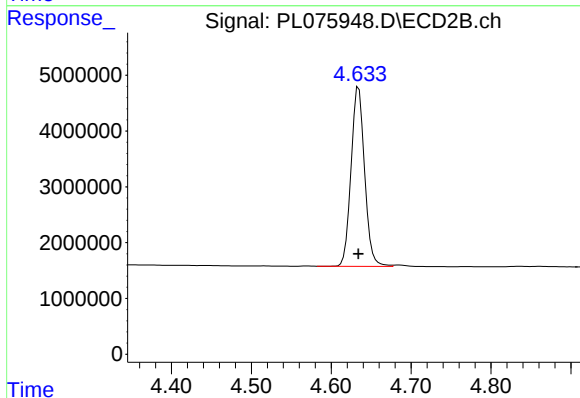


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 37964265
Conc: 20.02 ng/ml

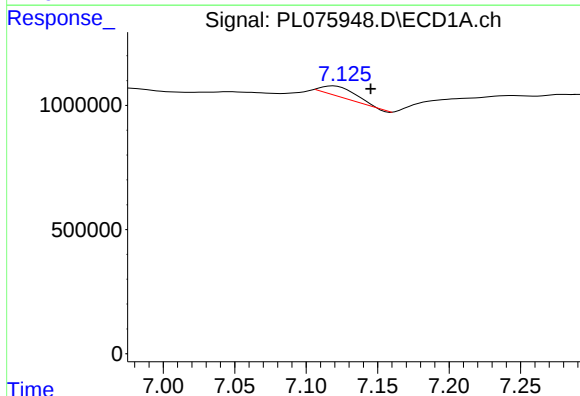


#7 delta-BHC

R.T.: 7.120 min
Delta R.T.: -0.026 min
Response: 672435
Conc: 0.86 ng/ml

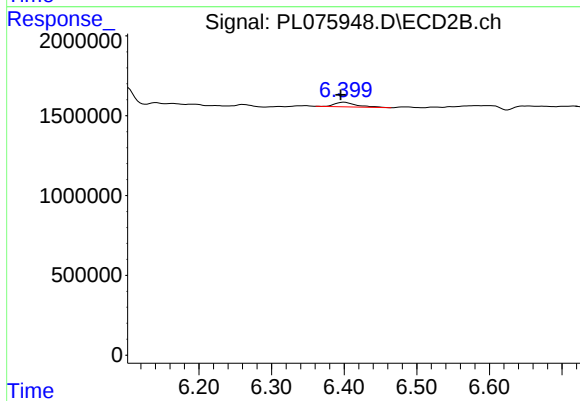

#7 delta-BHC


R.T.: 6.400 min
Delta R.T.: 0.005 min
Response: 604588
Conc: 0.27 ng/ml

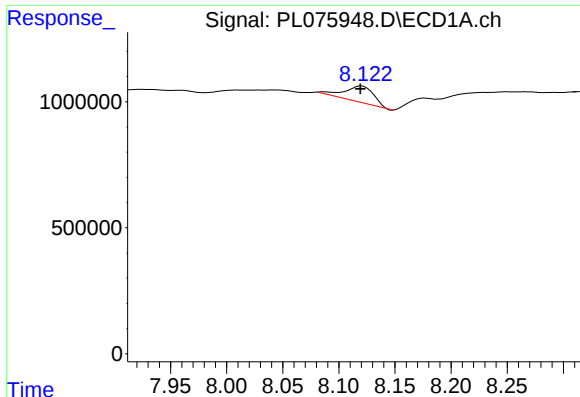

#8 Heptachlor epoxide


R.T.: 8.121 min
Delta R.T.: 0.002 min
Response: 1181842
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

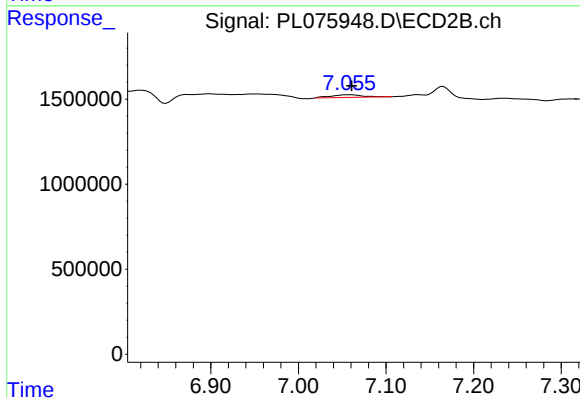


#8 Heptachlor epoxide

R.T.: 7.058 min
Delta R.T.: -0.003 min
Response: 395970
Conc: 0.21 ng/ml

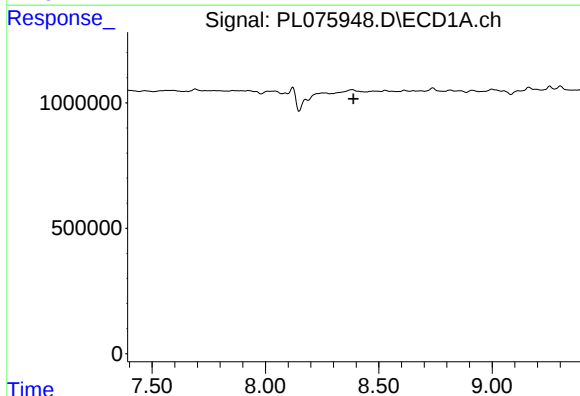


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.389 min
Response: 0
Conc: N.D.

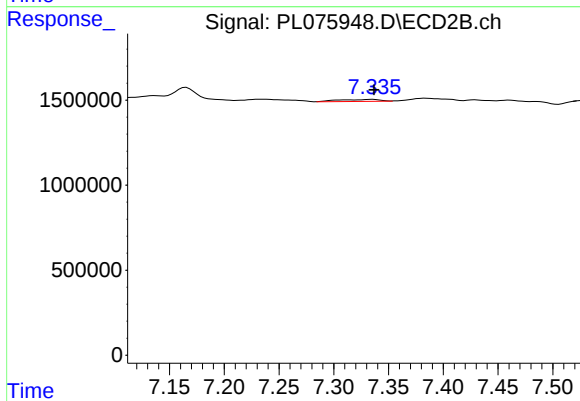

#10 gamma-Chlordane


R.T.: 7.336 min
Delta R.T.: 0.000 min
Response: 300306
Conc: 0.16 ng/ml

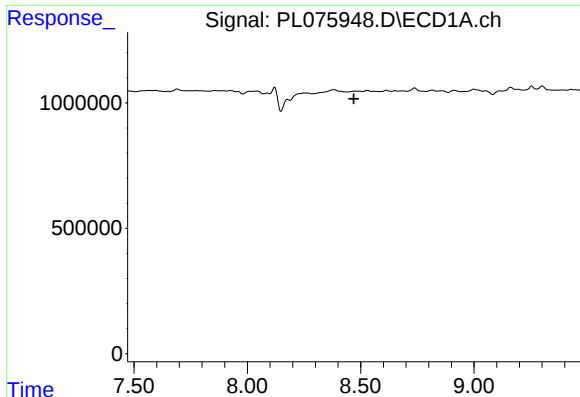

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

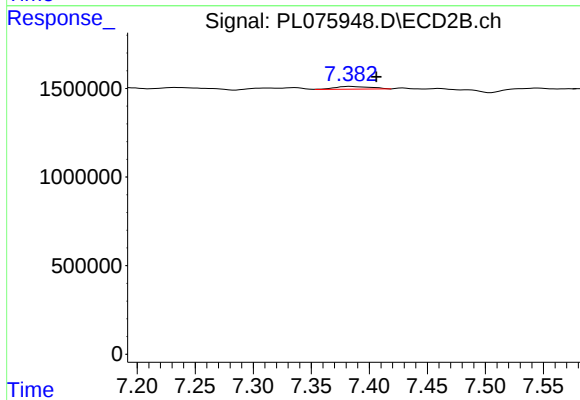


#11 alpha-Chlordane

R.T.: 7.383 min
Delta R.T.: -0.023 min
Response: 328707
Conc: 0.17 ng/ml

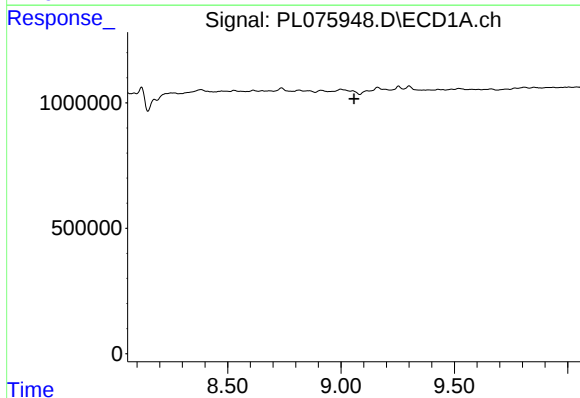


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

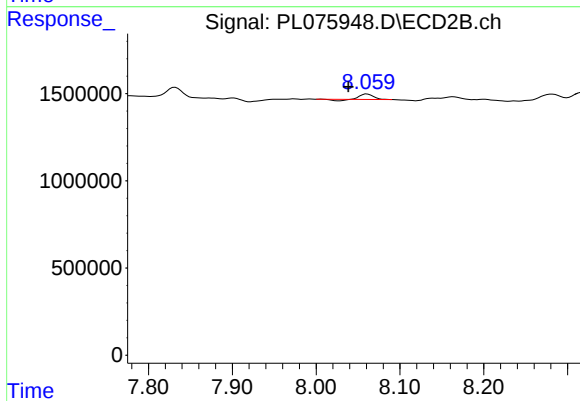

#14 Endrin


R.T.: 8.061 min
Delta R.T.: 0.023 min
Response: 279241
Conc: 0.18 ng/ml

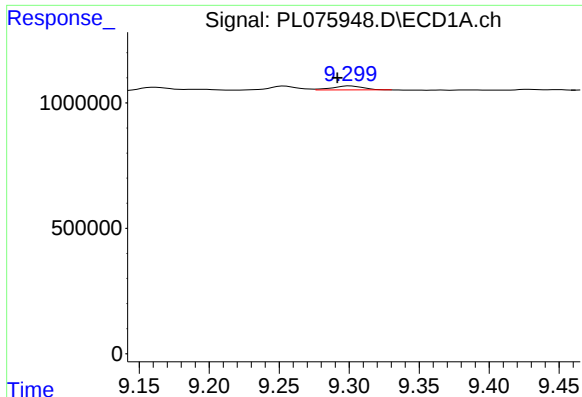

#15 Endosulfan II


R.T.: 9.300 min
Delta R.T.: 0.009 min
Response: 246103
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

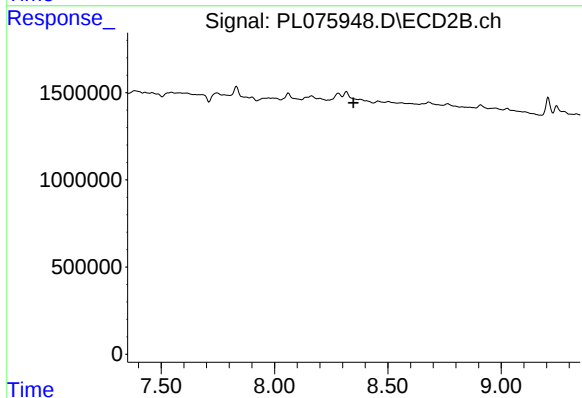


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

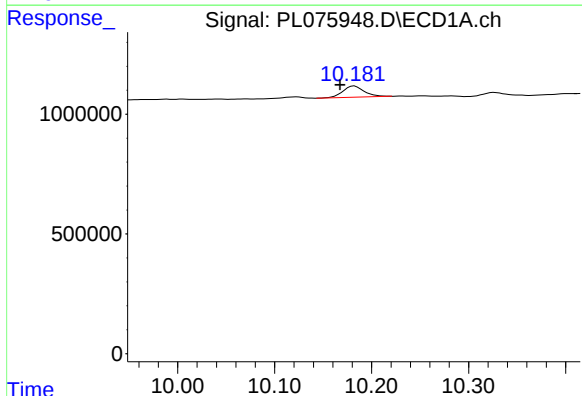


#21 Endrin ketone

R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 717066
Conc: 0.99 ng/ml

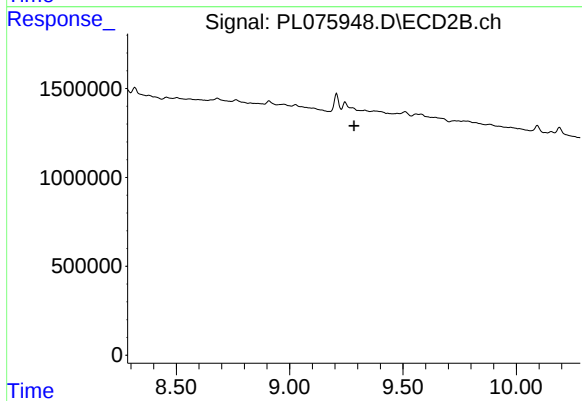

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

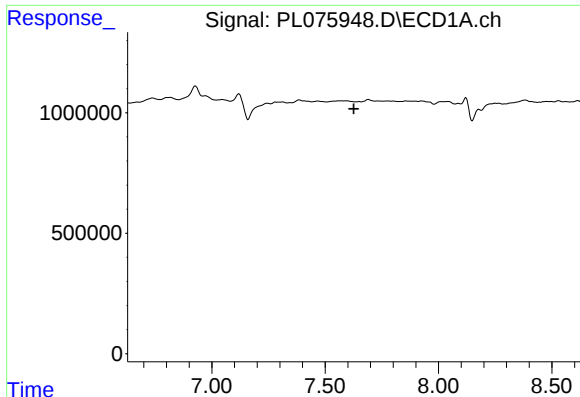

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.627 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

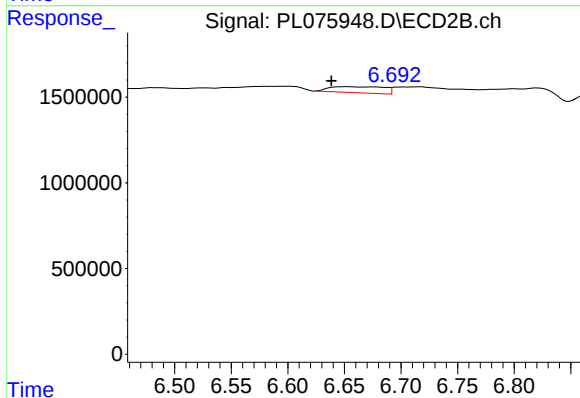


#24 Chlordane-2

R.T.: 6.654 min
Delta R.T.: 0.015 min
Response: 1174072
Conc: 16.88 ng/ml

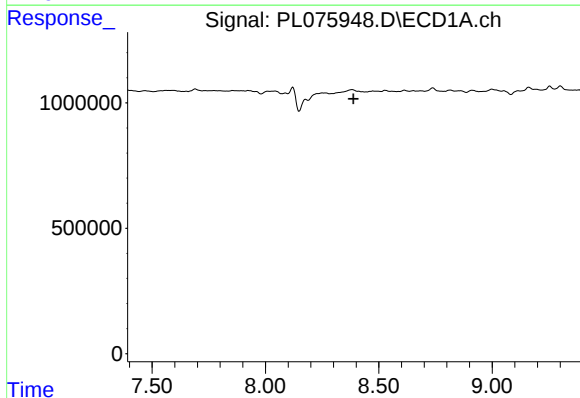


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

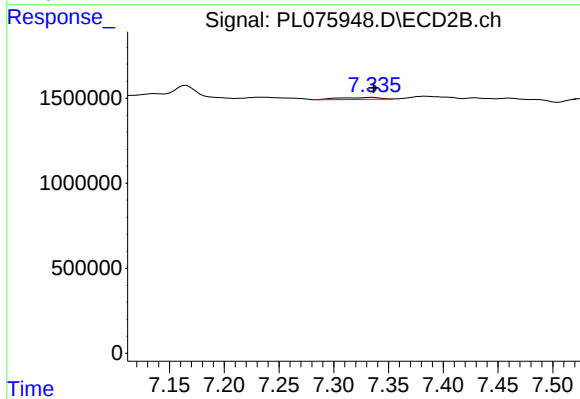

#25 Chlordane-3


R.T.: 7.336 min
Delta R.T.: 0.000 min
Response: 300306
Conc: 1.70 ng/ml

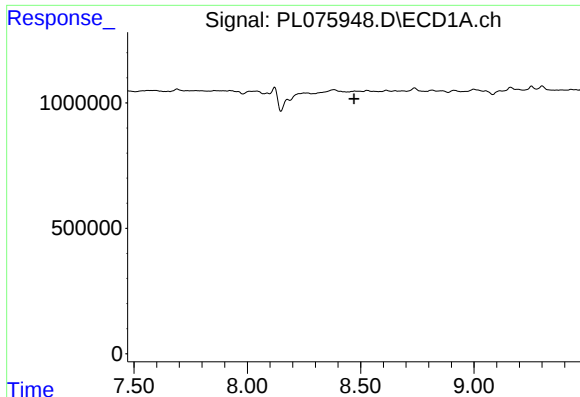

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

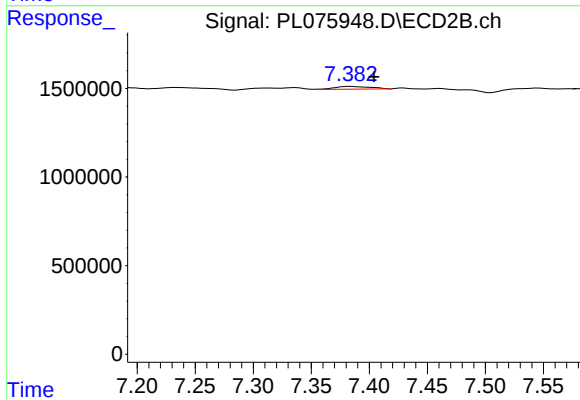


#26 Chlordane-4

R.T.: 7.383 min
Delta R.T.: -0.021 min
Response: 328707
Conc: 1.74 ng/ml

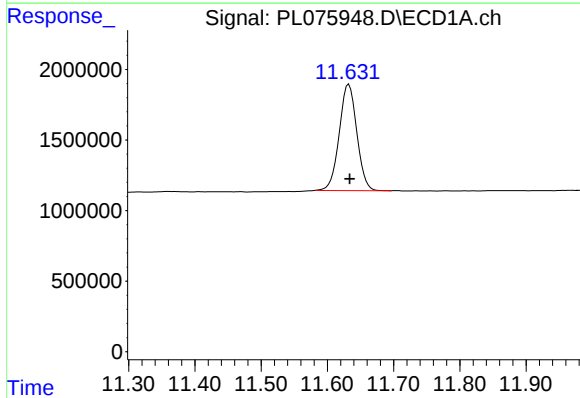

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: -0.001 min
Response: 13895601
Conc: 22.08 ng/ml

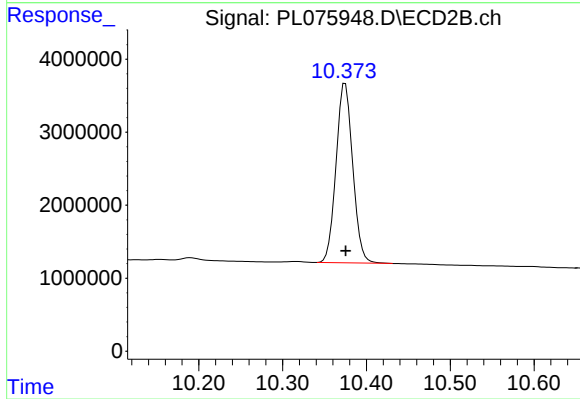

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 33989192
Conc: 22.13 ng/ml